


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030220\
 Data File : BN010035.D
 Acq On : 02 Mar 2020 11:46
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN021920.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 19 15:57:43 2020

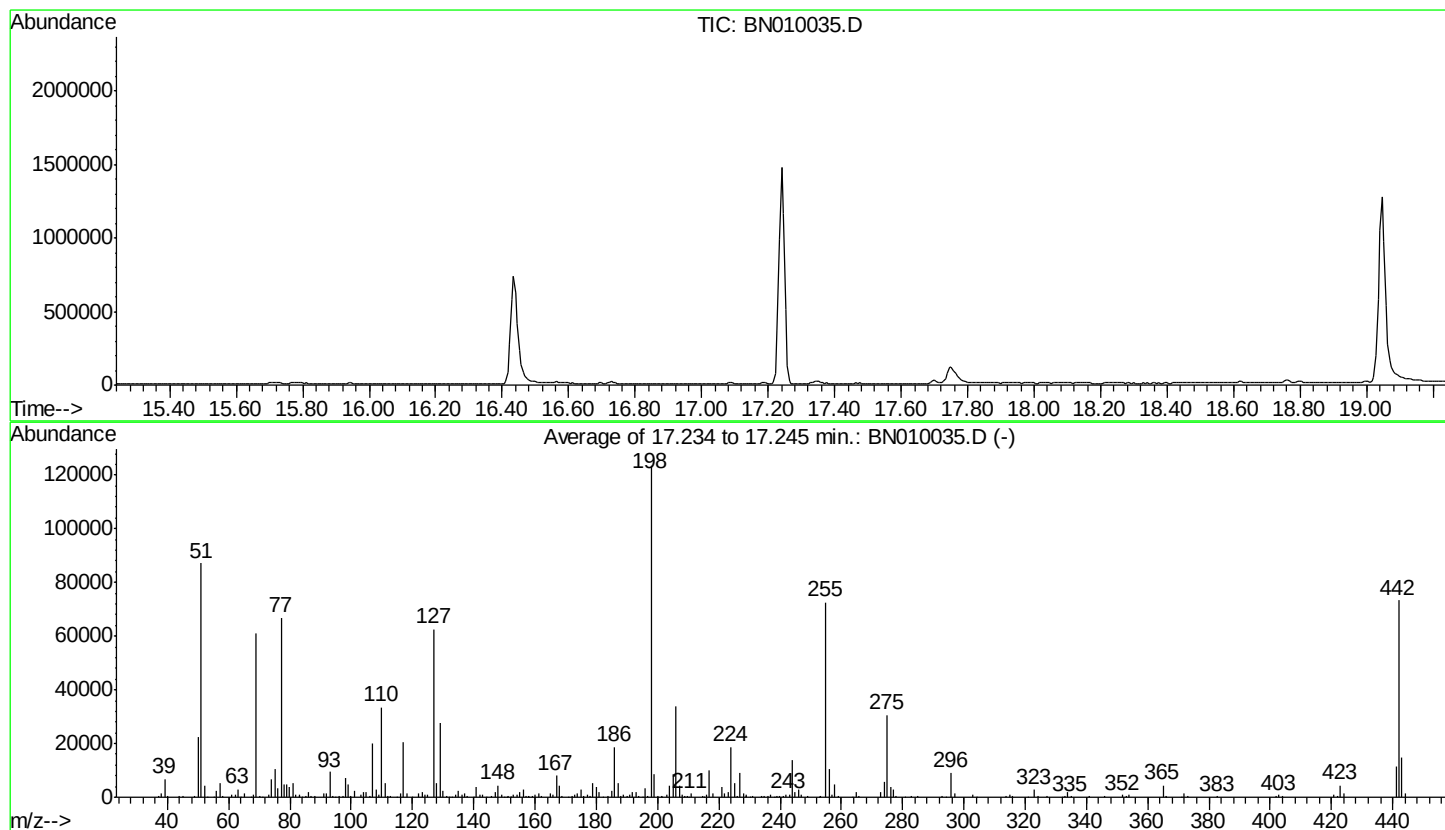

AutoFind: Scans 2422, 2423, 2424; Background Corrected with Scan 2416

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	70.6	87177	PASS
68	69	0.00	2	1.8	1117	PASS
69	198	0.00	100	49.6	61265	PASS
70	69	0.00	2	0.4	264	PASS
127	198	10	80	50.6	62514	PASS
197	198	0.00	2	0.5	603	PASS
198	198	100	100	100.0	123498	PASS
199	198	5	9	7.0	8690	PASS
275	198	10	60	24.8	30637	PASS
365	198	1	100	3.5	4317	PASS
441	198	0.01	100	9.4	11647	PASS
442	198	50	100	59.3	73240	PASS
443	442	15	24	20.2	14816	PASS