

Data File : BN010046.D

Acq On : 02 Mar 2020 18:49

Operator : CG/JU

Sample : L1619-01

Misc :

ALS Vial : 4 Sample Multiplier: 1




Quant Time: Mar 03 01:07:44 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Tue Mar 03 01:05:31 2020

Response via : Initial Calibration

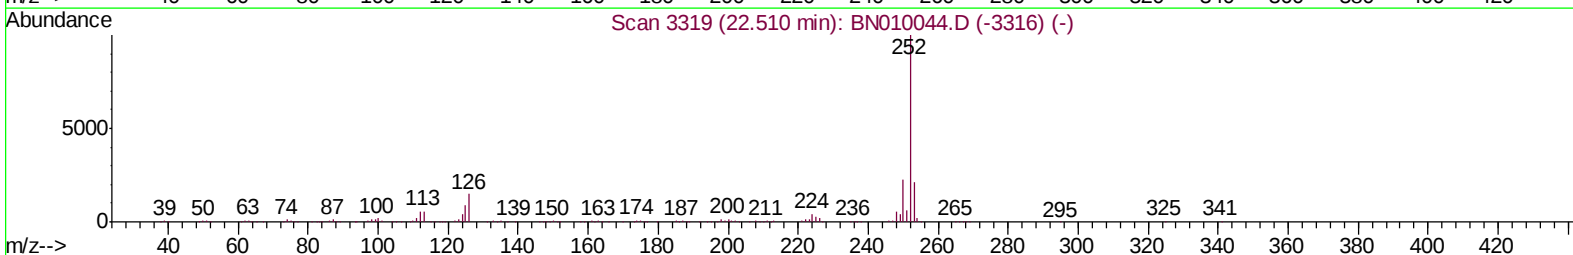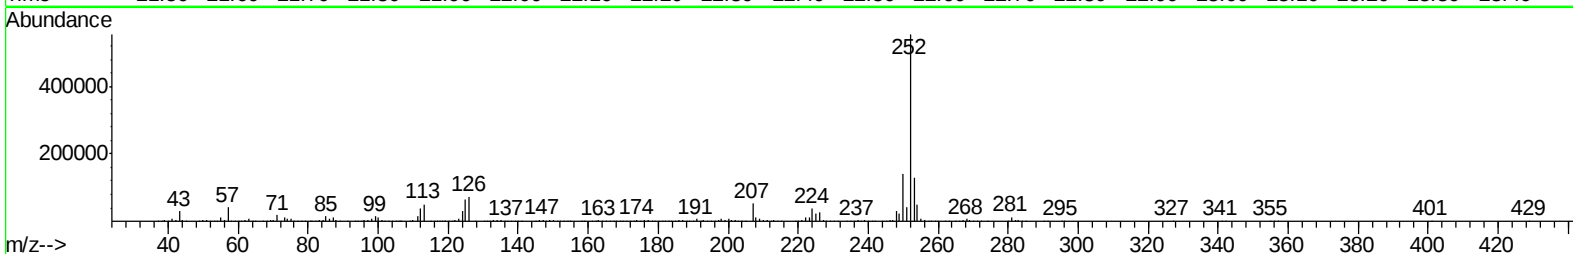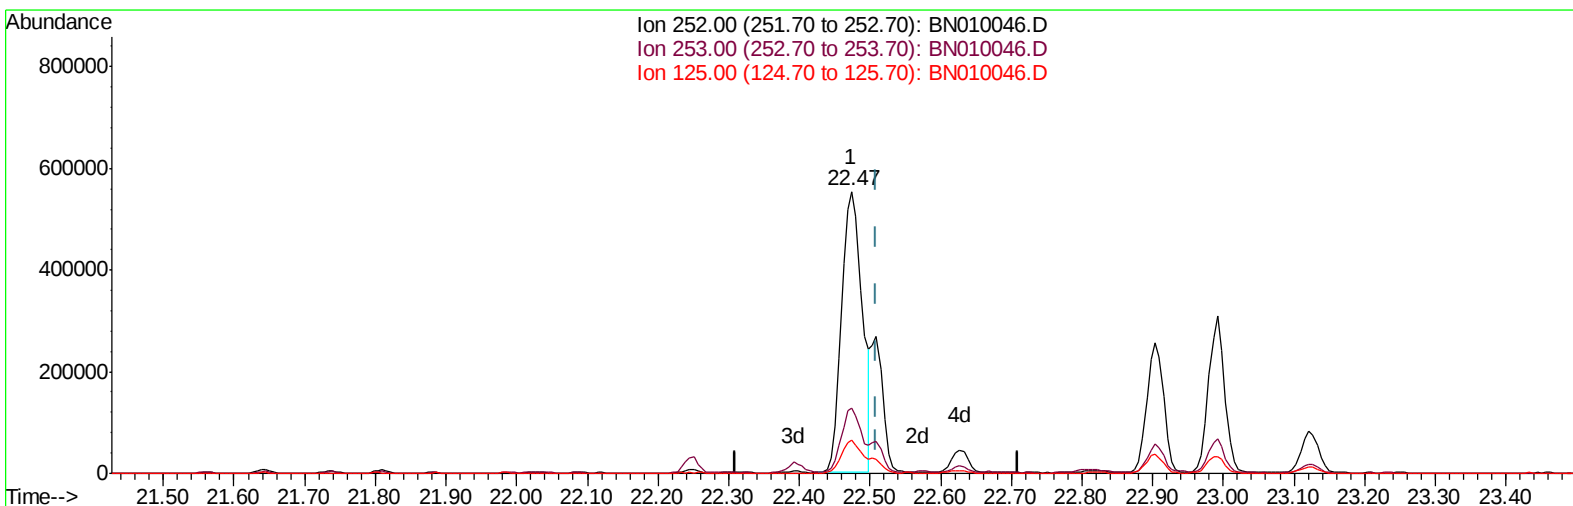

TIC: BN010046.D

(89) Benzo(k)fluoranthene

22.474min (-0.036) 33.07ng/ul

response 1131794

Ion	Exp%	Act%
252.00	100	100
253.00	22.50	23.21
125.00	10.20	11.69
0.00	0.00	0.00