
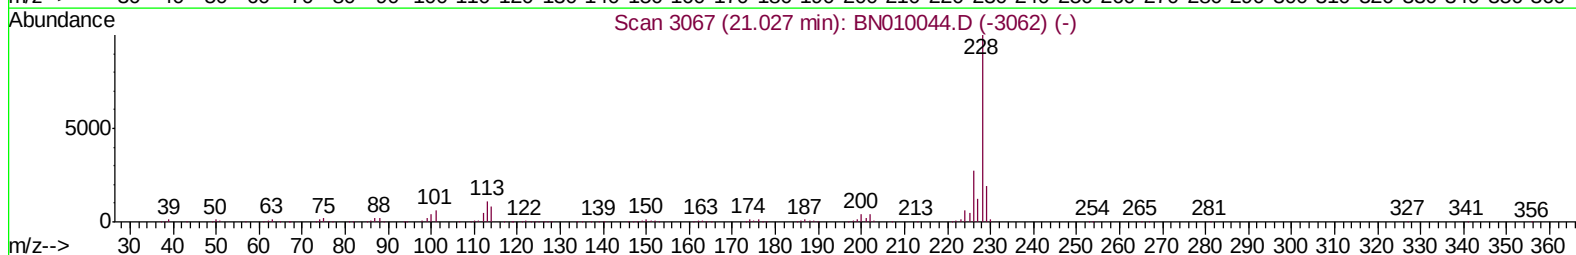
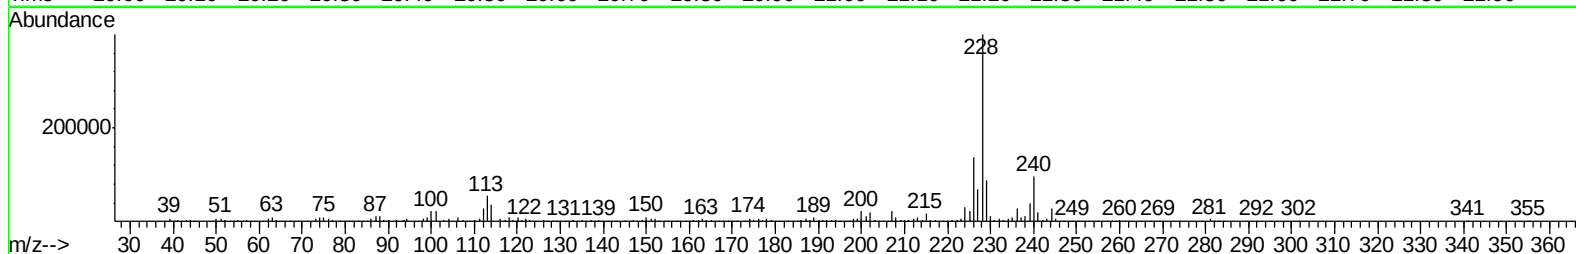


Data File : BN010047.D
Acq On : 02 Mar 2020 19:25
Operator : CG/JU
Sample : L1619-02MS
Misc :
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Mar 03 01:07:58 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 03 01:05:31 2020
Response via : Initial Calibration

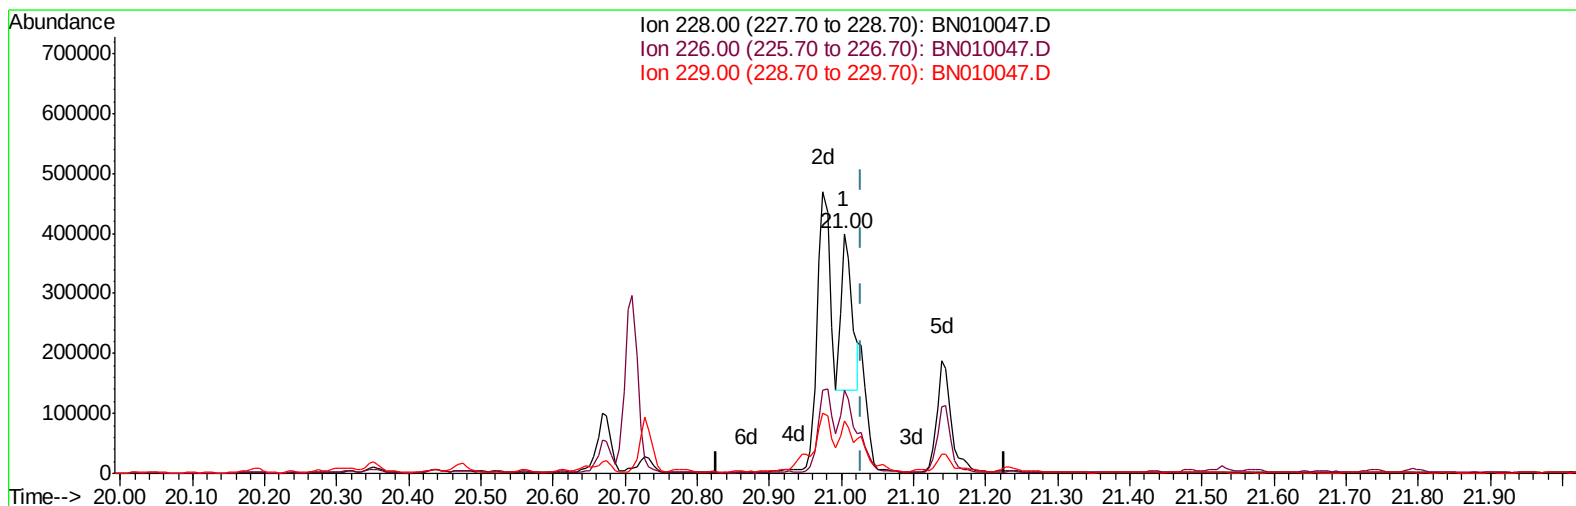

TIC: BN010047.D

(85) Chrysene

21.004min (-0.024) 7.92ng/ul

response 278808

Ion	Exp%	Act%
228.00	100	100
226.00	29.30	34.53
229.00	18.70	21.99
0.00	0.00	0.00