
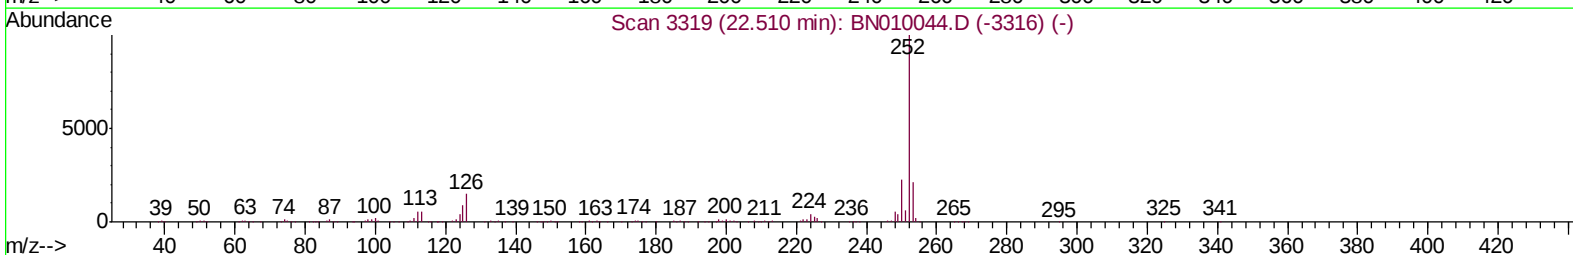
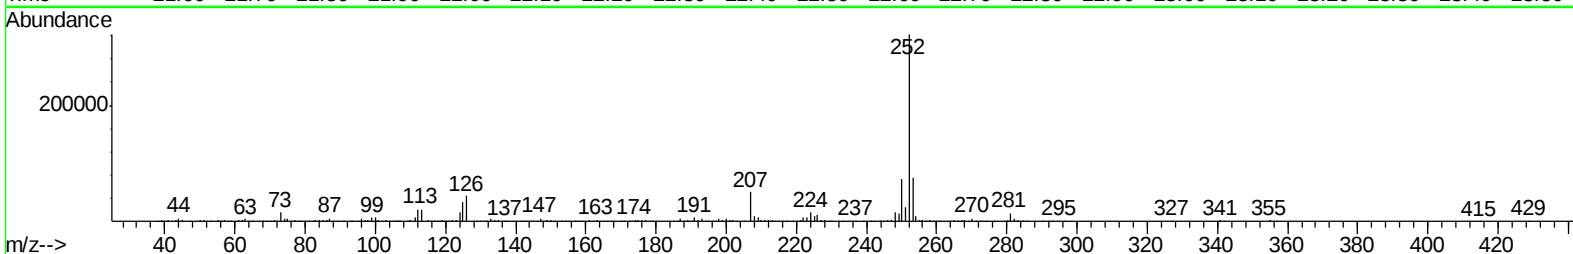


Data File : BN010047.D
Acq On : 02 Mar 2020 19:25
Operator : CG/JU
Sample : L1619-02MS
Misc :
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Mar 03 01:07:58 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 03 01:05:31 2020
Response via : Initial Calibration

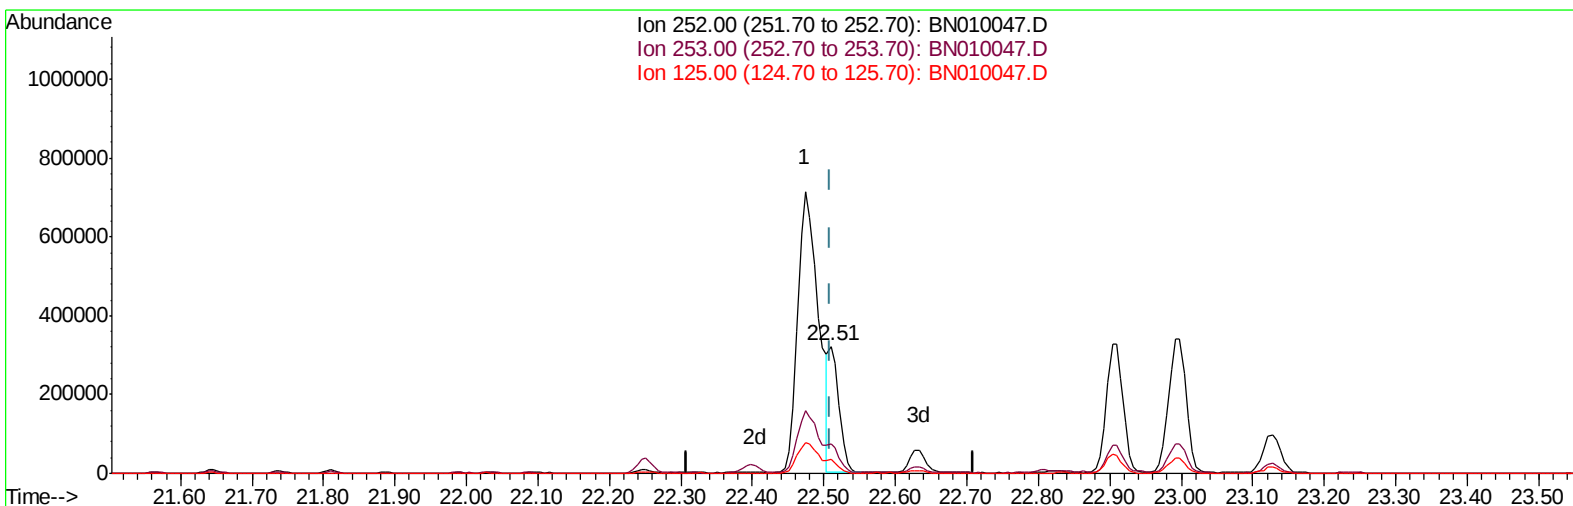

TIC: BN010047.D

(89) Benzo(k)fluoranthene

22.510min (+0.000) 8.82ng/ul m

response 309822

Ion	Exp%	Act%
252.00	100	100
253.00	22.50	23.17
125.00	10.20	10.71
0.00	0.00	0.00