

Data File : BN010047.D

Acq On : 02 Mar 2020 19:25

Operator : CG/JU

Sample : L1619-02MS

Misc :

ALS Vial : 5 Sample Multiplier: 1




Quant Time: Mar 03 01:07:58 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Tue Mar 03 01:05:31 2020

Response via : Initial Calibration

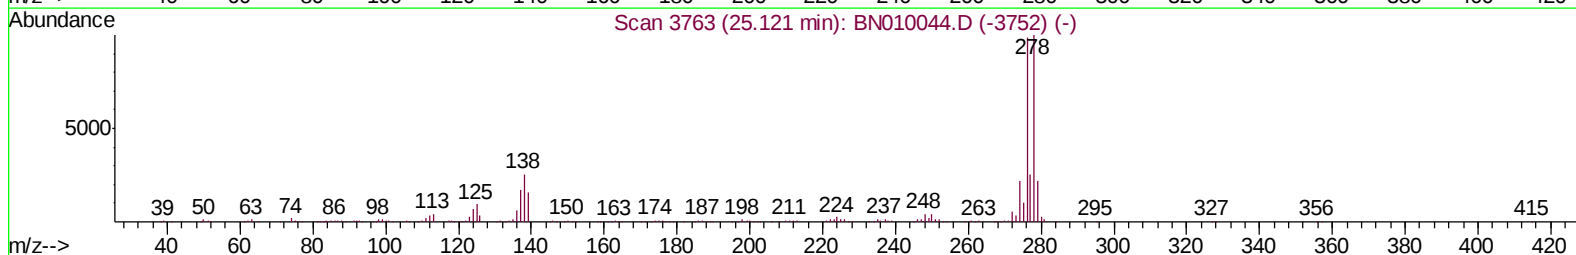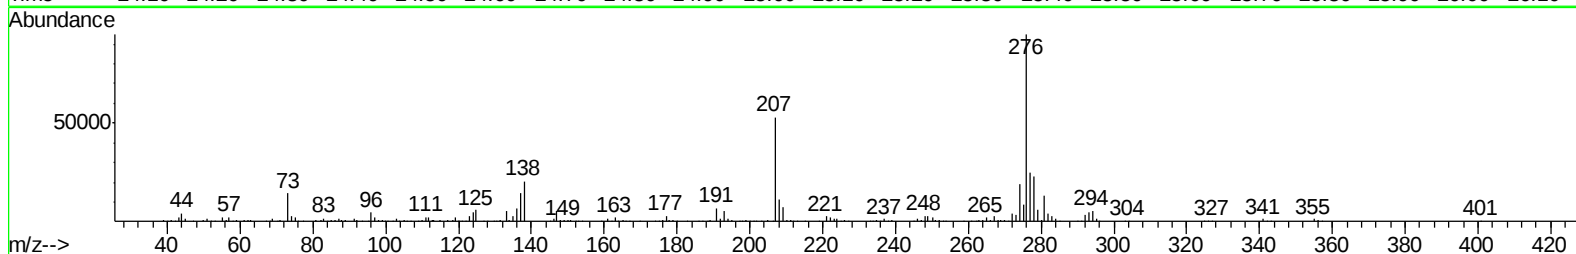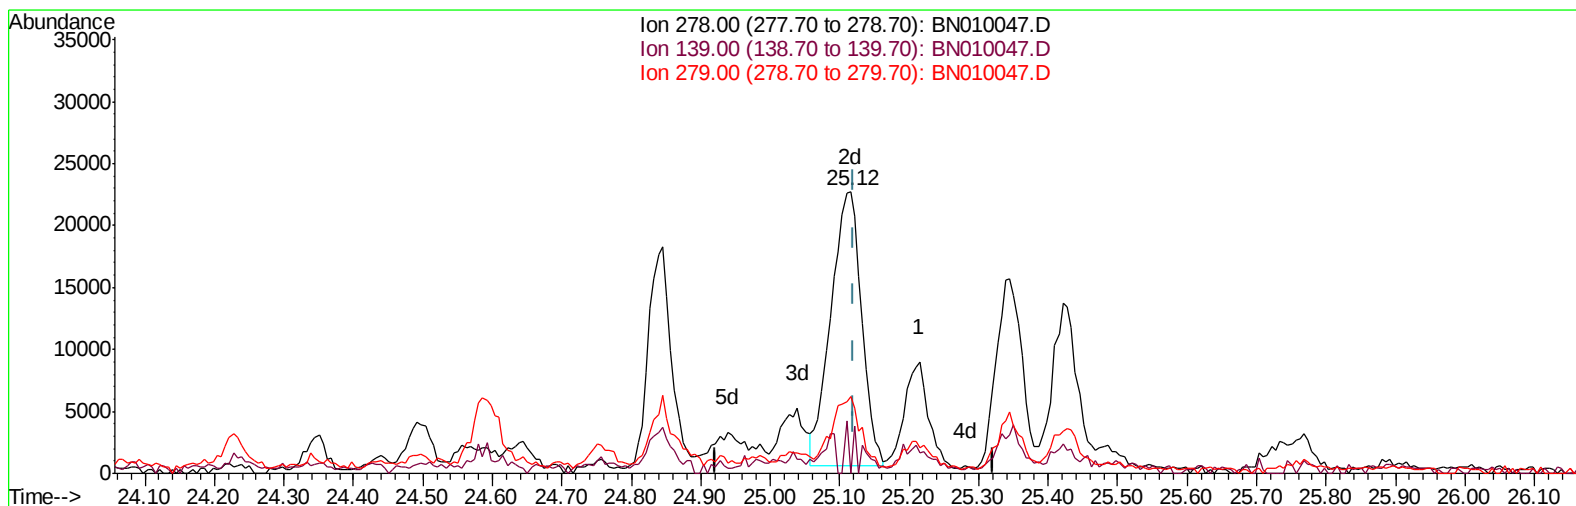

TIC: BN010047.D

(93) Dibenzo(a,h)anthracene

25.115min (-0.006) 2.00ng/ul m

response 67894

Ion	Exp%	Act%
278.00	100	100
139.00	16.20	0.00#
279.00	21.90	27.27#
0.00	0.00	0.00