
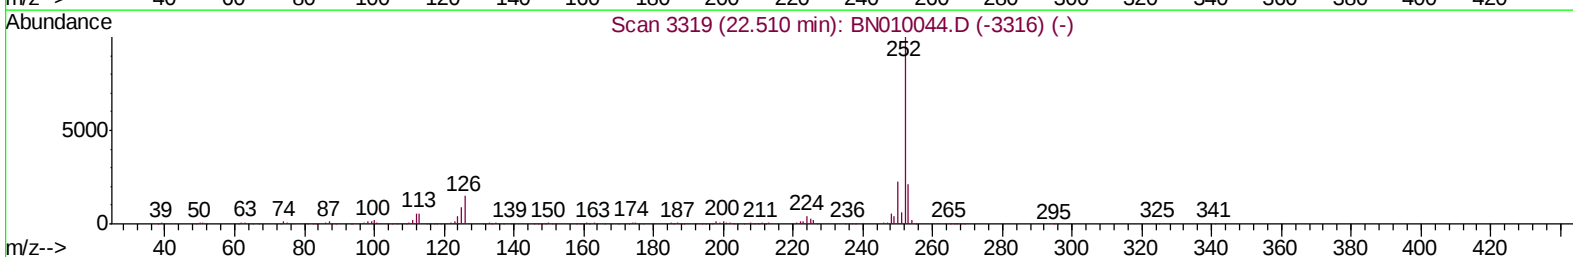
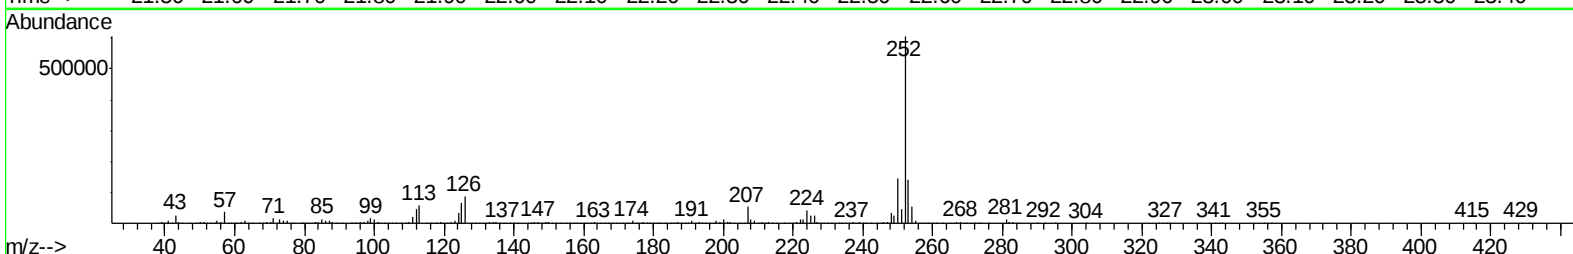


Data File : BN010048.D
Acq On : 02 Mar 2020 20:01
Operator : CG/JU
Sample : L1619-03MSD
Misc :
ALS Vial : 6 Sample Multiplier: 1

Quant Time: Mar 03 01:08:14 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 03 01:05:31 2020
Response via : Initial Calibration

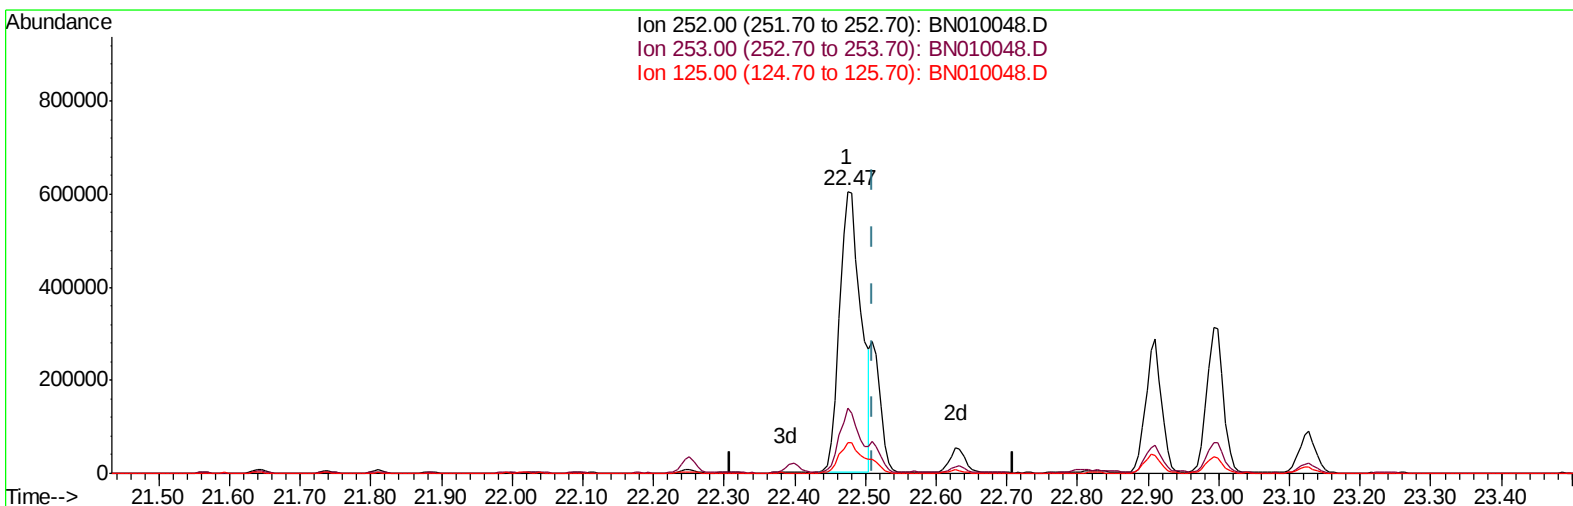

TIC: BN010048.D

(89) Benzo(k)fluoranthene

22.474min (-0.035) 39.49ng/ul

response 1283574

Ion	Exp%	Act%
252.00	100	100
253.00	22.50	23.41
125.00	10.20	11.00
0.00	0.00	0.00