

Data File : BN010048.D

Acq On : 02 Mar 2020 20:01

Operator : CG/JU

Sample : L1619-03MSD

Misc :

ALS Vial : 6 Sample Multiplier: 1




Quant Time: Mar 03 01:08:14 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Tue Mar 03 01:05:31 2020

Response via : Initial Calibration

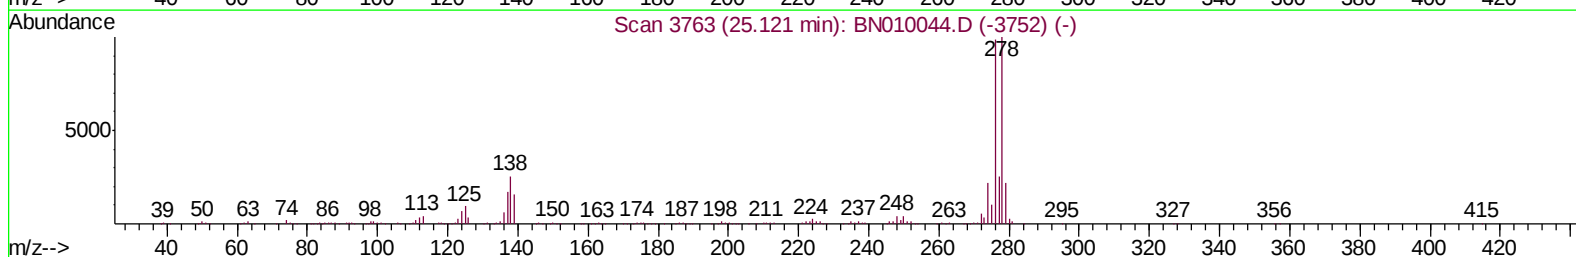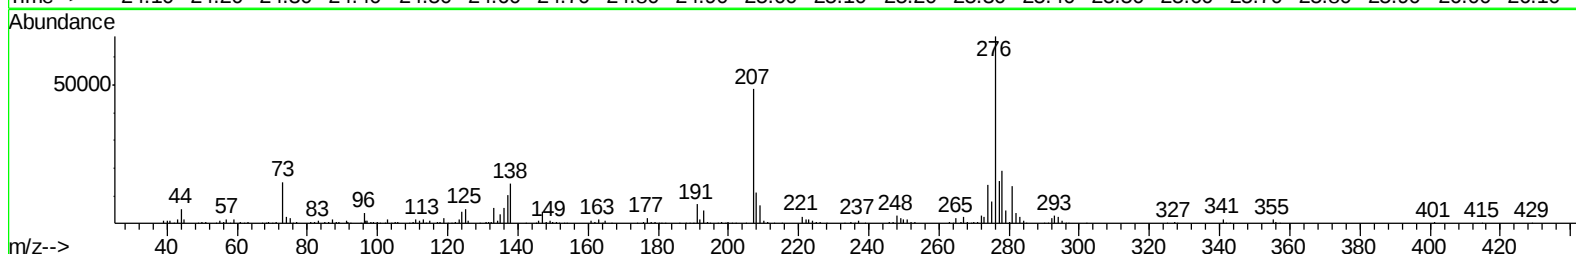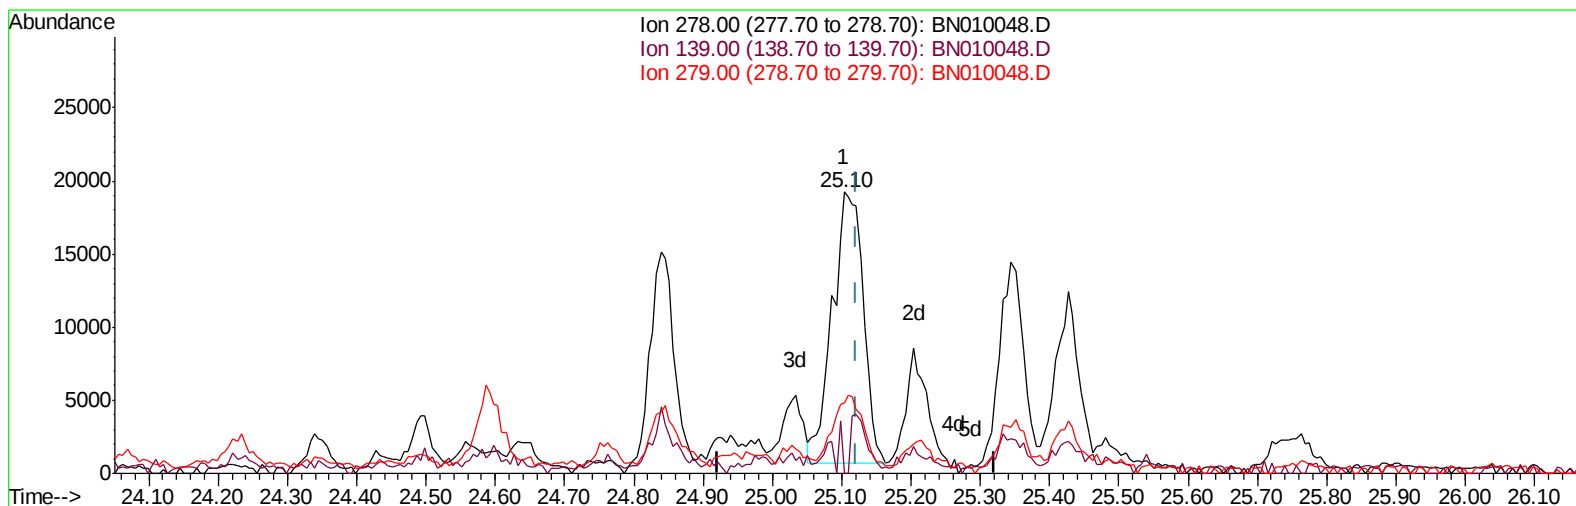

TIC: BN010048.D

(93) Dibenzo(a,h)anthracene

25.104min (-0.017) 1.83ng/ul m

response 57445

Ion	Exp%	Act%
278.00	100	100
139.00	16.20	0.00#
279.00	21.90	25.07
0.00	0.00	0.00