
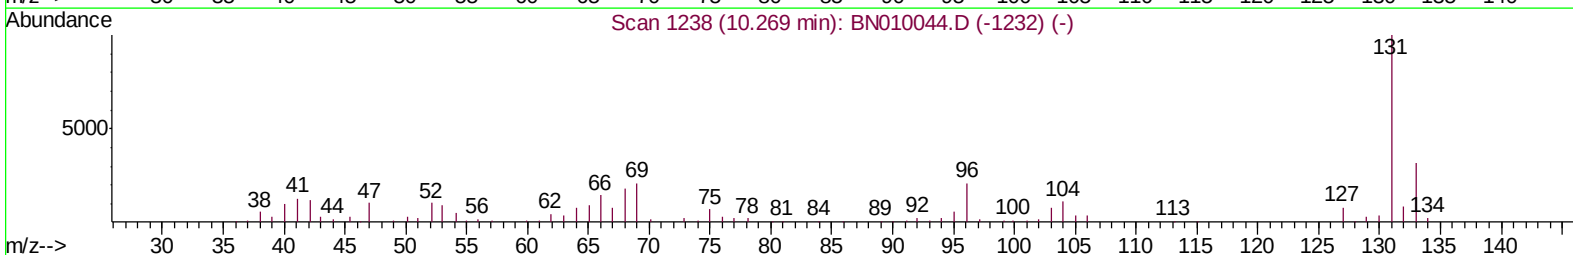
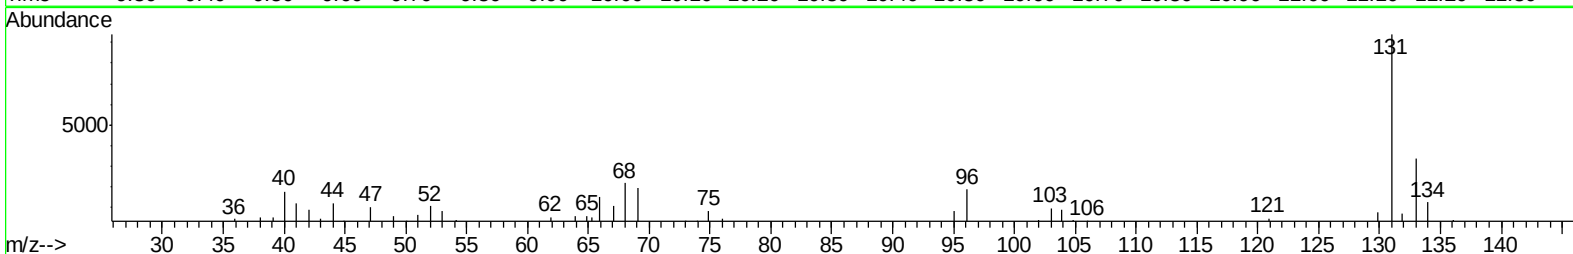


Data File : BN010049.D
Acq On : 02 Mar 2020 20:38
Operator : CG/JU
Sample : L1619-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Quant Time: Mar 03 01:08:34 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 03 01:05:31 2020
Response via : Initial Calibration

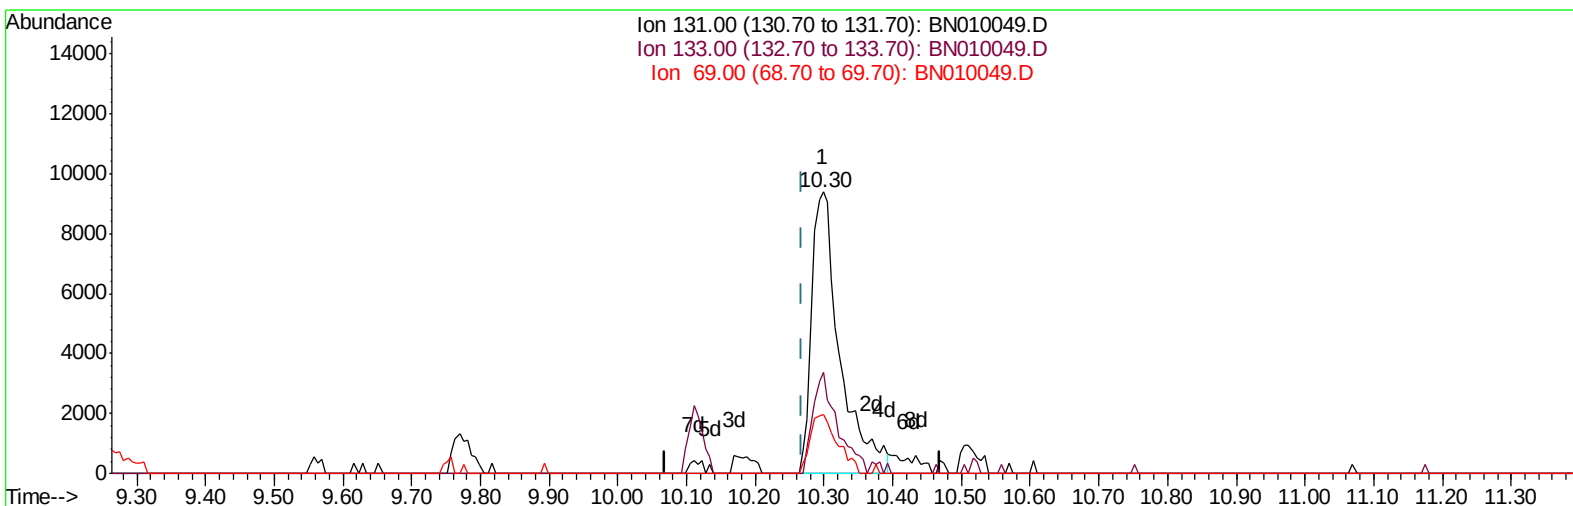

TIC: BN010049.D

(29) 4-Chloroaniline-d4 (S)
10.299min (+0.030) 3.42ng/ul m
response 26660

Ion	Exp%	Act%
131.00	100	100
133.00	33.00	35.98
69.00	22.10	21.00
0.00	0.00	0.00