
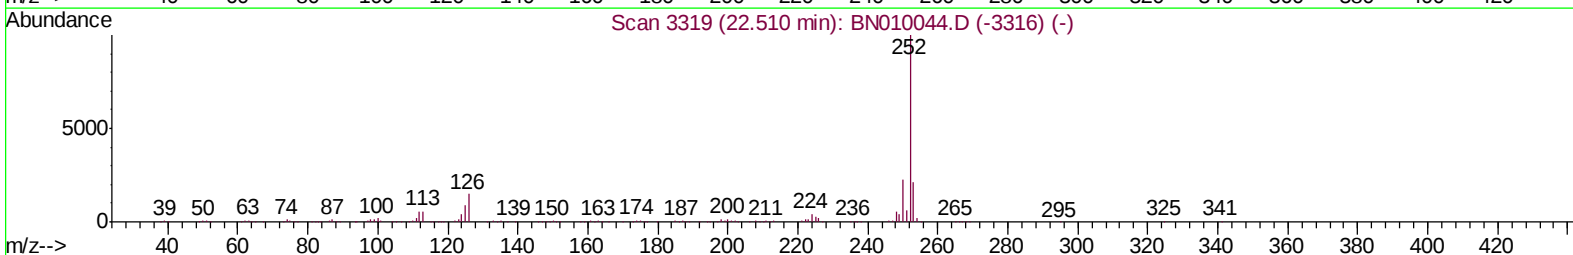
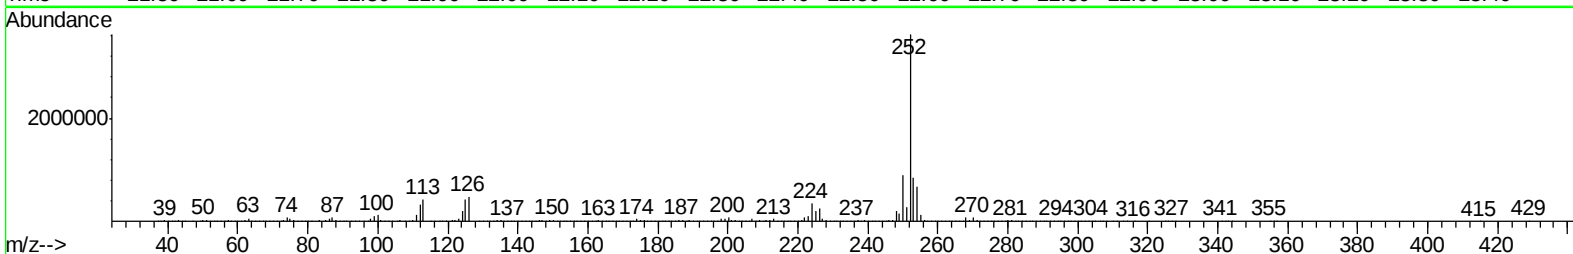


Data File : BN010049.D
Acq On : 02 Mar 2020 20:38
Operator : CG/JU
Sample : L1619-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Quant Time: Mar 03 01:08:34 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 03 01:05:31 2020
Response via : Initial Calibration

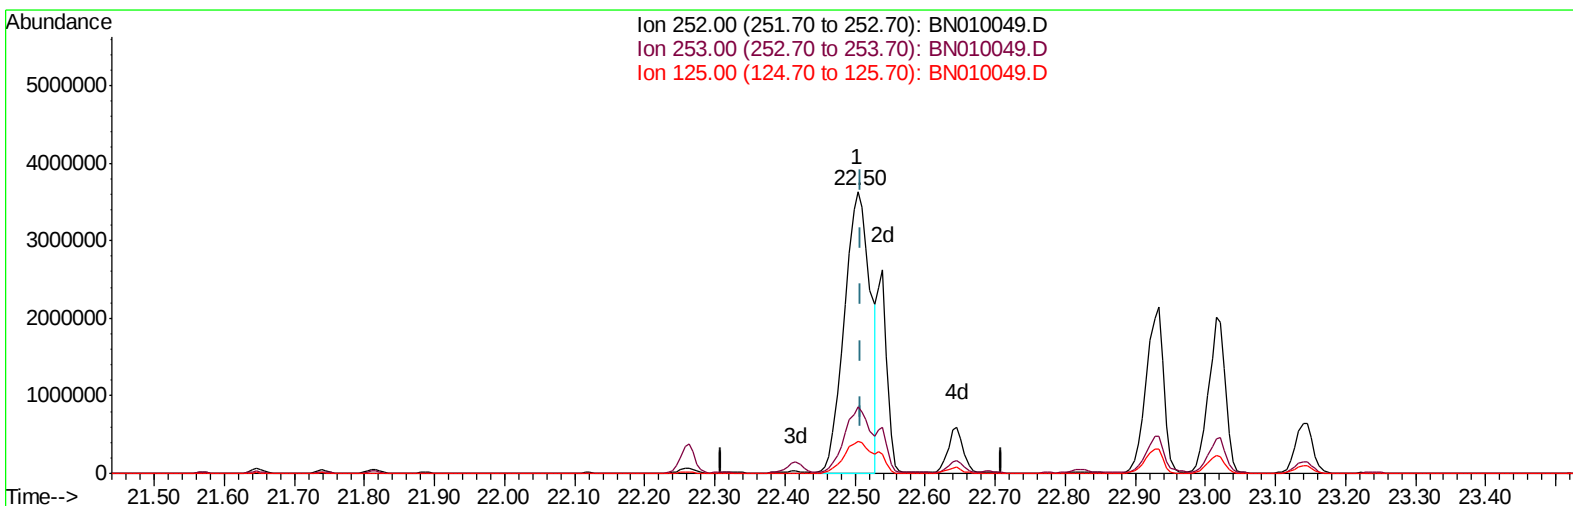

TIC: BN010049.D

(89) Benzo(k)fluoranthene

22.504min (-0.006) 280.99ng/ul

response 9262842

Ion	Exp%	Act%
252.00	100	100
253.00	22.50	23.46
125.00	10.20	11.34
0.00	0.00	0.00