

Data File : BN010049.D

Acq On : 02 Mar 2020 20:38

Operator : CG/JU

Sample : L1619-04

Misc :

ALS Vial : 7 Sample Multiplier: 1




Quant Time: Mar 03 01:08:34 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Tue Mar 03 01:05:31 2020

Response via : Initial Calibration

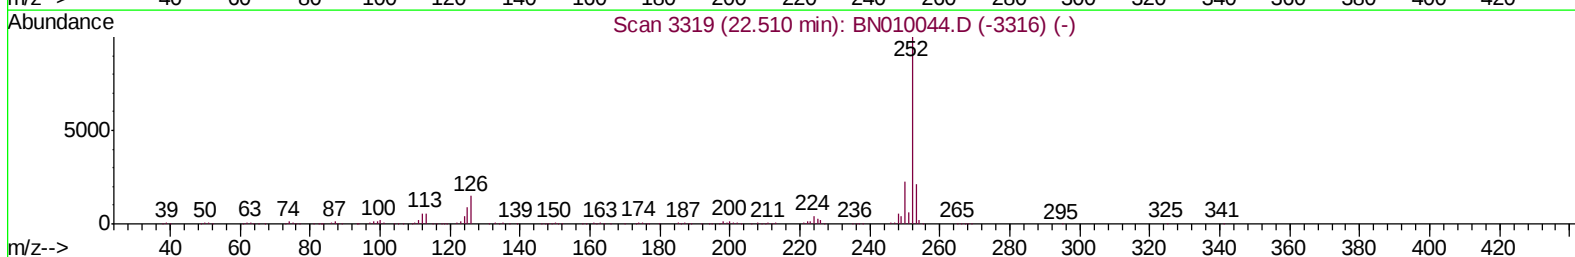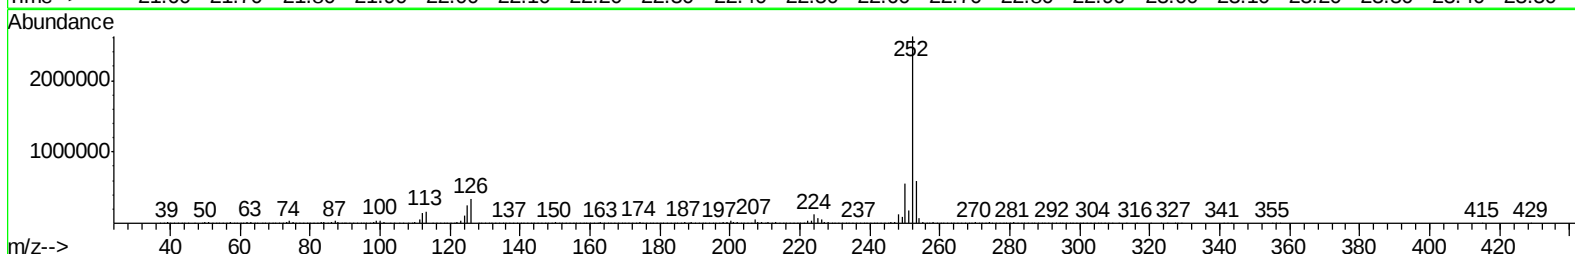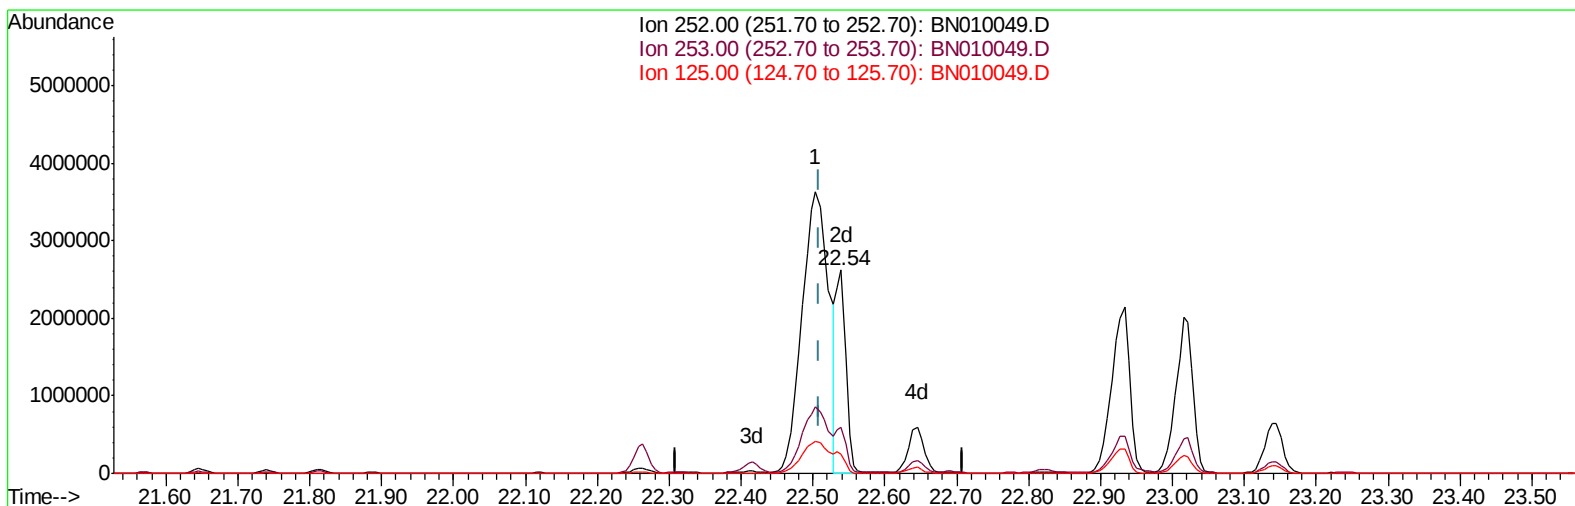

TIC: BN010049.D

(89) Benzo(k)fluoranthene

22.539min (+0.030) 76.32ng/ul m

response 2515933

Ion	Exp%	Act%
252.00	100	100
253.00	22.50	22.81
125.00	10.20	9.47
0.00	0.00	0.00