
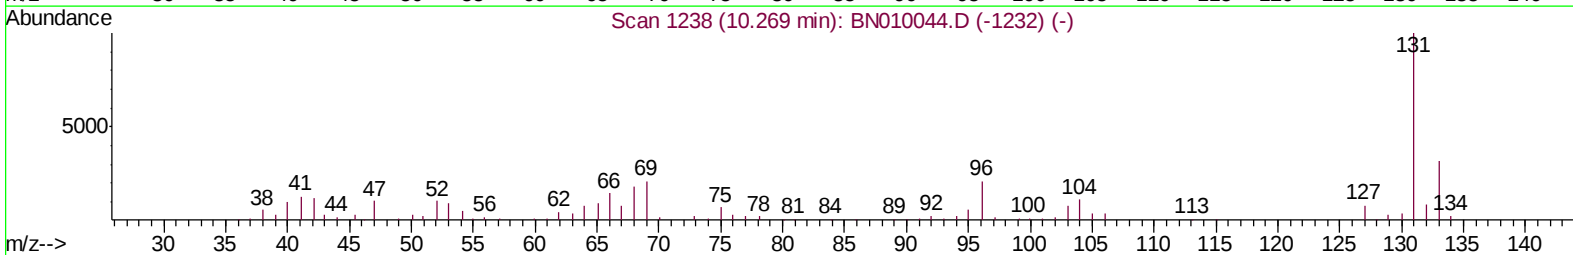
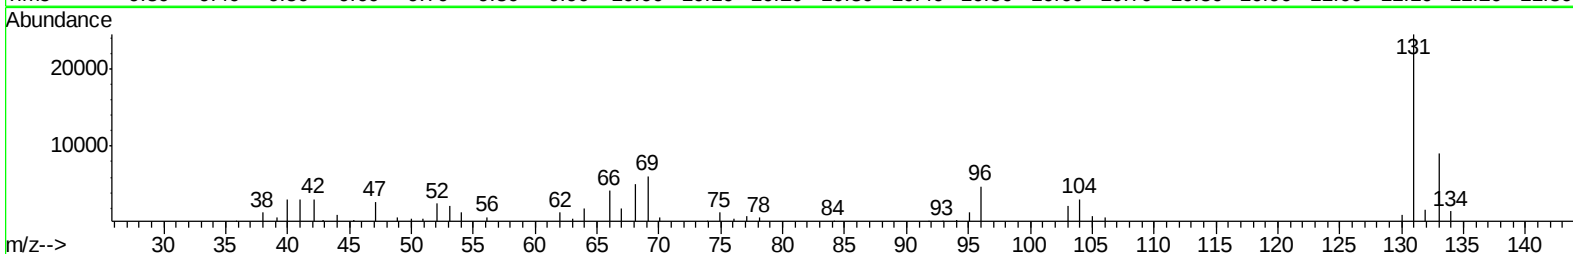


Data File : BN010051.D
Acq On : 02 Mar 2020 21:51
Operator : CG/JU
Sample : L1619-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Quant Time: Mar 03 01:08:59 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 03 01:05:31 2020
Response via : Initial Calibration

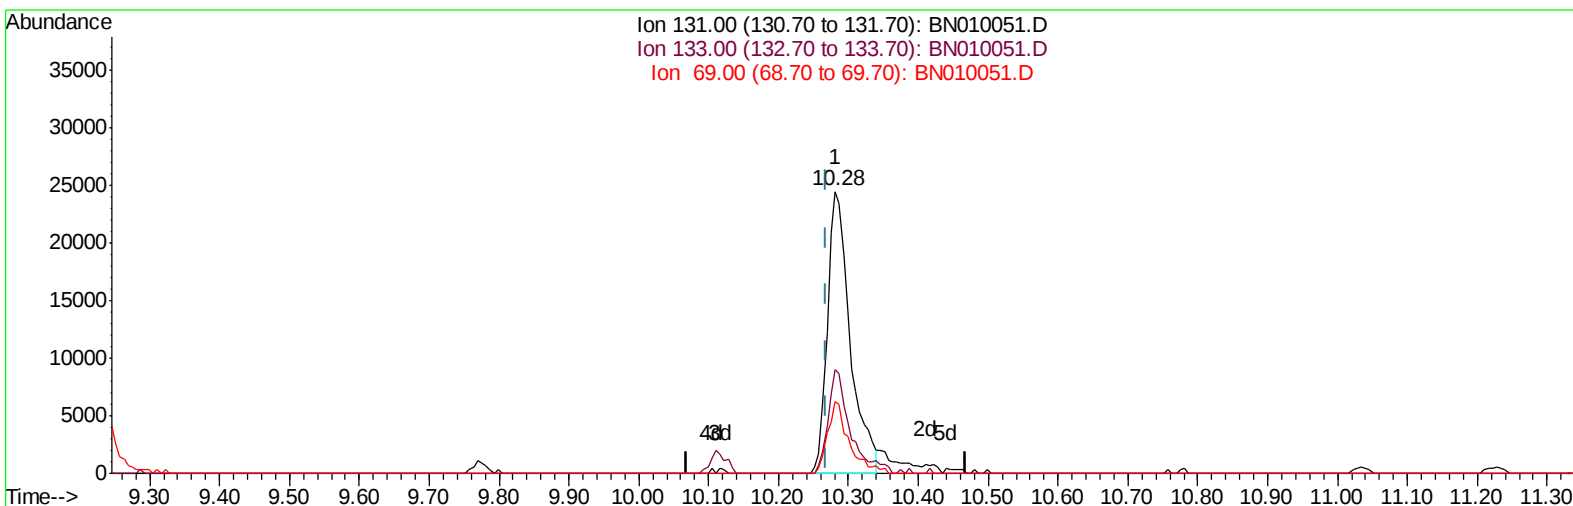

TIC: BN010051.D

(29) 4-Chloroaniline-d4 (S)
10.281min (+0.012) 7.85ng/ul
response 55048

Ion	Exp%	Act%
131.00	100	100
133.00	33.00	36.91
69.00	22.10	25.26
0.00	0.00	0.00