
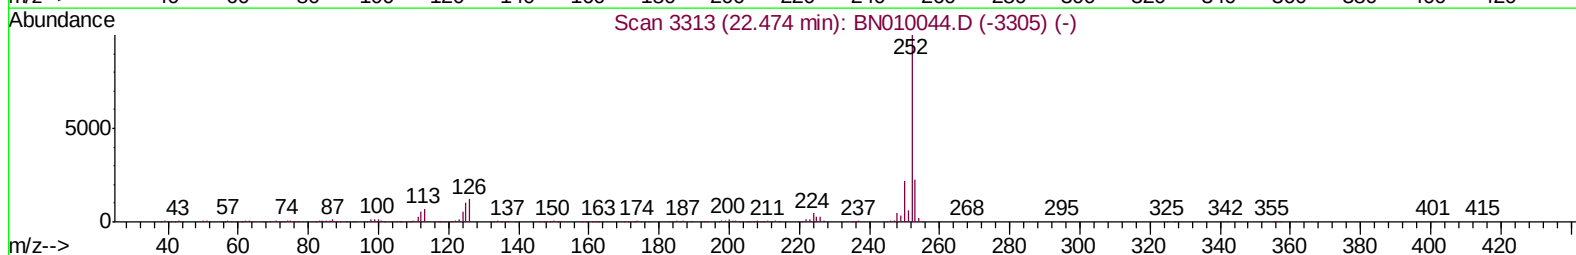
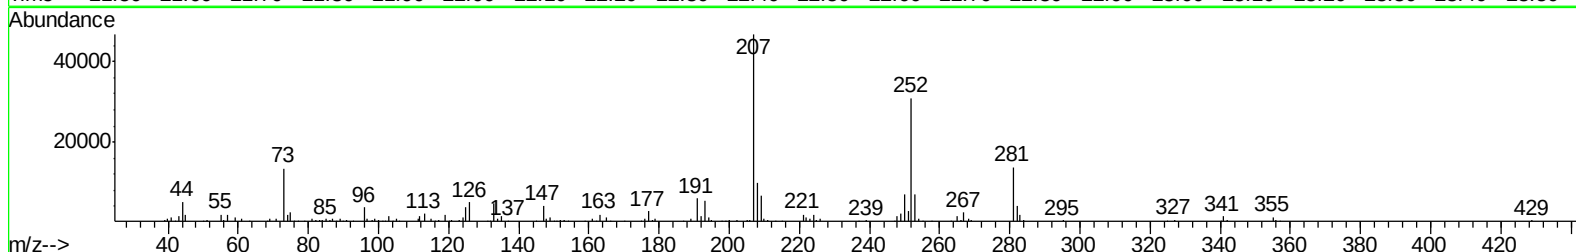


Data File : BN010051.D  
Acq On : 02 Mar 2020 21:51  
Operator : CG/JU  
Sample : L1619-06  
Misc :  
ALS Vial : 9 Sample Multiplier: 1

Quant Time: Mar 03 01:08:59 2020  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\SOM-EPA-BN021220MA.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Tue Mar 03 01:05:31 2020  
Response via : Initial Calibration

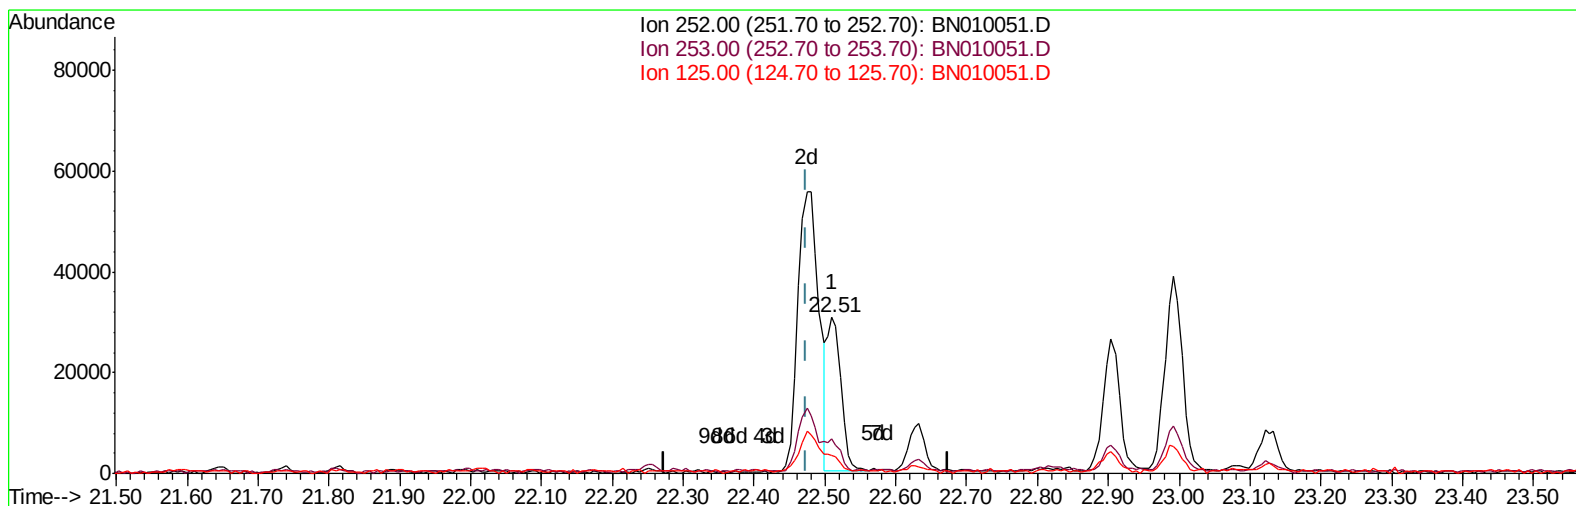

TIC: BN010051.D

(88) Benzo(b)fluoranthene  
22.510min (+0.035) 1.35ng/ul  
response 41912

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 252.00 | 100   | 100   |
| 253.00 | 21.20 | 22.42 |
| 125.00 | 10.00 | 11.88 |
| 0.00   | 0.00  | 0.00  |