
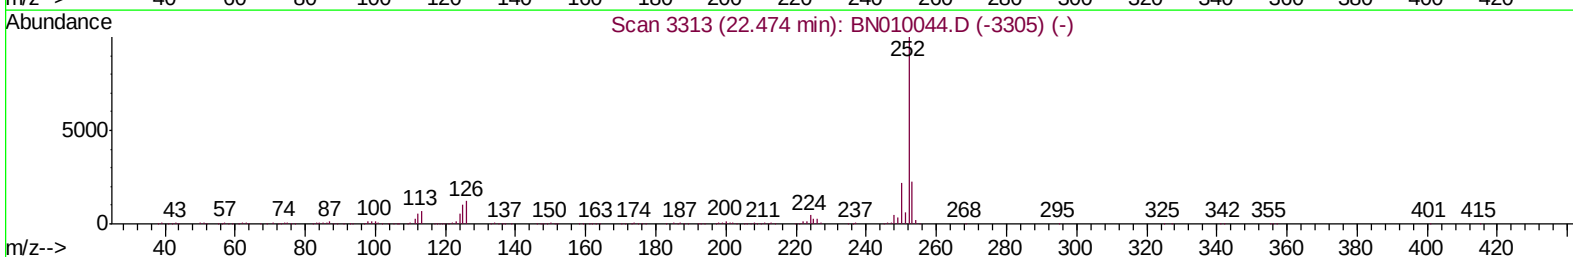
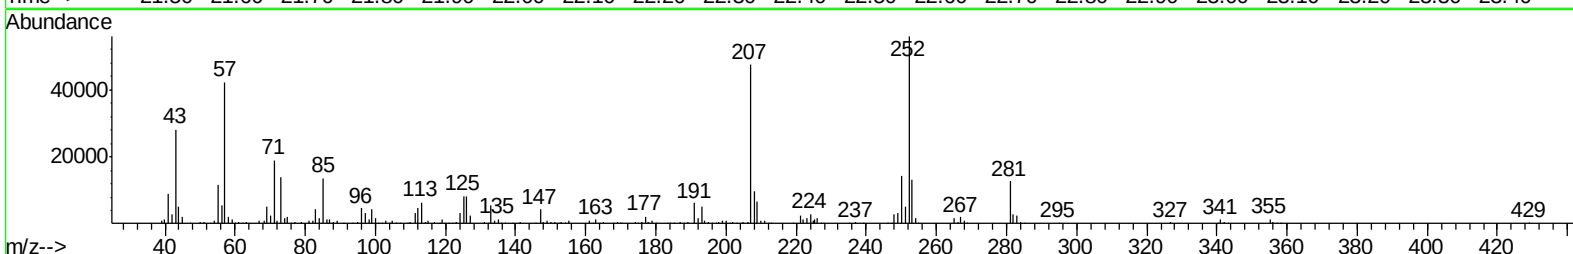


Data File : BN010051.D
Acq On : 02 Mar 2020 21:51
Operator : CG/JU
Sample : L1619-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Quant Time: Mar 03 01:08:59 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 03 01:05:31 2020
Response via : Initial Calibration

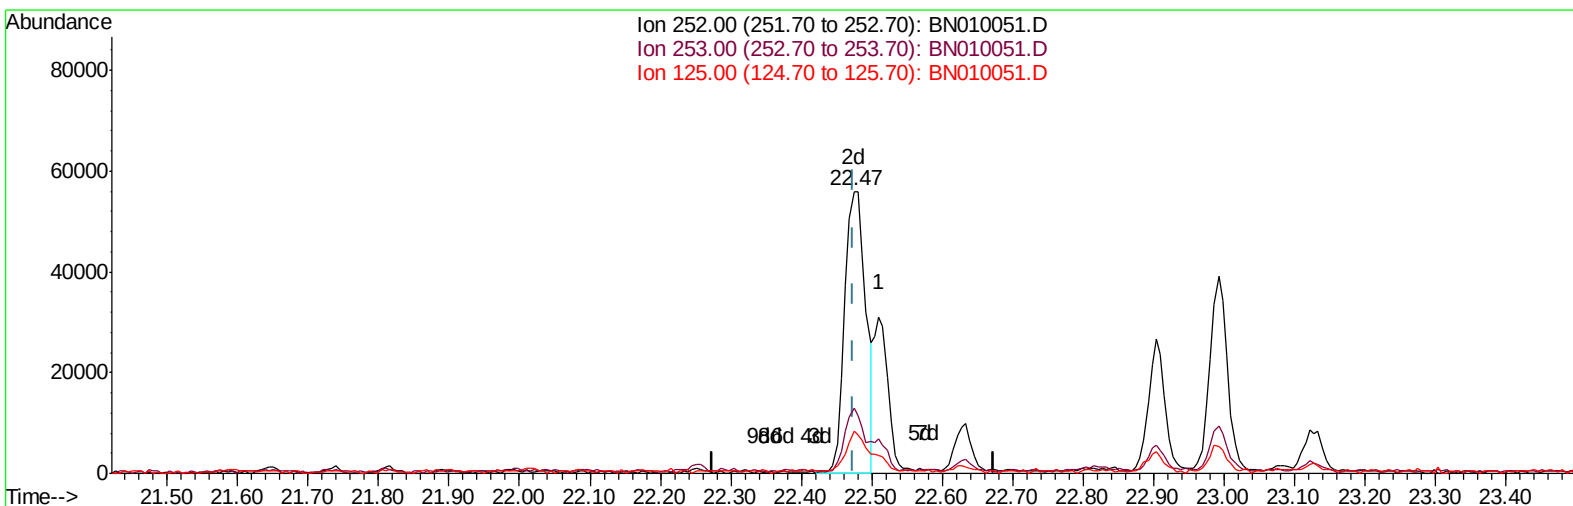

TIC: BN010051.D

(88) Benzo(b)fluoranthene

22.474min (+0.000) 3.74ng/ul m

response 116034

Ion	Exp%	Act%
252.00	100	100
253.00	21.20	23.42
125.00	10.00	15.01#
0.00	0.00	0.00