
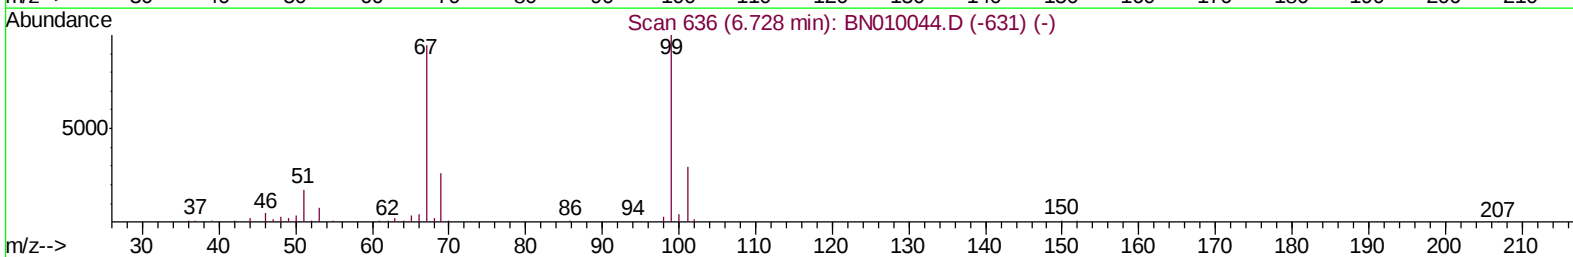
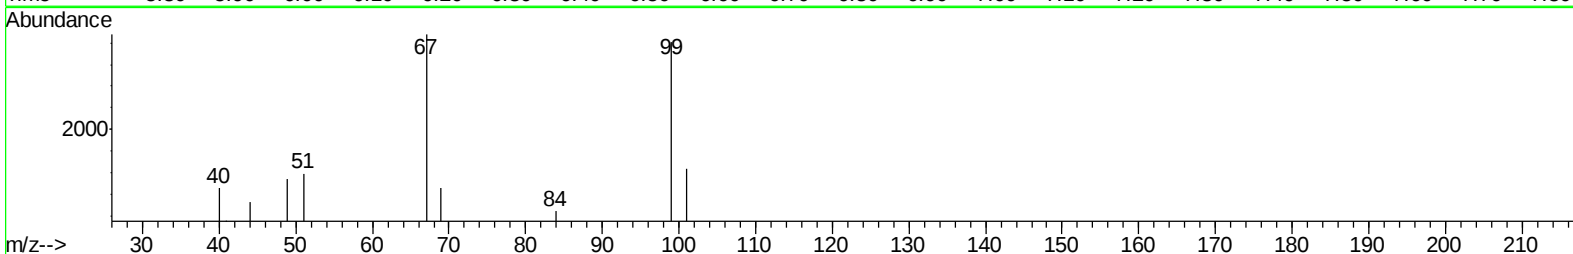


Data File : BN010054.D
Acq On : 02 Mar 2020 23:38
Operator : CG/JU
Sample : L1615-08DL 5X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Mar 03 01:09:44 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 03 01:05:31 2020
Response via : Initial Calibration

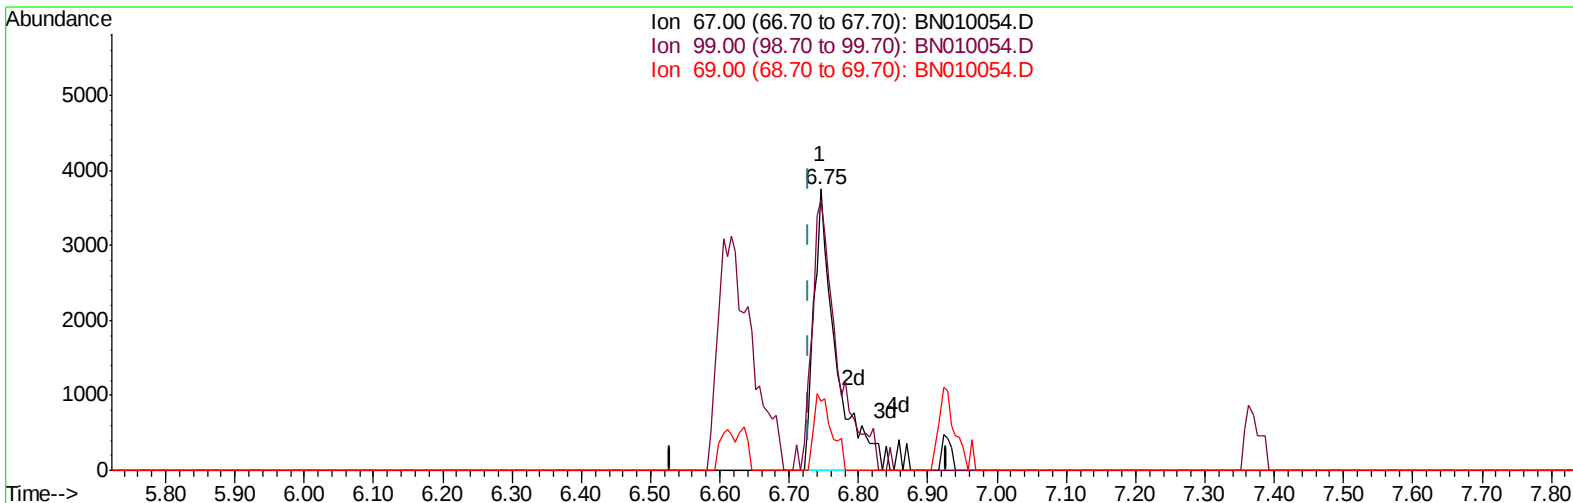

TIC: BN010054.D

(7) Bis-(2-Chloroethyl)ether-d8 (S)

6.746min (+0.018) 1.96ng/ul m

response 8281

Ion	Exp%	Act%
67.00	100	100
99.00	106.90	95.95
69.00	28.30	24.35
0.00	0.00	0.00