
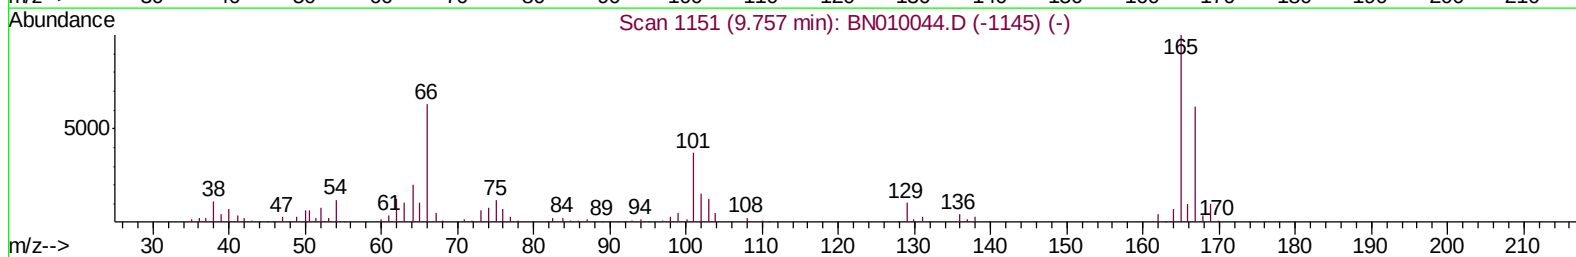
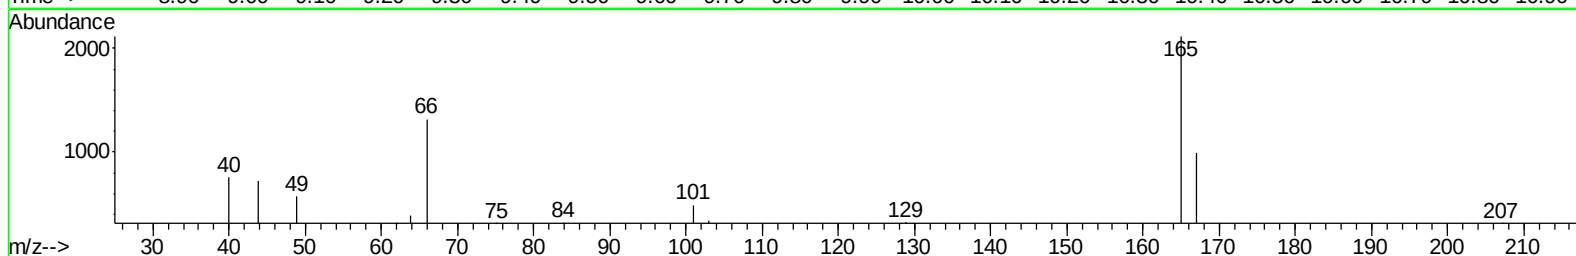


Data File : BN010054.D
Acq On : 02 Mar 2020 23:38
Operator : CG/JU
Sample : L1615-08DL 5X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Mar 03 01:09:44 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 03 01:05:31 2020
Response via : Initial Calibration

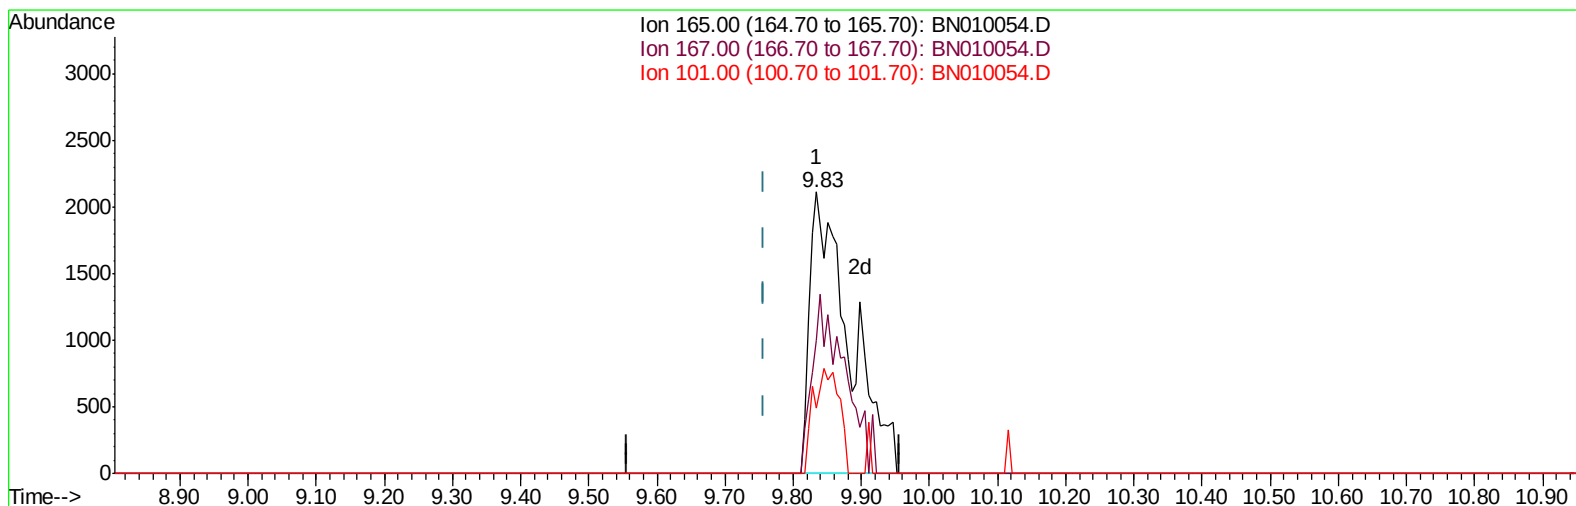

TIC: BN010054.D

(26) 2,4-Dichlorophenol-d3 (S)

9.834min (+0.077) 1.74ng/ul m

response 8504

Ion	Exp%	Act%
165.00	100	100
167.00	64.20	47.16#
101.00	36.10	23.27#
0.00	0.00	0.00