

Data File : BN010055.D

Acq On : 03 Mar 2020 00:14

Operator : CG/JU

Sample : SSTDCCC020EC

Misc :

ALS Vial : 2 Sample Multiplier: 1




Quant Time: Mar 03 01:10:00 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Tue Mar 03 01:05:31 2020

Response via : Initial Calibration

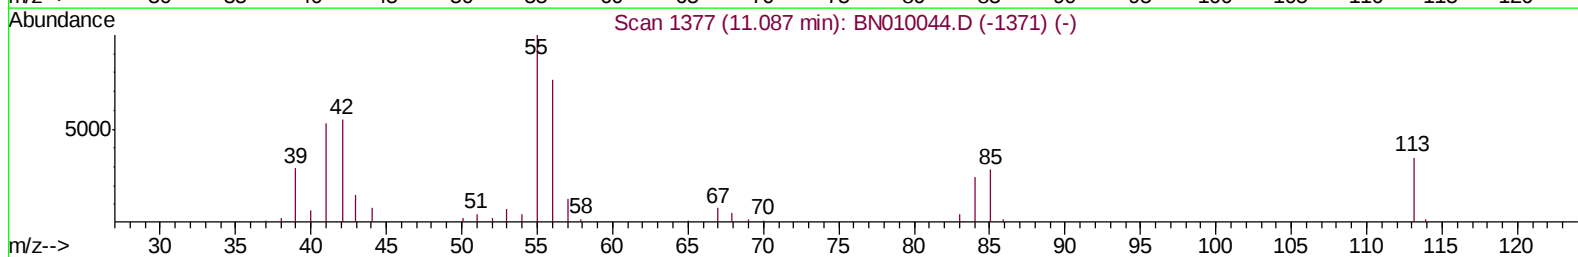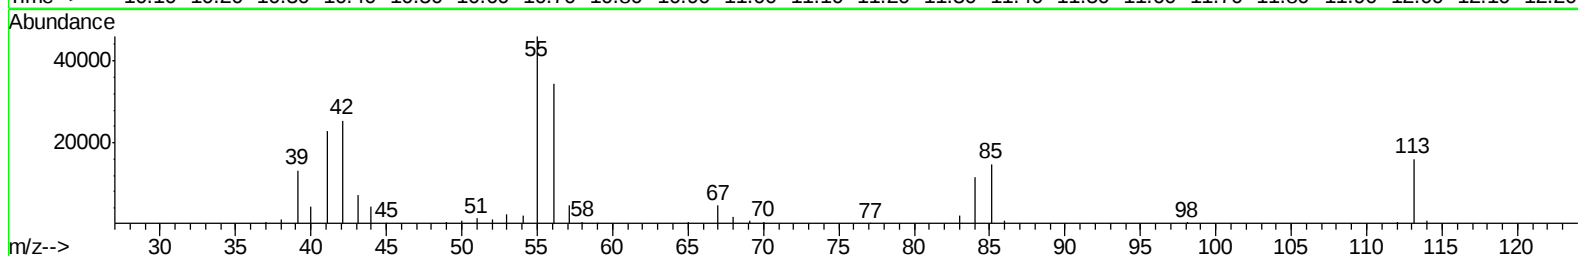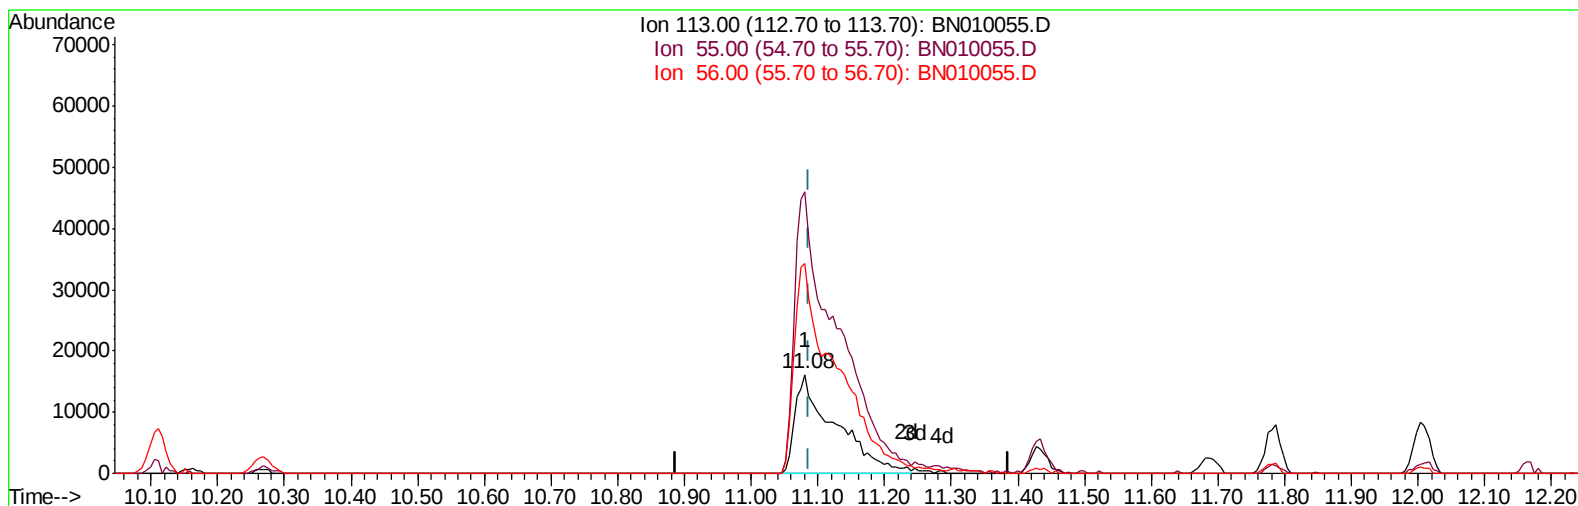

TIC: BN010055.D

(32) Caprolactam

11.081min (-0.006) 20.95ng/ul m

response 67400

Ion	Exp%	Act%
113.00	100	100
55.00	261.40	285.20
56.00	202.00	212.70
0.00	0.00	0.00