

Data File : BN010055.D

Acq On : 03 Mar 2020 00:14

Operator : CG/JU

Sample : SSTDCCC020EC

Misc :

ALS Vial : 2 Sample Multiplier: 1




Quant Time: Mar 03 01:10:00 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Tue Mar 03 01:05:31 2020

Response via : Initial Calibration

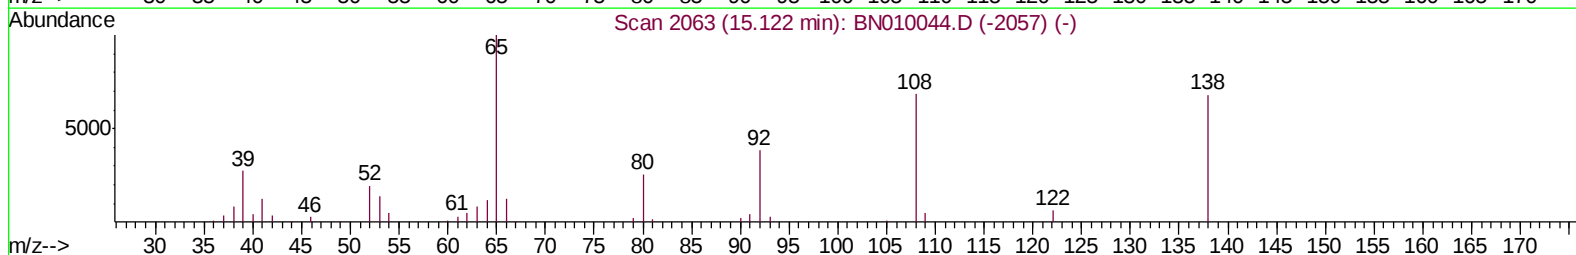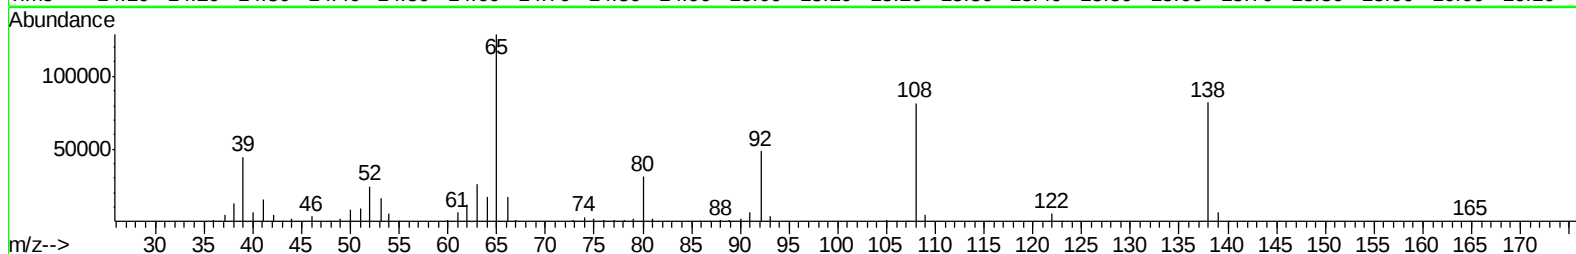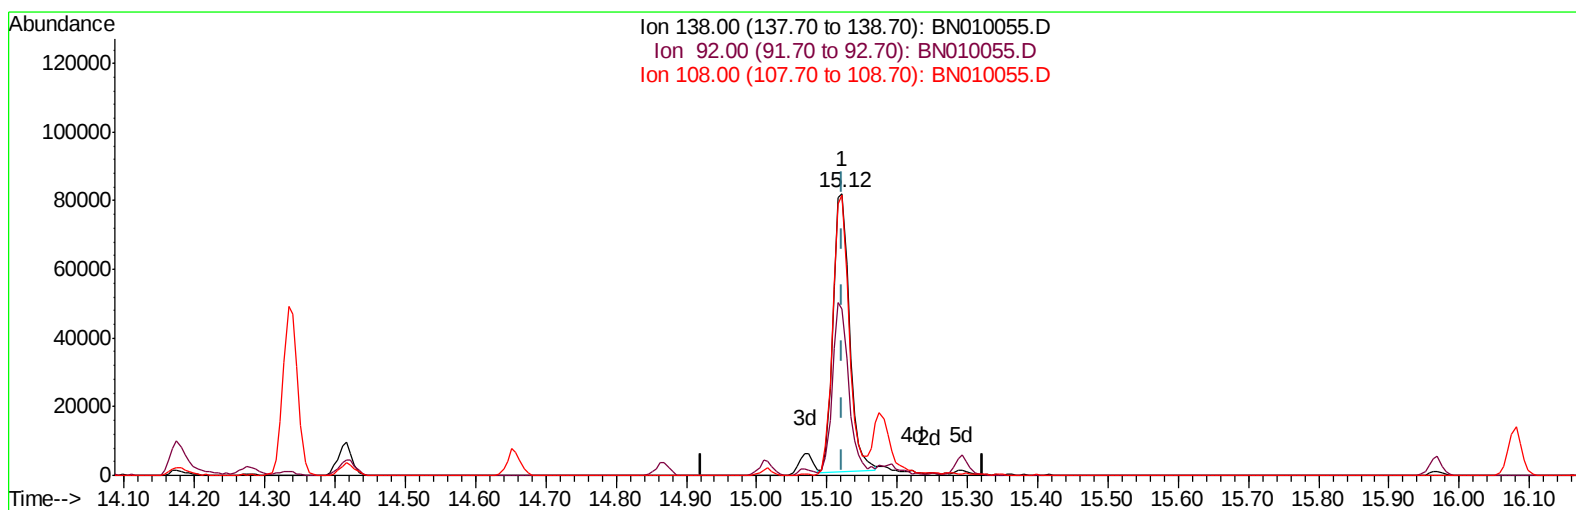

TIC: BN010055.D

(61) 4-Nitroaniline

15.122min (+0.000) 18.77ng/ul

response 131599

Ion	Exp%	Act%
138.00	100	100
92.00	59.70	59.24
108.00	90.40	99.42
0.00	0.00	0.00