
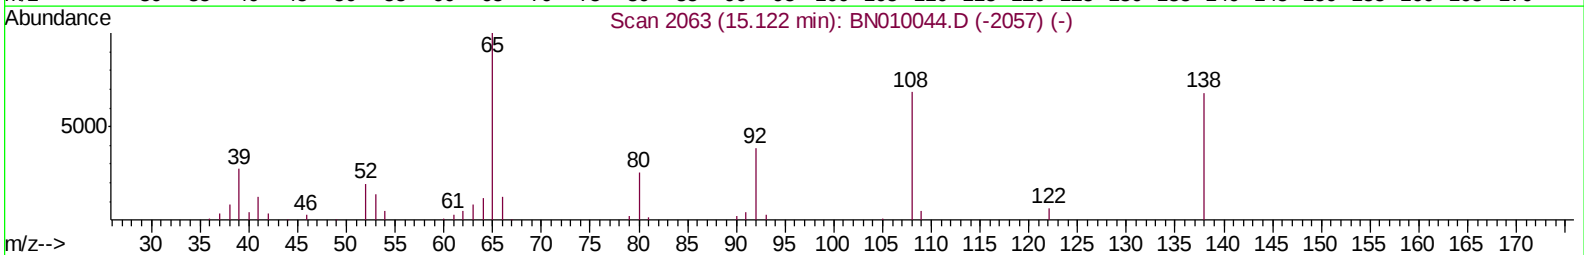
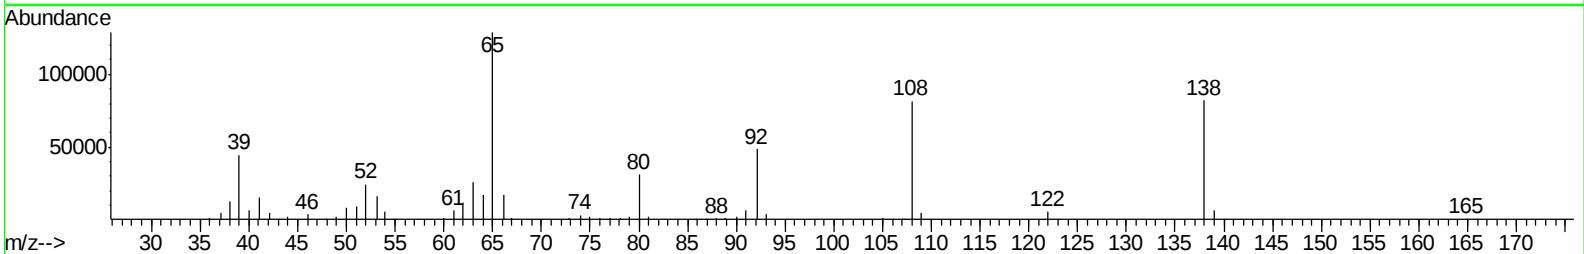


Data File : BN010055.D
Acq On : 03 Mar 2020 00:14
Operator : CG/JU
Sample : SSTDCCC020EC
Misc :
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Mar 03 01:10:00 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 03 01:05:31 2020
Response via : Initial Calibration

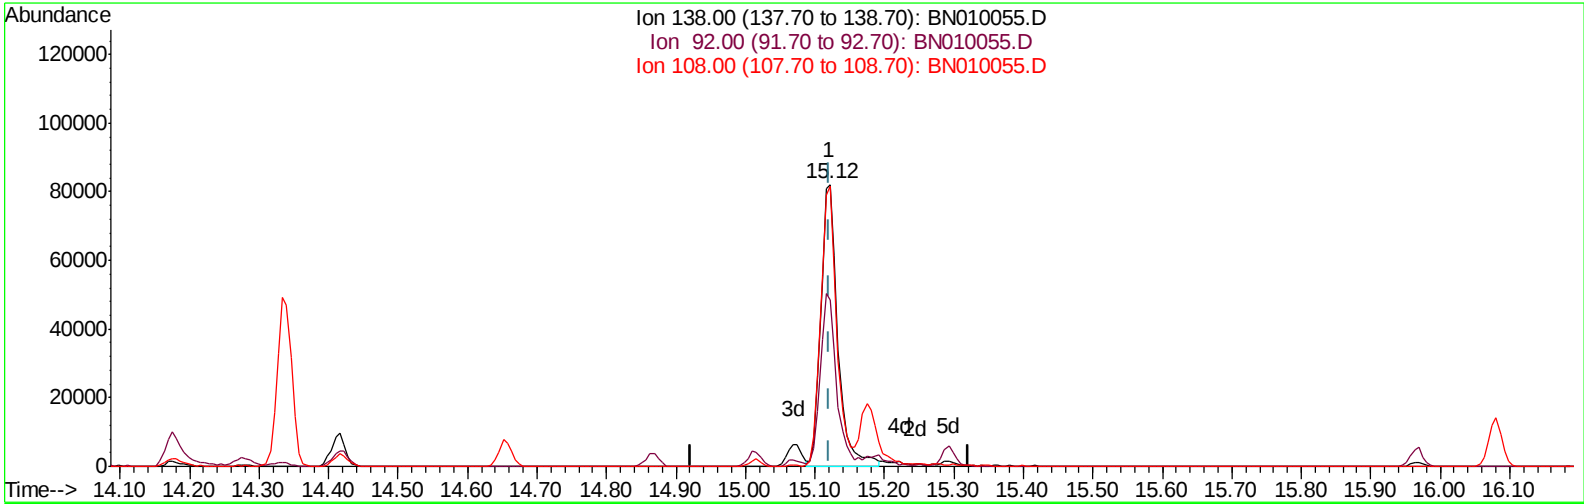

TIC: BN010055.D

(61) 4-Nitroaniline

15.122min (+0.000) 19.86ng/ul m

response 139230

Ion	Exp%	Act%
138.00	100	100
92.00	59.70	59.24
108.00	90.40	99.42
0.00	0.00	0.00