
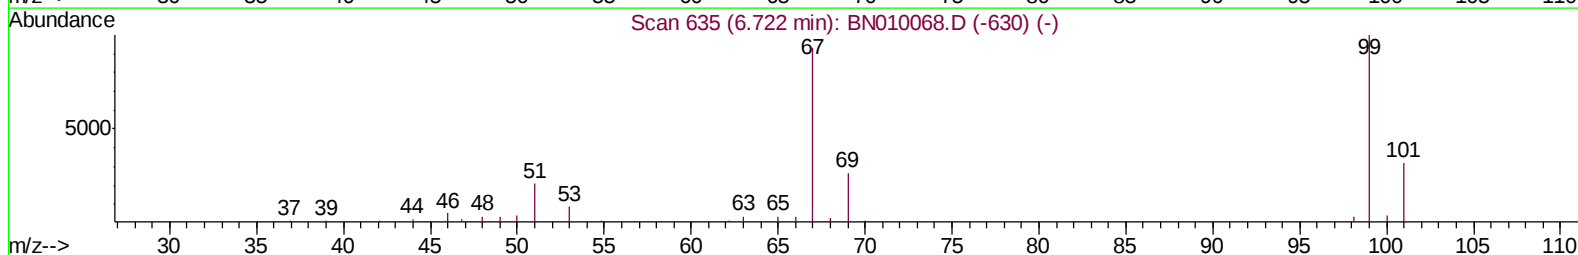
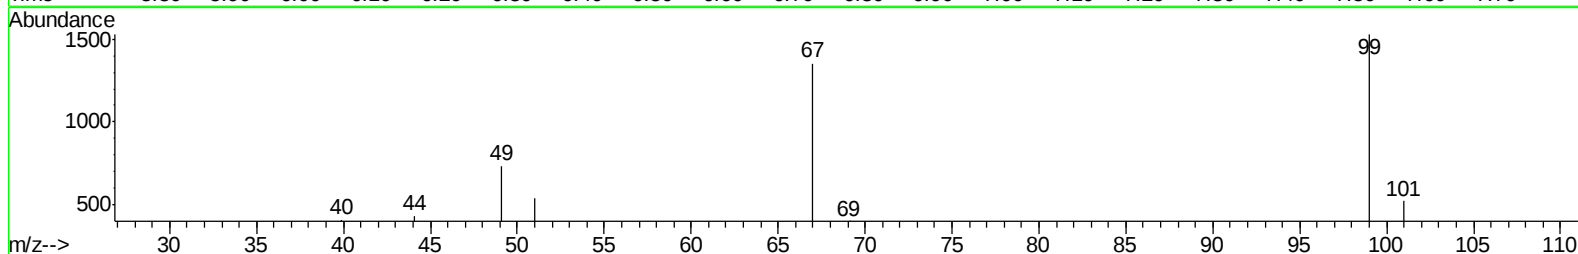


Data File : BN010075.D
Acq On : 03 Mar 2020 23:22
Operator : CG/JU
Sample : L1619-04DL 10X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Quant Time: Mar 04 01:33:01 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 04 01:30:16 2020
Response via : Initial Calibration

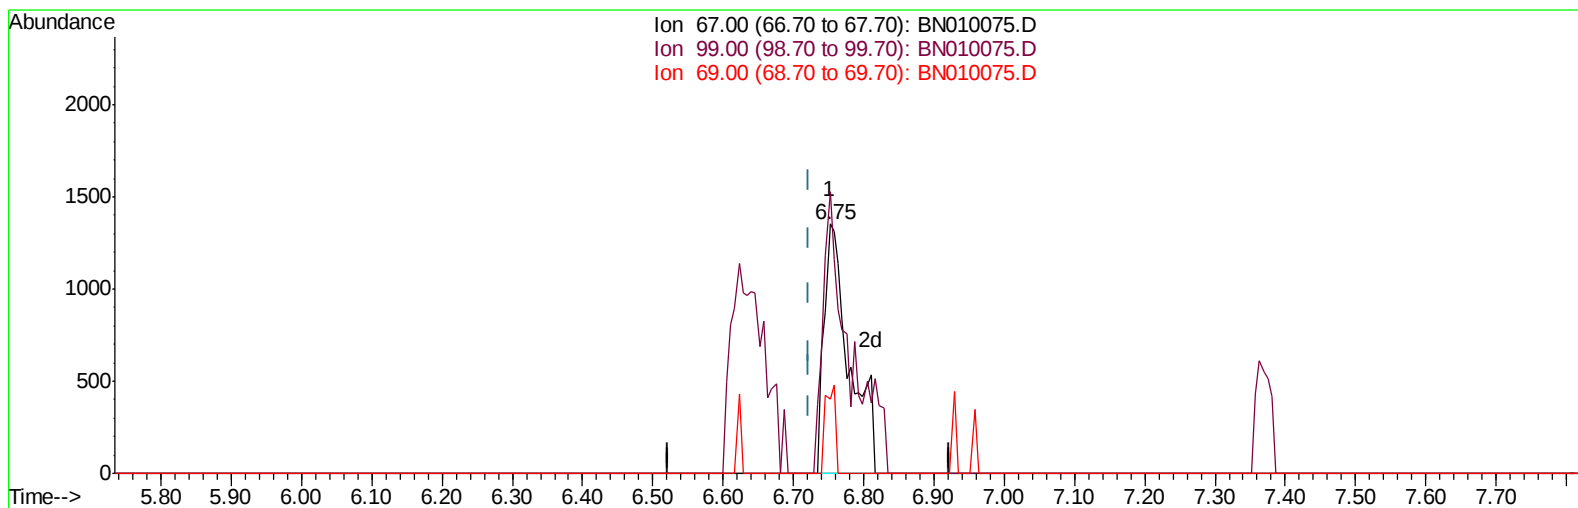

TIC: BN010075.D

(7) Bis-(2-Chloroethyl)ether-d8 (S)

6.752min (+0.030) 1.08ng/ul m

response 3381

Ion	Exp%	Act%
67.00	100	100
99.00	106.90	113.10
69.00	28.30	29.68
0.00	0.00	0.00