
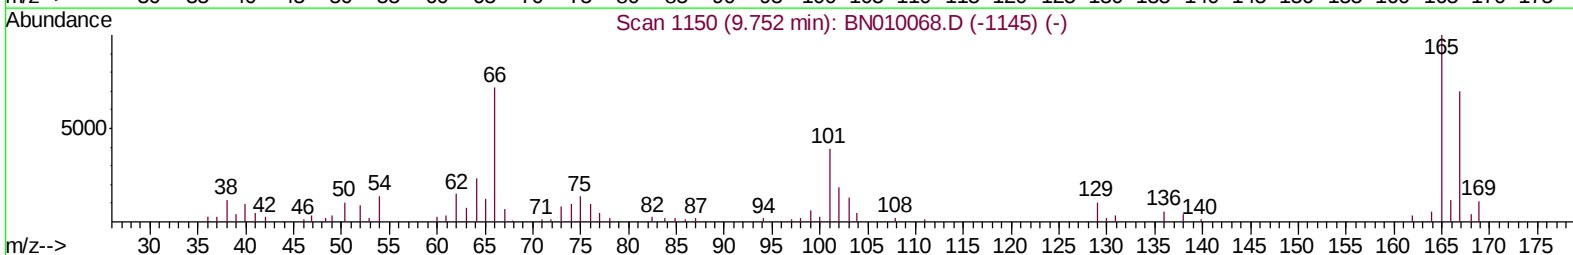
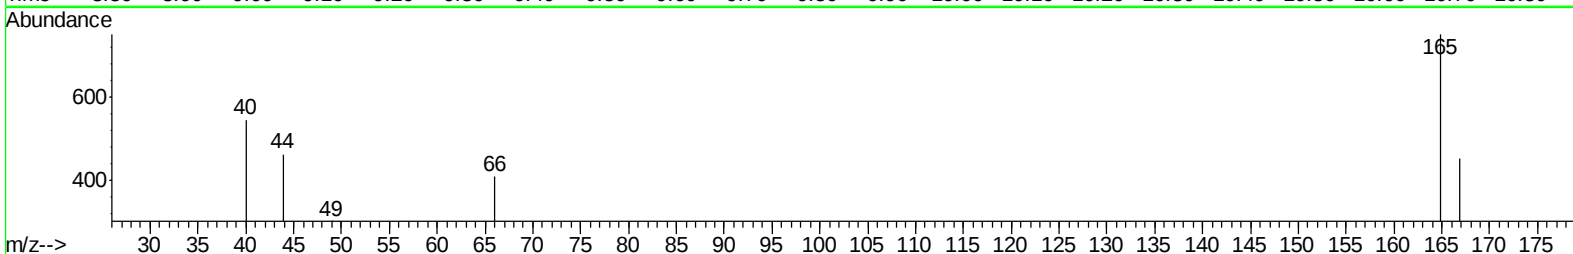


Data File : BN010075.D
Acq On : 03 Mar 2020 23:22
Operator : CG/JU
Sample : L1619-04DL 10X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Quant Time: Mar 04 01:33:01 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 04 01:30:16 2020
Response via : Initial Calibration

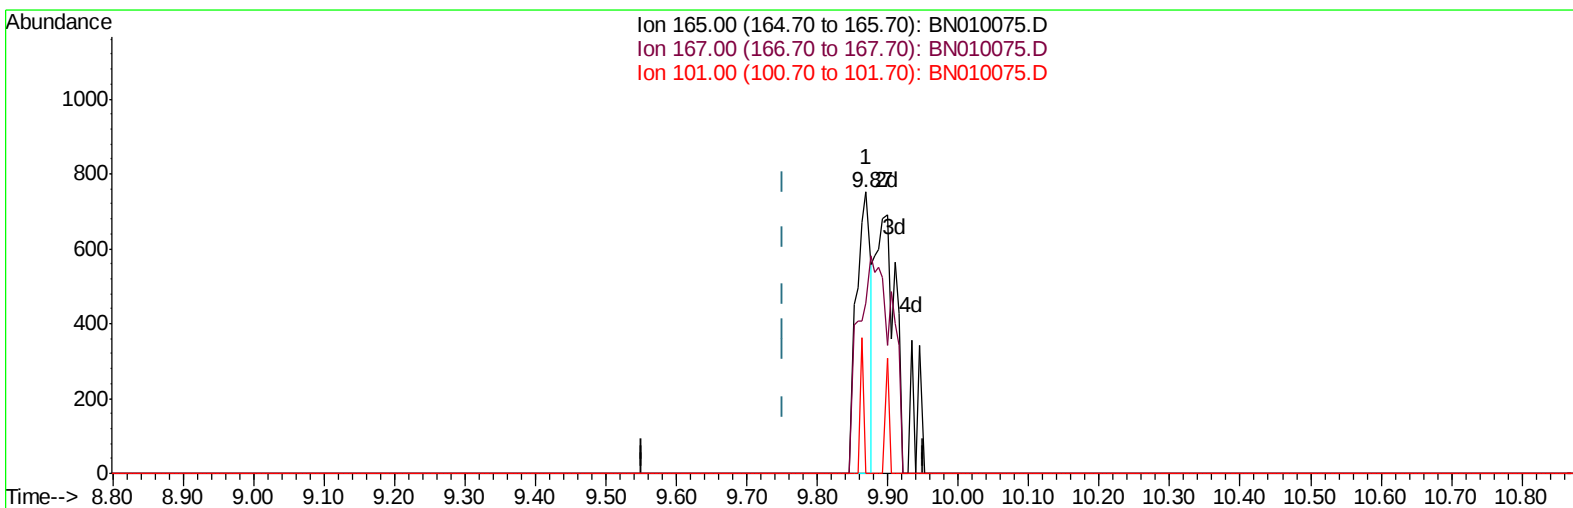

TIC: BN010075.D

(26) 2,4-Dichlorophenol-d3 (S)

9.869min (+0.118) 0.38ng/ul

response 1034

Ion	Exp%	Act%
165.00	100	100
167.00	64.20	60.37
101.00	36.10	0.00#
0.00	0.00	0.00