
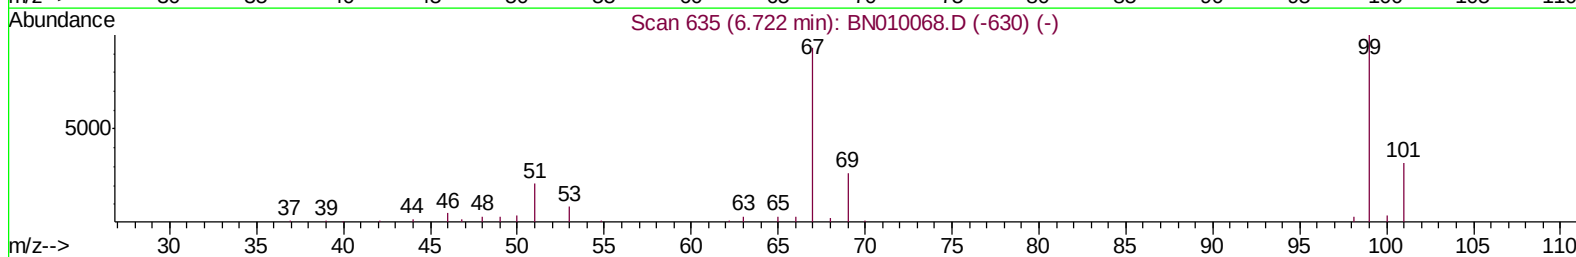
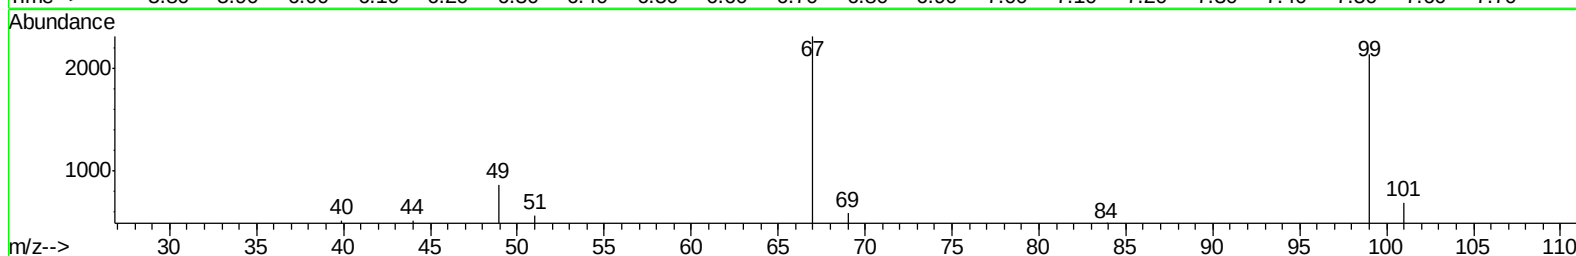


Data File : BN010076.D
Acq On : 03 Mar 2020 23:58
Operator : CG/JU
Sample : L1619-06DL 50X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Mar 04 01:33:14 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 04 01:30:16 2020
Response via : Initial Calibration

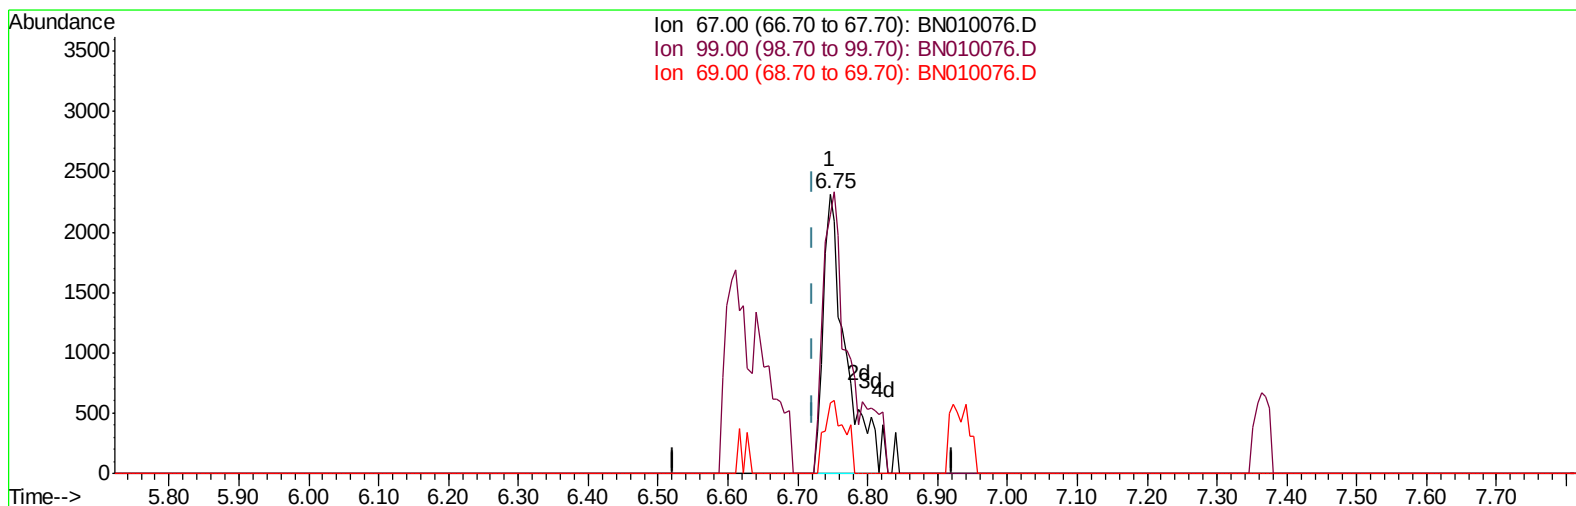

TIC: BN010076.D

(7) Bis-(2-Chloroethyl)ether-d8 (S)

6.746min (+0.024) 1.46ng/ul m

response 5037

Ion	Exp%	Act%
67.00	100	100
99.00	106.90	92.66
69.00	28.30	25.39
0.00	0.00	0.00