
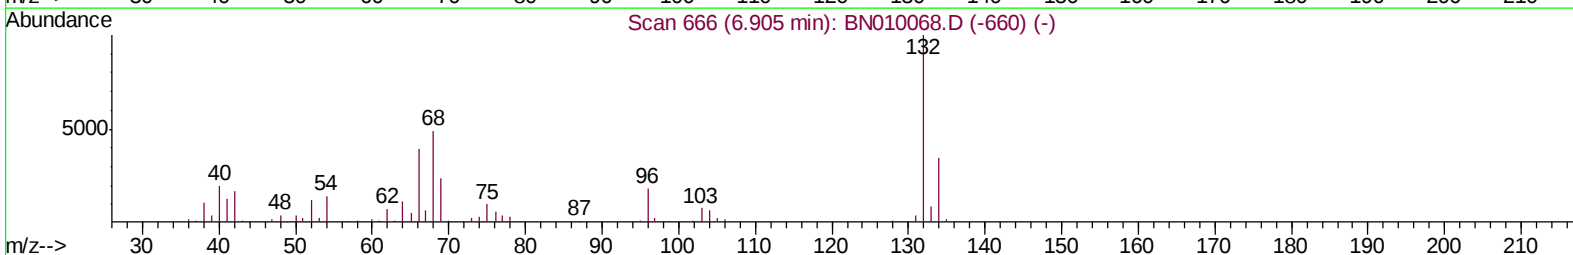
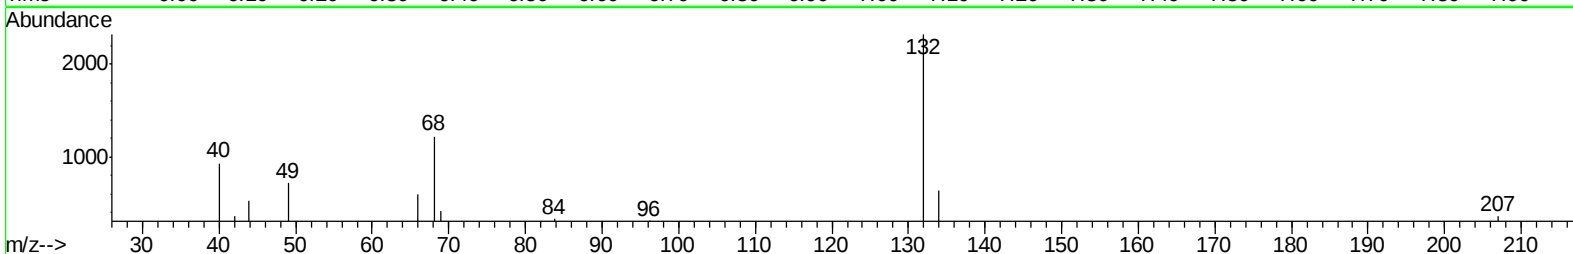


Data File : BN010076.D
Acq On : 03 Mar 2020 23:58
Operator : CG/JU
Sample : L1619-06DL 50X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Mar 04 01:33:14 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 04 01:30:16 2020
Response via : Initial Calibration

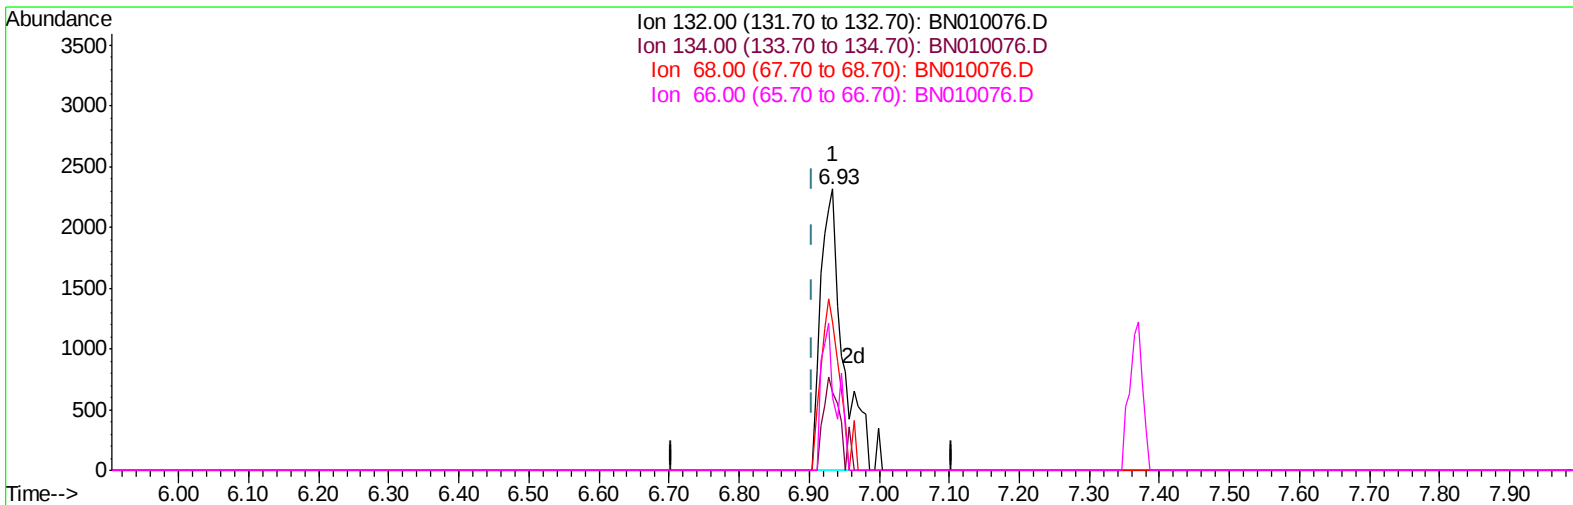

TIC: BN010076.D

(9) 2-Chlorophenol-d4 (S)

6.934min (+0.029) 1.36ng/ul m

response 5119

Ion	Exp%	Act%
132.00	100	100
134.00	32.10	27.52
68.00	48.60	52.85
66.00	37.30	26.06#