
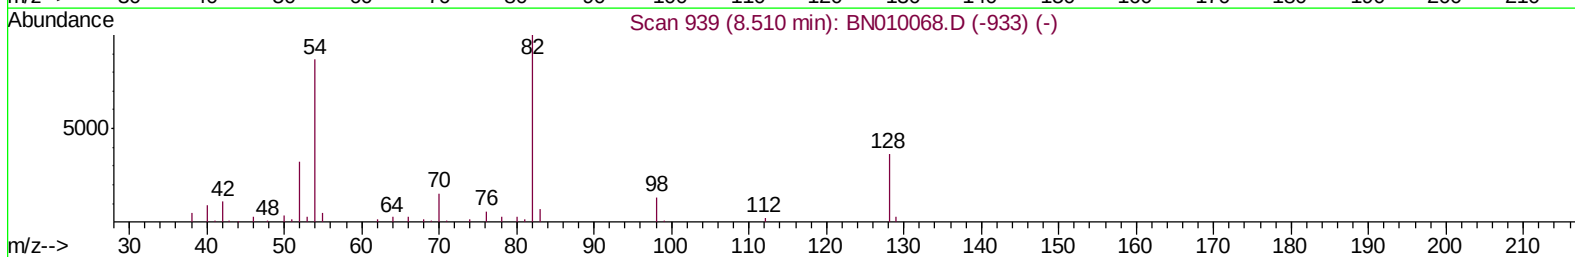
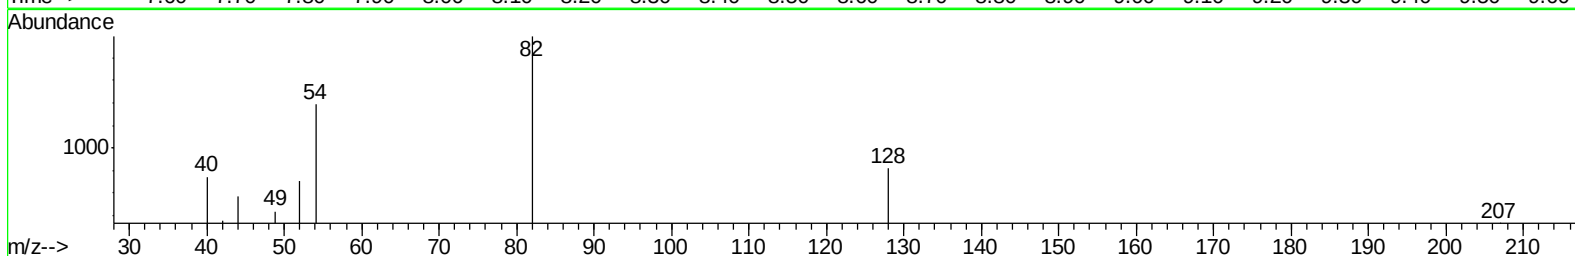


Data File : BN010076.D
Acq On : 03 Mar 2020 23:58
Operator : CG/JU
Sample : L1619-06DL 50X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Mar 04 01:33:14 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 04 01:30:16 2020
Response via : Initial Calibration

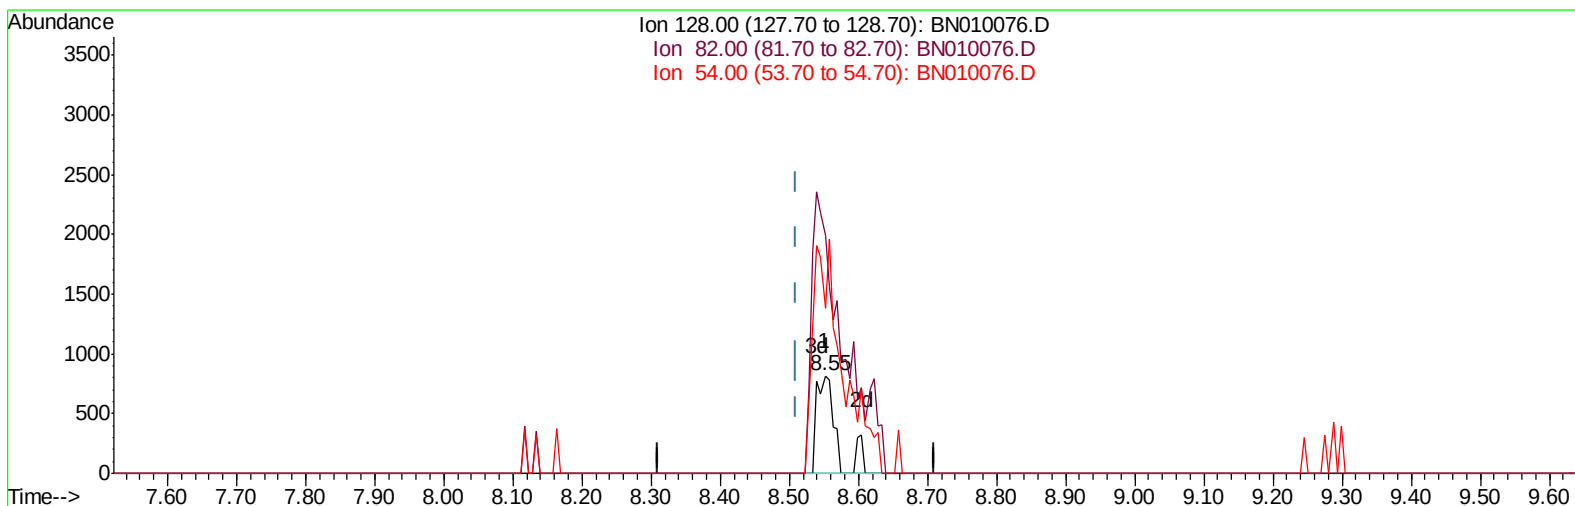

TIC: BN010076.D

(19) Nitrobenzene-d5 (S)
8.552min (+0.041) 0.98ng/ul m
response 1559

Ion	Exp%	Act%
128.00	100	100
82.00	271.60	243.70
54.00	200.30	169.52
0.00	0.00	0.00