
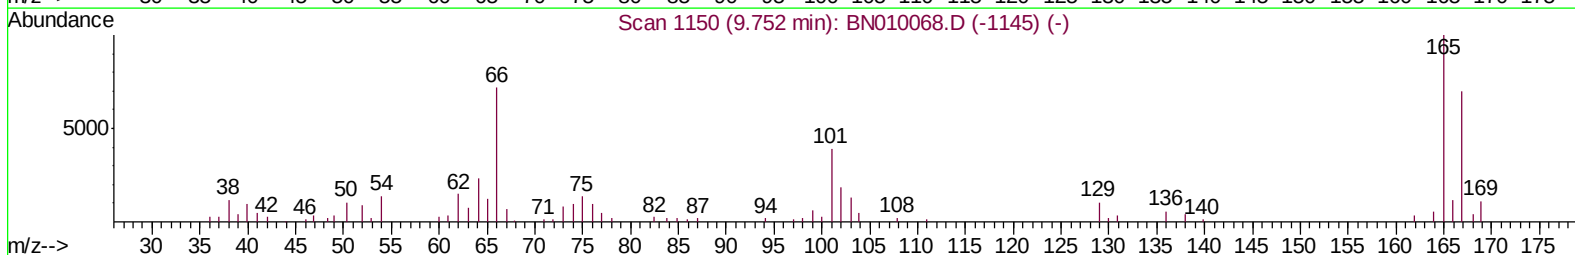
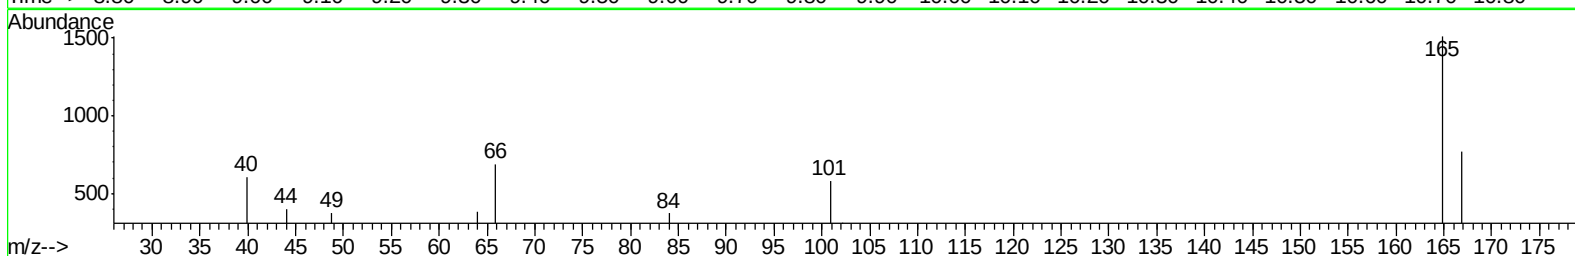


Data File : BN010076.D  
Acq On : 03 Mar 2020 23:58  
Operator : CG/JU  
Sample : L1619-06DL 50X  
Misc :  
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Mar 04 01:33:14 2020  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\SOM-EPA-BN021220MA.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Wed Mar 04 01:30:16 2020  
Response via : Initial Calibration

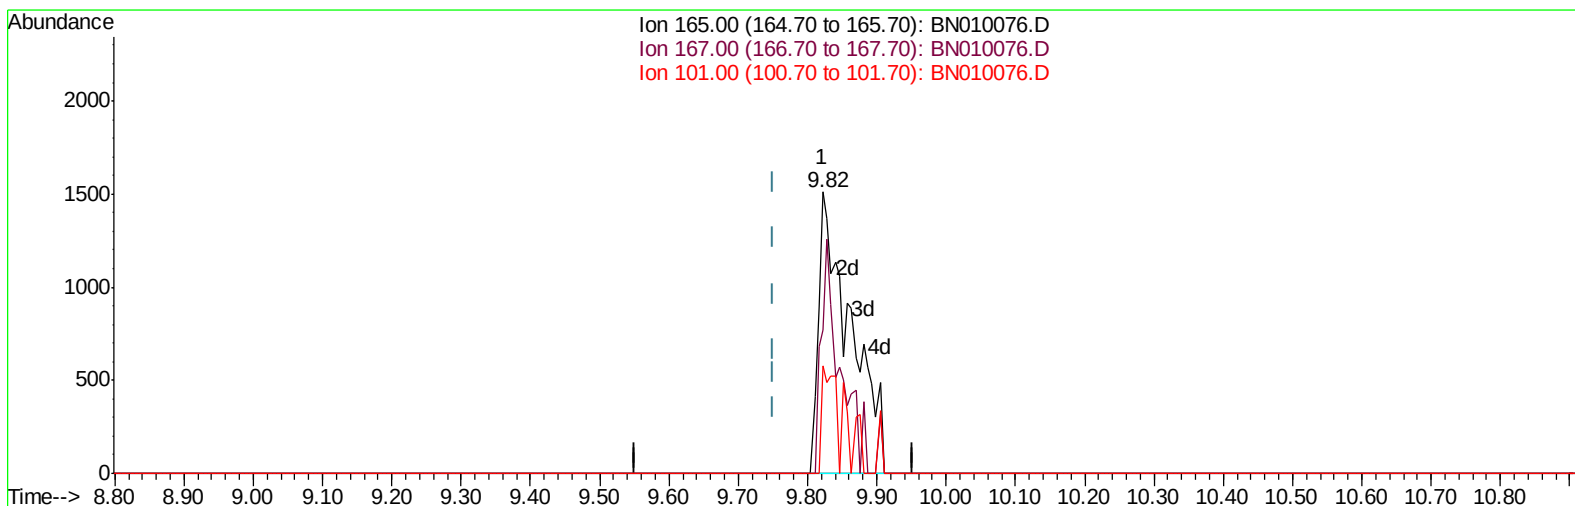

TIC: BN010076.D

(26) 2,4-Dichlorophenol-d3 (S)

9.822min (+0.071) 1.44ng/ul m

response 4788

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 165.00 | 100   | 100    |
| 167.00 | 64.20 | 50.93# |
| 101.00 | 36.10 | 38.43  |
| 0.00   | 0.00  | 0.00   |