
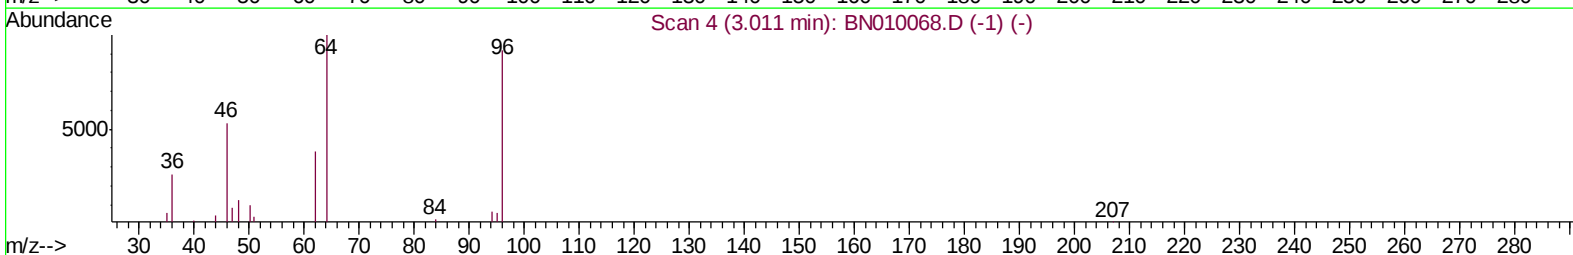
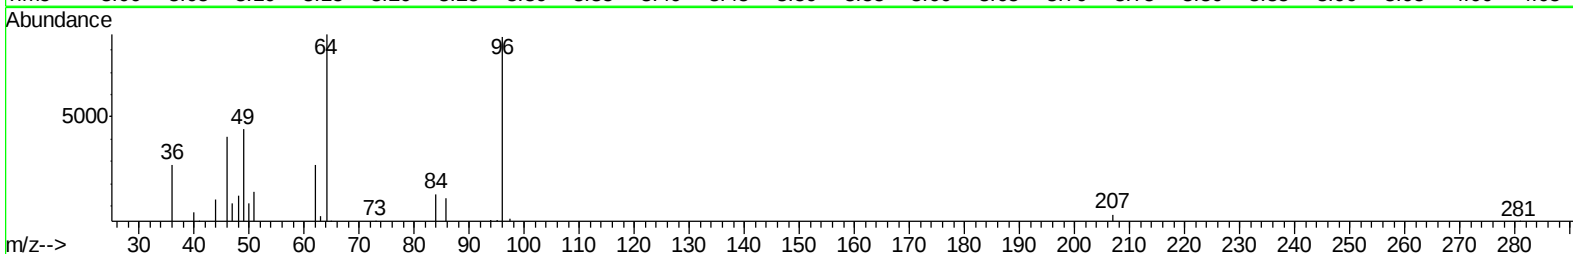


Data File : BN010077.D
Acq On : 04 Mar 2020 00:34
Operator : CG/JU
Sample : TEST BS
Misc :
ALS Vial : 21 Sample Multiplier: 1

Quant Time: Mar 04 01:33:26 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 04 01:30:16 2020
Response via : Initial Calibration

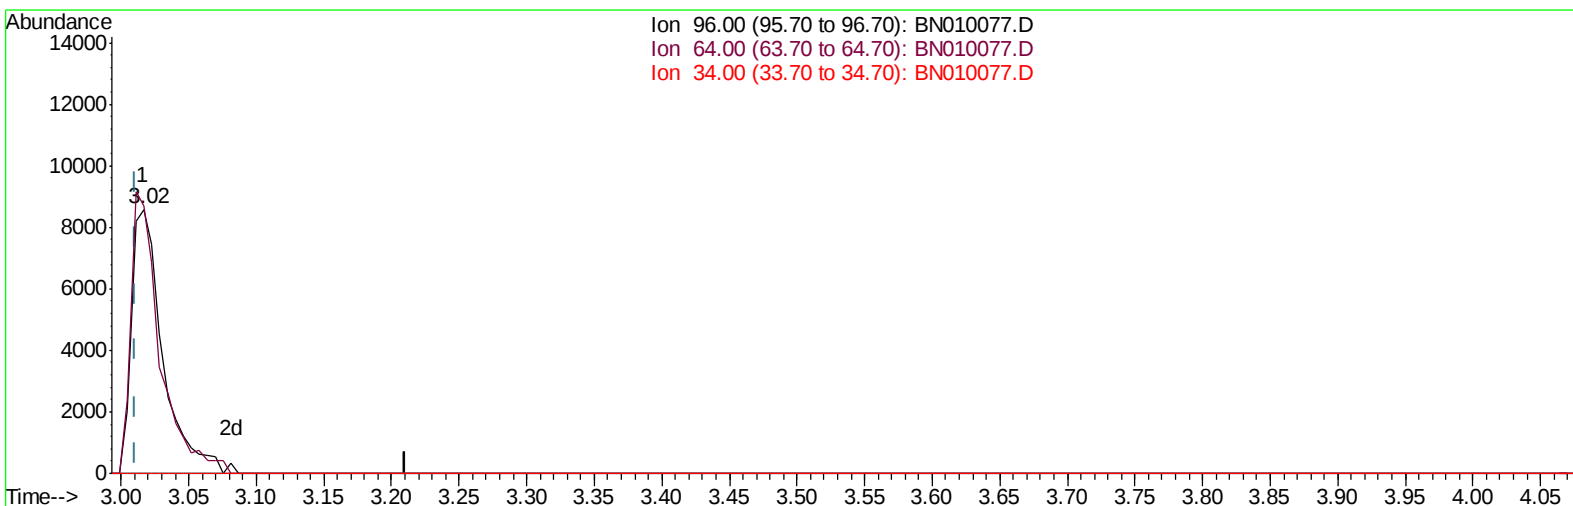

TIC: BN010077.D

(3) 1,4-Dioxane-d8 (S)

3.017min (+0.006) 7.00ng/uL m

response 13680

Ion	Exp%	Act%
96.00	100	100
64.00	93.60	101.47
34.00	0.00	0.00
0.00	0.00	0.00