
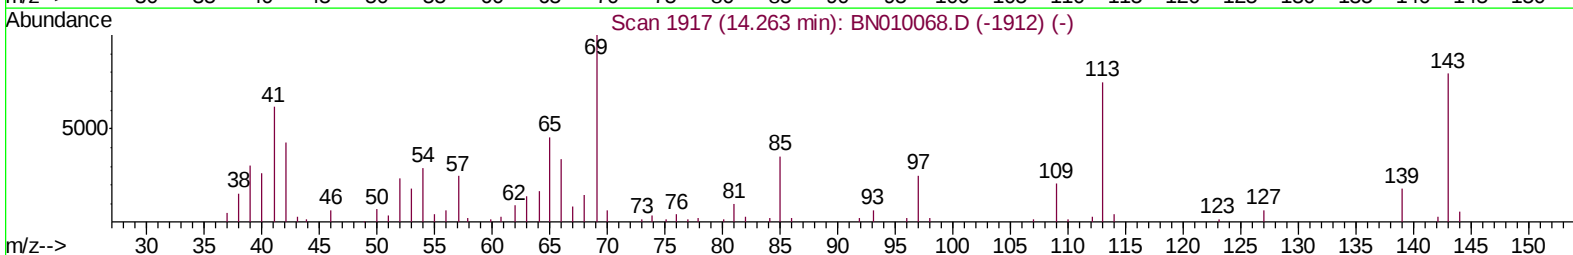
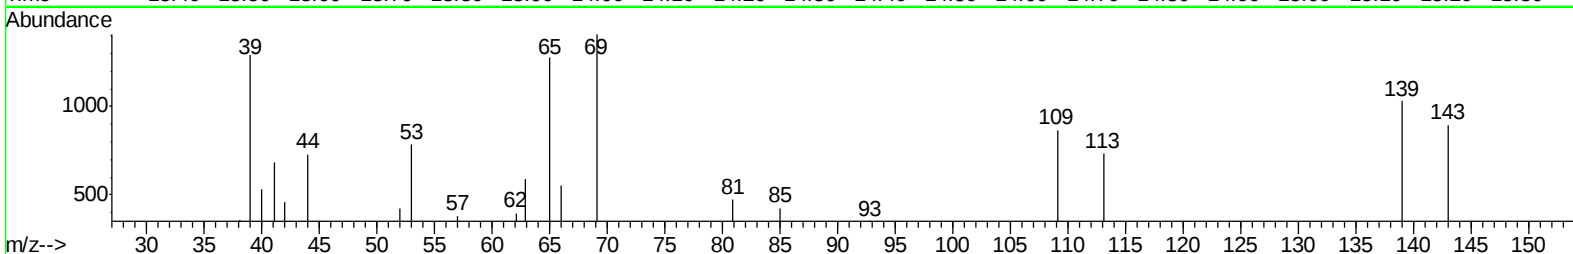


Data File : BN010077.D
Acq On : 04 Mar 2020 00:34
Operator : CG/JU
Sample : TEST BS
Misc :
ALS Vial : 21 Sample Multiplier: 1

Quant Time: Mar 04 01:33:26 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 04 01:30:16 2020
Response via : Initial Calibration

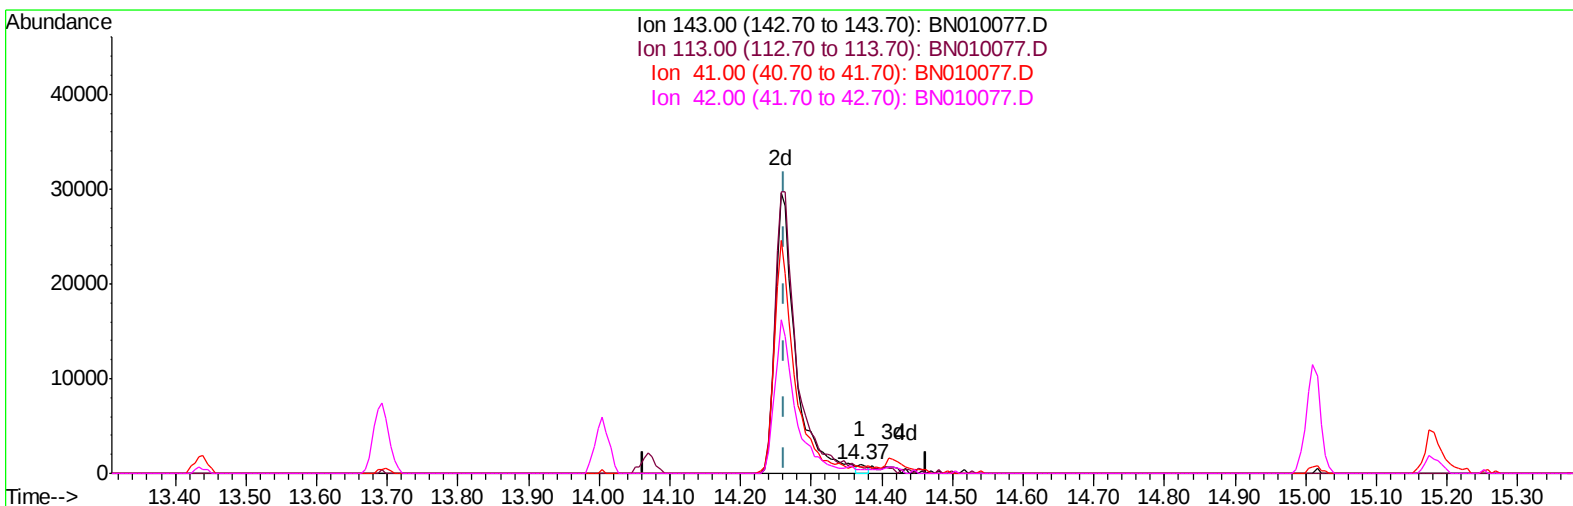

TIC: BN010077.D

(52) 4-Nitrophenol-d4 (S)
14.369min (+0.106) 0.44ng/ul

response 792

Ion	Exp%	Act%
143.00	100	100
113.00	86.40	81.83
41.00	66.00	76.48
42.00	43.20	51.17