
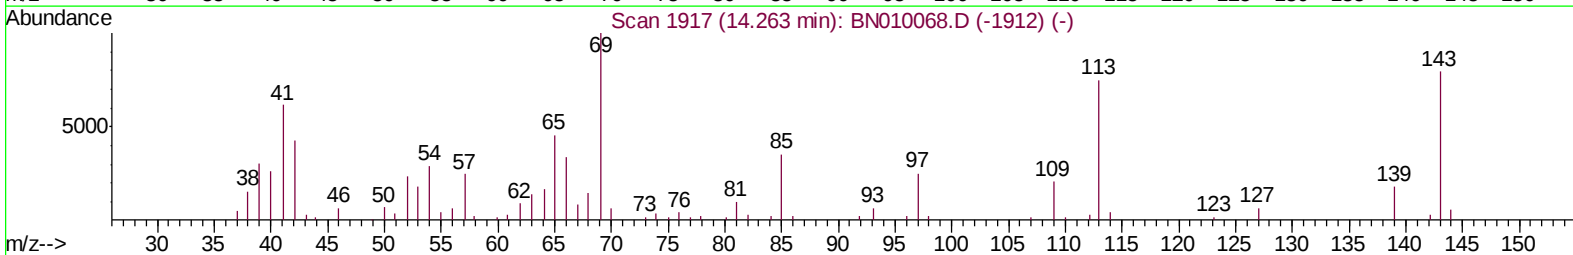
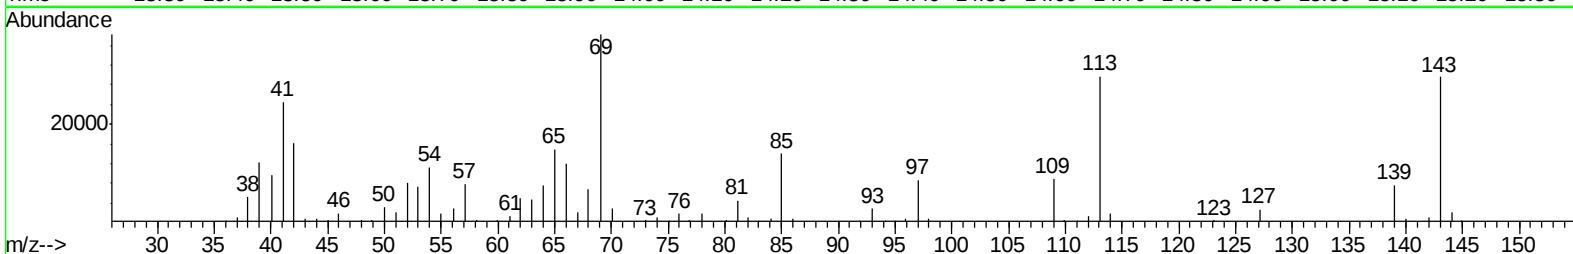


Data File : BN010077.D
Acq On : 04 Mar 2020 00:34
Operator : CG/JU
Sample : TEST BS
Misc :
ALS Vial : 21 Sample Multiplier: 1

Quant Time: Mar 04 01:33:26 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 04 01:30:16 2020
Response via : Initial Calibration

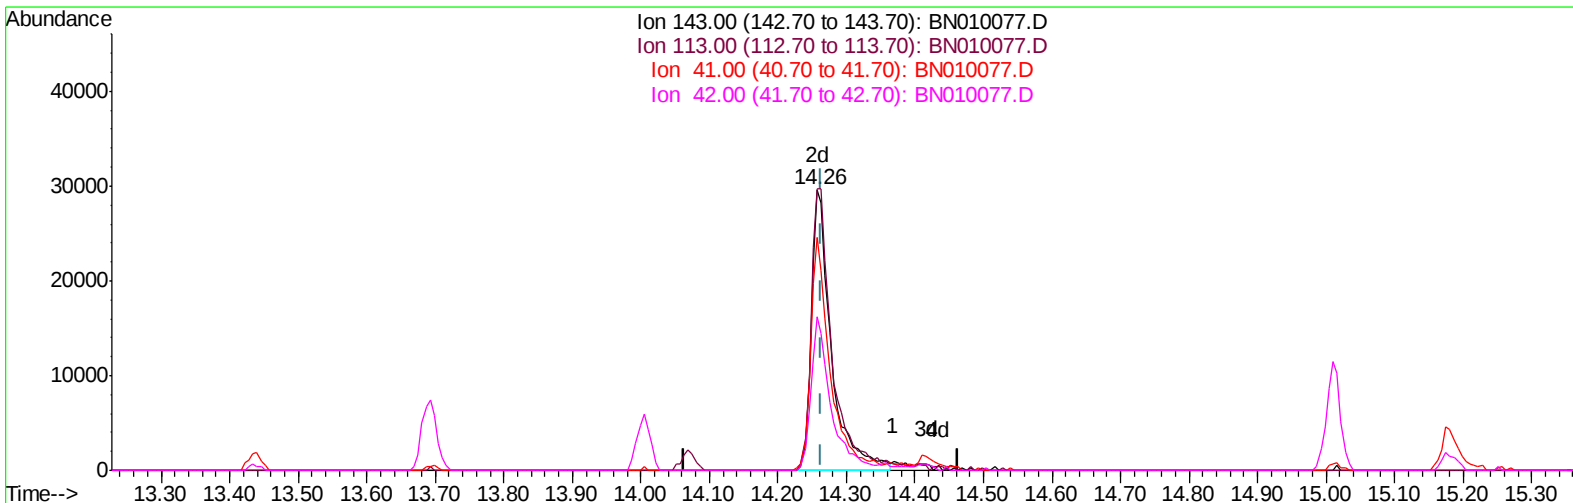

TIC: BN010077.D

(52) 4-Nitrophenol-d4 (S)
14.257min (-0.006) 33.53ng/ul m
response 60164

Ion	Exp%	Act%
143.00	100	100
113.00	86.40	100.41
41.00	66.00	83.00#
42.00	43.20	54.68#