
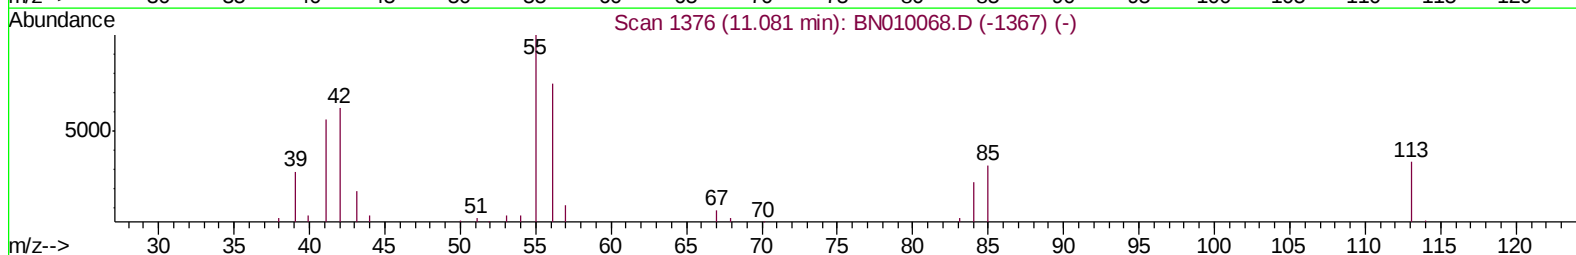
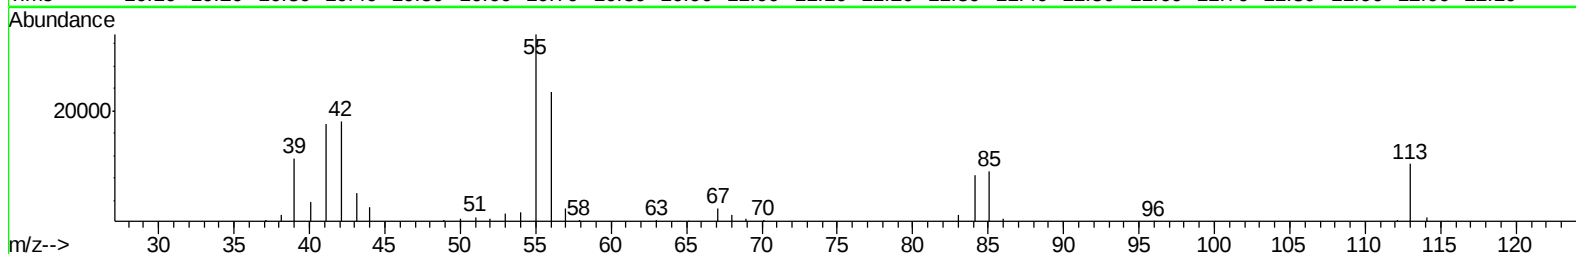


Data File : BN010078.D
Acq On : 04 Mar 2020 01:10
Operator : CG/JU
Sample : SSTDCCC020EC
Misc :
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Mar 04 03:01:38 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 04 01:30:16 2020
Response via : Initial Calibration

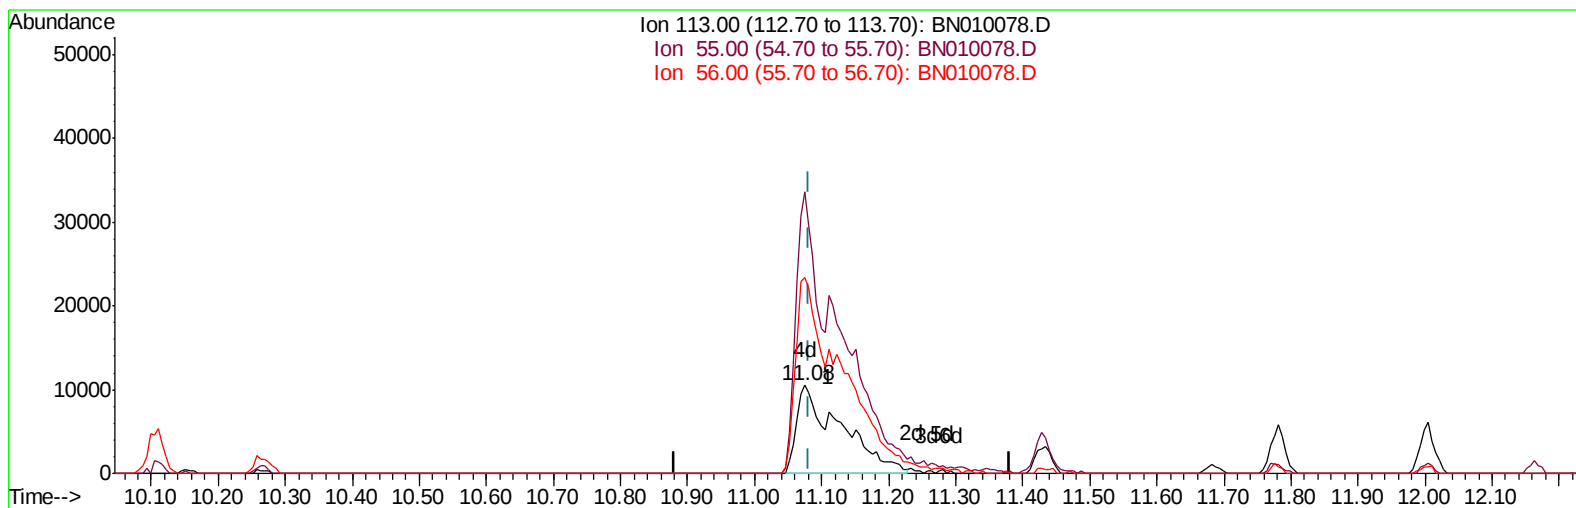

TIC: BN010078.D

(32) Caprolactam

11.075min (-0.006) 23.81ng/ul m

response 48651

Ion	Exp%	Act%
113.00	100	100
55.00	261.40	319.92#
56.00	202.00	222.46
0.00	0.00	0.00