

Data File : BN010069.D
Acq On : 03 Mar 2020 19:44
Operator : CG/JU
Sample : PB127247BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK47

Quant Time: Mar 04 01:32:22 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 04 01:30:16 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.36	152	44982	20.00	ng/ul	0.00
18) Naphthalene-d8	10.11	136	191879	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.01	164	128593	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.77	188	279956	20.00	ng/ul	0.00
78) Chrysene-d12	20.99	240	256241	20.00	ng/ul	0.00
86) Perylene-d12	23.09	264	278362	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.02	96	6130	5.60	ng/uL	0.00
5) Phenol-d5	6.57	99	116999	30.58	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.72	67	85917	32.54	ng/ul	0.00
9) 2-Chlorophenol-d4	6.90	132	96706	33.57	ng/ul	0.00
13) 4-Methylphenol-d8	8.08	113	99433	32.67	ng/ul	0.00
19) Nitrobenzene-d5	8.51	128	46744	33.30	ng/ul	0.00
22) 2-Nitrophenol-d4	9.22	143	52515	34.19	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.76	165	92270	31.25	ng/ul	0.00
29) 4-Chloroaniline-d4	10.27	131	133022	40.10	ng/ul	0.00
44) Dimethylphthalate-d6	13.44	166	331310	34.49	ng/ul	0.00
47) Acenaphthylene-d8	13.69	160	381853	33.76	ng/ul	0.00
52) 4-Nitrophenol-d4	14.36	143	440	0.25	ng/ul	0.09
58) Fluorene-d10	15.02	176	290430	35.02	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.19	200	32367	18.61	ng/ul	0.00
71) Anthracene-d10	16.87	188	446059	34.76	ng/ul	0.00
79) Pyrene-d10	19.17	212	496025	37.04	ng/ul	0.00
90) Benzo(a)pyrene-d12	22.95	264	486066	34.97	ng/ul	0.00


Target Compounds					Qvalue	
15) N-Nitroso-di-n-propylamine	8.07	70	2839	1.096	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN010069.D
Acq On : 03 Mar 2020 19:44
Operator : CG/JU
Sample : PB127247BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK47

Quant Time: Mar 04 01:32:22 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 04 01:30:16 2020
Response via : Initial Calibration

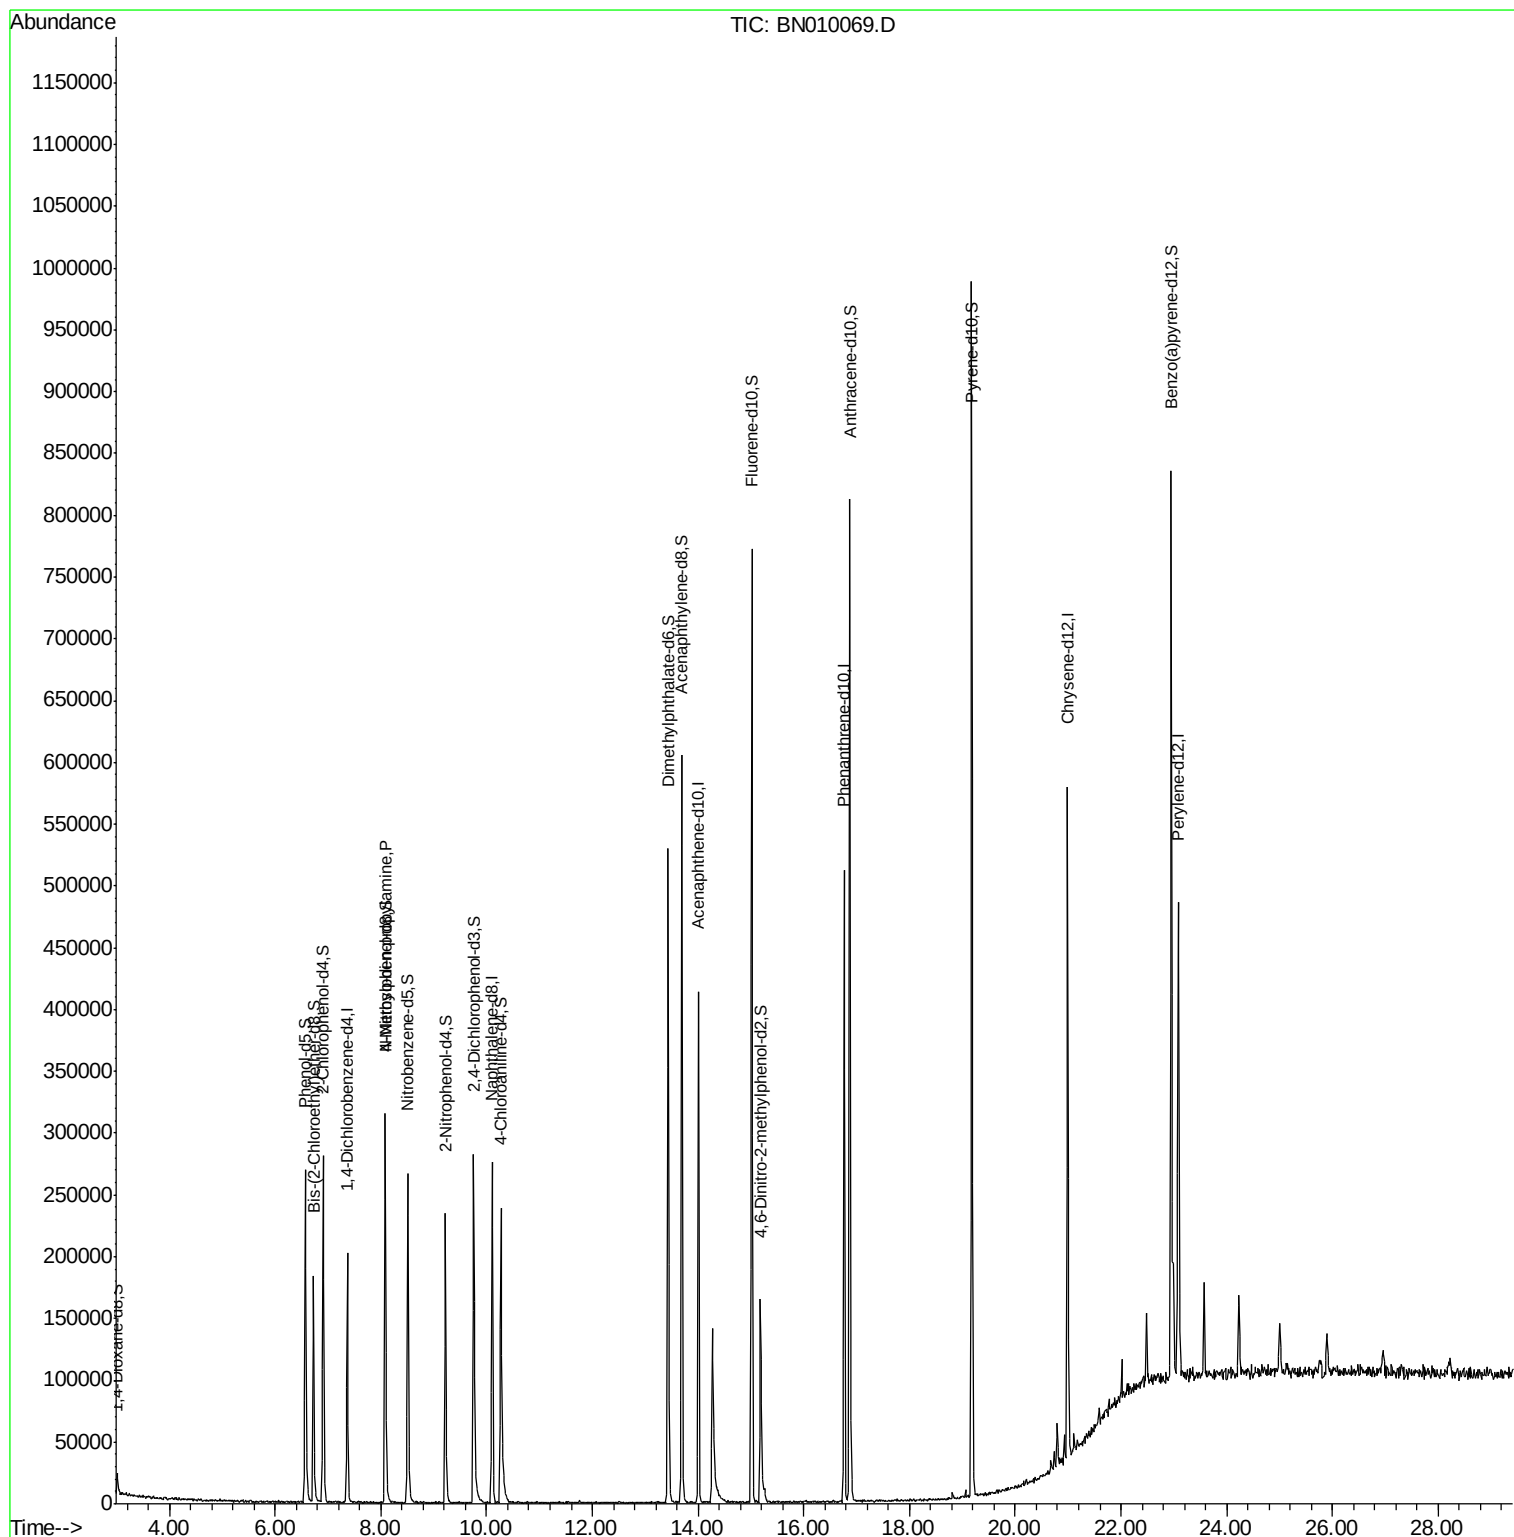

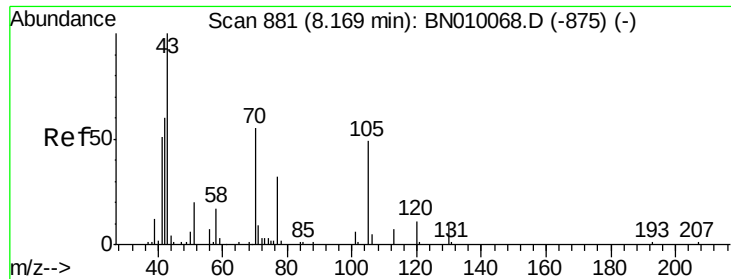

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.096 ng/ul
 RT: 8.07 min Scan# 865
 Delta R.T. -0.09 min
 Lab File: BN010069.D
 Acq: 03 Mar 2020 19:44

Instrument :
 BNA_N
 ClientSampleId :
 SBLK47

Tgt Ion: 70 Resp: 2839
 Ion Ratio Lower Upper
 70 100
 42 497.0 72.6 108.8#
 101 0.0 7.7 11.5#
 130 0.0 14.7 22.1#

