

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030320\
Quantitation Report (QT Reviewed)


Data File : BN010054.D
Acq On : 02 Mar 2020 23:38
Operator : CG/JU
Sample : L1615-08DL 5X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Mar 03 03:04:06 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 03 01:05:31 2020
Response via : Initial Calibration

Instrument :
BNA_N
Client Sample Id :
DBDN2DL

Manual Integrations
APPROVED

mohammad
3/4/2020 7:50:58 AM

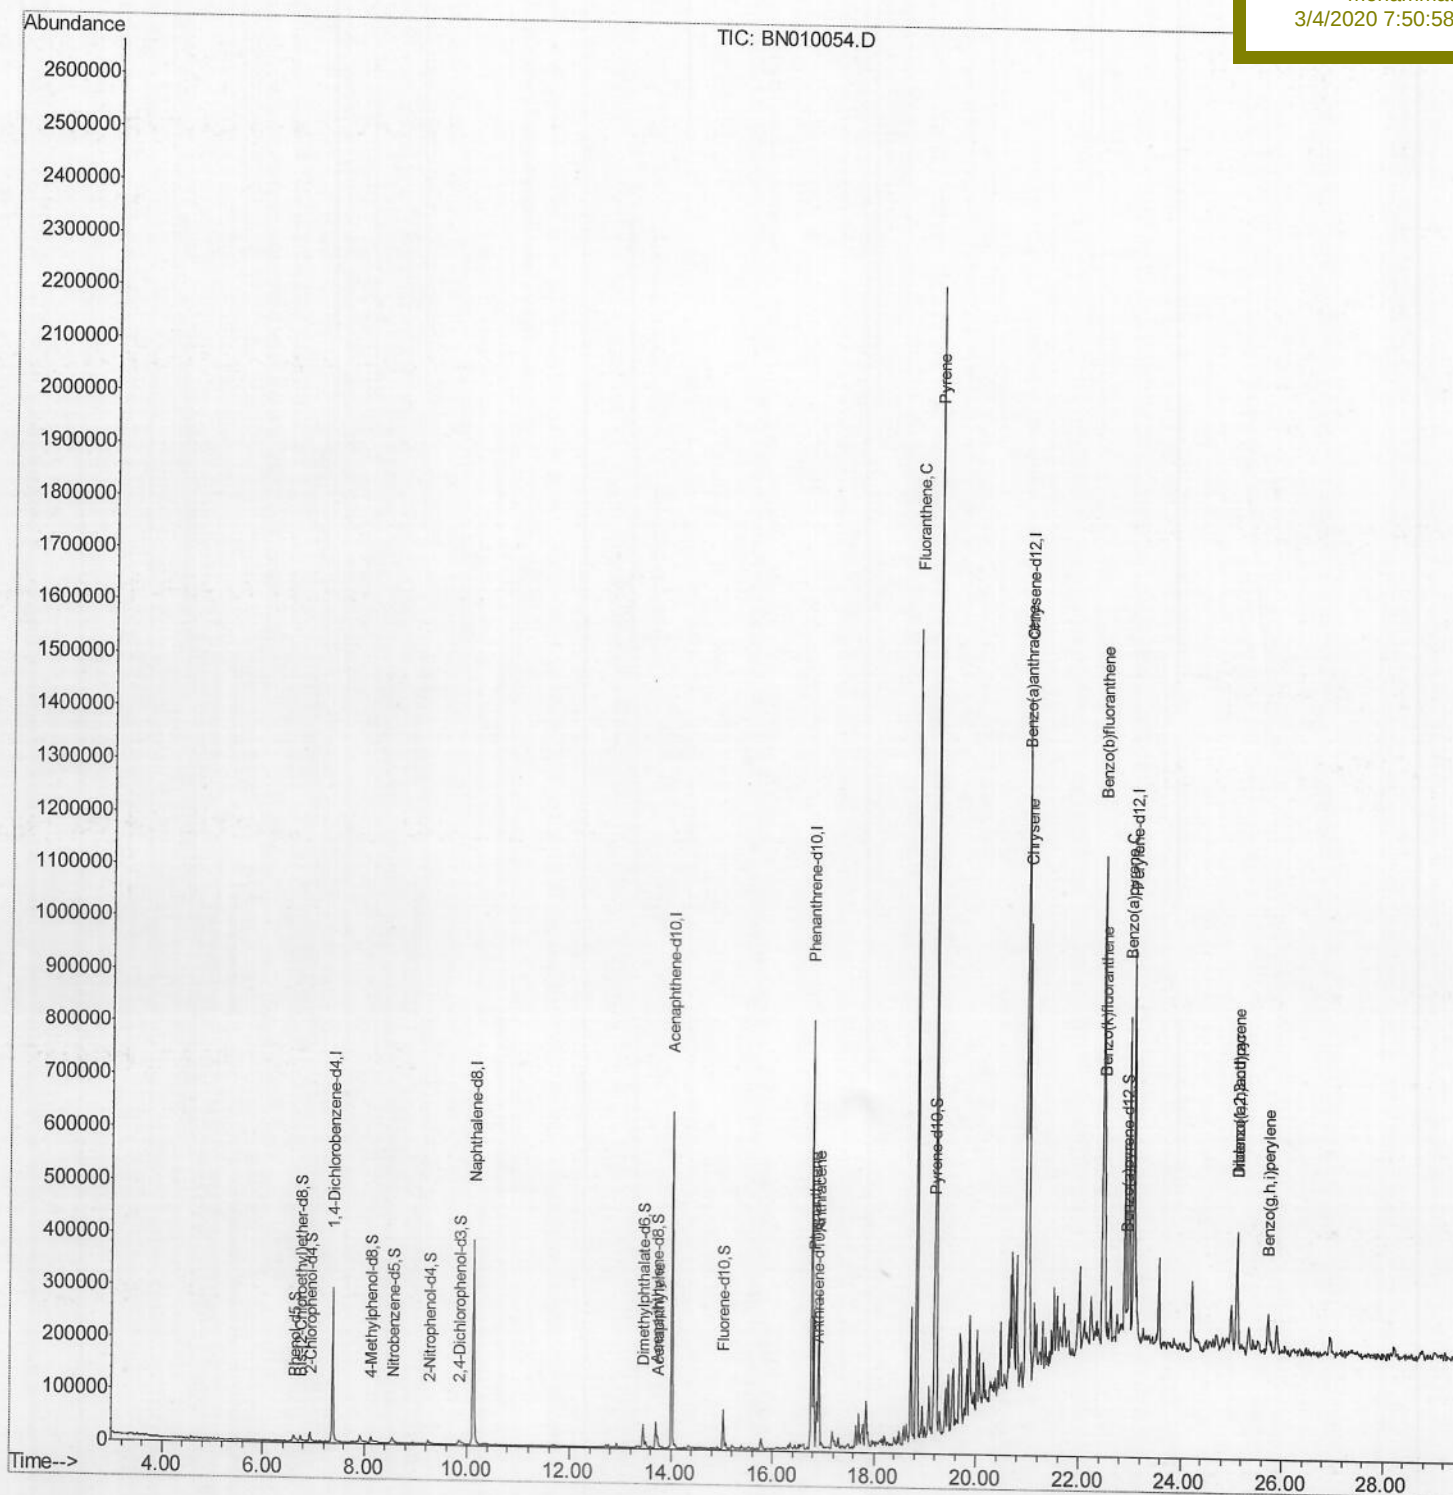

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030320\
Quantitation Report (Qedit)




Data File : BN010054.D
Acq On : 02 Mar 2020 23:38
Operator : CG/JU
Sample : L1615-08DL 5X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Mar 03 01:09:44 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 03 01:05:31 2020
Response via : Initial Calibration

Instrument :
BNA_N
Client Sampled :
DBDN2DL

Manual Integrations
APPROVED

mohammad
3/4/2020 7:50:58 AM

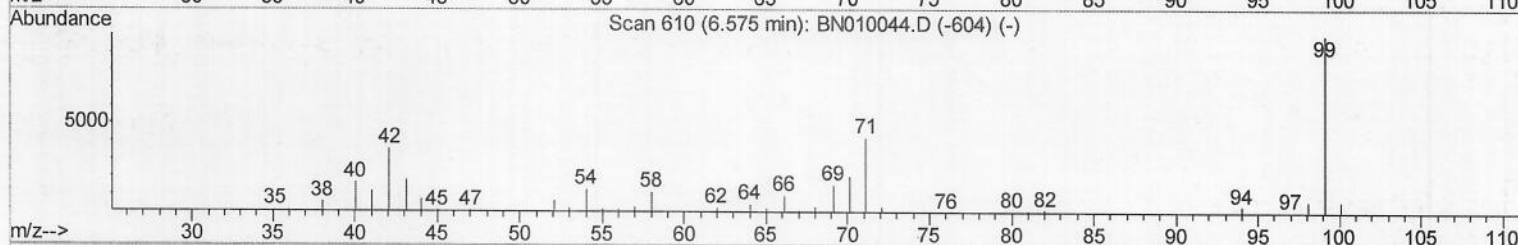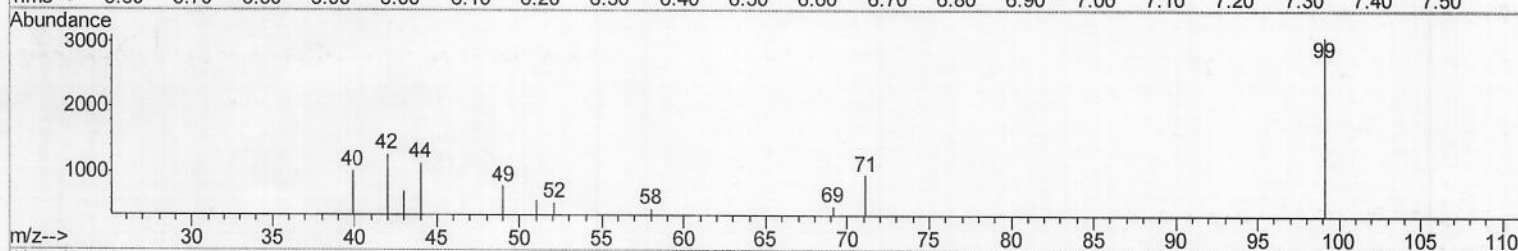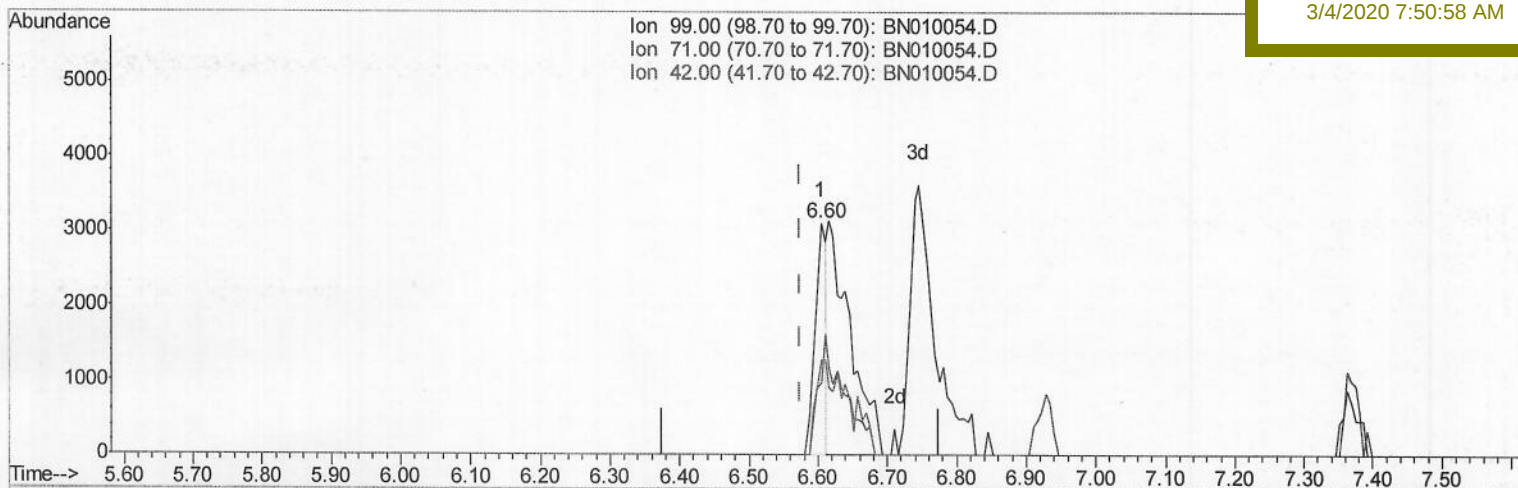

TIC: BN010054.D

(5) Phenol-d5 (S)

6.605min (+0.029) 0.57ng/ul

response 3459

Ion	Exp%	Act%
99.00	100	100
71.00	38.10	31.34
42.00	28.80	41.29#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030320\
Quantitation Report (Qedit)

Data File : BN010054.D

Acq On : 02 Mar 2020 23:38

Operator : CG/JU

Sample : L1615-08DL 5X

Misc :

ALS Vial : 12 Sample Multiplier: 1

Quant Time: Mar 03 01:09:44 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Tue Mar 03 01:05:31 2020

Response via : Initial Calibration

Instrument :

BNA_N

Client Sampled :




DBDN2DL

Manual Integrations

APPROVED

mohammad

3/4/2020 7:50:58 AM

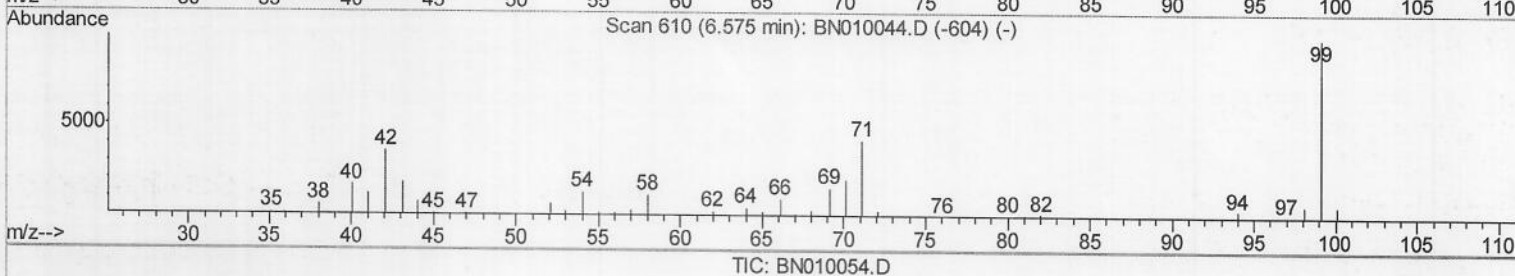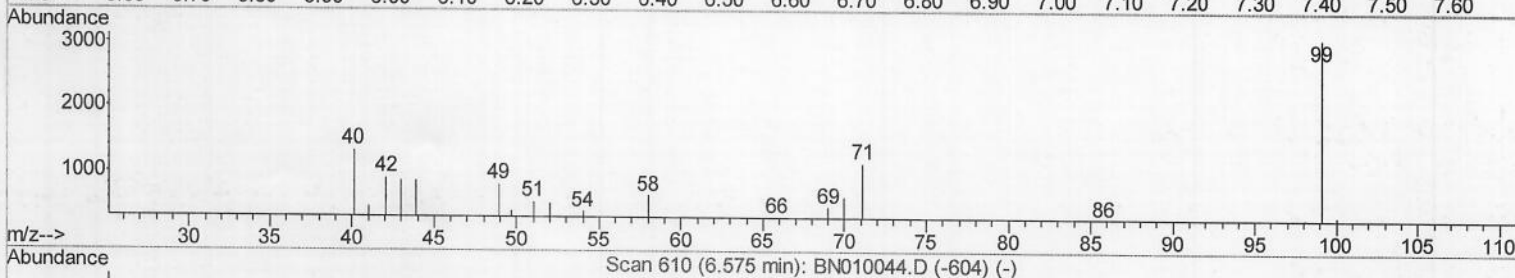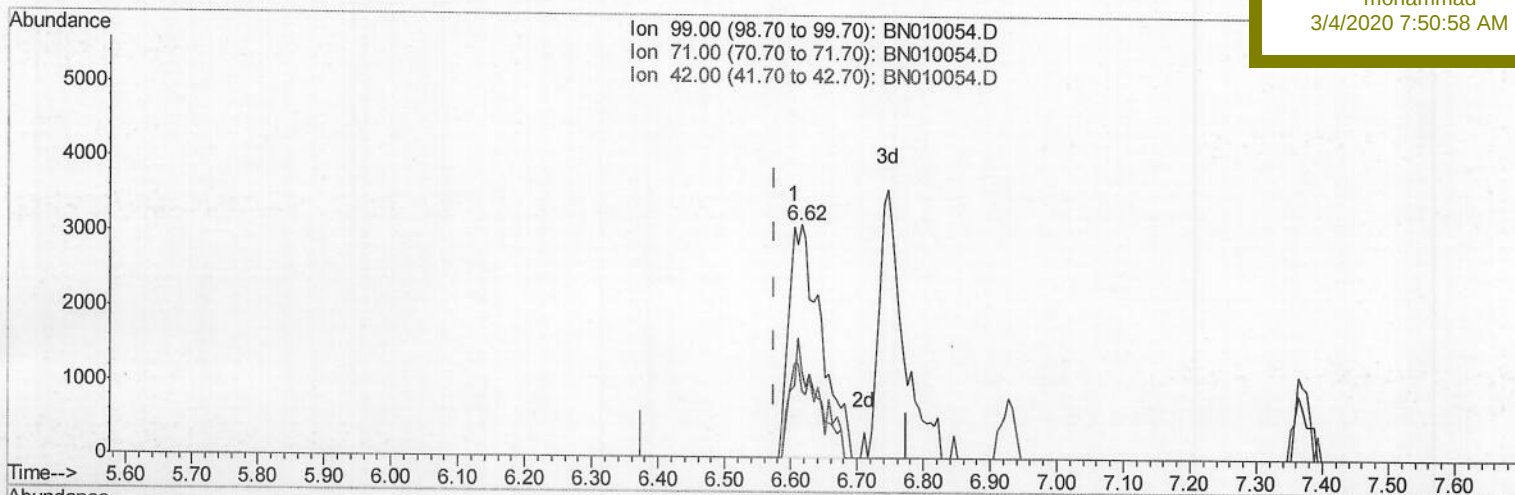

(5) Phenol-d5 (S)

6.616min (+0.041) 1.72ng/ul m

response 10502

Ion	Exp%	Act%
99.00	100	100
71.00	38.10	37.14
42.00	28.80	28.91
0.00	0.00	0.00

JU 03/05/20

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030320\
Quantitation Report (Qedit)




Data File : BN010054.D
Acq On : 02 Mar 2020 23:38
Operator : CG/JU
Sample : L1615-08DL 5X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Mar 03 01:09:44 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 03 01:05:31 2020
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
DBDN2DL

Manual Integrations
APPROVED

mohammad
3/4/2020 7:50:58 AM

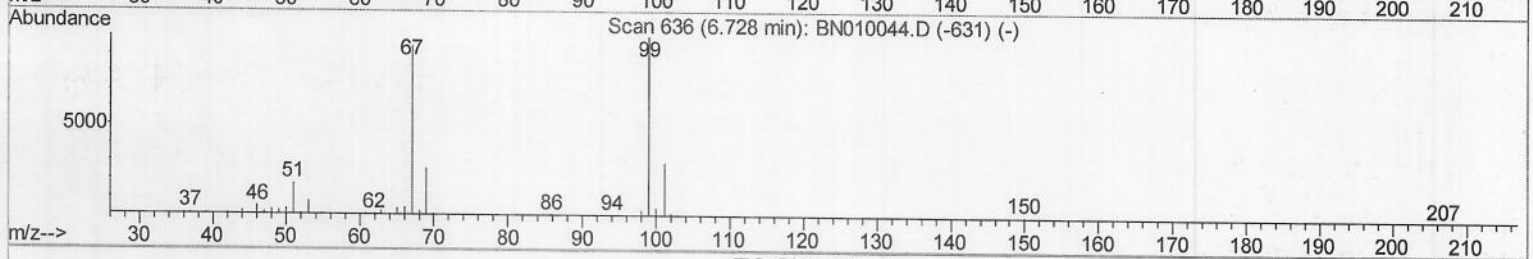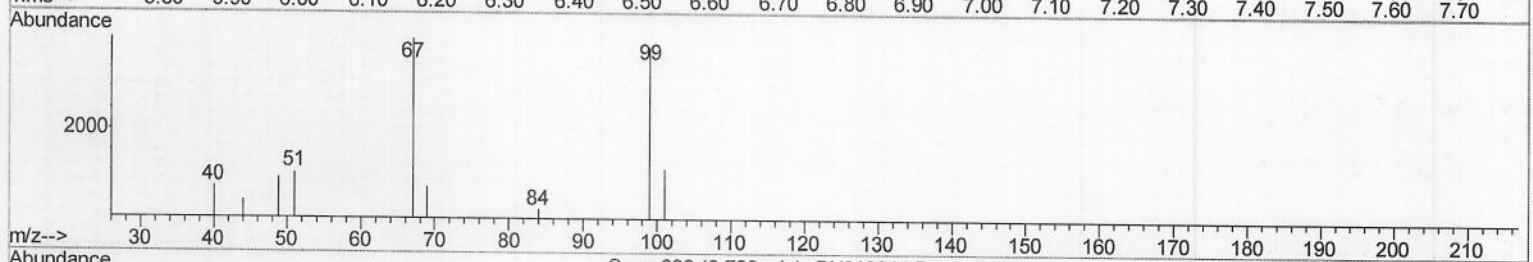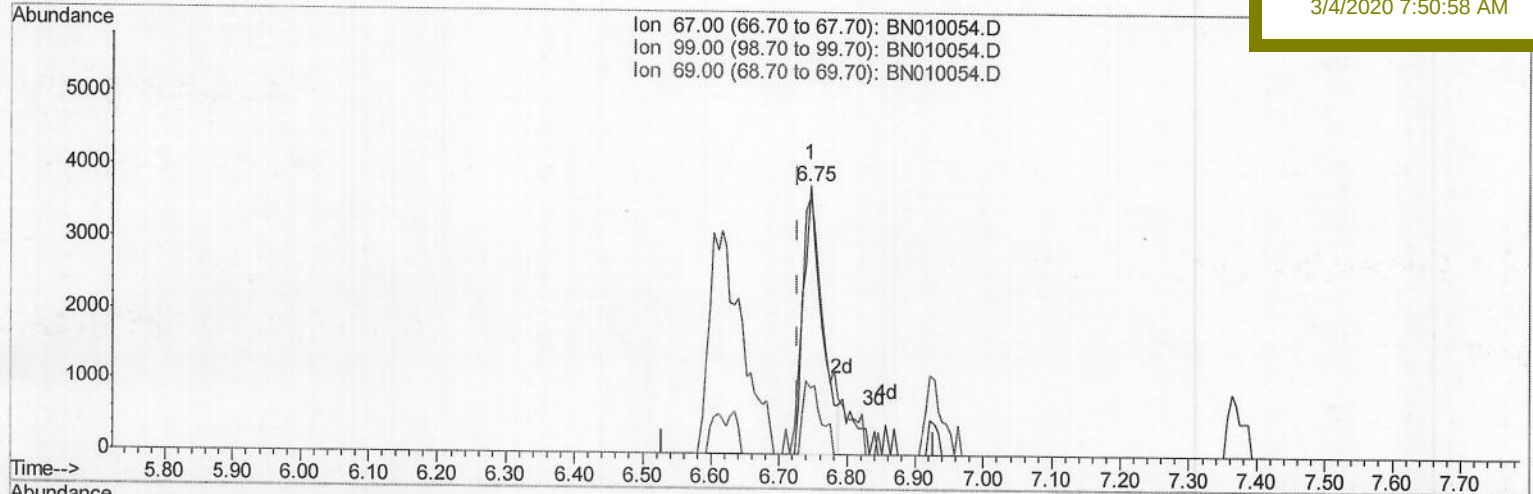

TIC: BN010054.D

(7) Bis-(2-Chloroethyl)ether-d8 (S)

6.746min (+0.018) 1.68ng/ul

response 7099

Ion	Exp%	Act%
67.00	100	100
99.00	106.90	95.95
69.00	28.30	24.35
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030320\
Quantitation Report (Qedit)




Data File : BN010054.D
Acq On : 02 Mar 2020 23:38
Operator : CG/JU
Sample : L1615-08DL 5X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Mar 03 01:09:44 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 03 01:05:31 2020
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
DBDN2DL

Manual Integrations
APPROVED

mohammad
3/4/2020 7:50:58 AM

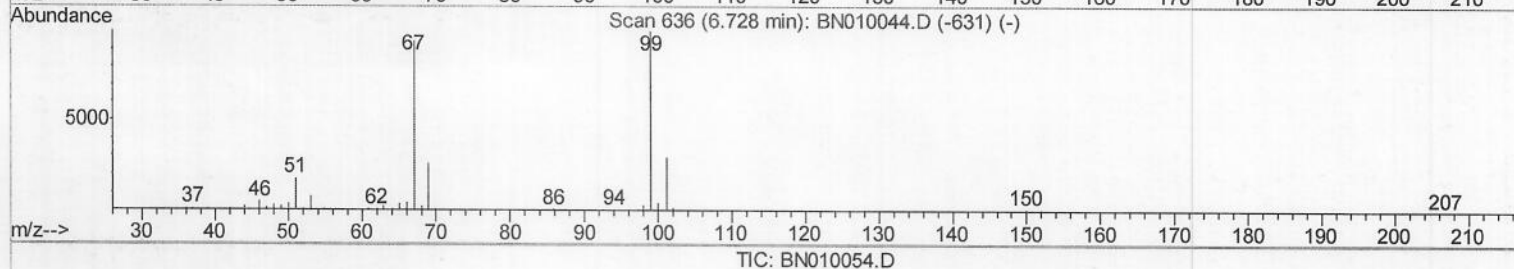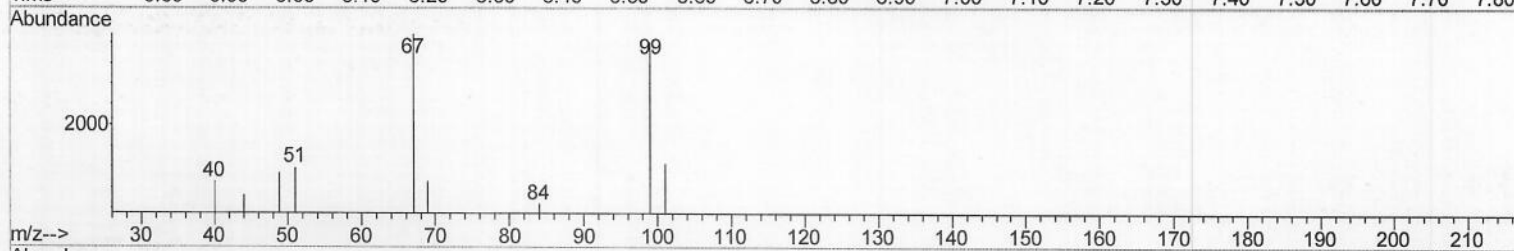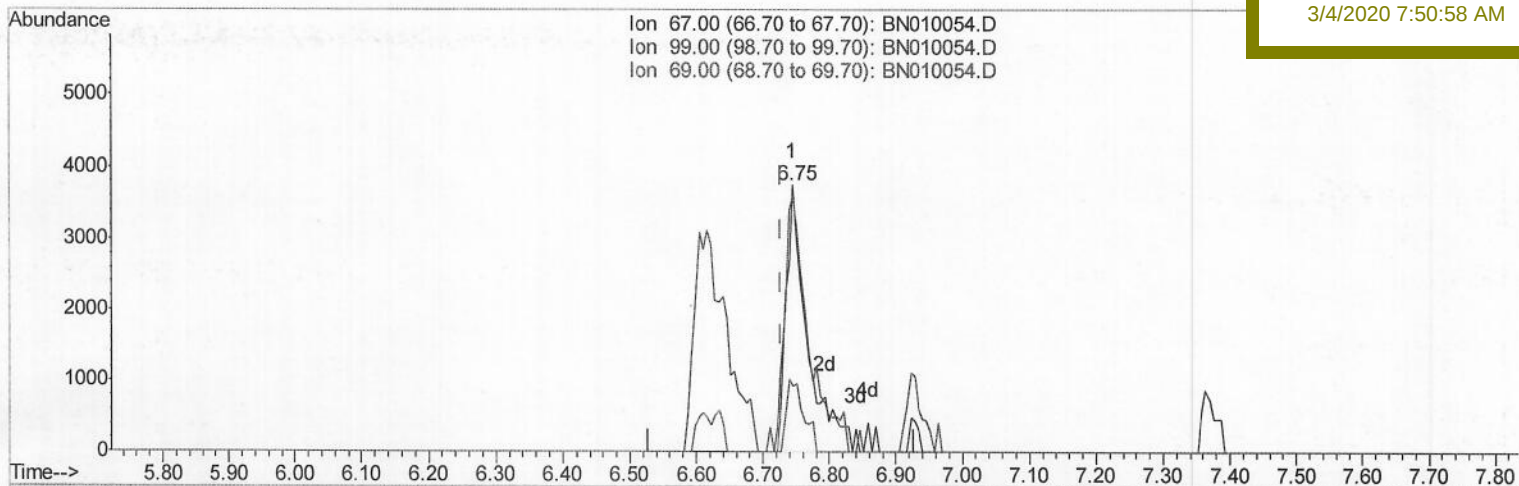

(7) Bis-(2-Chloroethyl)ether-d8 (S)

6.746min (+0.018) 1.96ng/ul m

response 8281

Ion	Exp%	Act%
67.00	100	100
99.00	106.90	95.95
69.00	28.30	24.35
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030320\
Quantitation Report (Qedit)




Data File : BN010054.D
Acq On : 02 Mar 2020 23:38
Operator : CG/JU
Sample : L1615-08DL 5X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Mar 03 01:09:44 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 03 01:05:31 2020
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
DBDN2DL

Manual Integrations
APPROVED

mohammad
3/4/2020 7:50:58 AM

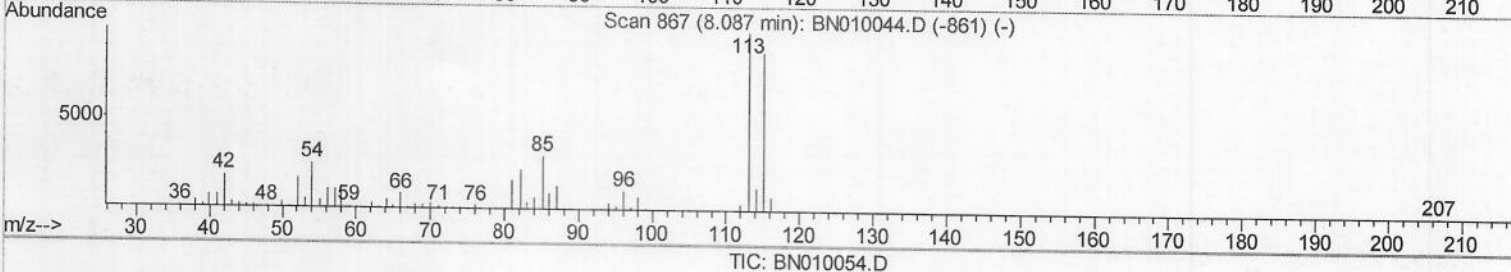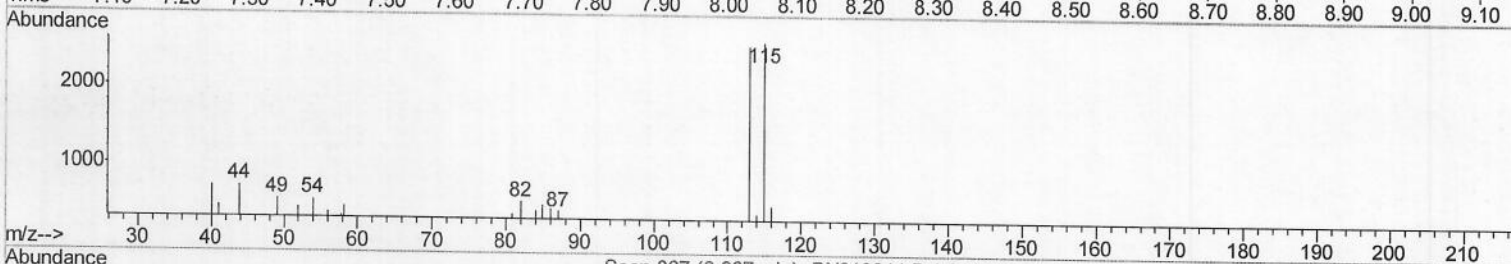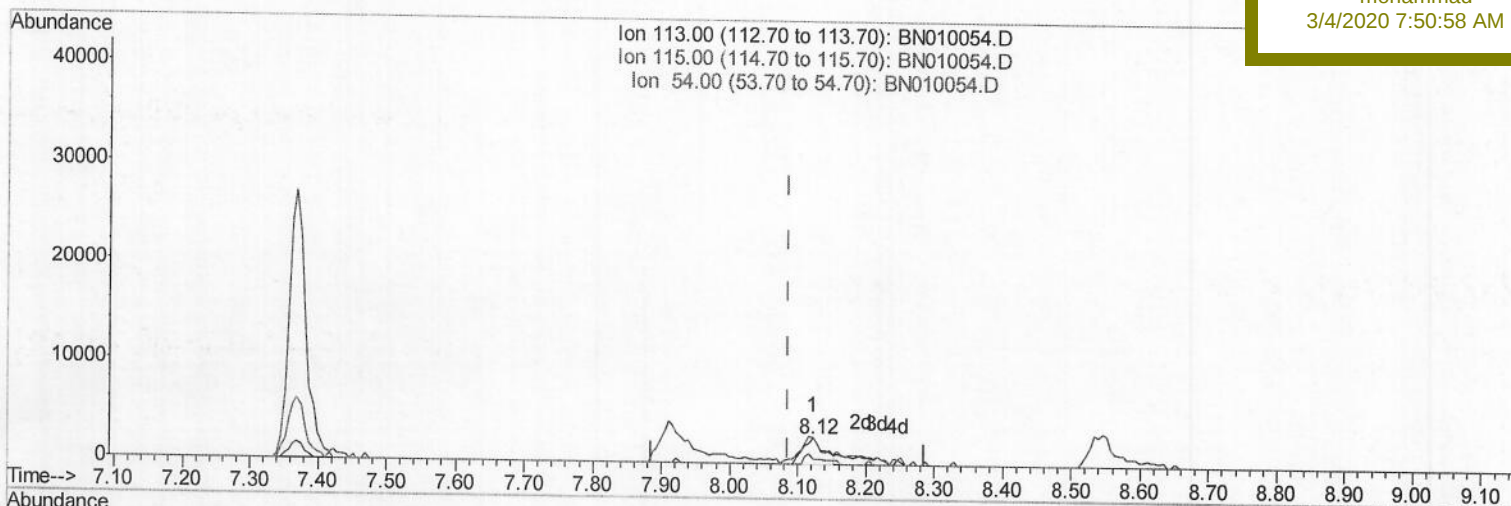

TIC: BN010054.D

(13) 4-Methylphenol-d8 (S)

8.122min (+0.035) 1.07ng/ul

response 5214

Ion	Exp%	Act%
113.00	100	100
115.00	90.70	101.60
54.00	21.20	21.55
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030320\
Quantitation Report (Qedit)




Data File : BN010054.D
Acq On : 02 Mar 2020 23:38
Operator : CG/JU
Sample : L1615-08DL 5X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Mar 03 01:09:44 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 03 01:05:31 2020
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
DBDN2DL

Manual Integrations
APPROVED

mohammad
3/4/2020 7:50:58 AM

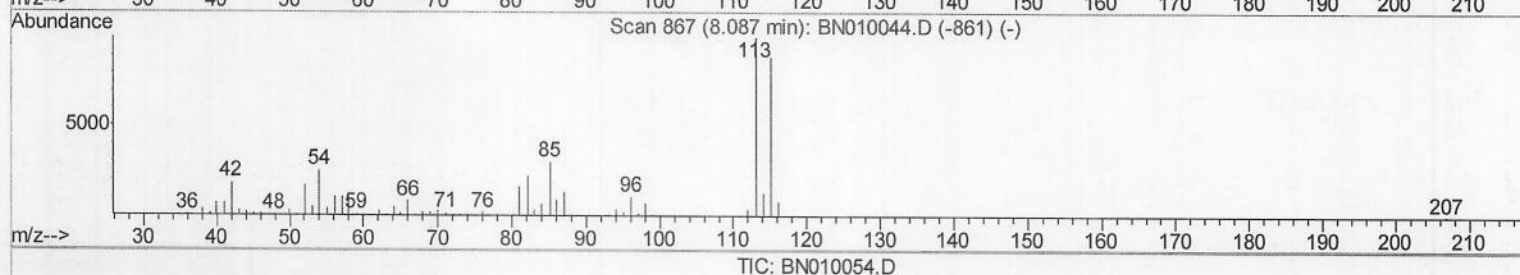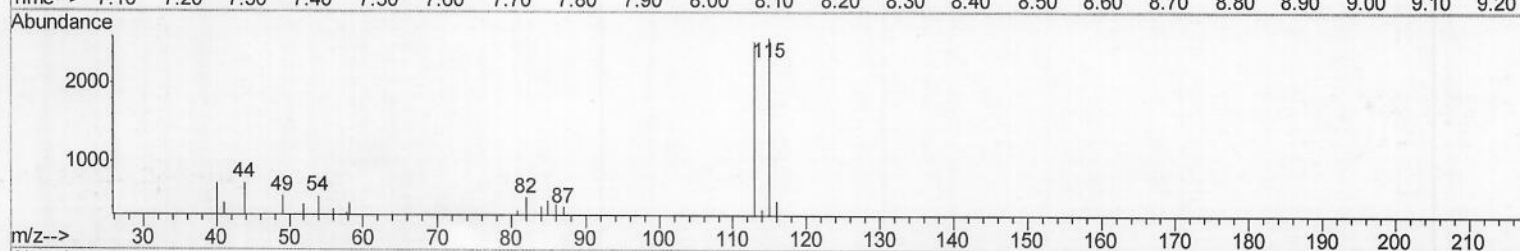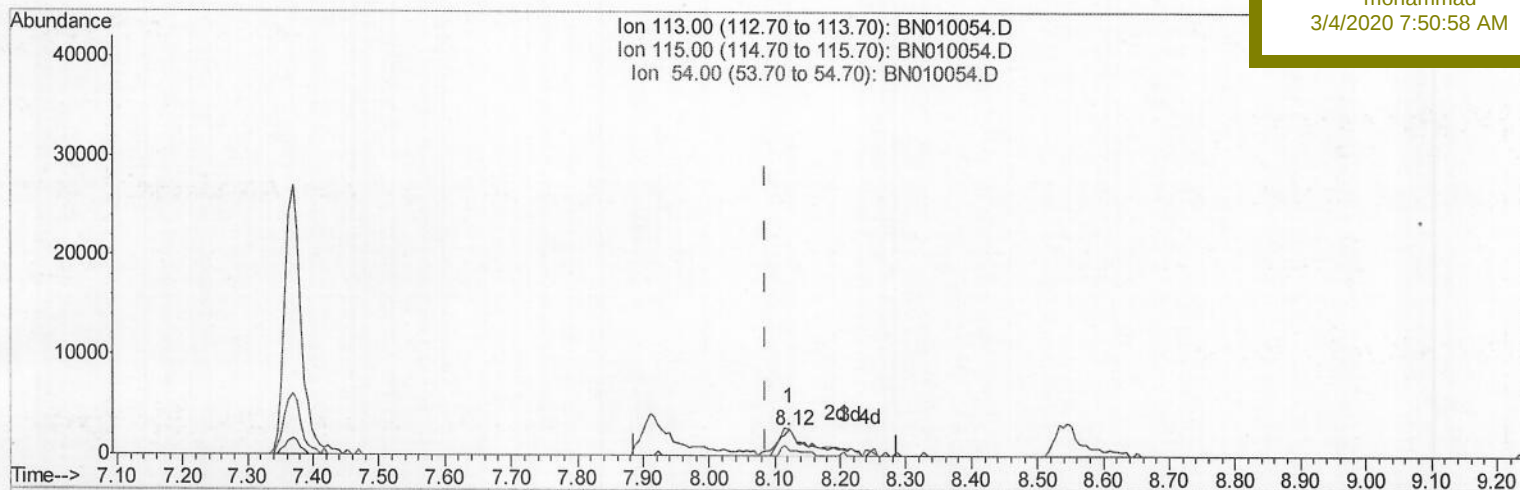

(13) 4-Methylphenol-d8 (S)

8.122min (+0.035) 1.75ng/ul m

response 8492

Ion	Exp%	Act%
113.00	100	100
115.00	90.70	101.60
54.00	21.20	21.55
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030320\
Quantitation Report (Qedit)




Data File : BN010054.D
Acq On : 02 Mar 2020 23:38
Operator : CG/JU
Sample : L1615-08DL 5X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Mar 03 01:09:44 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 03 01:05:31 2020
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
DBDN2DL

Manual Integrations
APPROVED

mohammad
3/4/2020 7:50:58 AM

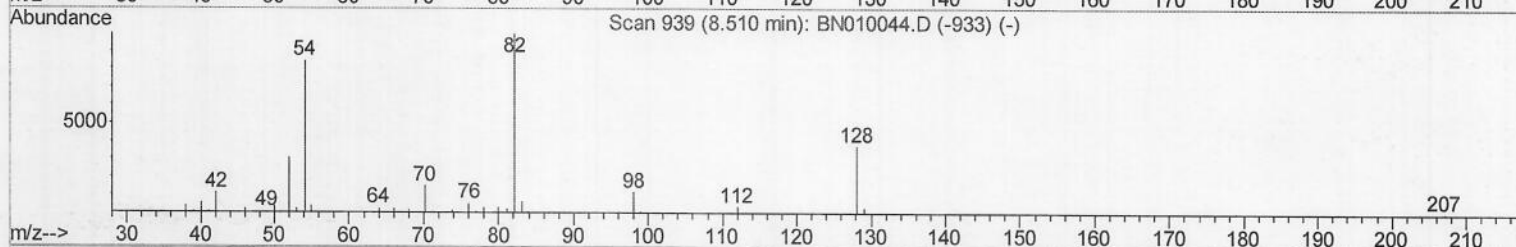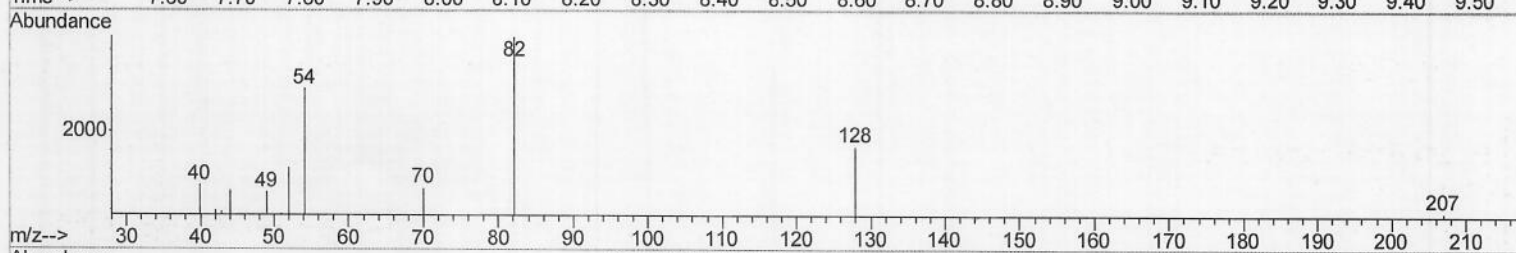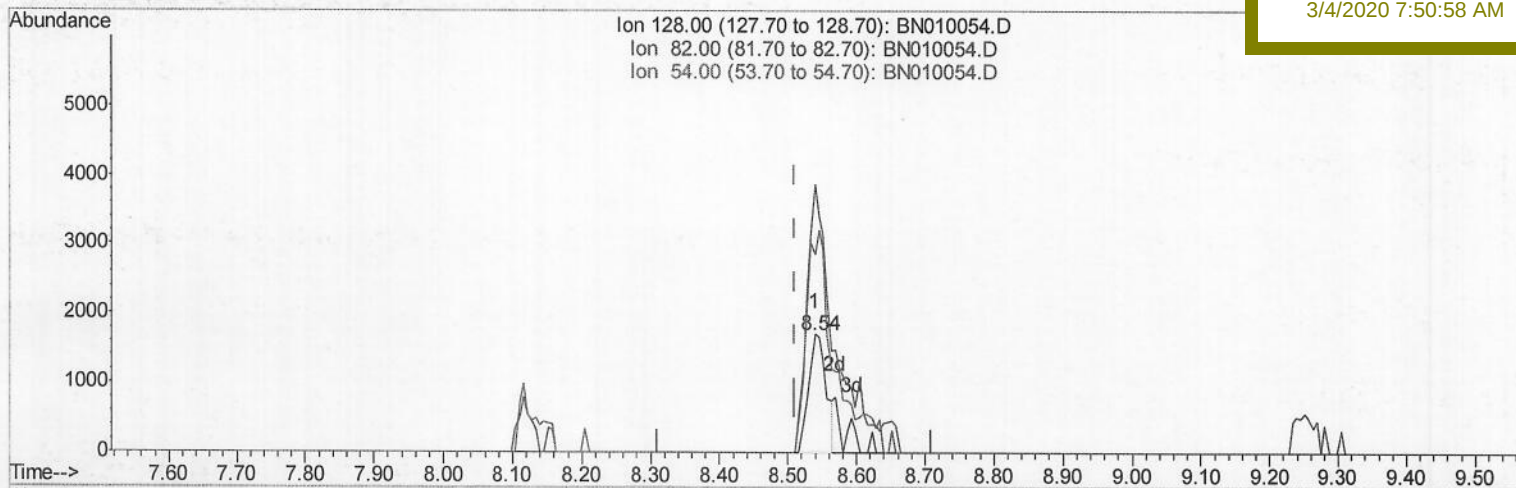

TIC: BN010054.D

(19) Nitrobenzene-d5 (S)

8.540min (+0.029) 1.30ng/ul

response 3021

Ion	Exp%	Act%
128.00	100	100
82.00	271.60	227.86
54.00	200.30	167.37
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030320\
Quantitation Report (Qedit)




Data File : BN010054.D
Acq On : 02 Mar 2020 23:38
Operator : CG/JU
Sample : L1615-08DL 5X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Mar 03 01:09:44 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 03 01:05:31 2020
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
DBDN2DL

Manual Integrations
APPROVED

mohammad
3/4/2020 7:50:58 AM

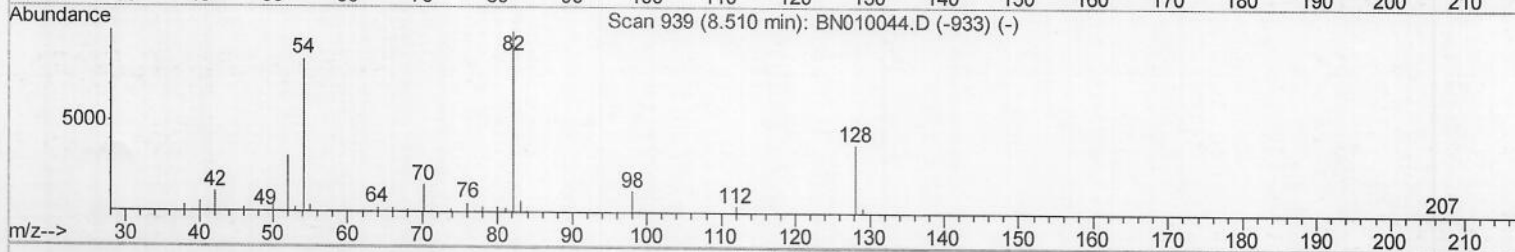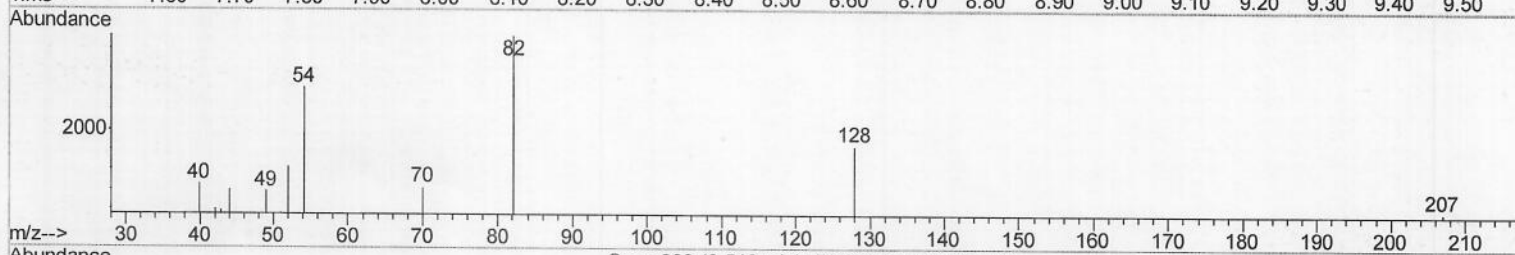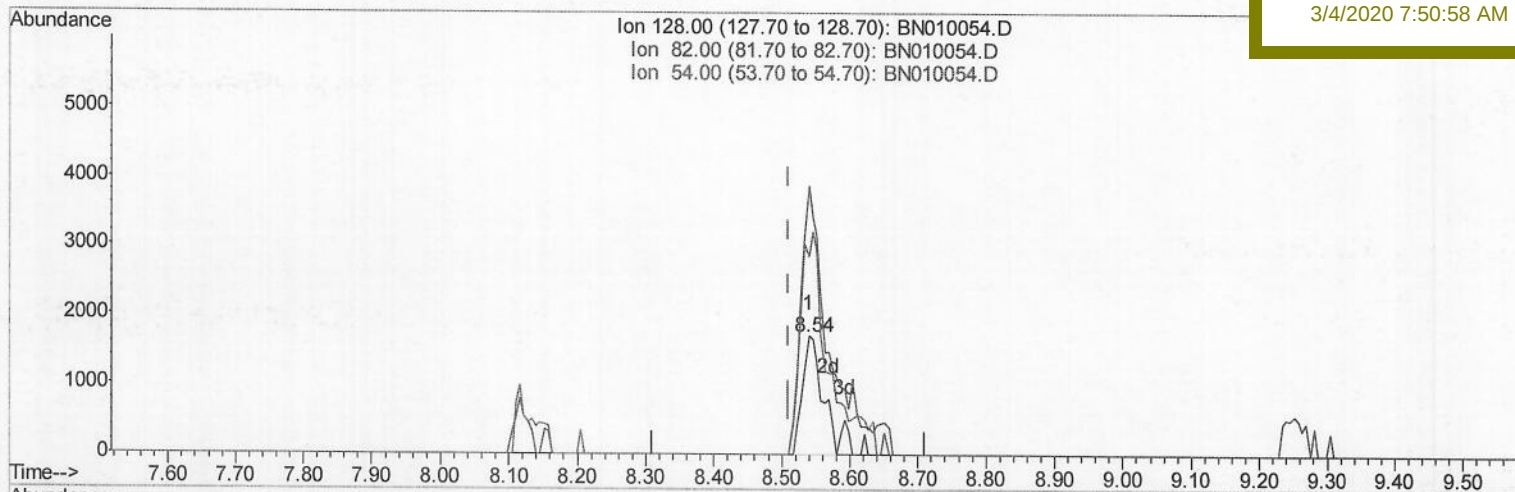

TIC: BN010054.D

(19) Nitrobenzene-d5 (S)

8.540min (+0.029) 1.48ng/ul m

response 3448

Ion	Exp%	Act%
128.00	100	100
82.00	271.60	227.86
54.00	200.30	167.37
0.00	0.00	0.00

5JU 03/05/20

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030320\
Quantitation Report (Qedit)




Data File : BN010054.D
Acq On : 02 Mar 2020 23:38
Operator : CG/JU
Sample : L1615-08DL 5X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Mar 03 01:09:44 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 03 01:05:31 2020
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
DBDN2DL

Manual Integrations
APPROVED

mohammad
3/4/2020 7:50:58 AM

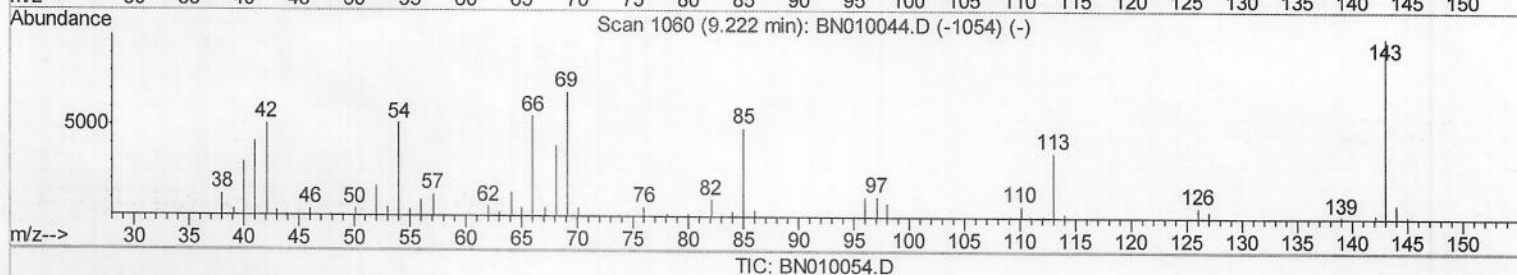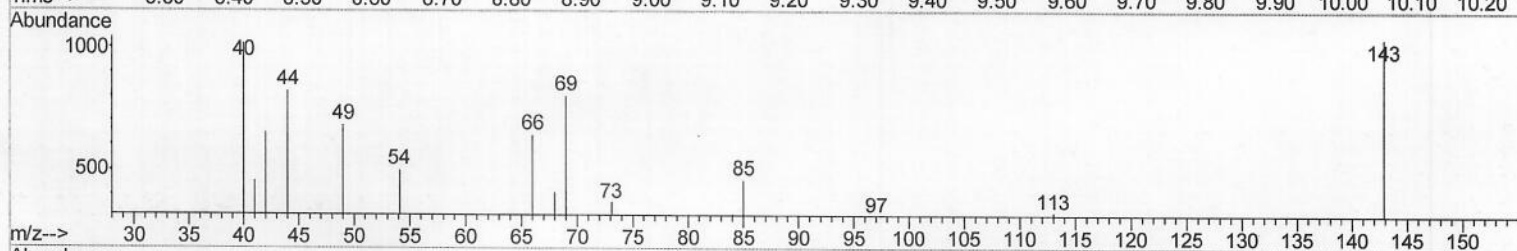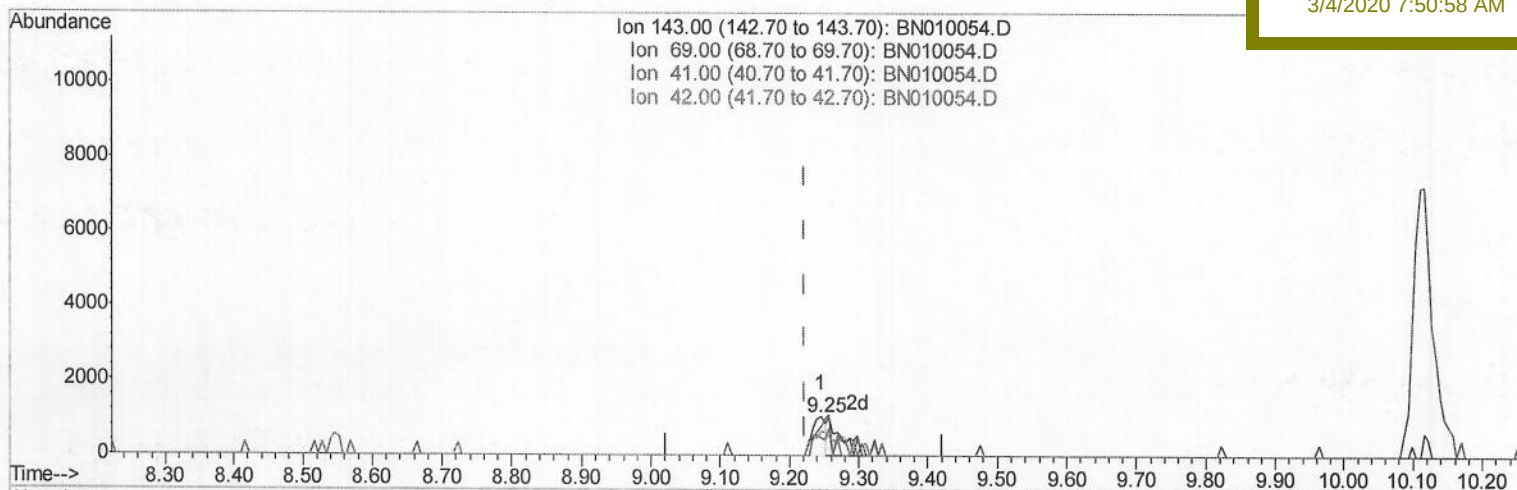

TIC: BN010054.D

(22) 2-Nitrophenol-d4 (S)
9.246min (+0.024) 0.55ng/ul
response 1412

Ion	Exp%	Act%
143.00	100	100
69.00	60.40	77.09#
41.00	36.00	43.50#
42.00	42.10	62.75#




Data File : BN010054.D
Acq On : 02 Mar 2020 23:38
Operator : CG/JU
Sample : L1615-08DL 5X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Mar 03 01:09:44 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 03 01:05:31 2020
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
DBDN2DL

Manual Integrations
APPROVED

mohammad
3/4/2020 7:50:58 AM

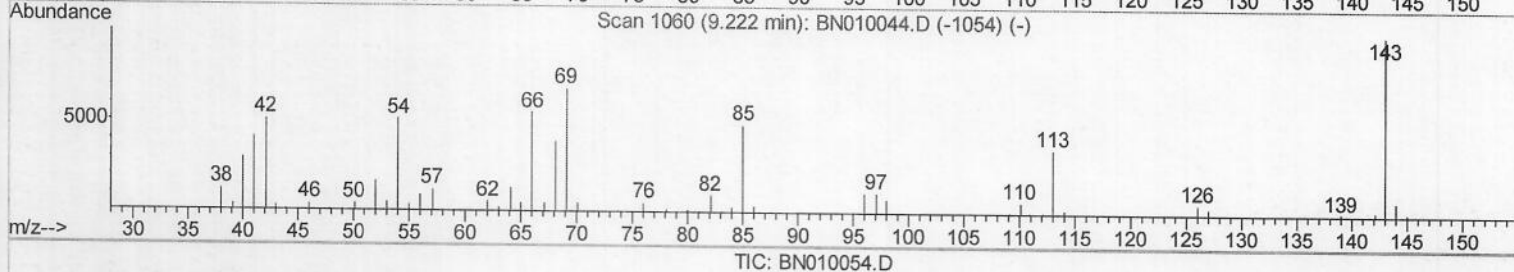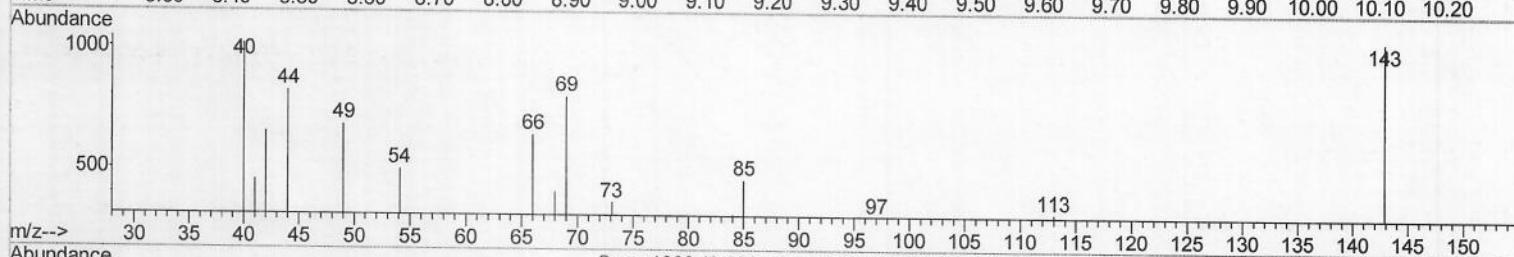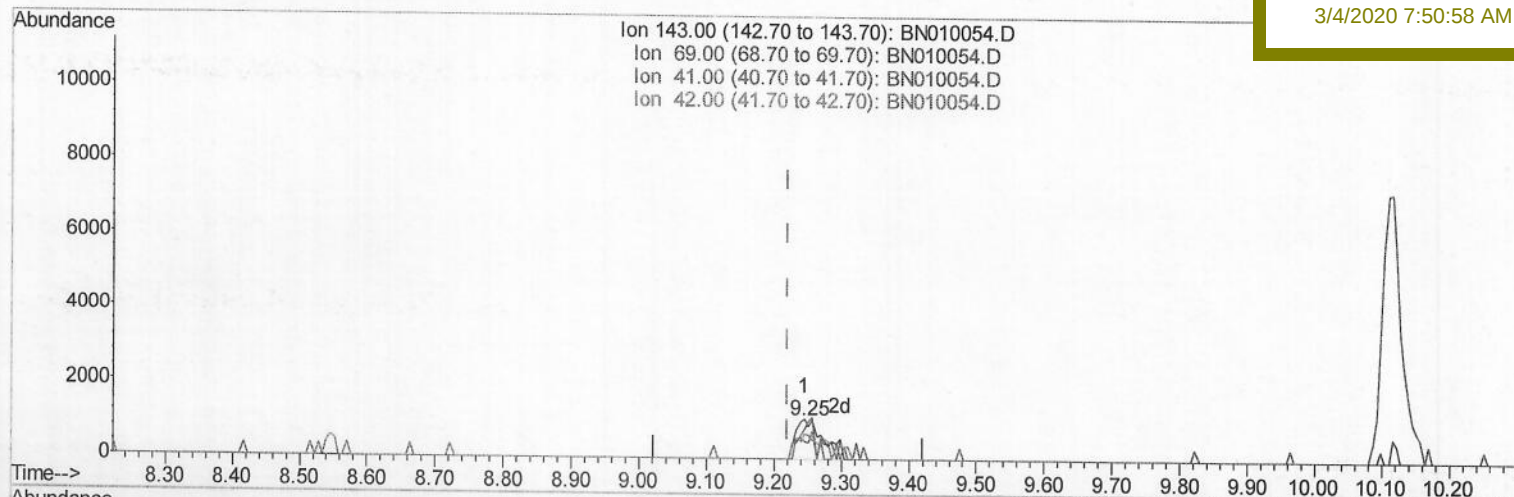

TIC: BN010054.D

(22) 2-Nitrophenol-d4 (S)

9.246min (+0.024) 1.17ng/ul m

> J003/05/20

response 2974

Ion	Exp%	Act%
143.00	100	100
69.00	60.40	77.09#
41.00	36.00	43.50#
42.00	42.10	62.75#

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030320\
Quantitation Report (Qedit)

Data File : BN010054.D

Acq On : 02 Mar 2020 23:38

Operator : CG/JU

Sample : L1615-08DL 5X

Misc :

ALS Vial : 12 Sample Multiplier: 1

Quant Time: Mar 03 01:09:44 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Tue Mar 03 01:05:31 2020

Response via : Initial Calibration

Instrument :




BNA_N

ClientSampleId :

DBDN2DL

Manual Integrations
APPROVED

mohammad
3/4/2020 7:50:58 AM

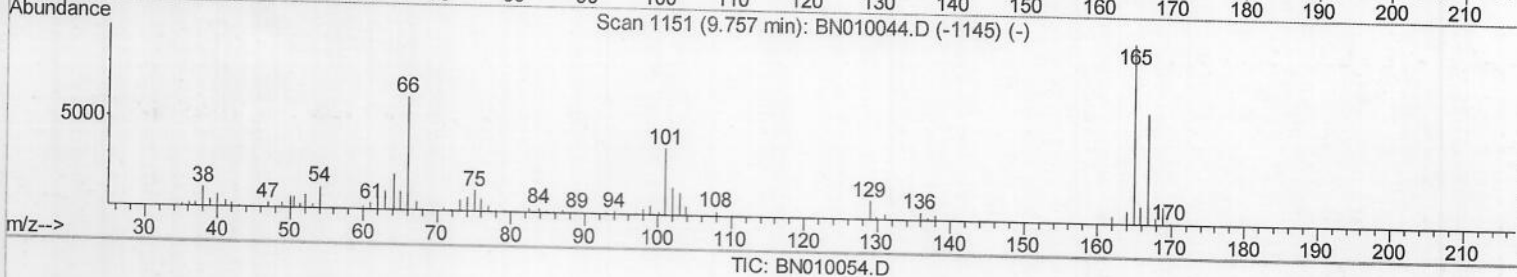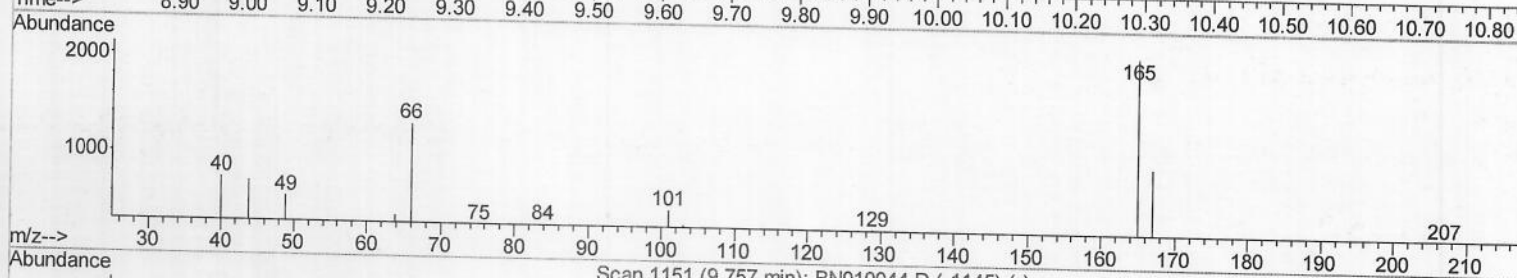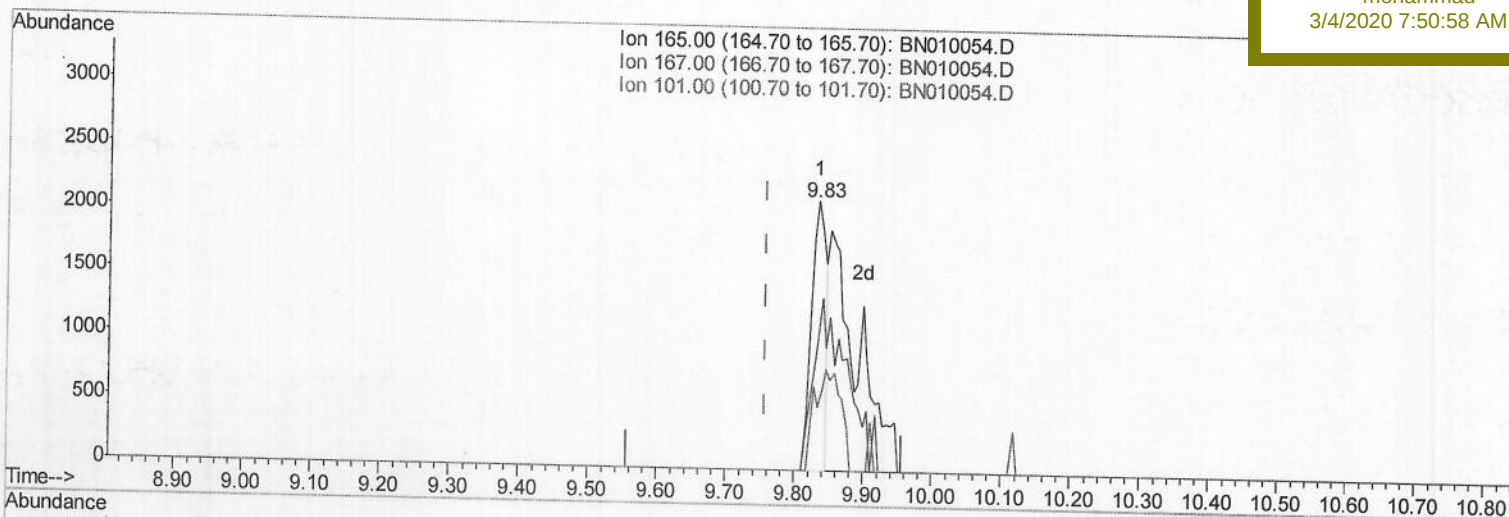

(26) 2,4-Dichlorophenol-d3 (S)

9.834min (+0.077) 0.65ng/ul

response 3175

Ion	Exp%	Act%
165.00	100	100
167.00	64.20	47.16#
101.00	36.10	23.27#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030320\
Quantitation Report (Qedit)




Data File : BN010054.D
Acq On : 02 Mar 2020 23:38
Operator : CG/JU
Sample : L1615-08DL 5X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Mar 03 01:09:44 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 03 01:05:31 2020
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
DBDN2DL

Manual Integrations
APPROVED

mohammad
3/4/2020 7:50:58 AM

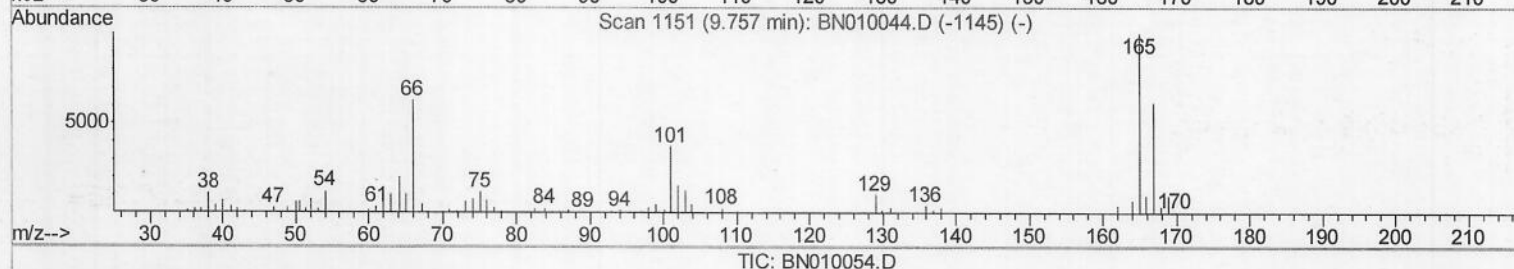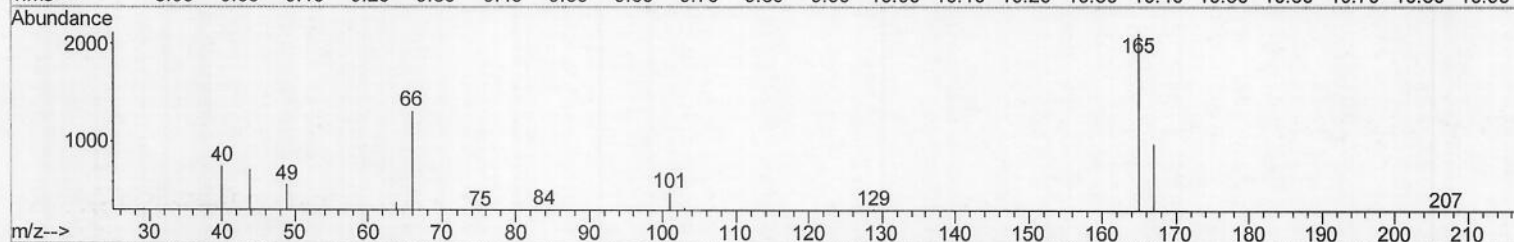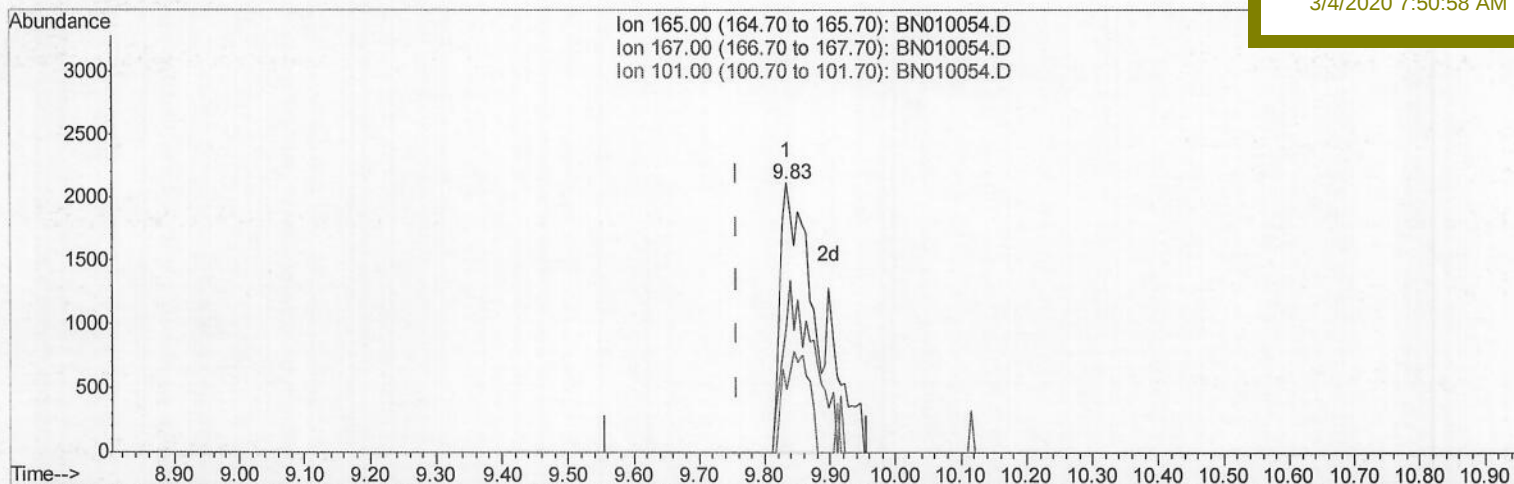

(26) 2,4-Dichlorophenol-d3 (S)

9.834min (+0.077) 1.74ng/ul m

response 8504

Ion	Exp%	Act%
165.00	100	100
167.00	64.20	47.16#
101.00	36.10	23.27#
0.00	0.00	0.00

>JU 03/05/20

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030320\
Quantitation Report (Qedit)




Data File : BN010054.D
Acq On : 02 Mar 2020 23:38
Operator : CG/JU
Sample : L1615-08DL 5X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Mar 03 01:09:44 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 03 01:05:31 2020
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
DBDN2DL

Manual Integrations
APPROVED

mohammad
3/4/2020 7:50:58 AM

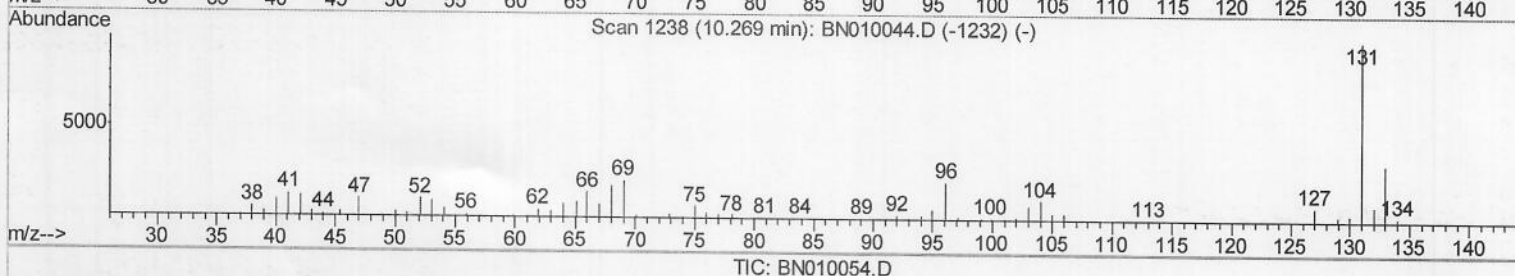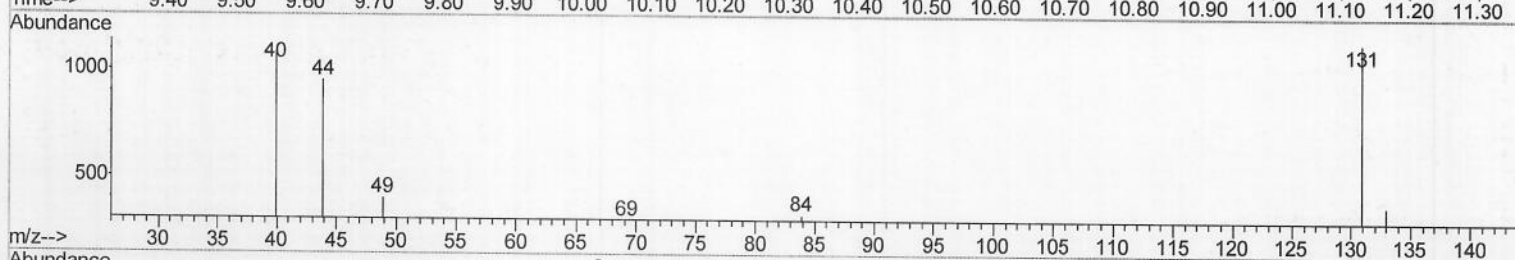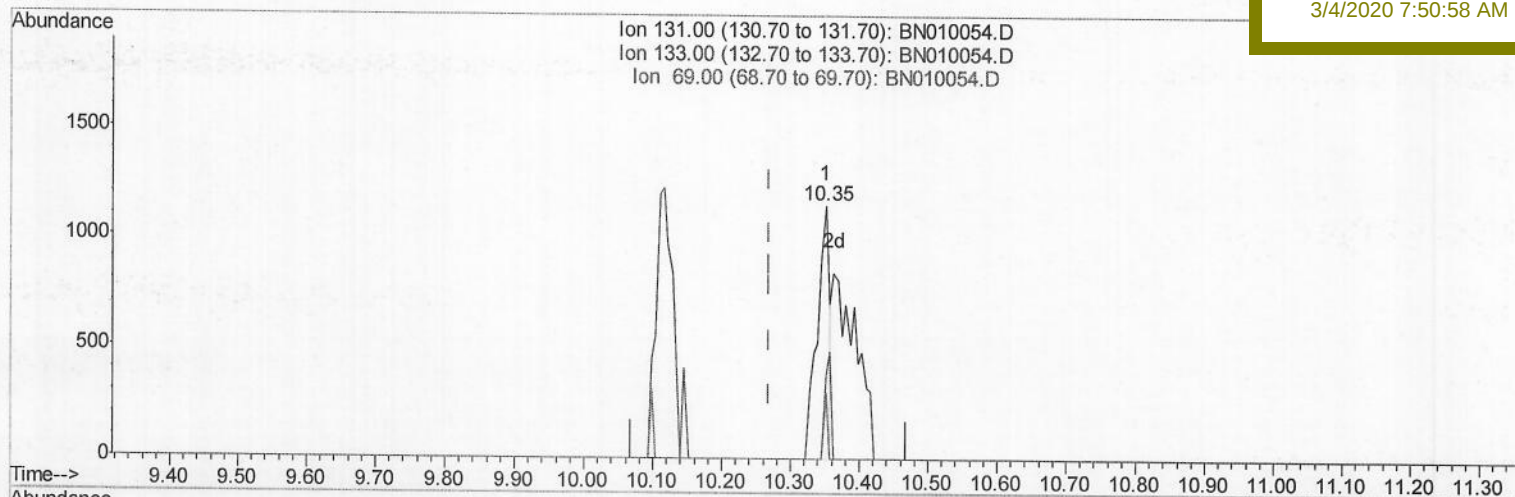

TIC: BN010054.D

(29) 4-Chloroaniline-d4 (S)

10.351min (+0.082) 0.26ng/ul

response 1432

Ion	Exp%	Act%
131.00	100	100
133.00	33.00	32.81
69.00	22.10	26.44
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030320\
Quantitation Report (Qedit)




Data File : BN010054.D
Acq On : 02 Mar 2020 23:38
Operator : CG/JU
Sample : L1615-08DL 5X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Mar 03 01:09:44 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 03 01:05:31 2020
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
DBDN2DL

Manual Integrations
APPROVED

mohammad
3/4/2020 7:50:58 AM

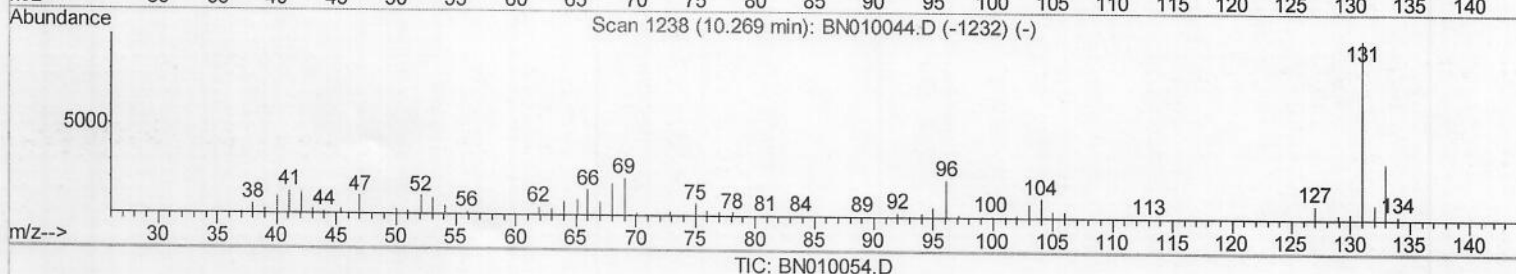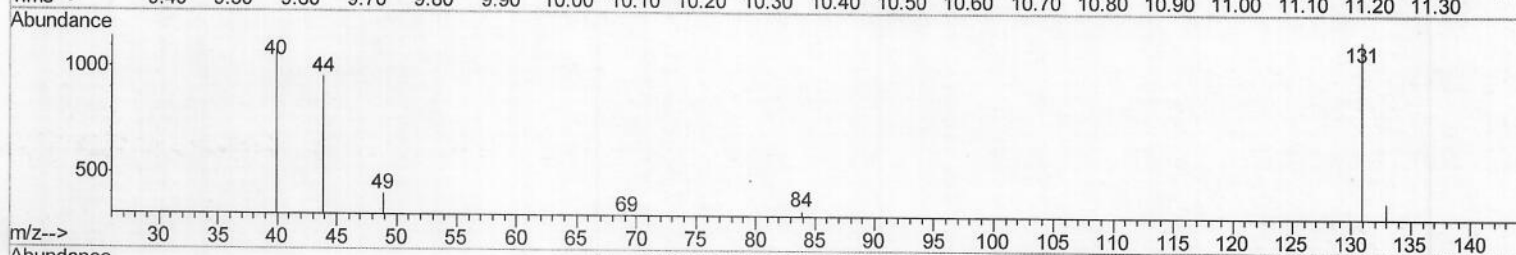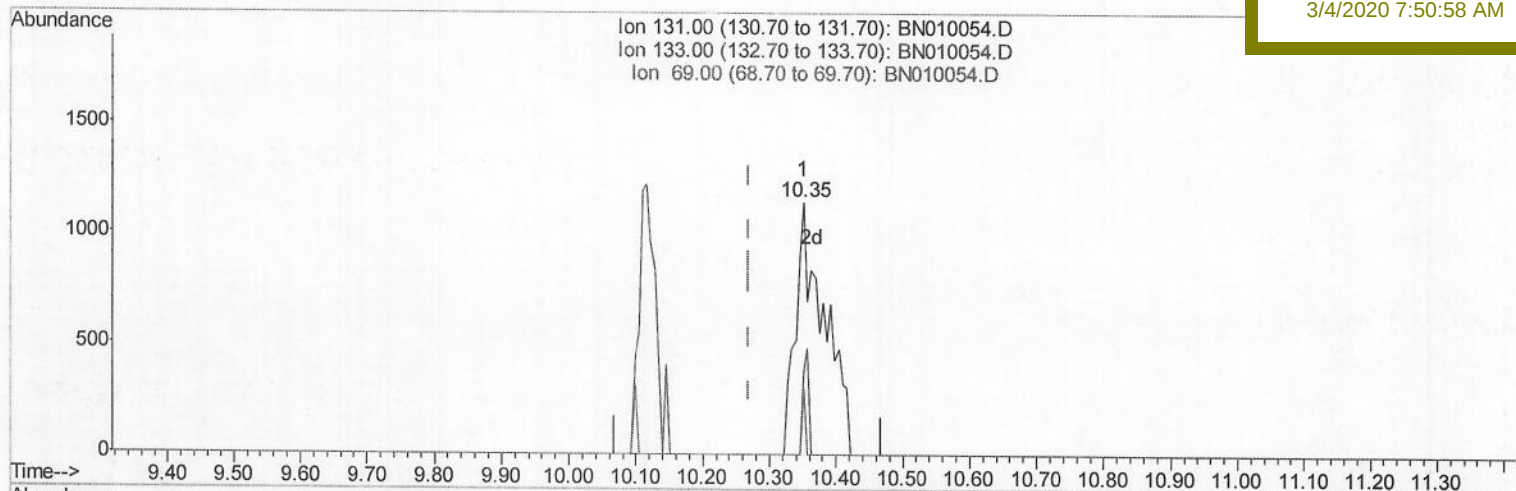

(29) 4-Chloroaniline-d4 (S)

10.351min (+0.082) 0.62ng/ul m

response 3410

Ion	Exp%	Act%
131.00	100	100
133.00	33.00	32.81
69.00	22.10	26.44
0.00	0.00	0.00

JU 03/05/20

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030320\
Quantitation Report (Qedit)




Data File : BN010054.D
Acq On : 02 Mar 2020 23:38
Operator : CG/JU
Sample : L1615-08DL 5X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Mar 03 01:09:44 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 03 01:05:31 2020
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
DBDN2DL

Manual Integrations
APPROVED

mohammad
3/4/2020 7:50:58 AM

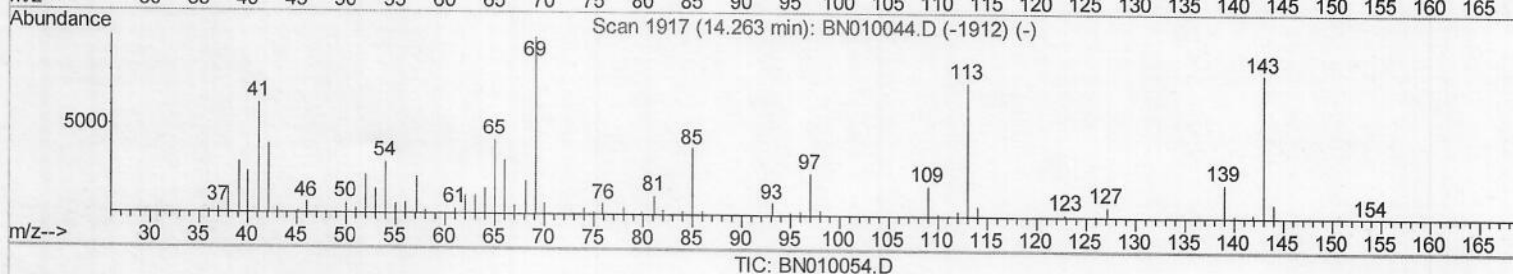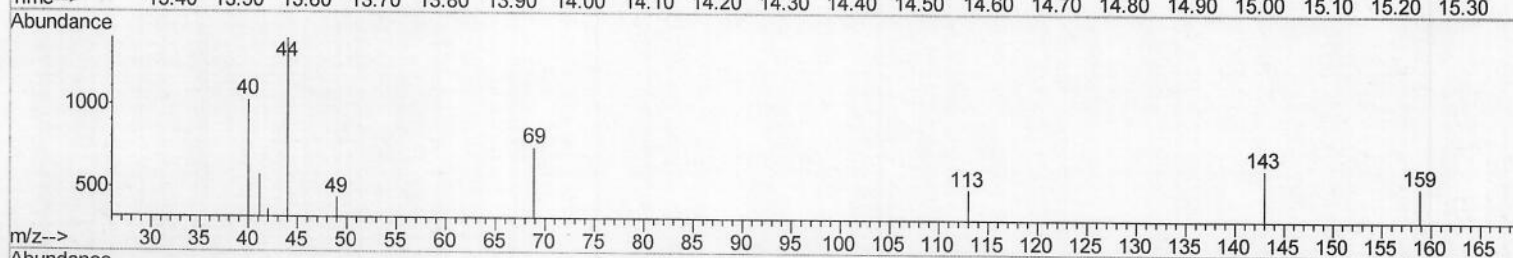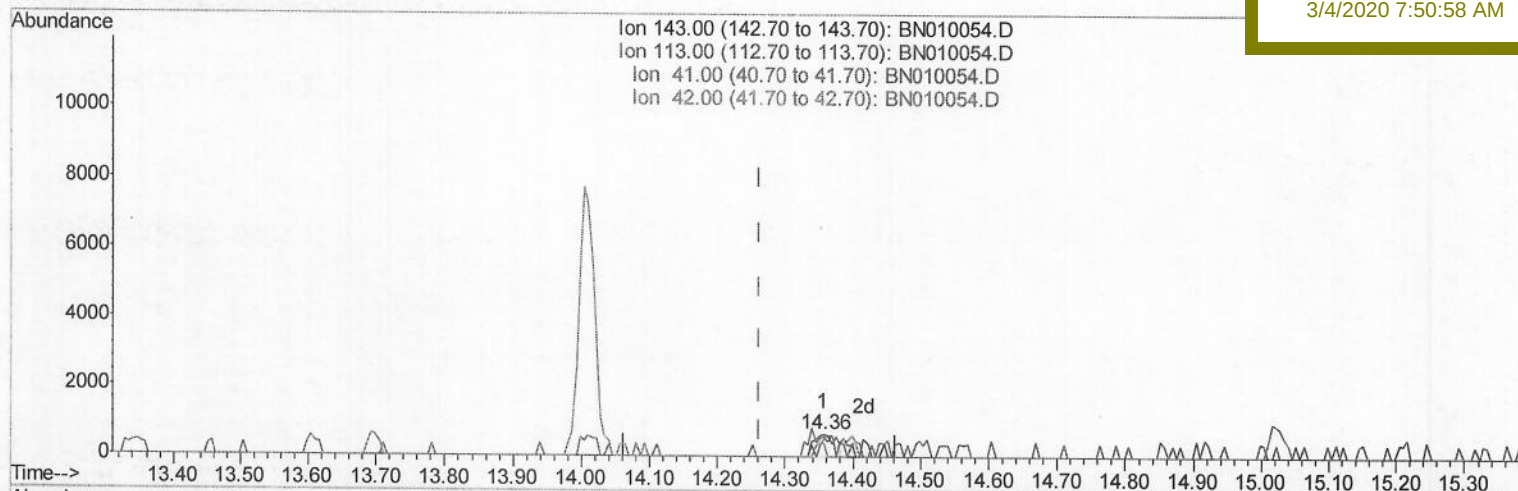

TIC: BN010054.D

(52) 4-Nitrophenol-d4 (S)

14.357min (+0.094) 0.50ng/ul

response 1413

Ion	Exp%	Act%
143.00	100	100
113.00	86.40	80.22
41.00	66.00	91.46#
42.00	43.20	59.02#

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030320\
Quantitation Report (Qedit)




Data File : BN010054.D
Acq On : 02 Mar 2020 23:38
Operator : CG/JU
Sample : L1615-08DL 5X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Mar 03 01:09:44 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 03 01:05:31 2020
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
DBDN2DL

Manual Integrations
APPROVED

mohammad
3/4/2020 7:50:58 AM

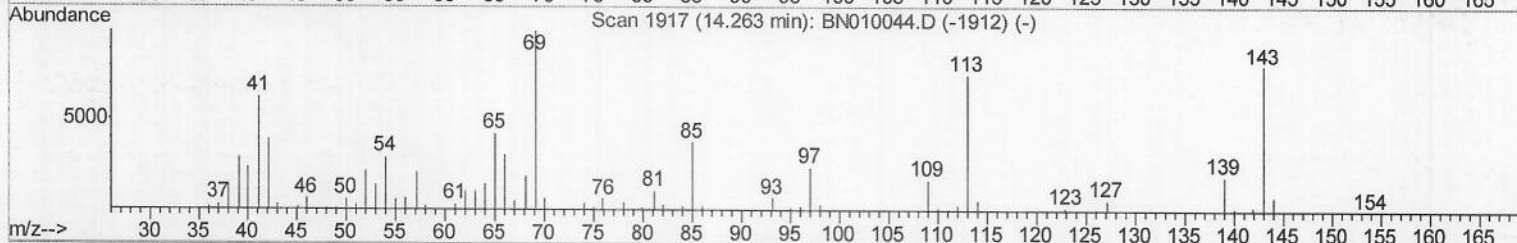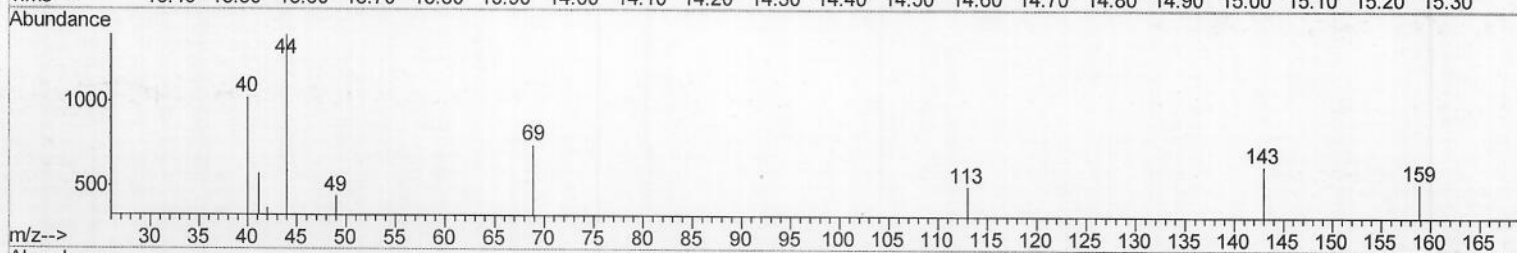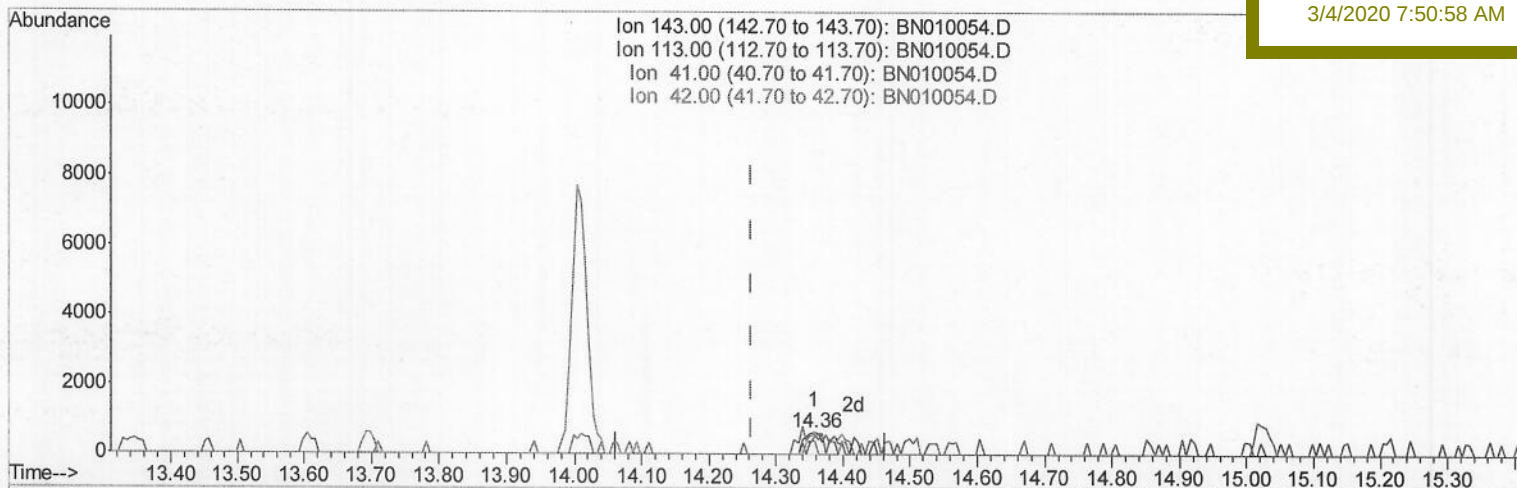

TIC: BN010054.D

(52) 4-Nitrophenol-d4 (S)

14.357min (+0.094) 0.64ng/ul m

response 1821

Ion	Exp%	Act%
143.00	100	100
113.00	86.40	80.22
41.00	66.00	91.46#
42.00	43.20	59.02#

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030320\
Quantitation Report (Qedit)




Data File : BN010054.D
Acq On : 02 Mar 2020 23:38
Operator : CG/JU
Sample : L1615-08DL 5X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Mar 03 01:09:44 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 03 01:05:31 2020
Response via : Initial Calibration

Instrument :
BNA_N
Client Sampled :
DBDN2DL

Manual Integrations
APPROVED

mohammad
3/4/2020 7:50:58 AM

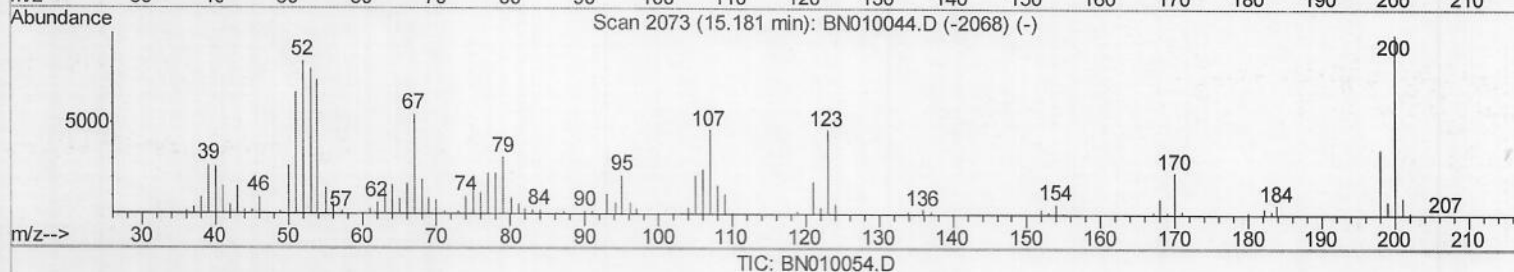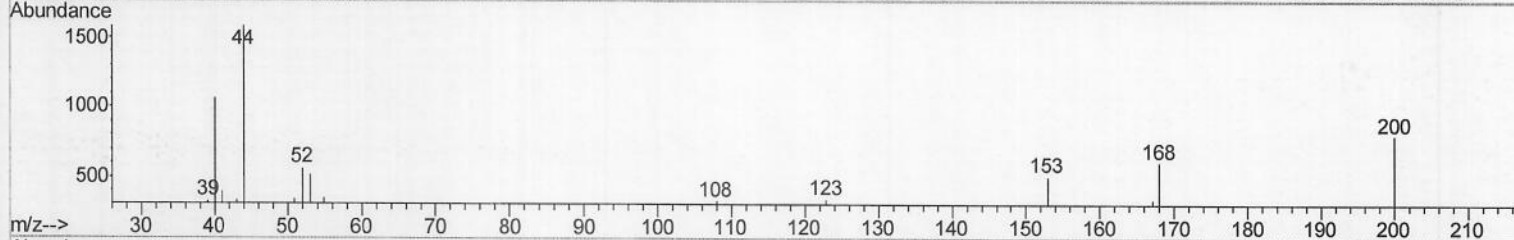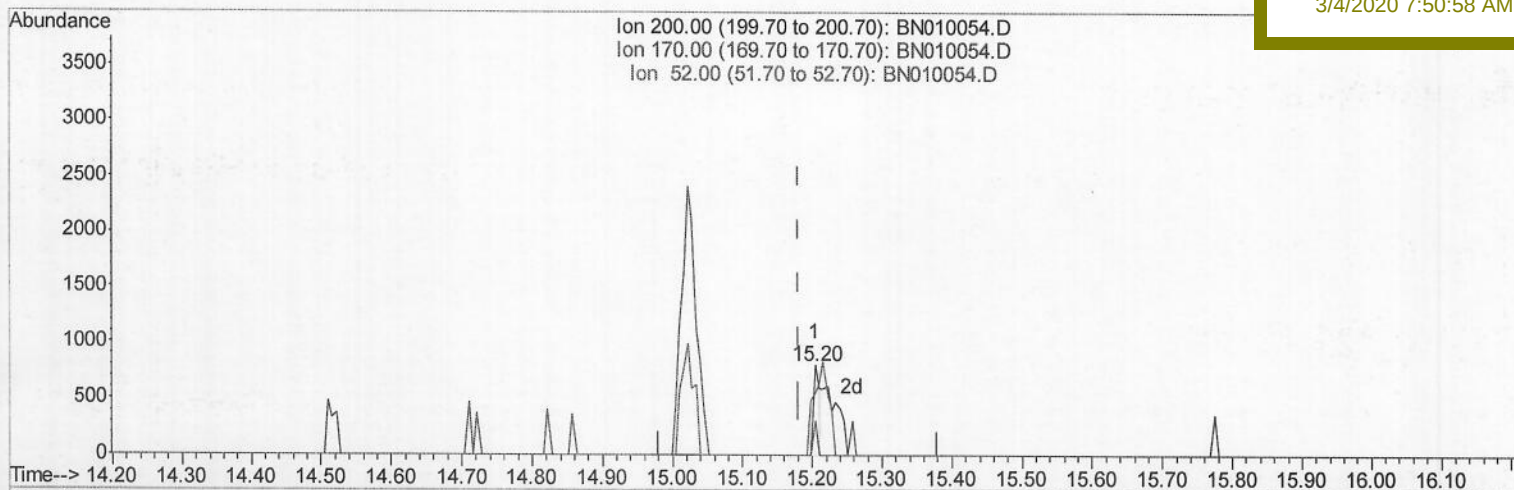

(63) 4,6-Dinitro-2-methylphenol-d2 (S)

15.204min (+0.024) 0.18ng/ul

response 490

Ion	Exp%	Act%
200.00	100	100
170.00	22.10	38.72#
52.00	71.30	70.30
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030320\
Quantitation Report (Qedit)




Data File : BN010054.D
Acq On : 02 Mar 2020 23:38
Operator : CG/JU
Sample : L1615-08DL 5X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Mar 03 01:09:44 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 03 01:05:31 2020
Response via : Initial Calibration

Instrument :
BNA_N
Client Sample Id :
DBDN2DL

Manual Integrations
APPROVED

mohammad
3/4/2020 7:50:58 AM

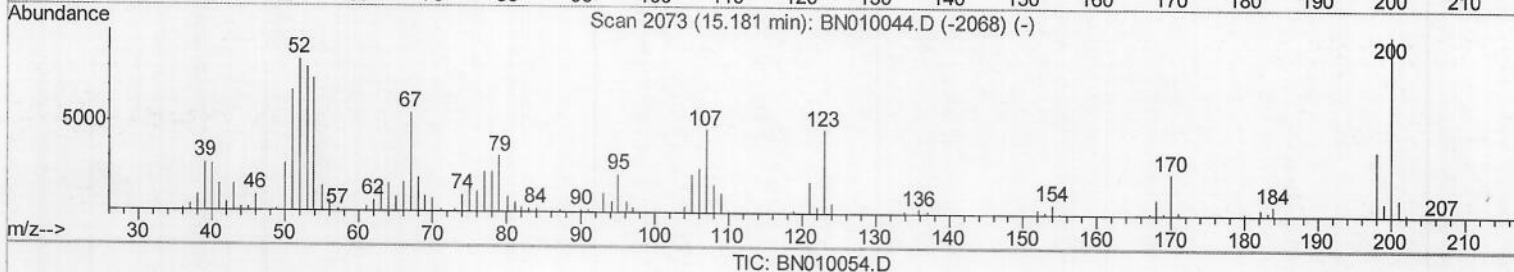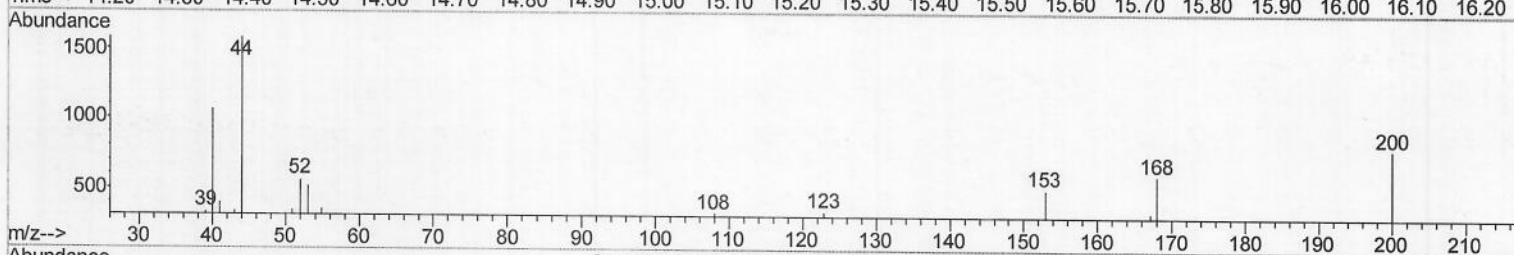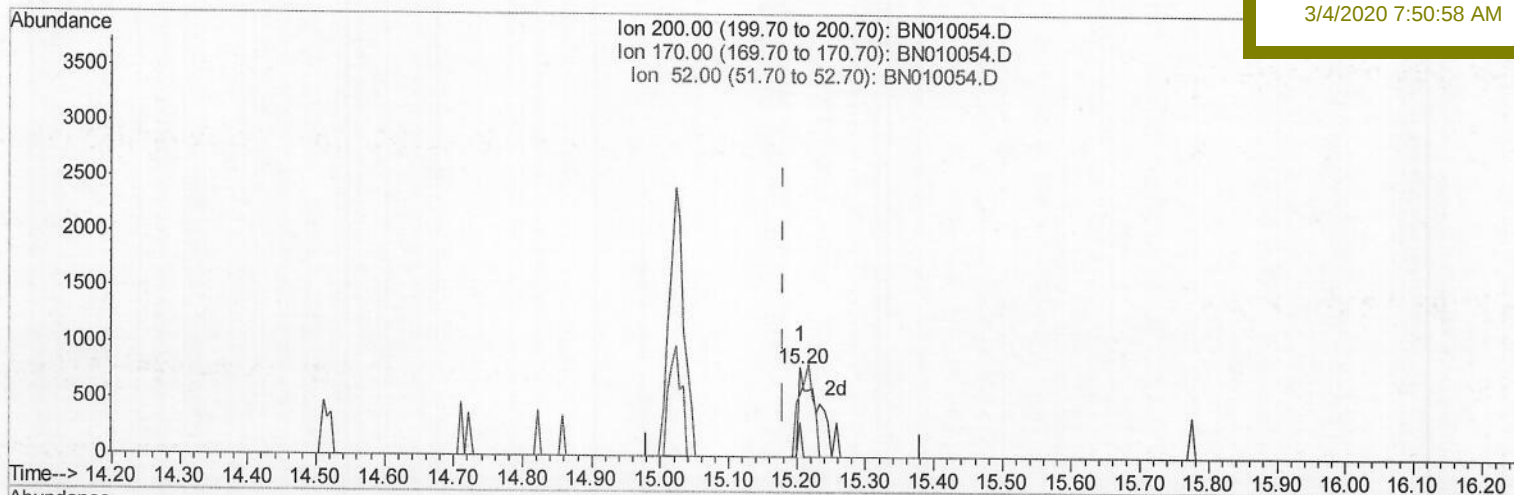

(63) 4,6-Dinitro-2-methylphenol-d2 (S)

15.204min (+0.024) 0.54ng/ul m

response 1477

Ion	Exp%	Act%
200.00	100	100
170.00	22.10	38.72#
52.00	71.30	70.30
0.00	0.00	0.00

250 09/05/20

Data File : BN010054.D
Acq On : 02 Mar 2020 23:38
Operator : CG/JU
Sample : L1615-08DL 5X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBDN2DL

Quant Time: Mar 03 03:04:06 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 03 01:05:31 2020
Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
3/4/2020 7:50:58 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.37	152	71819	20.00	ng/ul	0.00
18) Naphthalene-d8	10.12	136	317887	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.01	164	209188	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.77	188	438872	20.00	ng/ul	0.00
78) Chrysene-d12	20.99	240	414773	20.00	ng/ul	0.00
86) Perylene-d12	23.07	264	437247	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.03	96	416	0.24	ng/uL	0.02
5) Phenol-d5	6.62	99	10502m	1.72	ng/ul	0.04
7) Bis-(2-Chloroethyl) ether-d	6.75	67	8281m	1.96	ng/ul	0.02
9) 2-Chlorophenol-d4	6.93	132	8123	1.77	ng/ul	0.02
13) 4-Methylphenol-d8	8.12	113	8492m	1.75	ng/ul	0.04
19) Nitrobenzene-d5	8.54	128	3448m	1.48	ng/ul	0.03
22) 2-Nitrophenol-d4	9.25	143	2974m	1.17	ng/ul	0.02
26) 2,4-Dichlorophenol-d3	9.83	165	8504m	1.74	ng/ul	0.08
29) 4-Chloroaniline-d4	10.35	131	3410m	0.62	ng/ul	0.08
44) Dimethylphthalate-d6	13.45	166	33361	2.14	ng/ul	0.02
47) Acenaphthylene-d8	13.70	160	34512	1.88	ng/ul	0.00
52) 4-Nitrophenol-d4	14.36	143	1821m	0.64	ng/ul	0.09
58) Fluorene-d10	15.02	176	28789	2.13	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.20	200	1477m	0.54	ng/ul	0.02
71) Anthracene-d10	16.87	188	46398	2.31	ng/ul	0.00
79) Pyrene-d10	19.17	212	50662	2.34	ng/ul	0.00
90) Benzo(a)pyrene-d12	22.94	264	52015	2.38	ng/ul	0.00

3/03/05/20

Target Compounds

					Qvalue	
48) Acenaphthylene	13.73	152	21330	1.071	ng/ul	97
70) Phenanthrene	16.81	178	147548	5.891	ng/ul	98
72) Anthracene	16.90	178	184794	7.217	ng/ul	99
77) Fluoranthene	18.84	202	834186	28.433	ng/ul	98
80) Pyrene	19.20	202	1164377	38.938	ng/ul	98
83) Benzo(a)anthracene	20.97	228	370878	13.012	ng/ul	95
85) Chrysene	21.02	228	501640	17.877	ng/ul	99
88) Benzo(b)fluoranthene	22.47	252	550564	19.421	ng/ul	97
89) Benzo(k)fluoranthene	22.50	252	190895	7.111	ng/ul	98
91) Benzo(a)pyrene	22.99	252	264218	10.362	ng/ul	98
92) Indeno(1,2,3-cd)pyrene	25.12	276	115081	3.802	ng/ul	99
93) Dibenzo(a,h)anthracene	25.10	278	30993	1.197	ng/ul#	89
94) Benzo(g,h,i)perylene	25.73	276	66159	2.606	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed