

Quantitation Report (Qedit)


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN030320\
Data File : BN010068.D
Acq On : 03 Mar 2020 19:05
Operator : CG/JU
Sample : SSTDCCC020
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_N
LabSampleId :
SSTD02077

Manual Integrations
APPROVED

mohammad
3/4/2020 7:51:54 AM

Quant Time: Mar 03 19:39:47 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 03 12:28:17 2020
Response via : Initial Calibration

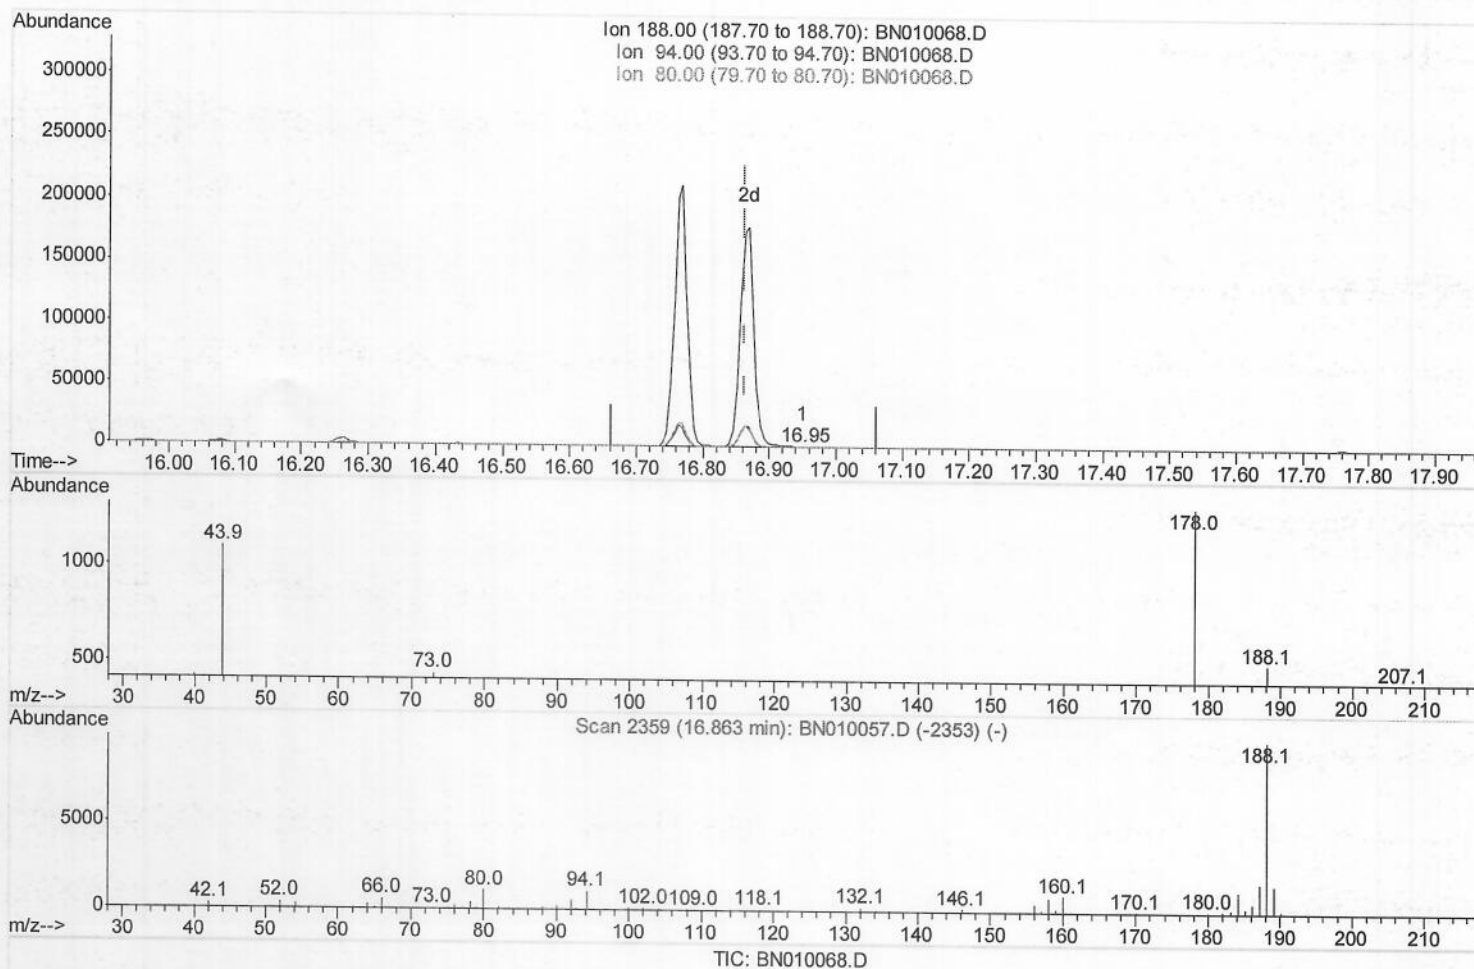

(71) Anthracene-d10 (S)

16.951min (+0.088) 0.02ng/ul

response 303

Ion	Exp%	Act%
188.00	100	100
94.00	11.80	0.00#
80.00	11.10	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030320\
 Data File : BN010068.D
 Acq On : 03 Mar 2020 19:05
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 LabSampleId :
 SSTD02077

Manual Integrations
 APPROVED

mohammad
 3/4/2020 7:51:54 AM

Quant Time: Mar 03 19:39:47 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 03 12:28:17 2020
 Response via : Initial Calibration

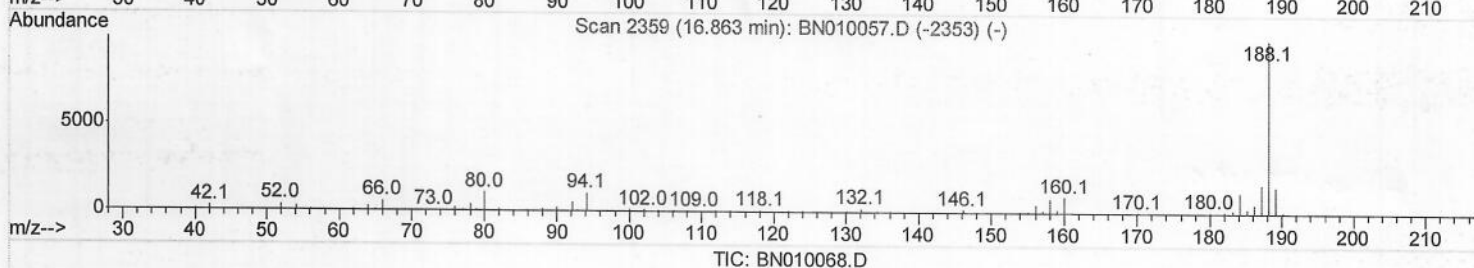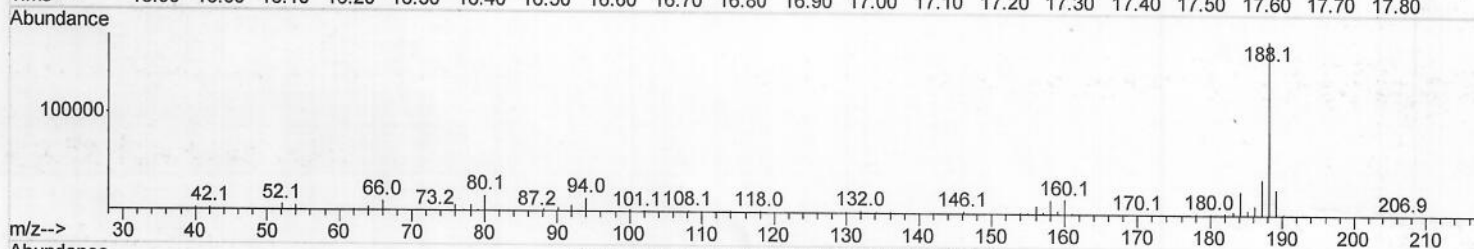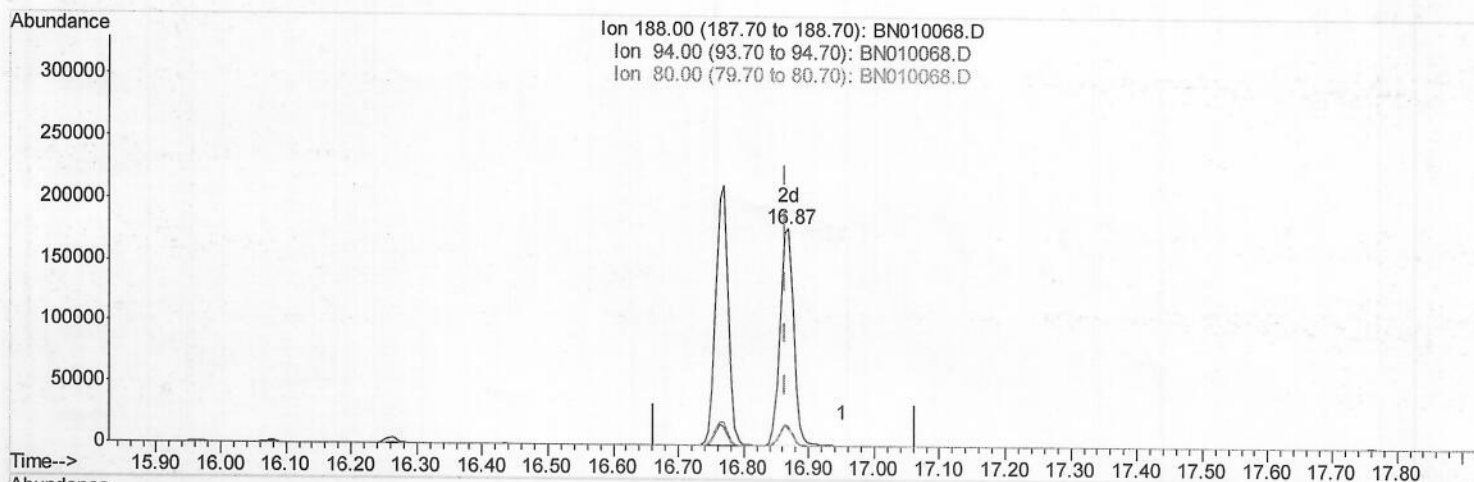

(71) Anthracene-d10 (S)

16.869min (+0.006) 19.90ng/ul m>JU 03/04/20

response 258583

Ion	Exp%	Act%
188.00	100	100
94.00	11.80	7.88#
80.00	11.10	9.10
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN030320\
Data File : BN010068.D
Acq On : 03 Mar 2020 19:05
Operator : CG/JU
Sample : SSTDCCC020
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_N
LabSampleId :
SSTD02077

Manual Integrations
APPROVED

mohammad
3/4/2020 7:51:54 AM

Quant Time: Mar 03 19:39:47 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 03 12:28:17 2020
Response via : Initial Calibration

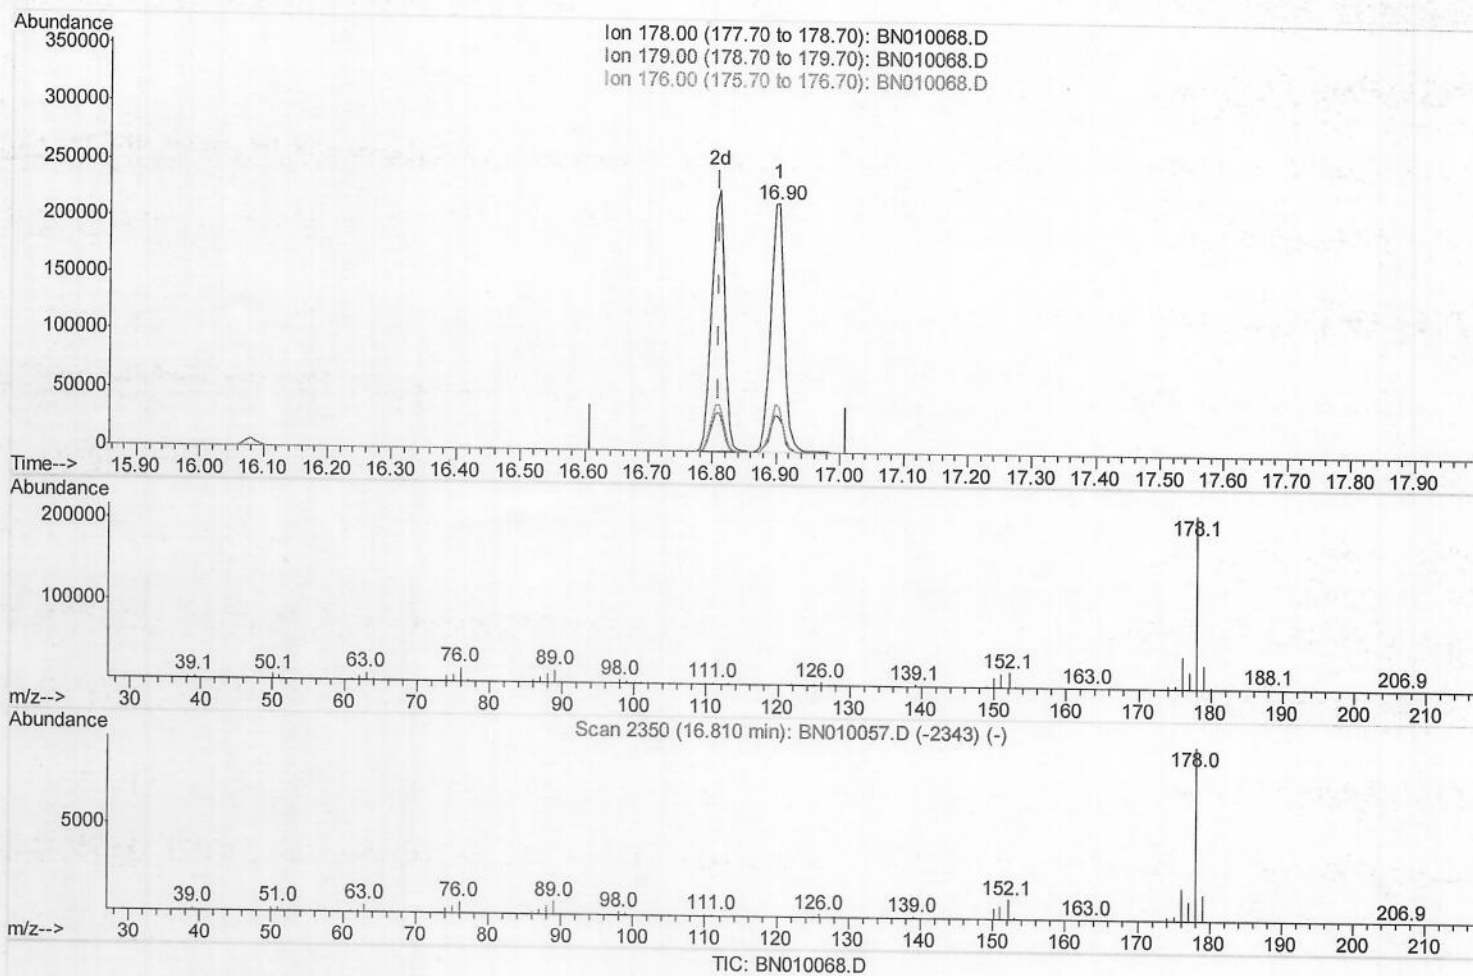

(70) Phenanthrene

16.904min (+0.094) 20.17ng/ul

response 326371

Ion	Exp%	Act%
178.00	100	100
179.00	15.60	14.14
176.00	18.30	18.39
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN030320\
Data File : BN010068.D
Acq On : 03 Mar 2020 19:05
Operator : CG/JU
Sample : SSTDCCC020
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_N
LabSampleId :
SSTD02077

Manual Integrations
APPROVED

mohammad
3/4/2020 7:51:54 AM

Quant Time: Mar 03 19:39:47 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 03 12:28:17 2020
Response via : Initial Calibration

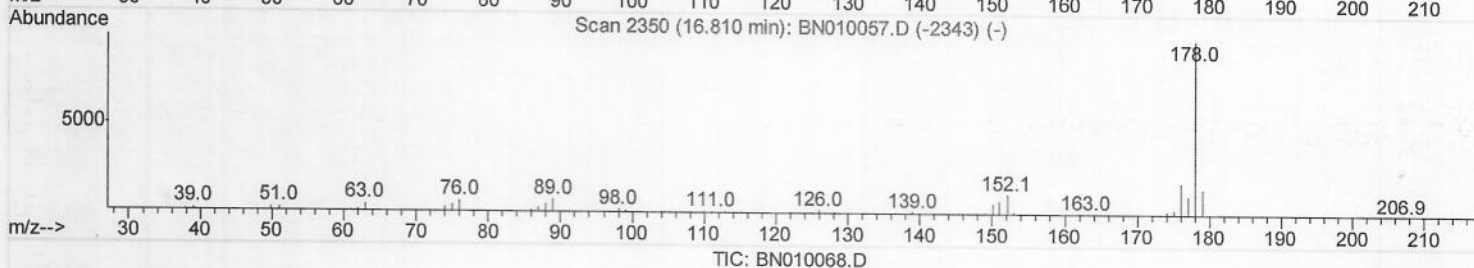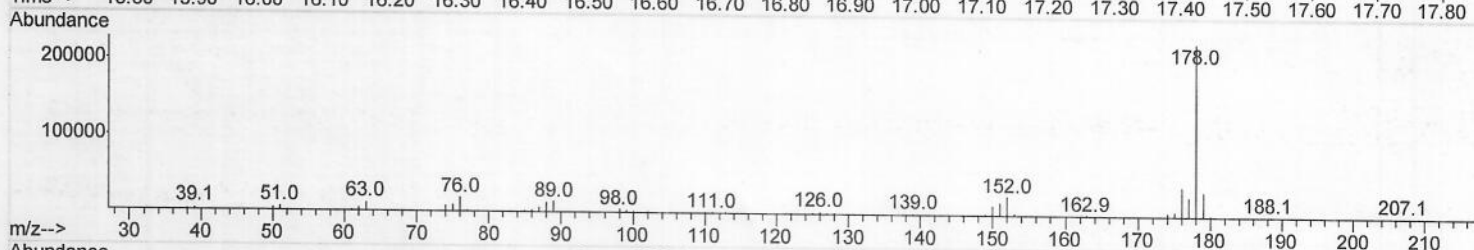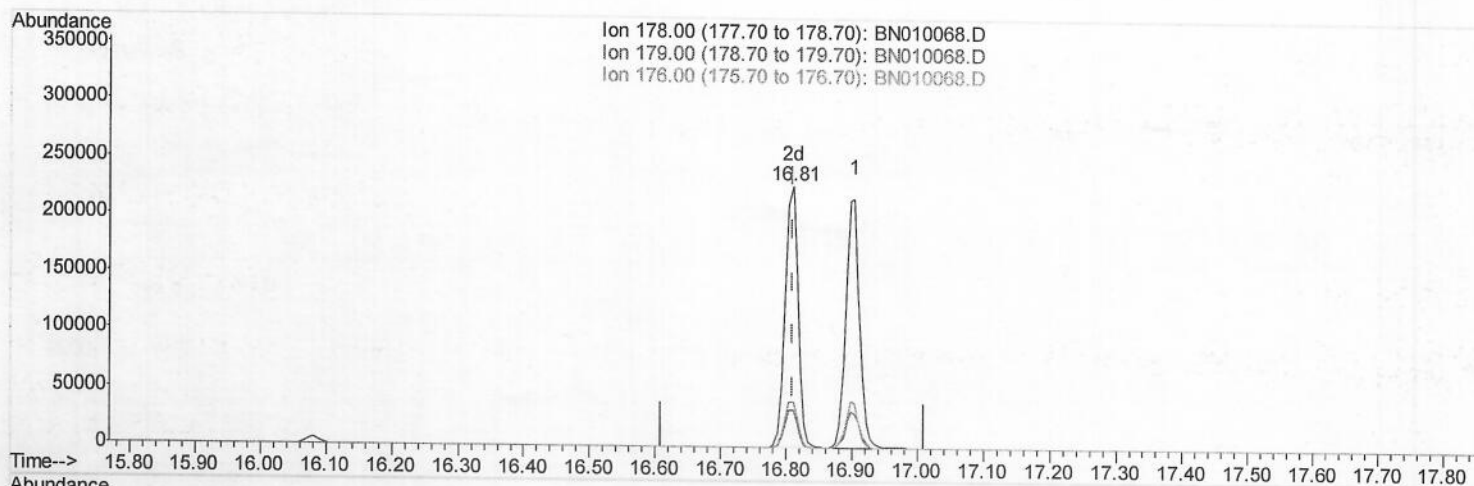

(70) Phenanthrene

16.810min (+0.000) 19.49ng/ul mssju 03/04/20

response 315321

Ion	Exp%	Act%
178.00	100	100
179.00	15.60	14.69
176.00	18.30	17.55
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN030320\
 Data File : BN010068.D
 Acq On : 03 Mar 2020 19:05
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 LabSampleId :
 SSTD02077

Manual Integrations
 APPROVED

mohammad
 3/4/2020 7:51:54 AM

Quant Time: Mar 03 19:39:47 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 03 12:28:17 2020
 Response via : Initial Calibration

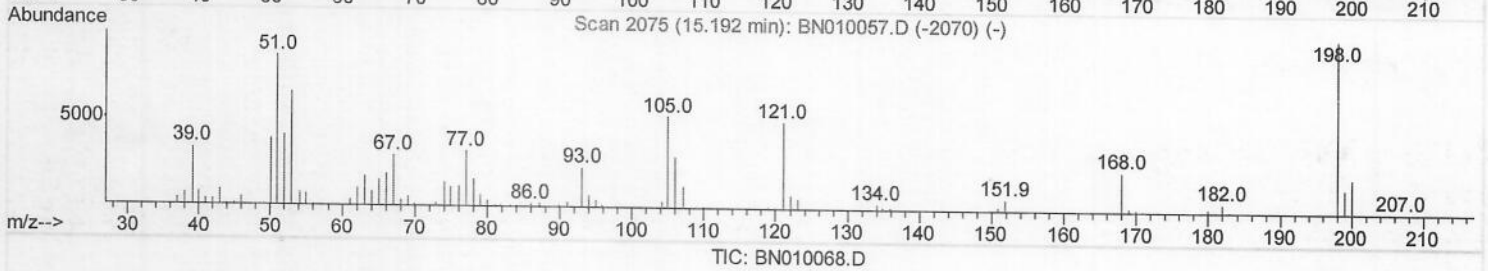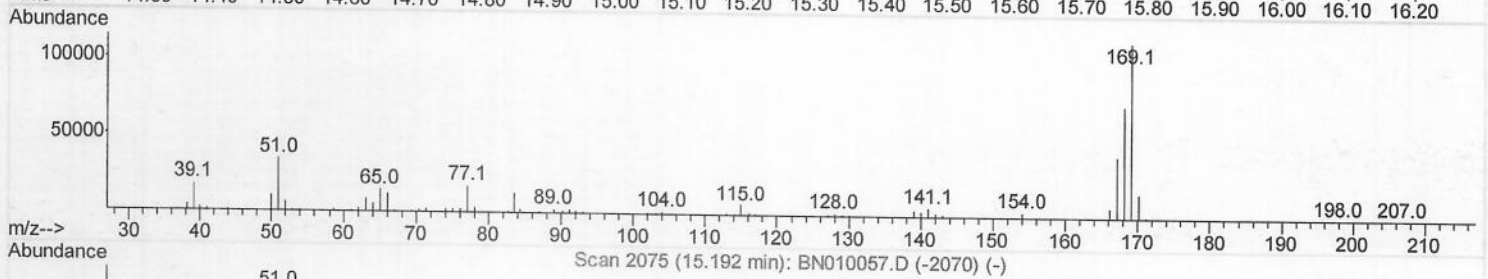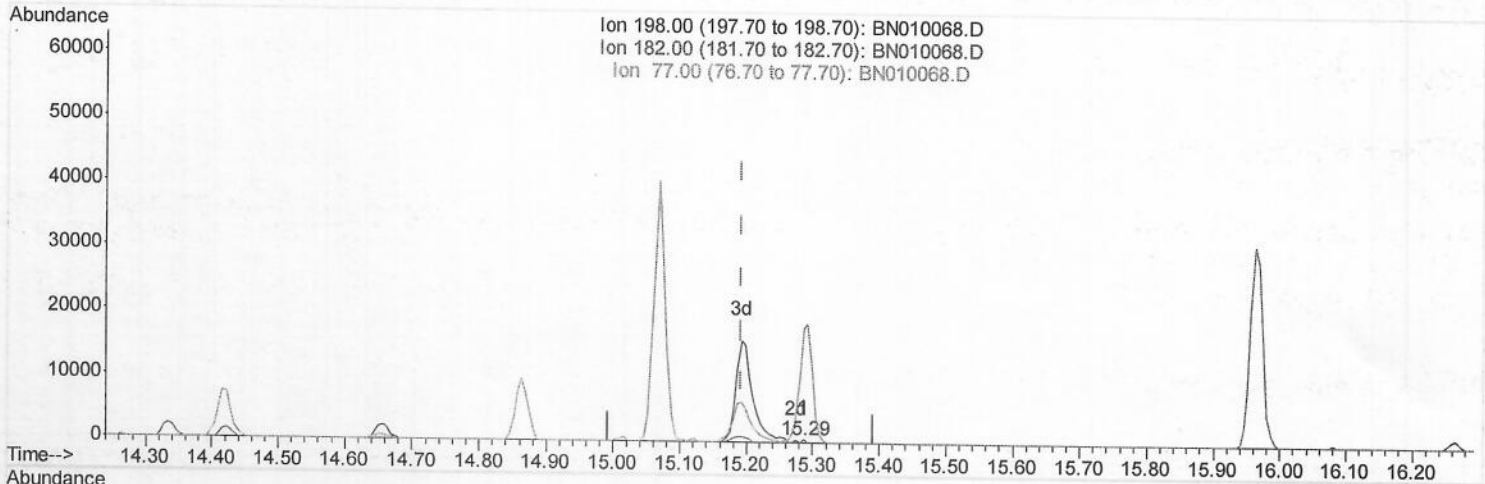

(64) 4,6-Dinitro-2-methylphenol

15.287min (+0.094) 0.09ng/ul

response 179

Ion	Exp%	Act%
198.00	100	100
182.00	4.60	0.00#
77.00	31.40	3483.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN030320\
 Data File : BN010068.D
 Acq On : 03 Mar 2020 19:05
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 LabSampleId :
 SSTD02077

Manual Integrations
 APPROVED

mohammad
 3/4/2020 7:51:54 AM

Quant Time: Mar 03 19:39:47 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 03 12:28:17 2020
 Response via : Initial Calibration

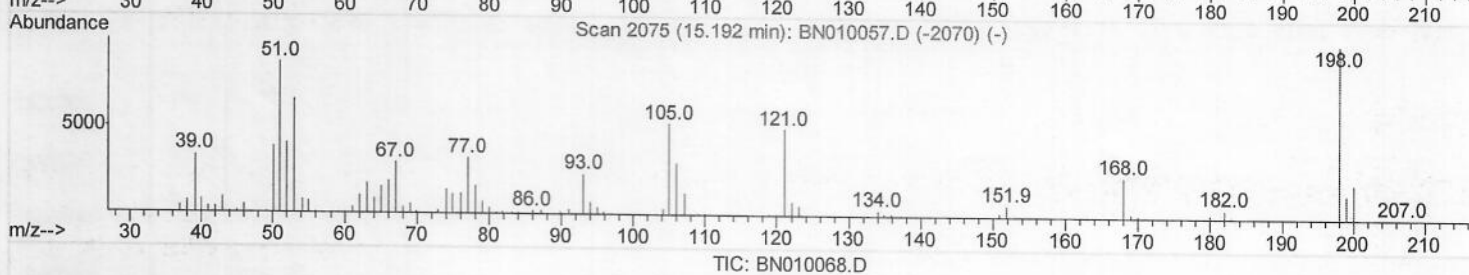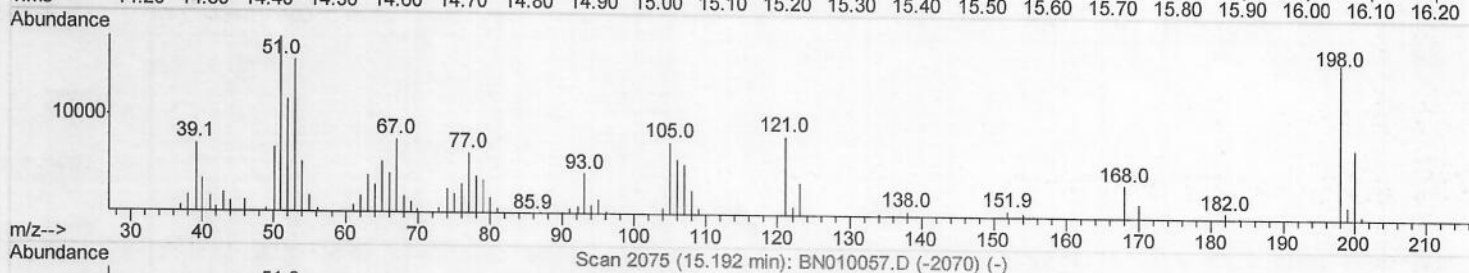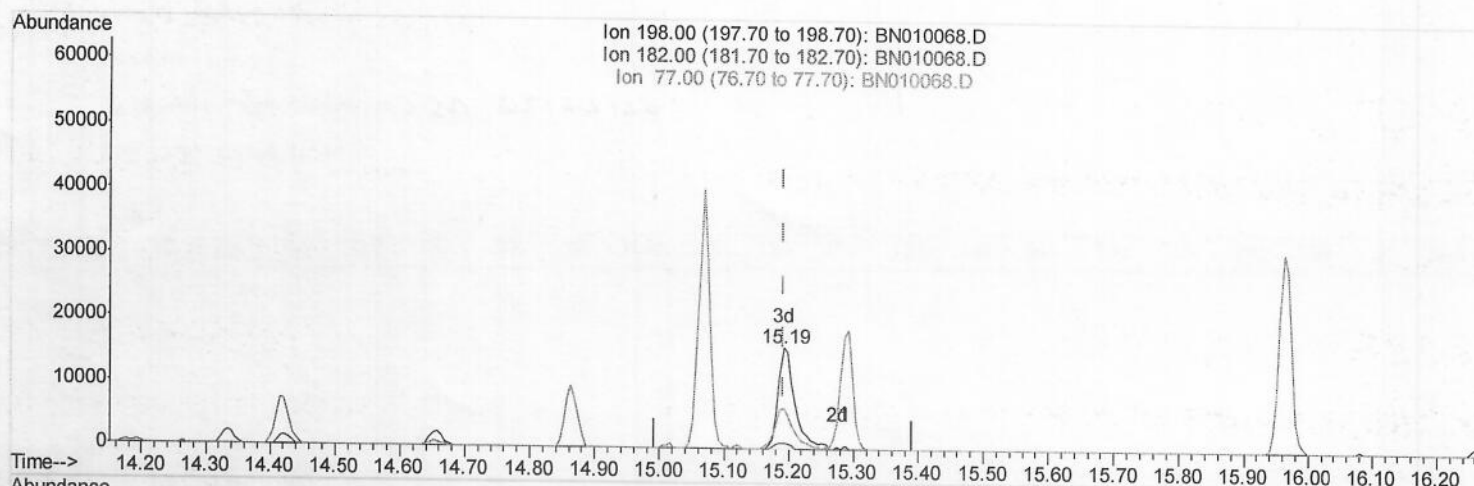

(64) 4,6-Dinitro-2-methylphenol

15.192min (0.000) 15.05ng/ul m *50 03/04/20*

response 28549

Ion	Exp%	Act%
198.00	100	100
182.00	4.60	5.47
77.00	31.40	39.82#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN030320\
 Data File : BN010068.D
 Acq On : 03 Mar 2020 19:05
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 LabSampleId :
 SSTD02077

Manual Integrations
 APPROVED

mohammad
 3/4/2020 7:51:54 AM

Quant Time: Mar 03 19:36:57 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 03 12:28:17 2020
 Response via : Initial Calibration

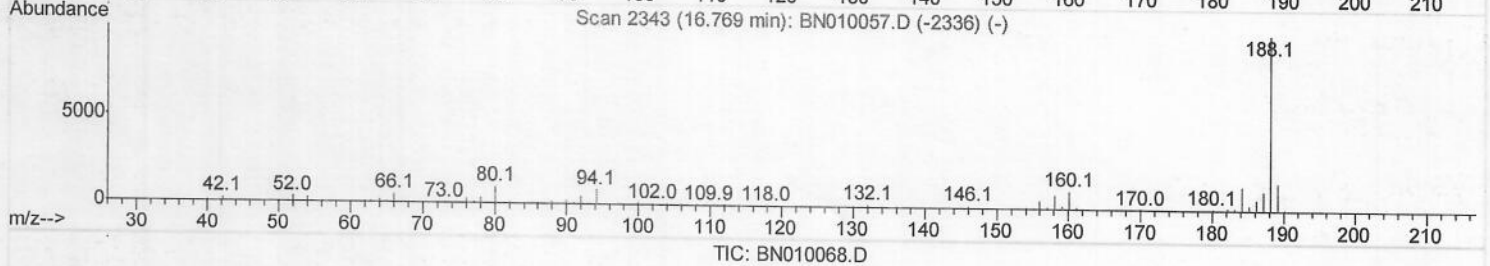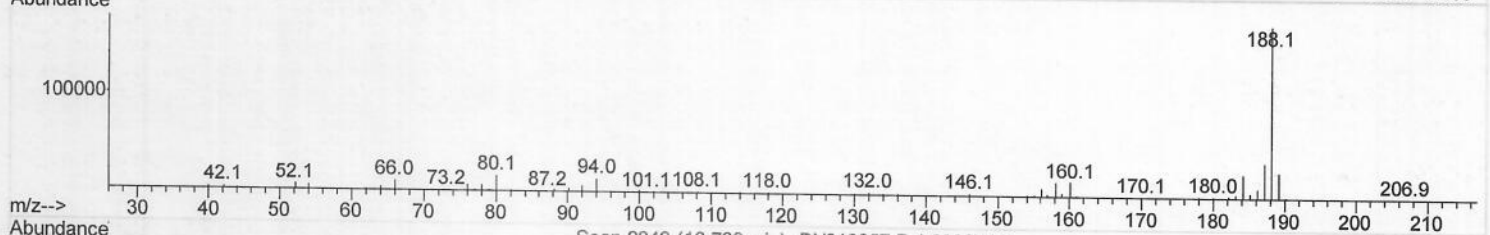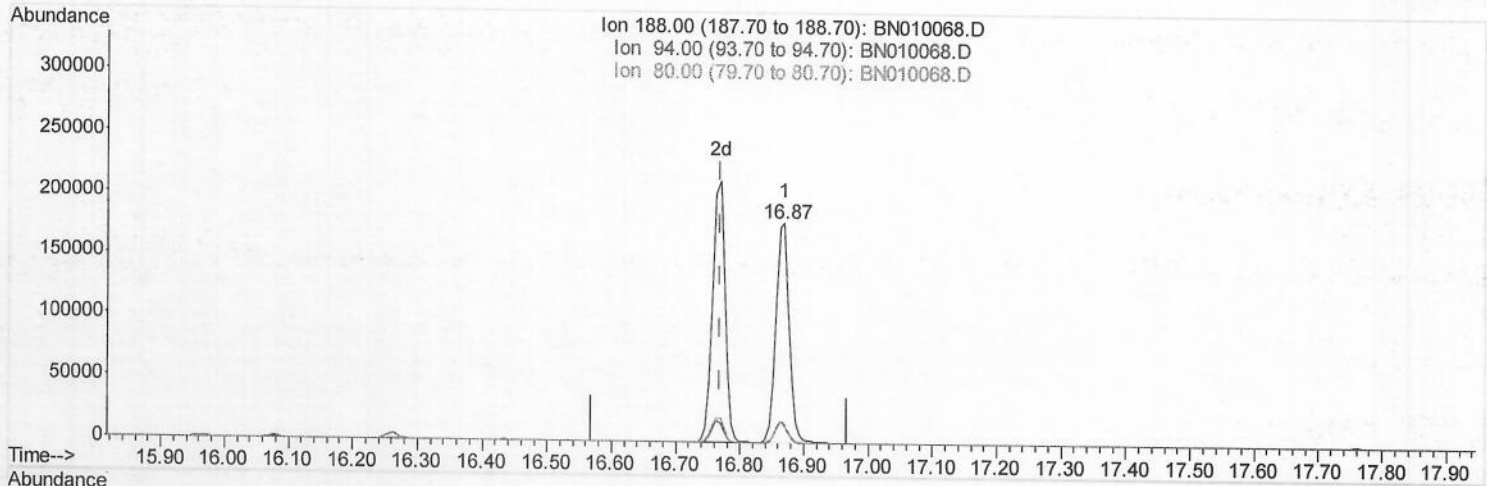

(62) Phenanthrene-d10 (I)
 16.869min (+0.100) 20.00ng/ul
 response 257560

Ion	Exp%	Act%
188.00	100	100
94.00	9.40	7.88
80.00	10.90	9.10
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN030320\
 Data File : BN010068.D
 Acq On : 03 Mar 2020 19:05
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 LabSampleId :
 SSTD02077

Manual Integrations
 APPROVED

mohammad
 3/4/2020 7:51:54 AM

Quant Time: Mar 03 19:36:57 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 03 12:28:17 2020
 Response via : Initial Calibration

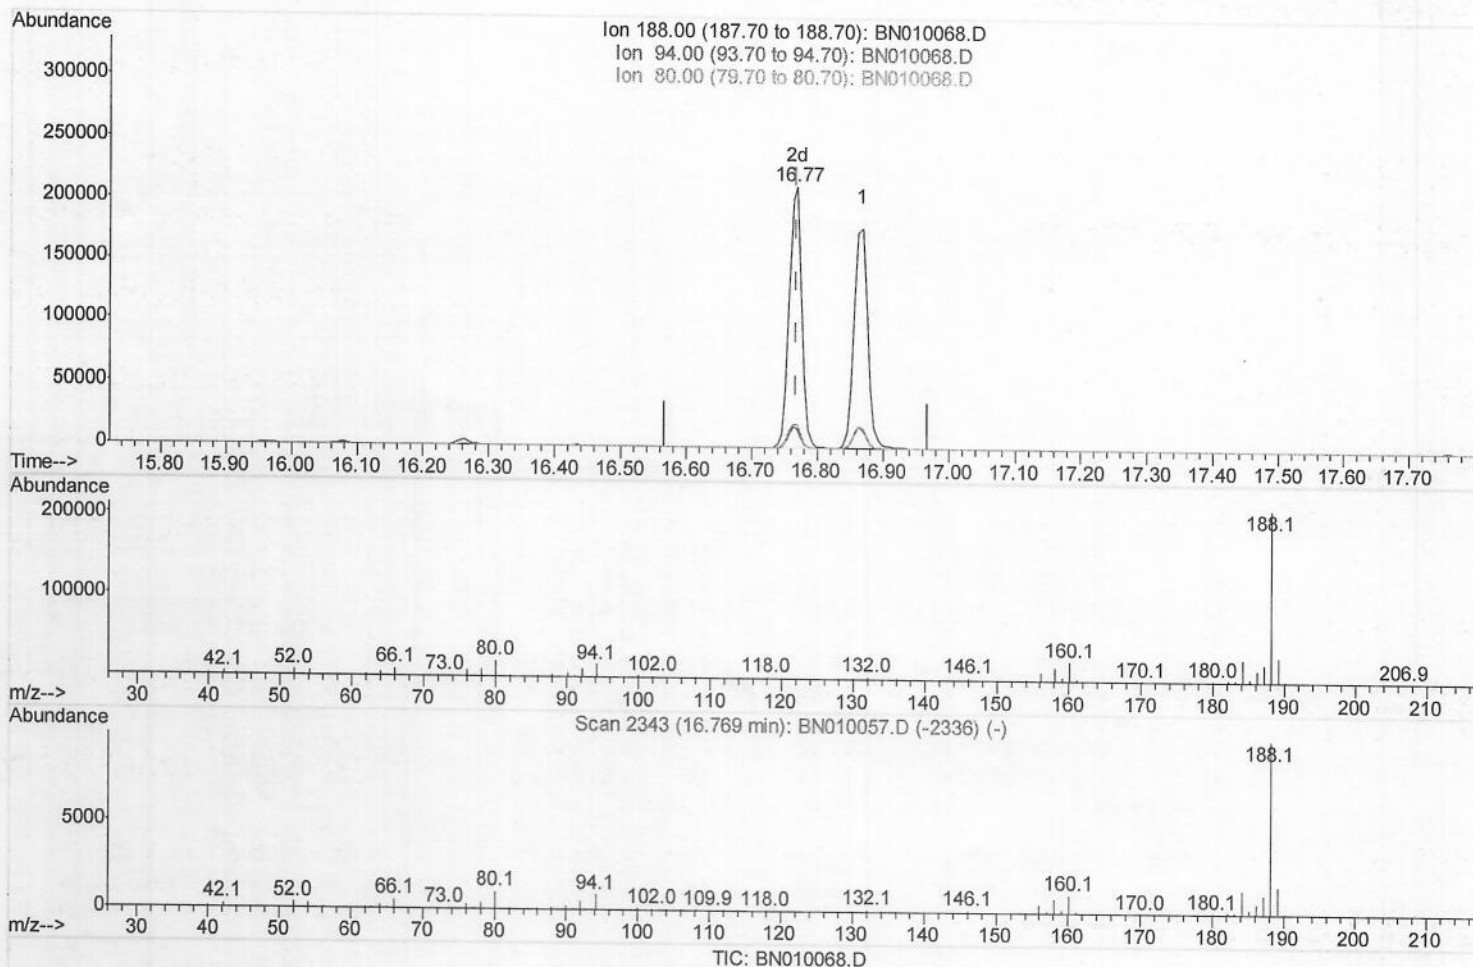

(62) Phenanthrene-d10 (I)

16.769min (0.000) 20.00ng/ul m 350 03/04/20

response 283514

Ion	Exp%	Act%
188.00	100	100
94.00	9.40	7.51#
80.00	10.90	9.12
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN030320\
 Data File : BN010068.D
 Acq On : 03 Mar 2020 19:05
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 LabSampleId :
 SSTD02077

Manual Integrations
 APPROVED

mohammad
 3/4/2020 7:51:54 AM

Quant Time: Mar 03 19:36:57 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 03 12:28:17 2020
 Response via : Initial Calibration

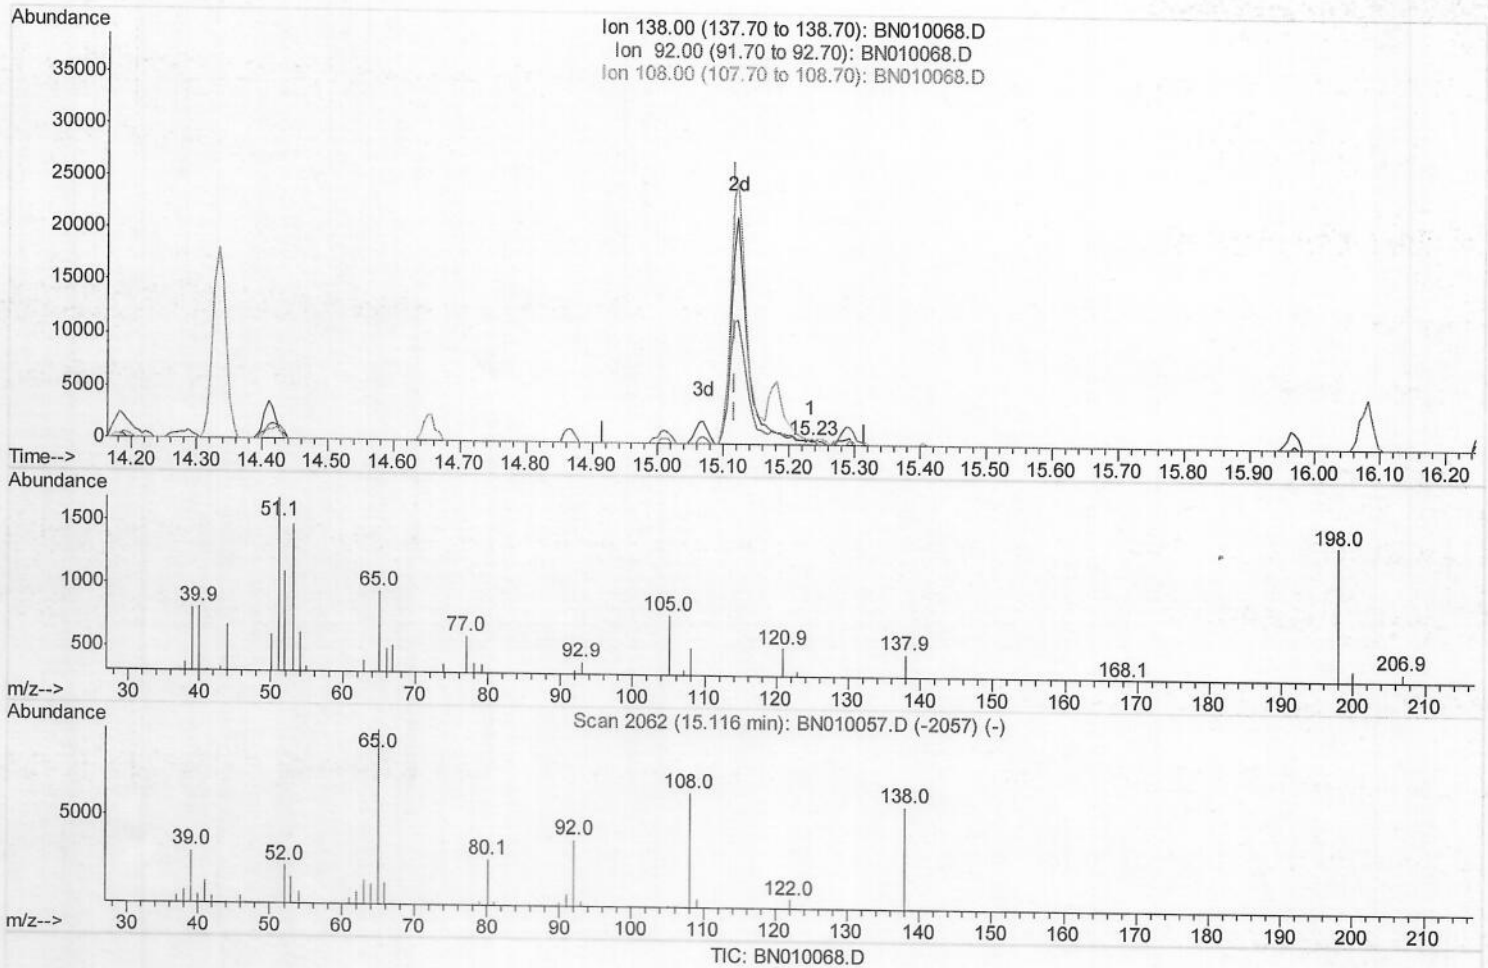

(61) 4-Nitroaniline

15.234min (+0.118) 0.05ng/ul

response 105

Ion	Exp%	Act%
138.00	100	100
92.00	59.70	68.17
108.00	90.40	107.19
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN030320\
 Data File : BN010068.D
 Acq On : 03 Mar 2020 19:05
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 LabSampleId :
 SSTD02077

Manual Integrations
 APPROVED

mohammad
 3/4/2020 7:51:54 AM

Quant Time: Mar 03 19:36:57 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 03 12:28:17 2020
 Response via : Initial Calibration

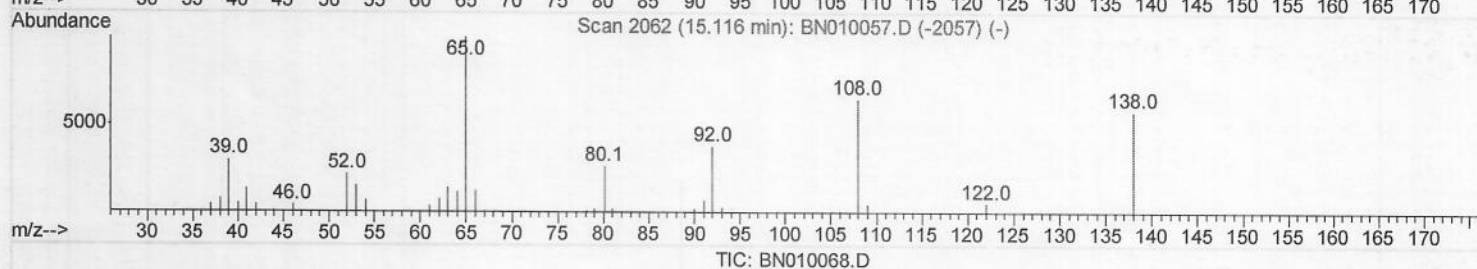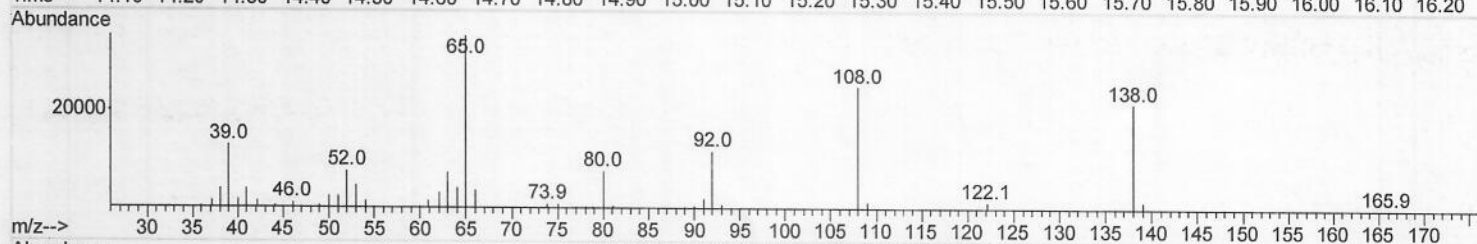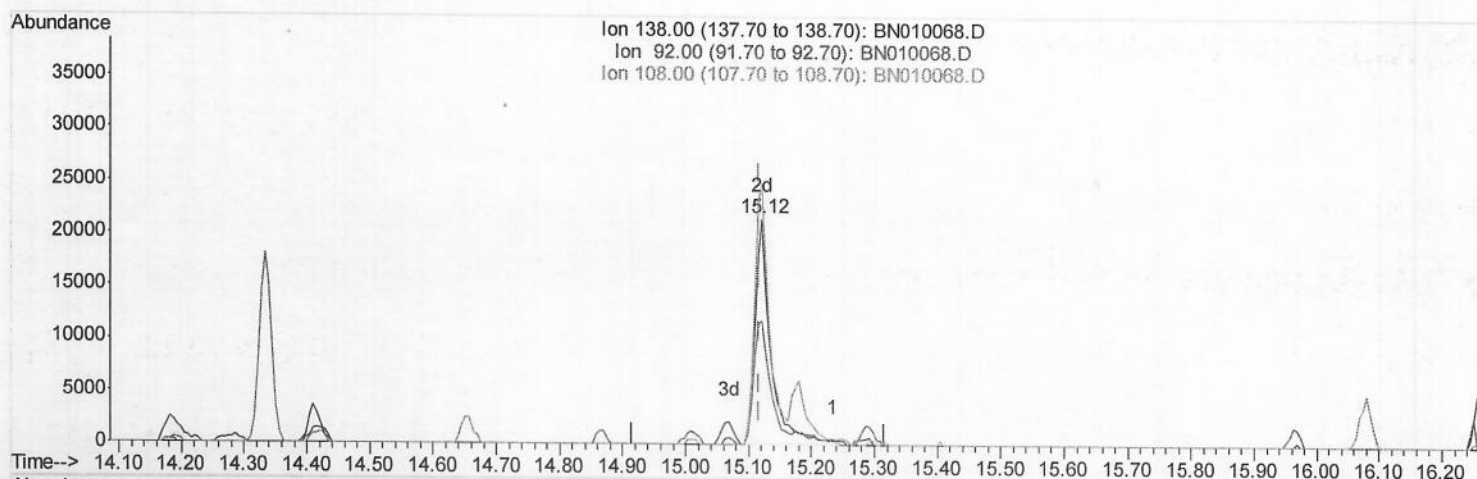

(61) 4-Nitroaniline

15.122min (+0.006) 17.44ng/ul m>JU 03104126

response 39481

Ion	Exp%	Act%
138.00	100	100
92.00	59.70	54.78
108.00	90.40	115.54#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN030320\
 Data File : BN010068.D
 Acq On : 03 Mar 2020 19:05
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 LabSampleId :
 SSTD02077

Manual Integrations
 APPROVED

mohammad
 3/4/2020 7:51:54 AM

Quant Time: Mar 03 19:36:57 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 03 12:28:17 2020
 Response via : Initial Calibration

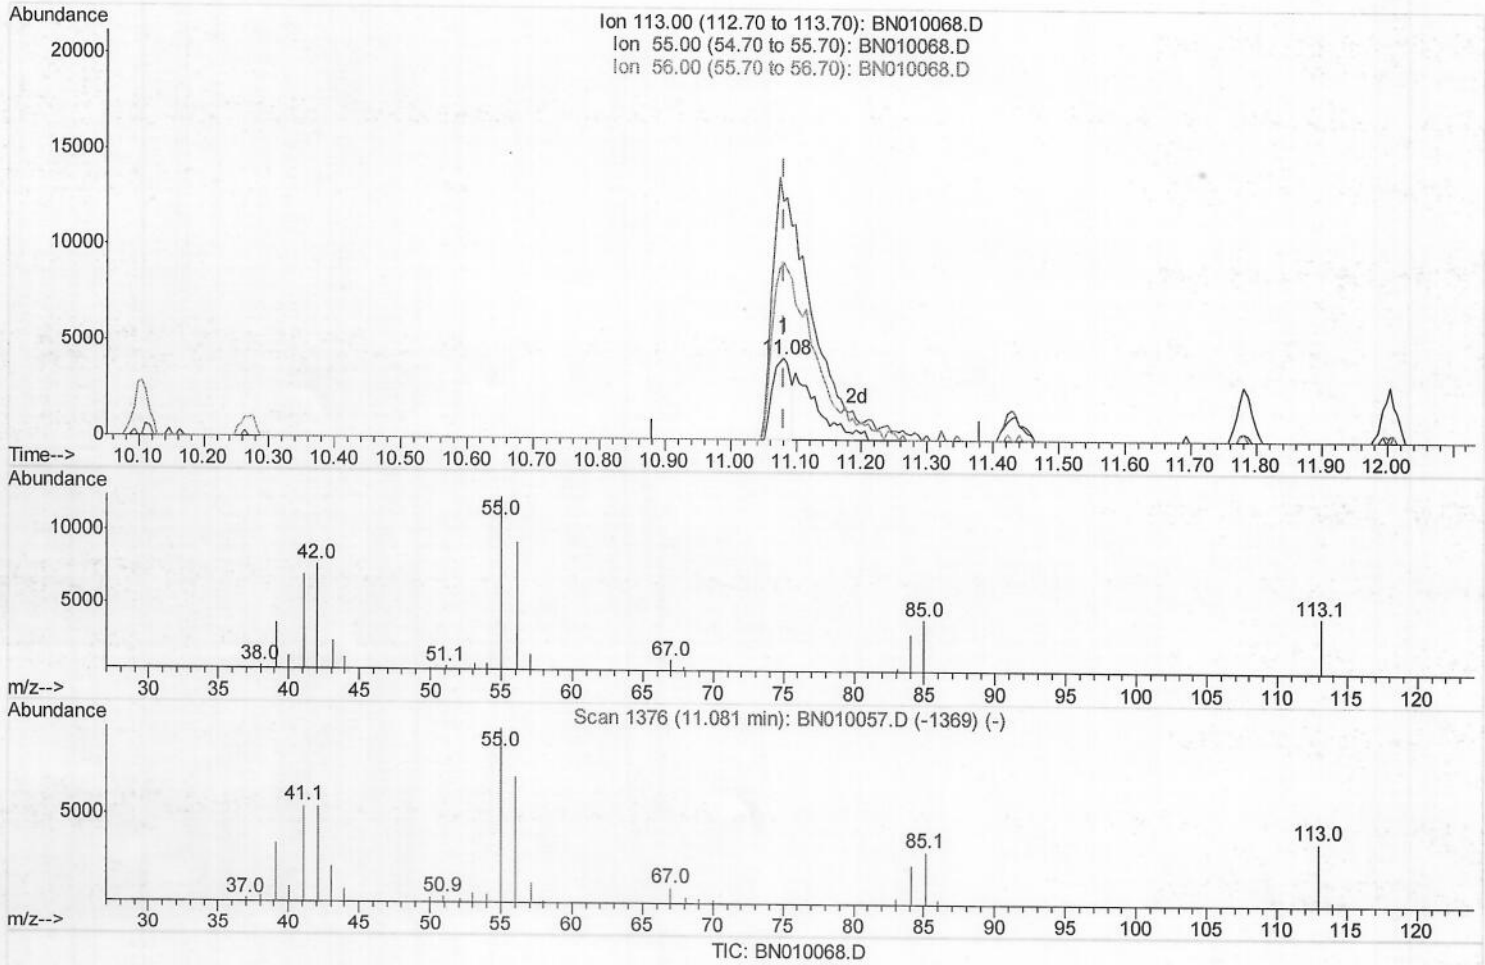

(32) Caprolactam

11.081min (0.000) 8.20ng/ul

response 7943

Ion	Exp%	Act%
113.00	100	100
55.00	261.40	295.63
56.00	202.00	220.40
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN030320\
 Data File : BN010068.D
 Acq On : 03 Mar 2020 19:05
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 LabSampleId :
 SSTD02077

Manual Integrations
 APPROVED

mohammad
 3/4/2020 7:51:54 AM

Quant Time: Mar 03 19:36:57 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 03 12:28:17 2020
 Response via : Initial Calibration

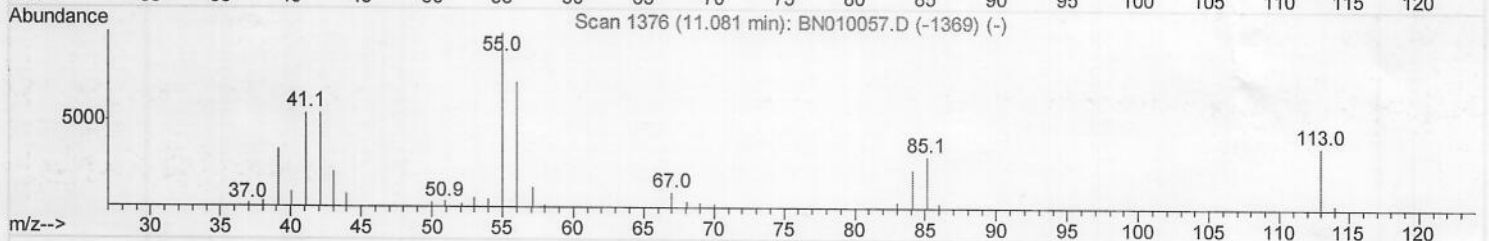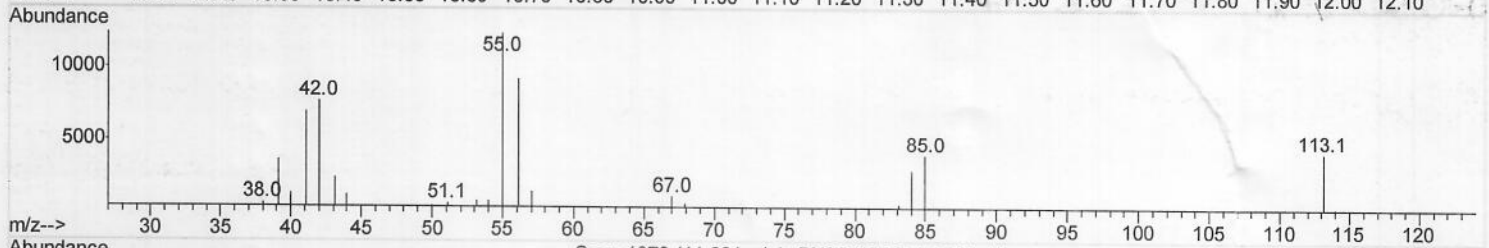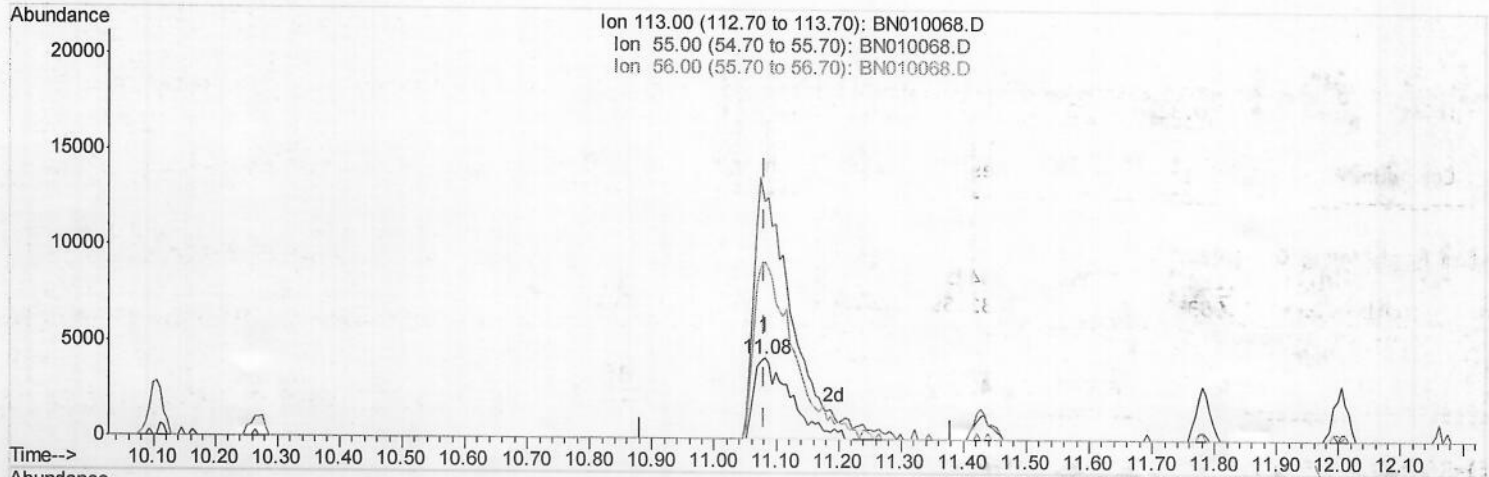

(32) Caprolactam

11.081min (0.000) 17.93ng/ul m>JU 03/04/20

response 17373

Ion	Exp%	Act%
113.00	100	100
55.00	261.40	295.63
56.00	202.00	220.40
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN030320\
 Data File : BN010068.D
 Acq On : 03 Mar 2020 19:05
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 LabSampleId :
 SSTD02077

Manual Integrations
 APPROVED

mohammad
 3/4/2020 7:51:54 AM

Quant Time: Mar 03 19:36:57 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 03 12:28:17 2020
 Response via : Initial Calibration

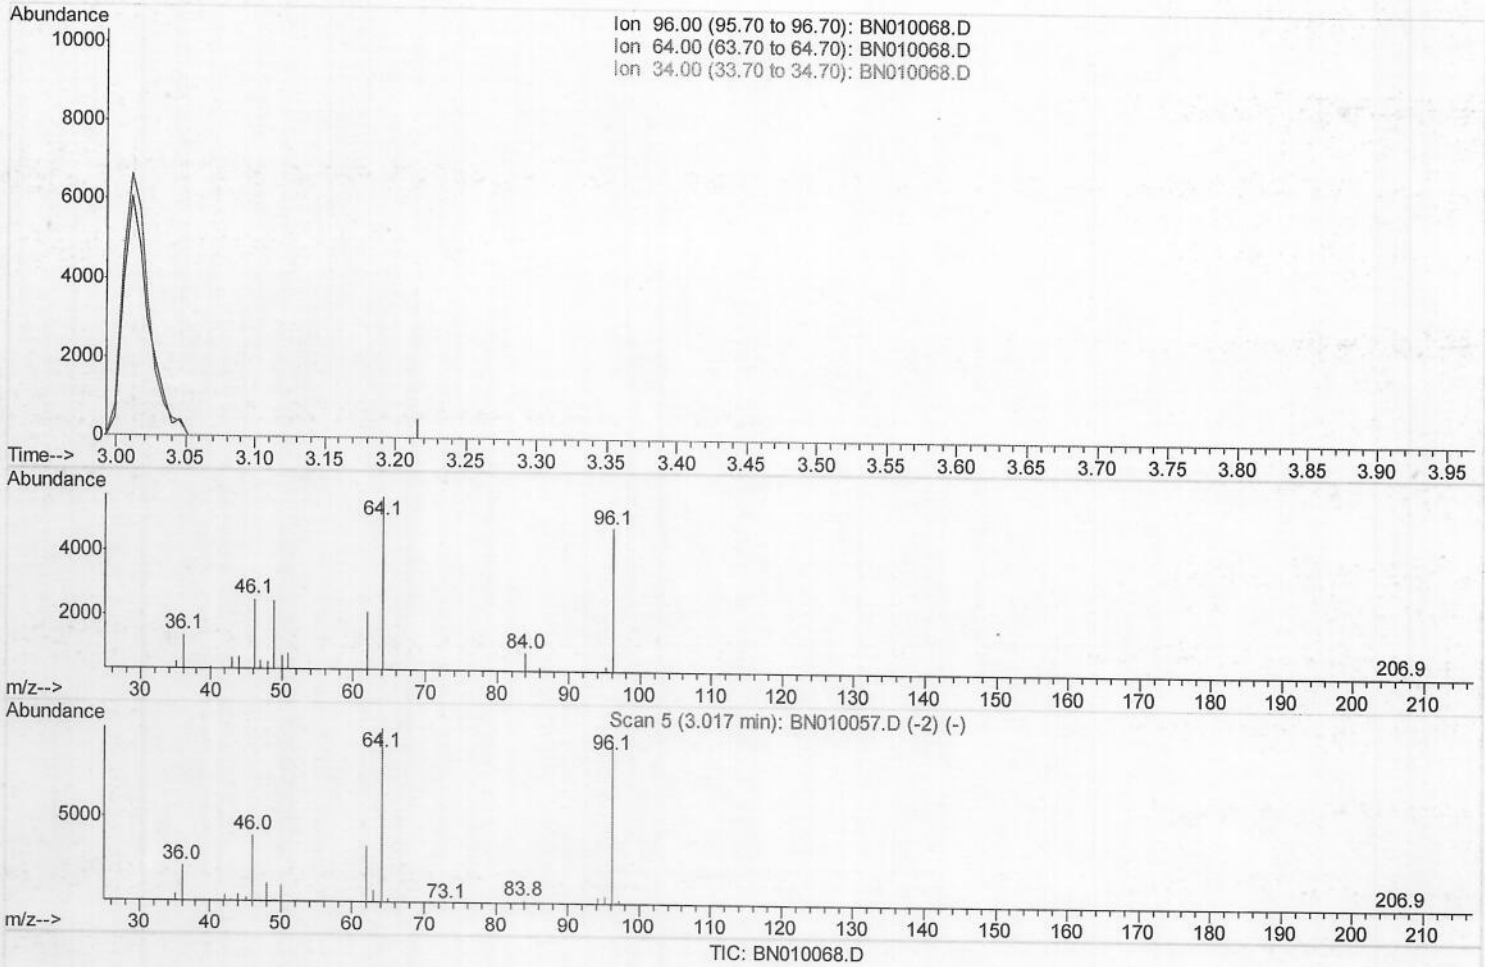

(3) 1,4-Dioxane-d8 (S)

3.017min (-3.017) 0.00ng/uL

response 0

Ion	Exp%	Act%
96.00	100	0.00
64.00	93.60	0.00#
34.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN030320\
 Data File : BN010068.D
 Acq On : 03 Mar 2020 19:05
 Operator : CG/JU
 Sample : SSTDC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 LabSampleId :
 SSTD02077

Manual Integrations
 APPROVED

mohammad
 3/4/2020 7:51:54 AM

Quant Time: Mar 03 19:36:57 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 03 12:28:17 2020
 Response via : Initial Calibration

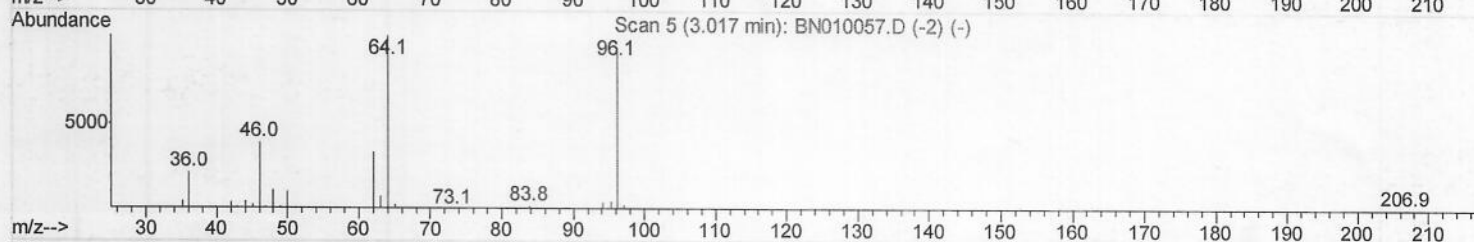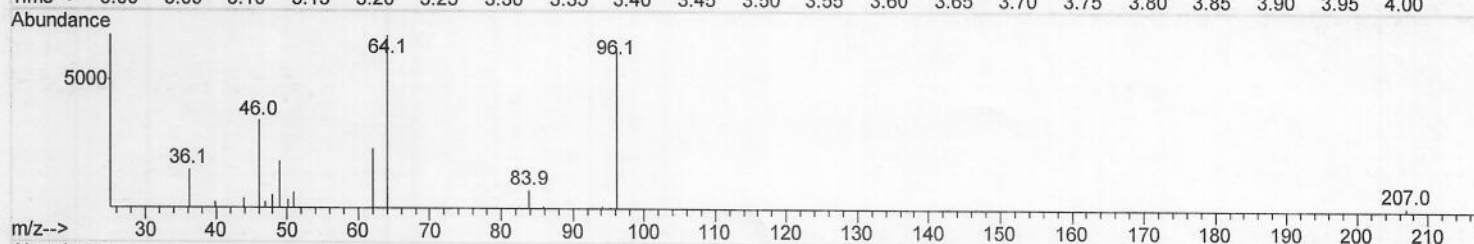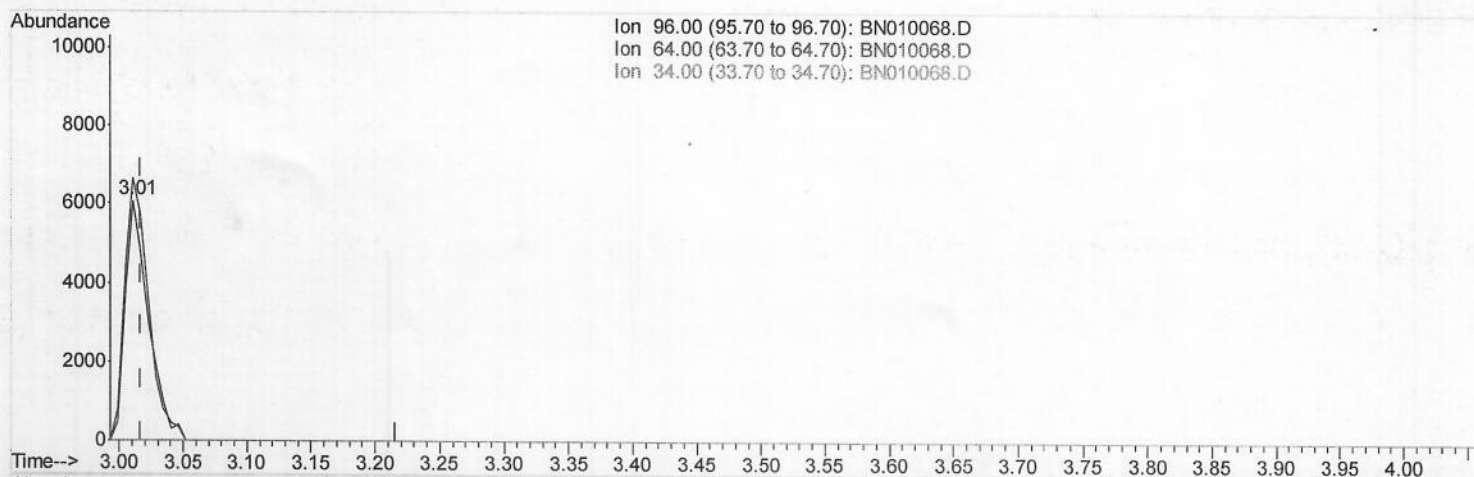

(3) 1,4-Dioxane-d8 (S)

3.011min (-0.006) 7.15ng/uL m>SV 03/04/20

response 7743

Ion	Exp%	Act%
96.00	100	100
64.00	93.60	109.24
34.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN030320\
 Data File : BN010068.D
 Acq On : 03 Mar 2020 19:05
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 LabSampleId :
 SSTD02077

Manual Integrations
 APPROVED

mohammad
 3/4/2020 7:51:54 AM

Quant Time: Mar 03 19:40:40 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 03 12:28:17 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.36	152	44538	20.00	ng/ul	0.00
18) Naphthalene-d8	10.10	136	186121	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.00	164	131749	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.77	188	283514m)	20.00	ng/ul	0.00
78) Chrysene-d12	20.99	240	269803	20.00	ng/ul	0.00
86) Perylene-d12	23.09	264	286700	20.00	ng/ul	0.00

>JU 03104120

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.01	96	7743m)	7.15	ng/uL	0.00
5) Phenol-d5	6.57	99	69778	18.42	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.72	67	46207	17.67	ng/ul	0.00
9) 2-Chlorophenol-d4	6.90	132	55739	19.54	ng/ul	0.00
13) 4-Methylphenol-d8	8.08	113	57711	19.15	ng/ul	0.00
19) Nitrobenzene-d5	8.51	128	26184	19.23	ng/ul	0.00
22) 2-Nitrophenol-d4	9.22	143	29935	20.09	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.75	165	59830	20.89	ng/ul	0.00
29) 4-Chloroaniline-d4	10.27	131	70901	22.04	ng/ul	0.00
44) Dimethylphthalate-d6	13.43	166	189699	19.28	ng/ul	0.00
47) Acenaphthylene-d8	13.69	160	215900	18.63	ng/ul	0.00
52) 4-Nitrophenol-d4	14.26	143	28473	15.84	ng/ul	0.00
58) Fluorene-d10	15.01	176	165799	19.51	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.18	200	26766	15.20	ng/ul	0.00
71) Anthracene-d10	16.87	188	258583m)	19.90	ng/ul	0.00
79) Pyrene-d10	19.17	212	279426	19.82	ng/ul	0.00
90) Benzo(a)pyrene-d12	22.95	264	289757	20.24	ng/ul	0.00

>JU 03104120

Target Compounds

					Ovalue
2) 1,4-Dioxane	3.05	88	8457	6.798	ng/uL 90
4) Benzaldehyde	6.53	77	30158	11.971	ng/ul 92
6) Phenol	6.59	94	77376	19.060	ng/ul# 84
8) Bis(2-Chloroethyl)ether	6.81	93	56621	17.746	ng/ul 96
10) 2-Chlorophenol	6.93	128	60089	20.002	ng/ul 97
11) 2-Methylphenol	7.82	108	56630	19.063	ng/ul 98
12) 2,2'-oxybis(1-Chloropropan	7.89	45	167981	21.476	ng/ul 99
14) Acetophenone	8.18	105	101426	20.655	ng/ul# 93
15) N-Nitroso-di-n-propylamine	8.17	70	53061	20.680	ng/ul# 83
16) 4-Methylphenol	8.15	108	63258	19.406	ng/ul 94
17) Hexachloroethane	8.40	117	27370	20.026	ng/ul 98
20) Nitrobenzene	8.55	77	82017	20.441	ng/ul 94
21) Isophorone	9.07	82	141360	20.018	ng/ul 98
23) 2-Nitrophenol	9.25	139	34697	20.817	ng/ul# 84
24) 2,4-Dimethylphenol	9.32	107	77242	21.344	ng/ul 98
25) Bis(2-Chloroethoxy)methane	9.55	93	77439	17.944	ng/ul 95
27) 2,4-Dichlorophenol	9.78	162	63257	21.894	ng/ul 98
28) Naphthalene	10.15	128	198491	19.777	ng/ul 99
30) 4-Chloroaniline	10.29	127	77987	23.670	ng/ul 98
31) Hexachlorobutadiene	10.44	225	41526	21.492	ng/ul 96
32) Caprolactam	11.08	113	17373m)	17.930	ng/ul 100
33) 4-Chloro-3-methylphenol	11.43	107	71558	21.660	ng/ul 95
34) 2-Methylnaphthalene	11.78	142	149607	21.467	ng/ul 95

>JU 03104120

Quantitation Report (QT Reviewed)

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN030320\
 Data File : BN010068.D
 Acq On : 03 Mar 2020 19:05
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 LabSampleId :
 SSTD02077

Manual Integrations
 APPROVED

mohammad
 3/4/2020 7:51:54 AM

Quant Time: Mar 03 19:40:40 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 03 12:28:17 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
35) 1-Methylnaphthalene	12.00	142	141644	20.277	ng/uL	99
37) 1,2,4,5-Tetrachlorobenzene	12.17	216	80159	20.526	ng/ul	93
38) Hexachlorocyclopentadiene	12.13	237	13286	7.863	ng/ul	94
39) 2,4,6-Trichlorophenol	12.43	196	49539	19.987	ng/ul	94
40) 2,4,5-Trichlorophenol	12.50	196	50040	18.820	ng/ul	98
41) 1,1'-Biphenyl	12.83	154	202366	19.999	ng/ul#	96
42) 2-Chloronaphthalene	12.86	162	155536	19.354	ng/ul	97
43) 2-Nitroaniline	13.09	65	59152	20.128	ng/ul	94
45) Dimethylphthalate	13.48	163	196963	19.181	ng/ul	98
46) 2,6-Dinitrotoluene	13.61	165	37649	18.729	ng/ul	92
48) Acenaphthylene	13.72	152	239853	19.120	ng/ul	99
49) 3-Nitroaniline	13.94	138	36373	19.599	ng/ul	99
50) Acenaphthene	14.07	153	165139	19.203	ng/ul	99
51) 2,4-Dinitrophenol	14.19	184	13570	11.758	ng/ul	92
53) 4-Nitrophenol	14.27	109	30784	18.982	ng/ul#	76
54) Dibenzofuran	14.41	168	238325	19.745	ng/ul	99
55) 2,4-Dinitrotoluene	14.42	165	59652	20.022	ng/ul#	96
56) 2,3,4,6-Tetrachlorophenol	14.66	232	46011	20.126	ng/ul	98
57) Diethylphthalate	14.86	149	204481	19.393	ng/ul	97
59) Fluorene	15.07	166	193066	19.059	ng/ul	99
60) 4-Chlorophenyl-phenylether	15.07	204	98969	19.810	ng/ul	89
61) 4-Nitroaniline	15.12	138	39481m	17.445	ng/ul	
64) 4,6-Dinitro-2-methylphenol	15.19	198	28549m	15.047	ng/ul	
65) N-Nitrosodiphenylamine	15.29	169	168627	20.046	ng/ul	98
66) 4-Bromophenyl-phenylether	15.97	248	57935	20.422	ng/ul	94
67) Hexachlorobenzene	16.08	284	64193	20.449	ng/ul	95
68) Atrazine	16.26	200	59582	18.671	ng/ul	91
69) Pentachlorophenol	16.44	266	28645	15.790	ng/ul	90
70) Phenanthrene	16.81	178	315321m	19.488	ng/ul	
72) Anthracene	16.90	178	326371	19.732	ng/ul	99
73) 1,2,3,4-Tetrachlorobenzene	12.79	216	76039	18.358	ng/uL	97
74) Pentachlorobenzene	14.33	250	76370	19.119	ng/uL	98
75) Carbazole	17.19	167	281277	19.310	ng/ul	97
76) Di-n-butylphthalate	17.76	149	339052	18.859	ng/ul#	98
77) Fluoranthene	18.84	202	362140	19.107	ng/ul	96
80) Pyrene	19.20	202	380179	19.545	ng/ul#	94
81) Butylbenzylphthalate	20.14	149	155959	19.504	ng/ul	100
82) 3,3'-Dichlorobenzidine	20.92	252	95983	16.317	ng/ul	97
83) Benzo(a)anthracene	20.97	228	369886	19.950	ng/ul	98
84) Bis(2-ethylhexyl)phthalate	20.93	149	223277	18.289	ng/ul	99
85) Chrysene	21.03	228	354914	19.444	ng/ul	99
87) Di-n-octyl phthalate	21.77	149	380915	17.554	ng/ul	100
88) Benzo(b)fluoranthene	22.47	252	362411	19.496	ng/ul	98
89) Benzo(k)fluoranthene	22.51	252	348907	19.823	ng/ul	99
91) Benzo(a)pyrene	23.00	252	345070	20.640	ng/ul#	97
92) Indeno(1,2,3-cd)pyrene	25.12	276	372384	18.760	ng/ul	93
93) Dibenzo(a,h)anthracene	25.12	278	311200	18.327	ng/ul#	94
94) Benzo(a,h,i)perylene	25.73	276	284620	17.101	ng/ul	96

250 03/04/20

250 03/04/20

Quantitation Report (QT Reviewed)

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030320\
 Data File : BN010068.D
 Acq On : 03 Mar 2020 19:05
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 LabSampleId :
 SSTD02077

Quant Time: Mar 03 19:40:40 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 03 12:28:17 2020
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mohammad
 3/4/2020 7:51:54 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)

(#) = qualifier out of range (m) = manual integration (+) = signals summed						