

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030320\

Quantitation Report (QT Reviewed)

Data File : BN010076.D

Acq On : 03 Mar 2020 23:58

Operator : CG/JU

Sample : L1619-06DL 5X

Misc :

ALS Vial : 20 Sample Multiplier: 1

Quant Time: Mar 04 02:50:56 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Wed Mar 04 01:30:16 2020

Response via : Initial Calibration

Instrument :

BNA_N

Client Sample ID :


DBDW0DL

Manual Integrations

APPROVED

mohammad

3/4/2020 7:52:16 AM

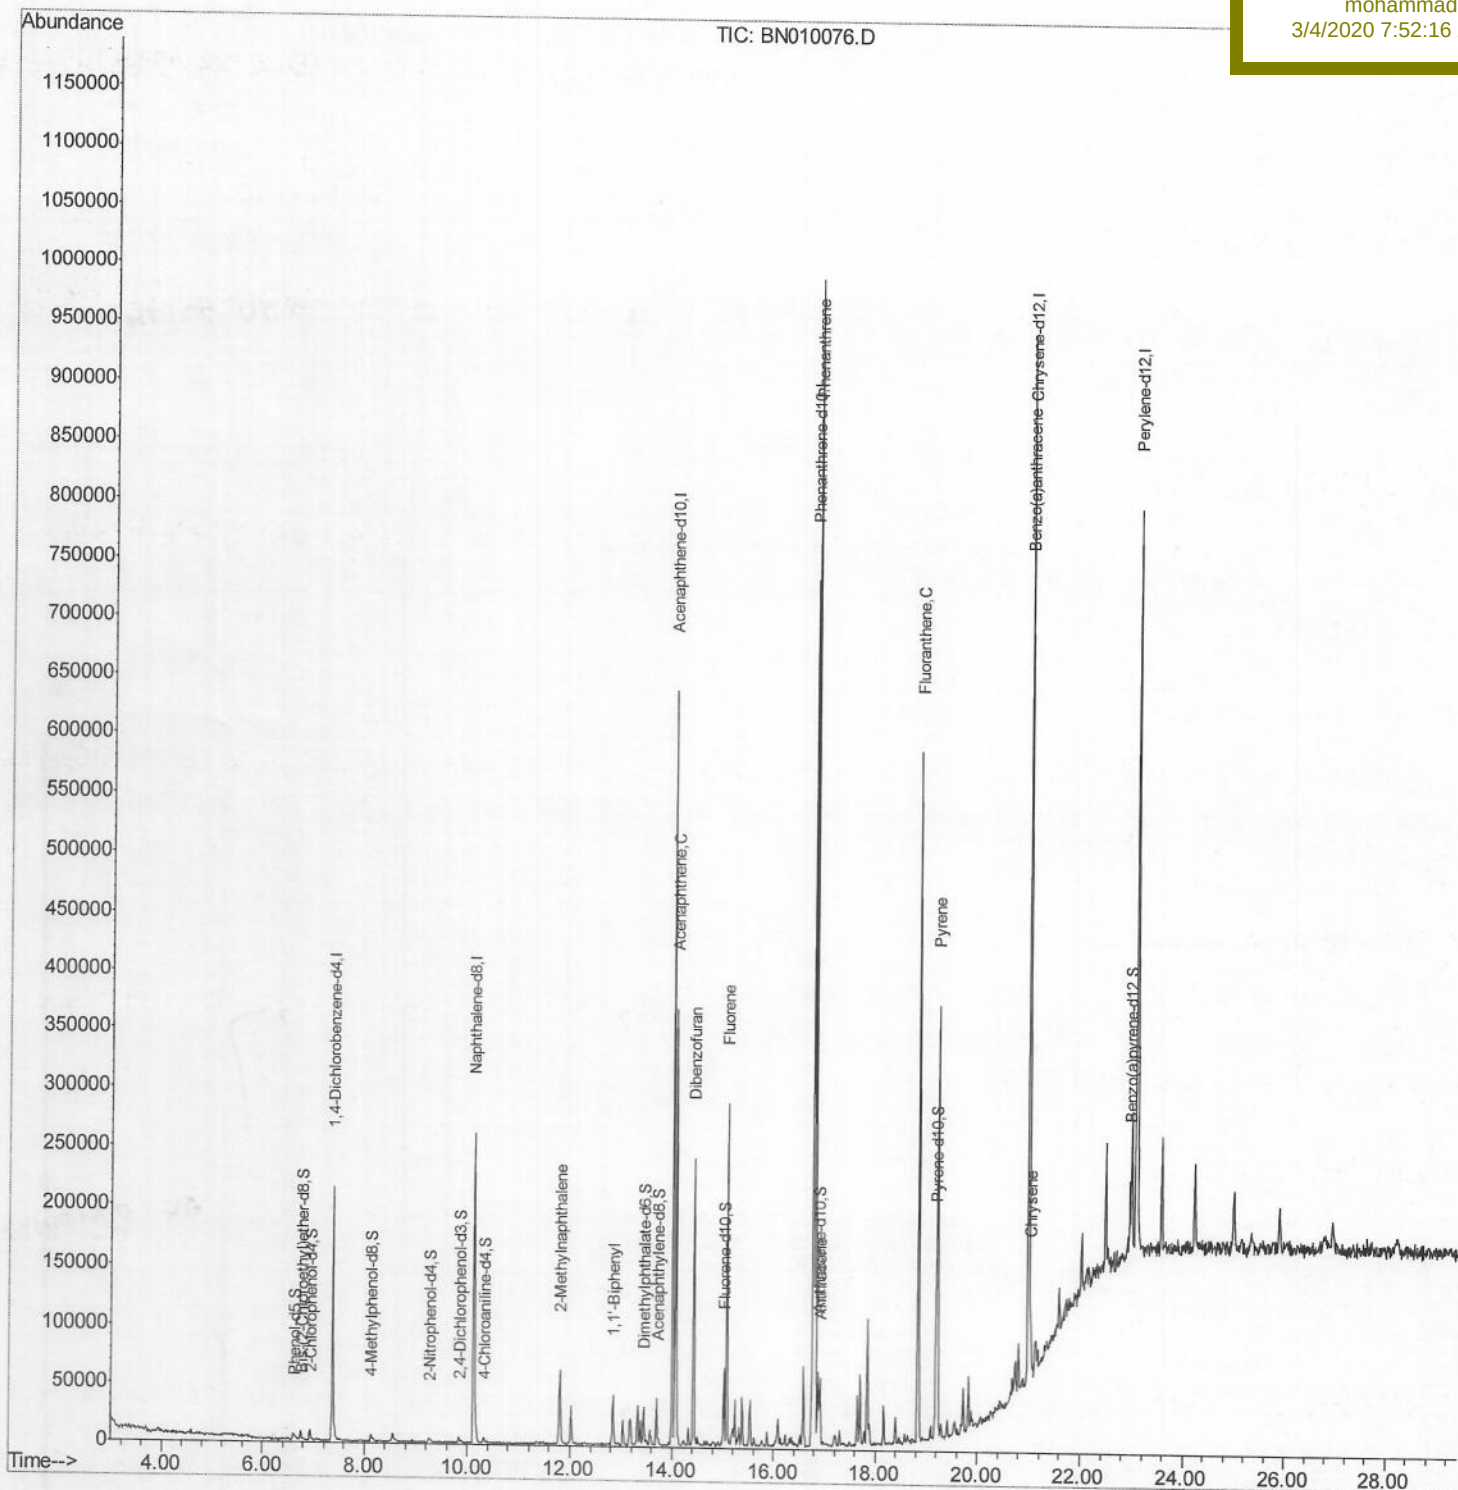

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030320\

Quantitation Report (Qedit)

Data File : BN010076.D

Acq On : 03 Mar 2020 23:58

Operator : CG/JU

Sample : L1619-06DL 50X

Misc :

ALS Vial : 20 Sample Multiplier: 1

Quant Time: Mar 04 01:33:14 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Wed Mar 04 01:30:16 2020

Response via : Initial Calibration

Instrument :

BNA_N

Client Sampled :




DBDW0DL

Manual Integrations

APPROVED

mohammad

3/4/2020 7:52:16 AM

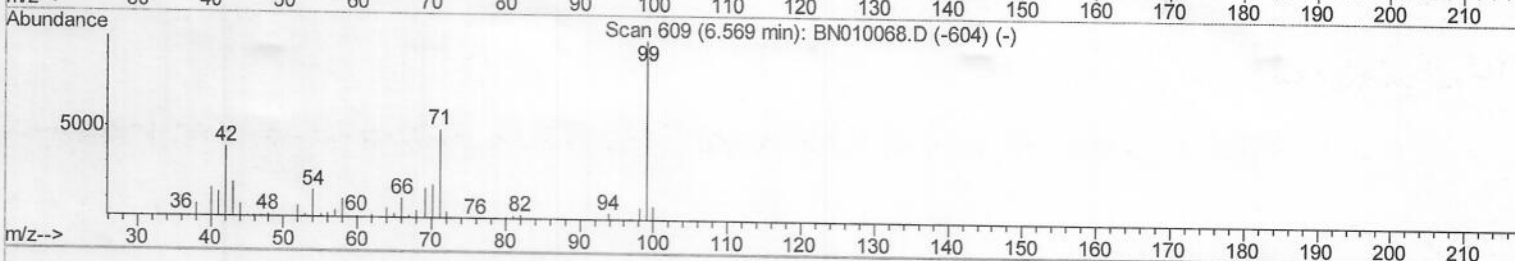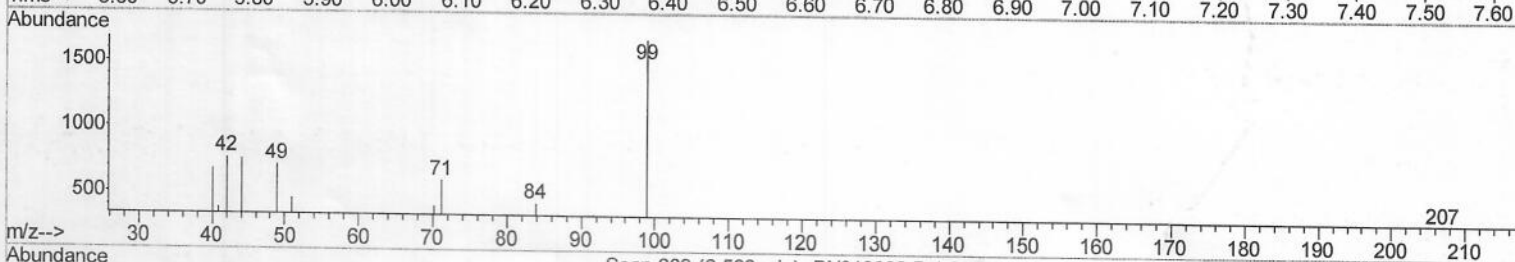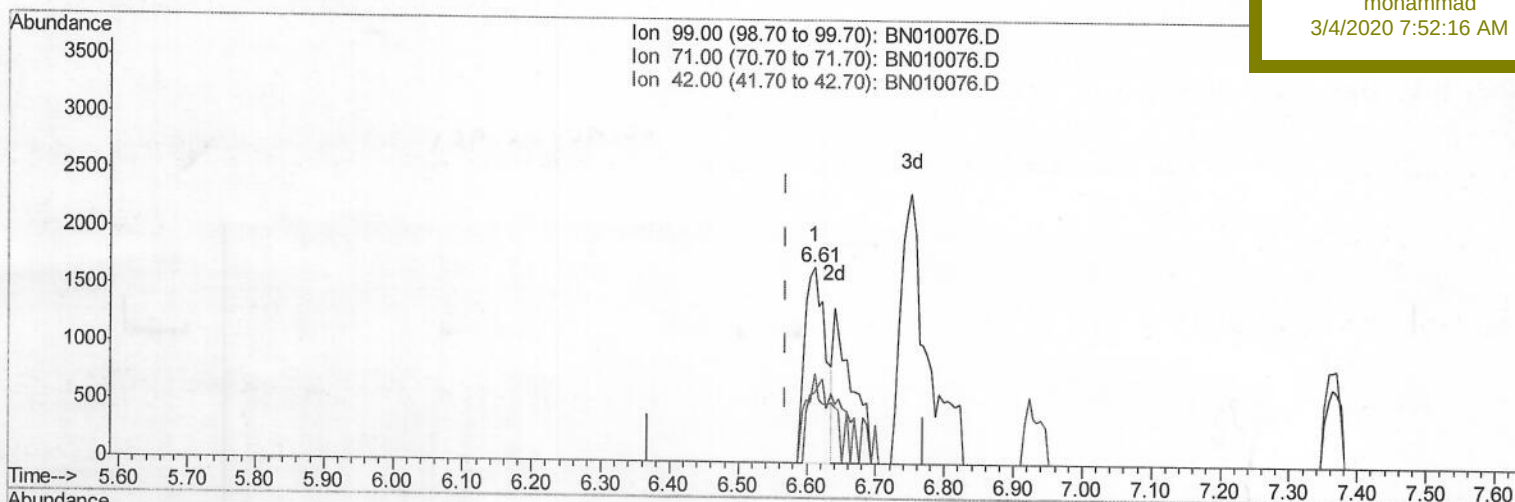

TIC: BN010076.D

(5) Phenol-d5 (S)

6.611min (+0.041) 0.70ng/ul

response 3502

Ion	Exp%	Act%
99.00	100	100
71.00	38.10	35.84
42.00	28.80	45.44#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030320\
Quantitation Report (Qedit)




Data File : BN010076.D
Acq On : 03 Mar 2020 23:58
Operator : CG/JU
Sample : L1619-06DL 50X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Mar 04 01:33:14 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 04 01:30:16 2020
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
DBDW0DL

Manual Integrations
APPROVED

mohammad
3/4/2020 7:52:16 AM

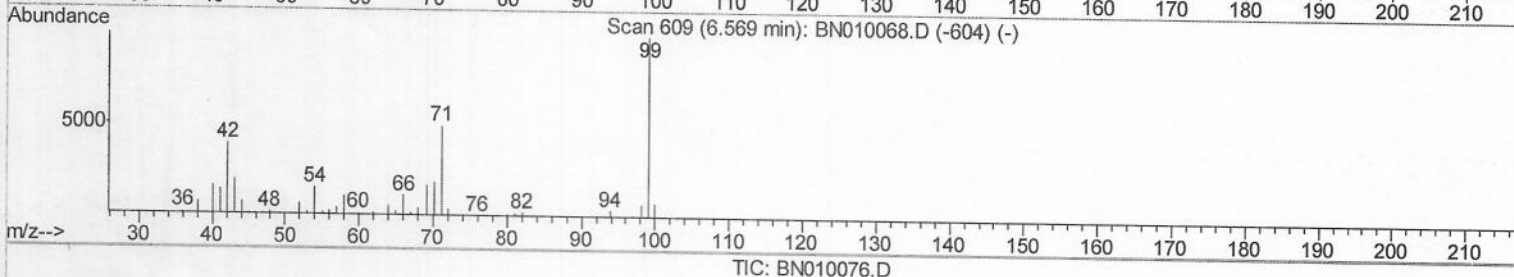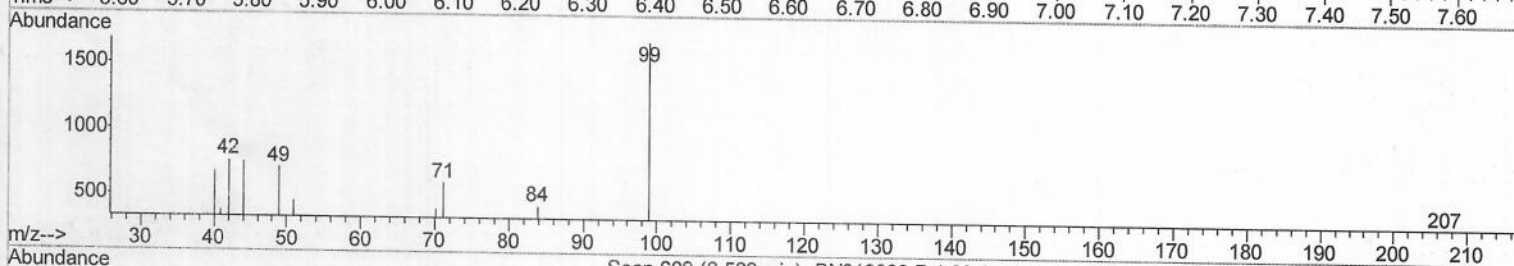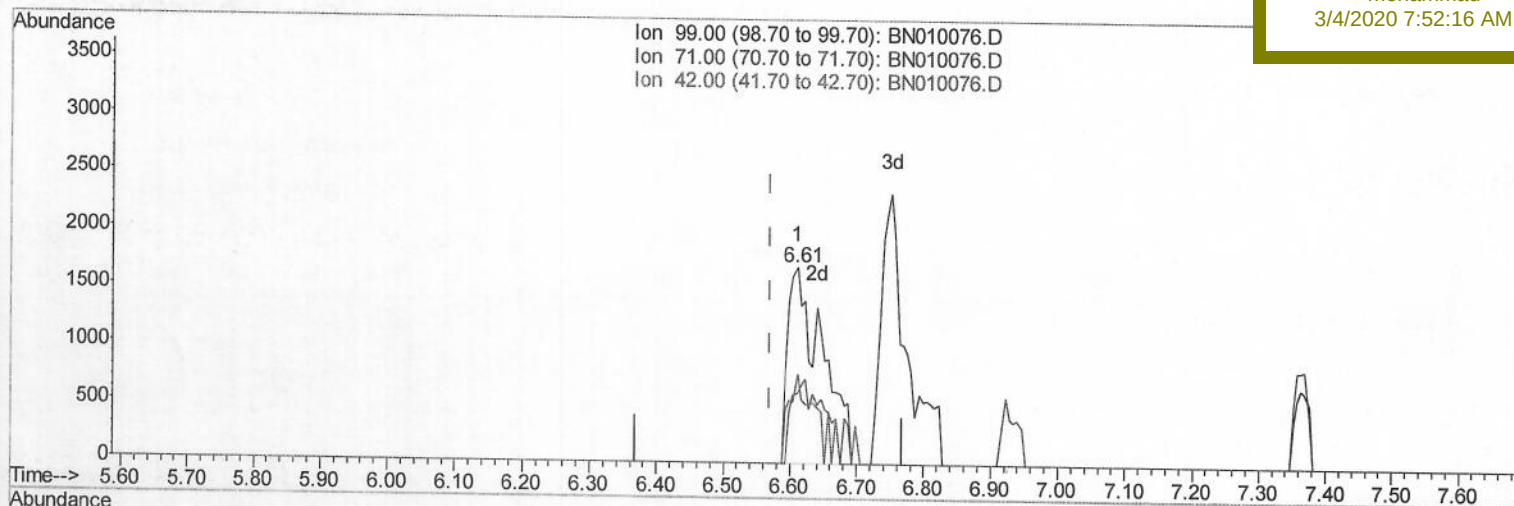

(5) Phenol-d5 (S)

6.611min (+0.041) 1.20ng/ul m

> JU 03/05/20

response 5998

Ion	Exp%	Act%
99.00	100	100
71.00	38.10	35.84
42.00	28.80	45.44#
0.00	0.00	0.00


Data File : BN010076.D
Acq On : 03 Mar 2020 23:58
Operator : CG/JU
Sample : L1619-06DL 50X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Mar 04 01:33:14 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 04 01:30:16 2020
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
DBDW0DL

Manual Integrations
APPROVED

mohammad
3/4/2020 7:52:16 AM

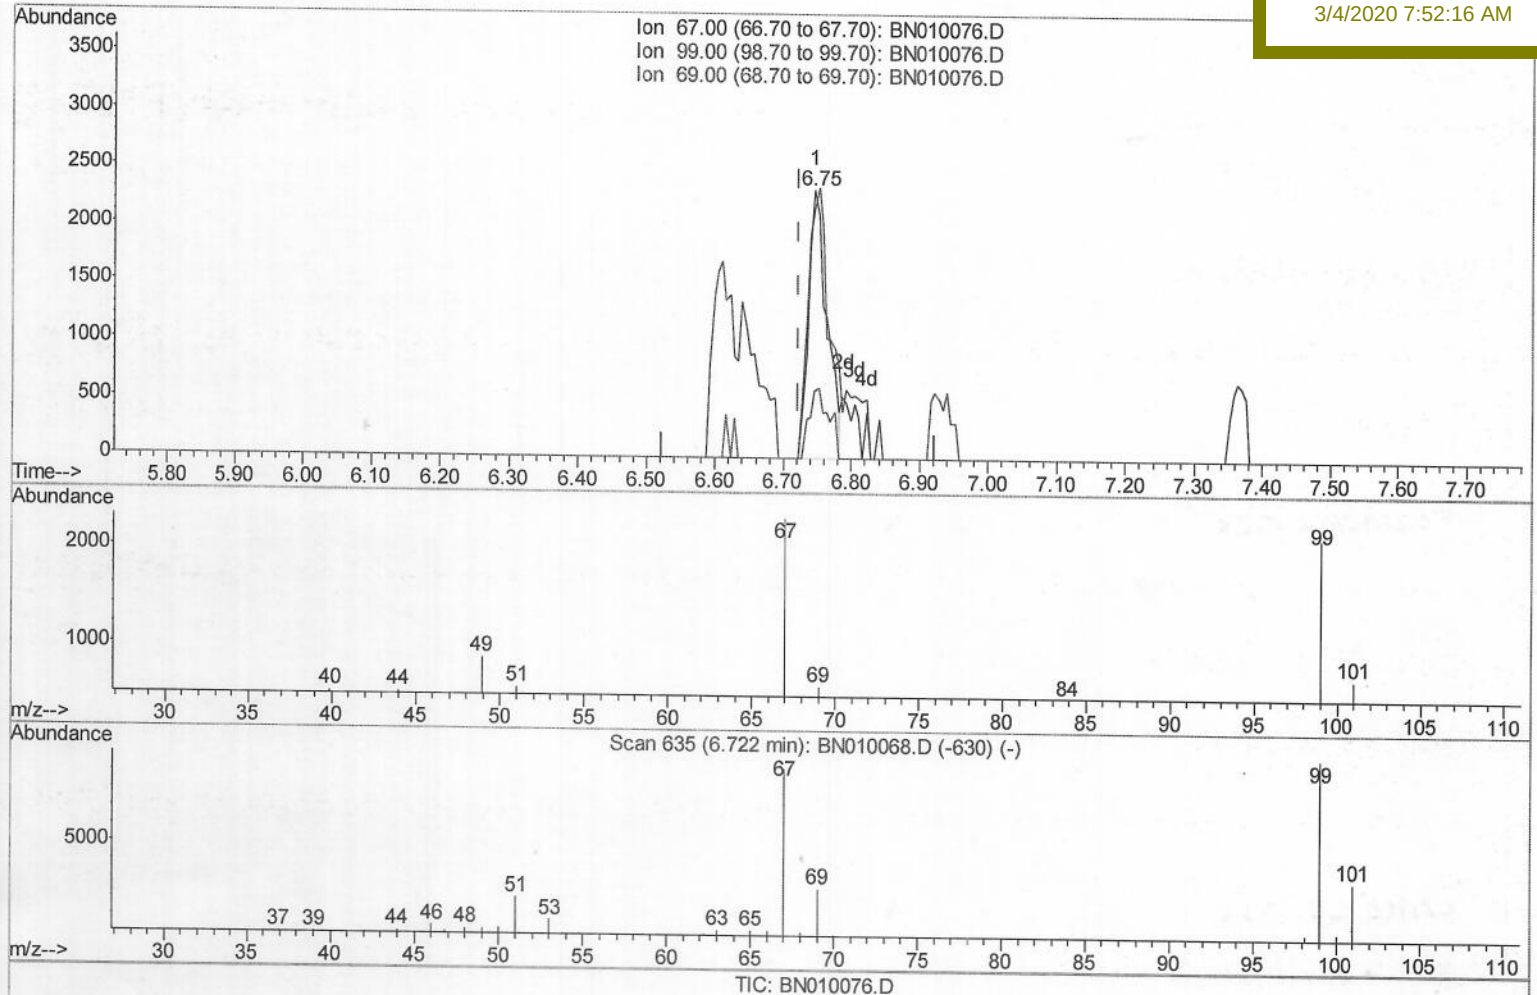

(7) Bis-(2-Chloroethyl)ether-d8 (S)

6.746min (+0.024) 1.24ng/ul

response 4271

Ion	Exp%	Act%
67.00	100	100
99.00	106.90	92.66
69.00	28.30	25.39
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030320\
Quantitation Report (Qedit)




Data File : BN010076.D
Acq On : 03 Mar 2020 23:58
Operator : CG/JU
Sample : L1619-06DL 50X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Mar 04 01:33:14 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 04 01:30:16 2020
Response via : Initial Calibration

Instrument :
BNA_N
Client Sampled :
DBDW0DL

Manual Integrations
APPROVED

mohammad
3/4/2020 7:52:16 AM

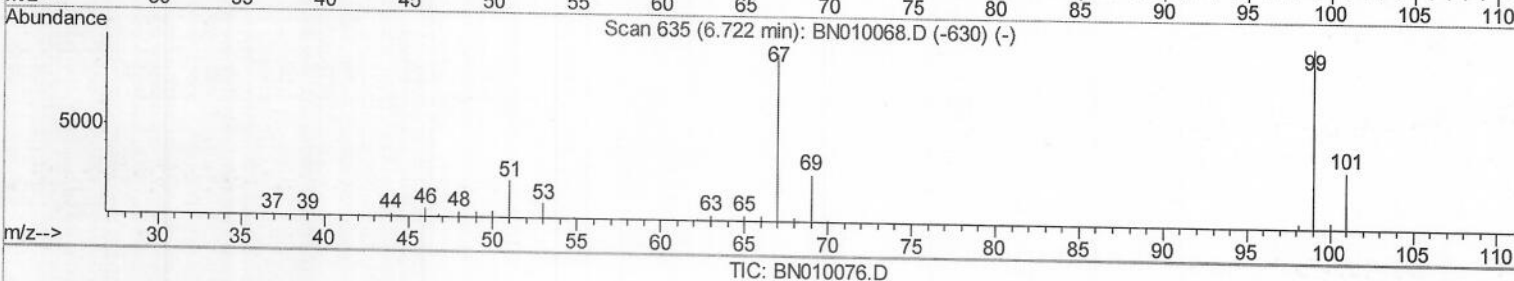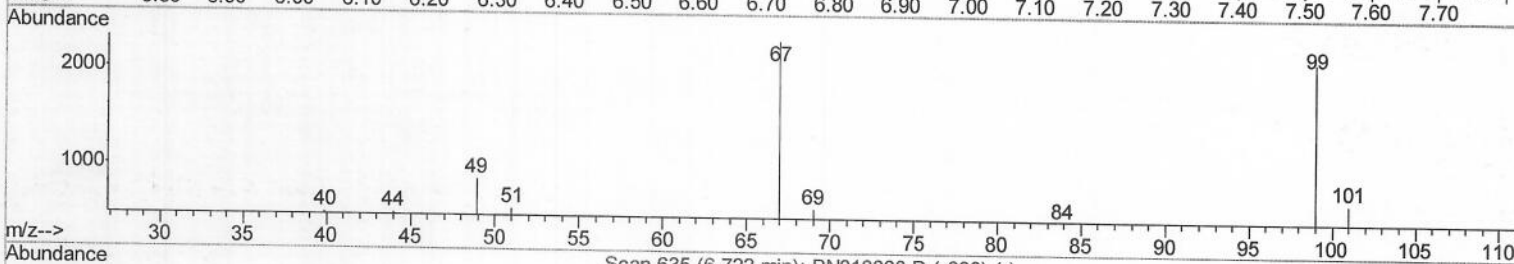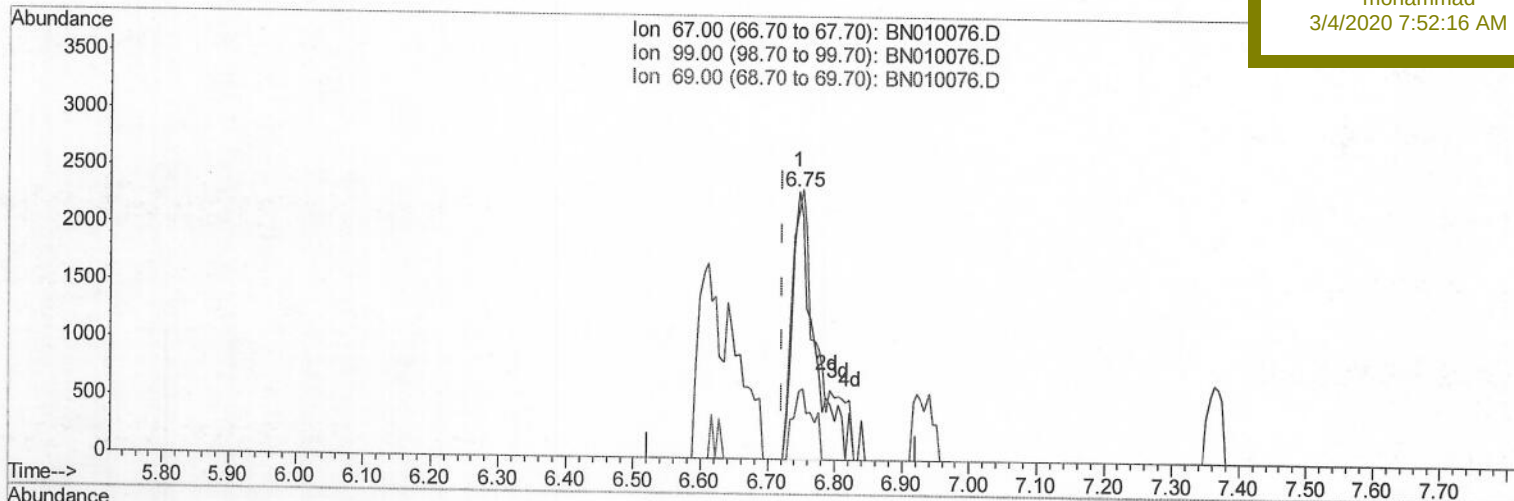

(7) Bis-(2-Chloroethyl)ether-d8 (S)

6.746min (+0.024) 1.46ng/ul m

response 5037

Ion	Exp%	Act%
67.00	100	100
99.00	106.90	92.66
69.00	28.30	25.39
0.00	0.00	0.00

> JU 03/05/20

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030320\
Quantitation Report (Qedit)




Data File : BN010076.D
Acq On : 03 Mar 2020 23:58
Operator : CG/JU
Sample : L1619-06DL 50X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Mar 04 01:33:14 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 04 01:30:16 2020
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
DBDW0DL

Manual Integrations
APPROVED

mohammad
3/4/2020 7:52:16 AM

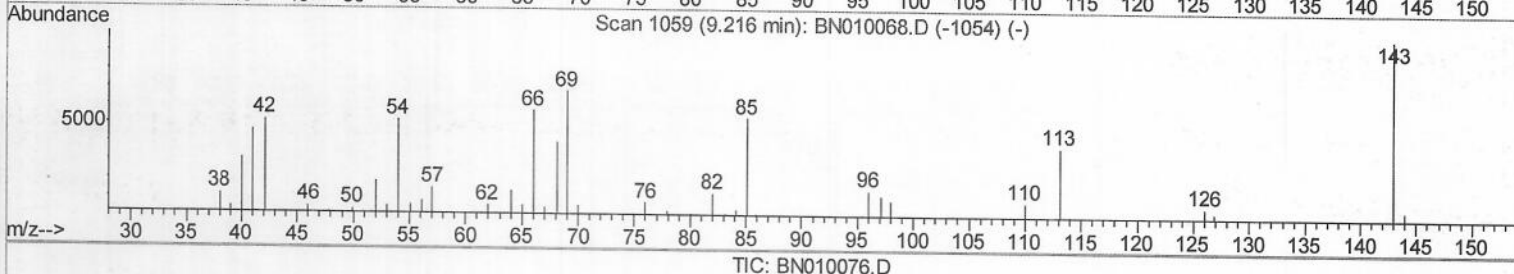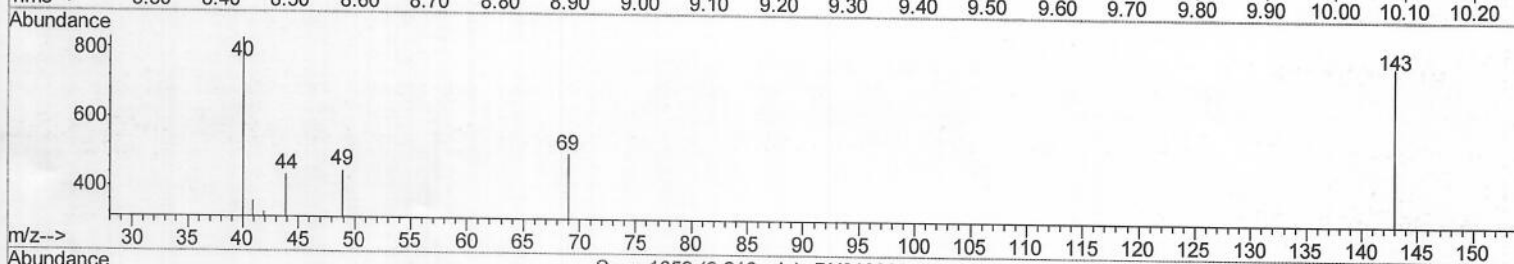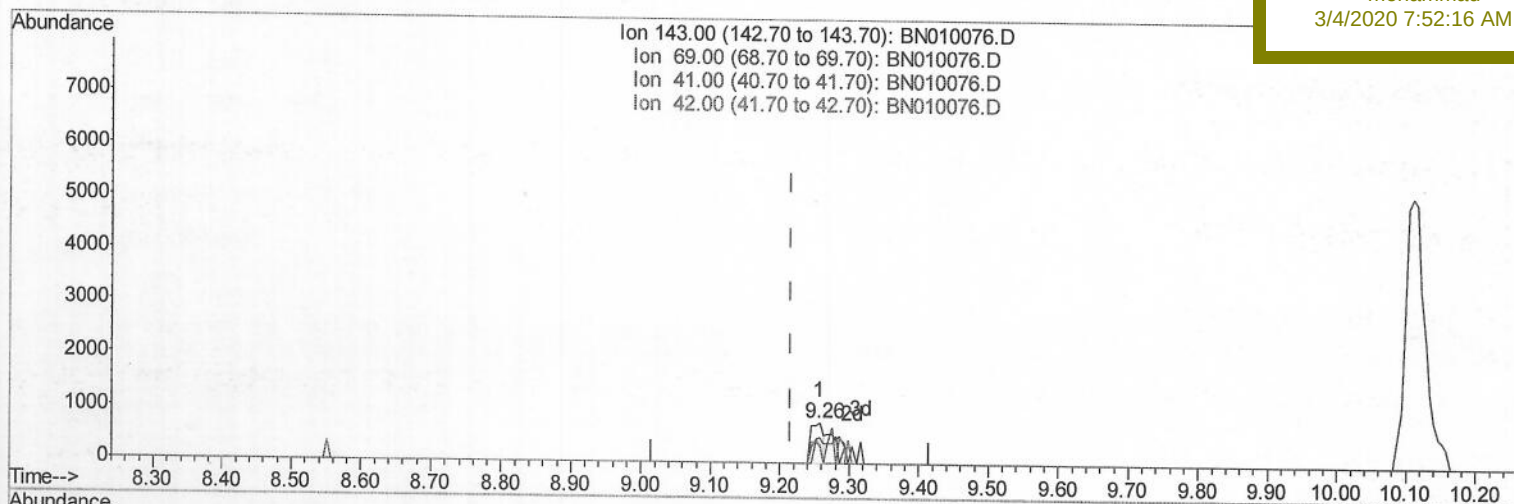

(22) 2-Nitrophenol-d4 (S)

9.258min (+0.041) 0.56ng/ul

response 970

Ion	Exp%	Act%
143.00	100	100
69.00	60.40	64.34
41.00	36.00	46.12#
42.00	42.10	41.86

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030320\

Quantitation Report (Qedit)

Data File : BN010076.D

Acq On : 03 Mar 2020 23:58

Operator : CG/JU

Sample : L1619-06DL 50X

Misc :

ALS Vial : 20 Sample Multiplier: 1

Quant Time: Mar 04 01:33:14 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Wed Mar 04 01:30:16 2020

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




DBDW0DL

Manual Integrations

APPROVED

mohammad

3/4/2020 7:52:16 AM

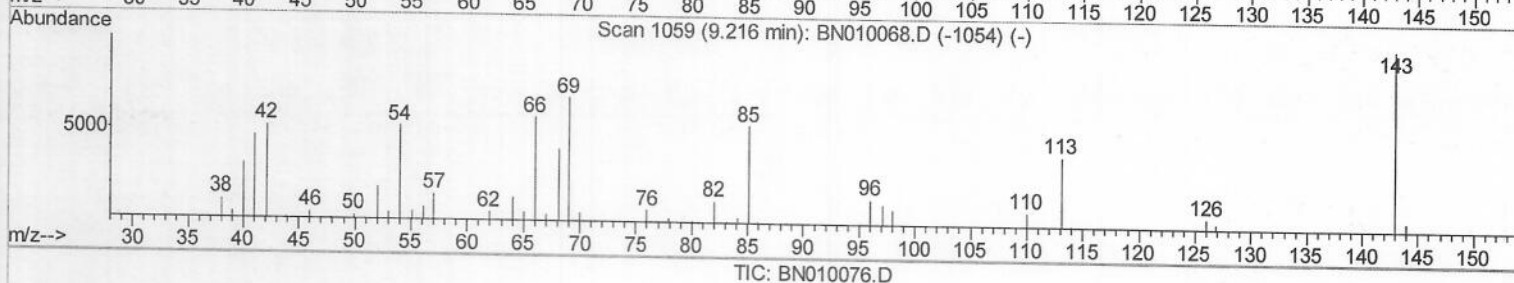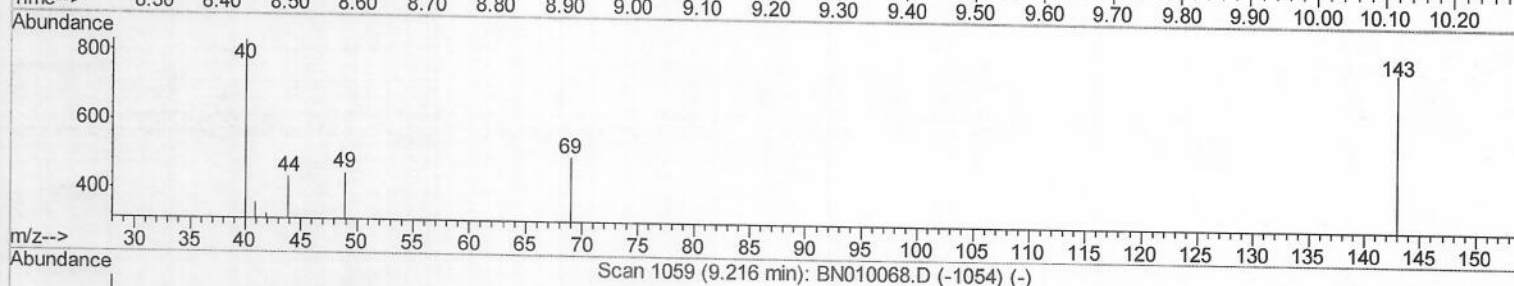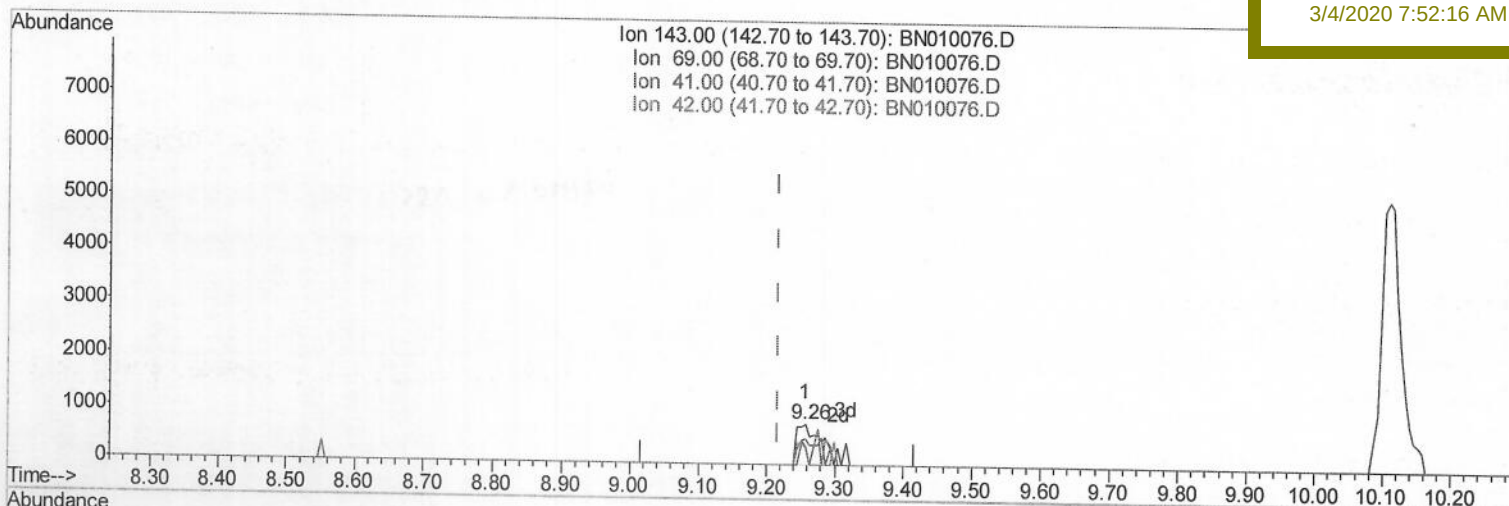

(22) 2-Nitrophenol-d4 (S)

9.258min (+0.041) 1.05ng/ul m

response 1812

Ion	Exp%	Act%
143.00	100	100
69.00	60.40	64.34
41.00	36.00	46.12#
42.00	42.10	41.86

> JU 03/05/20

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030320\
Quantitation Report (Qedit)




Data File : BN010076.D
Acq On : 03 Mar 2020 23:58
Operator : CG/JU
Sample : L1619-06DL 50X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Mar 04 01:33:14 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 04 01:30:16 2020
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
DBDW0DL

Manual Integrations
APPROVED

mohammad
3/4/2020 7:52:16 AM

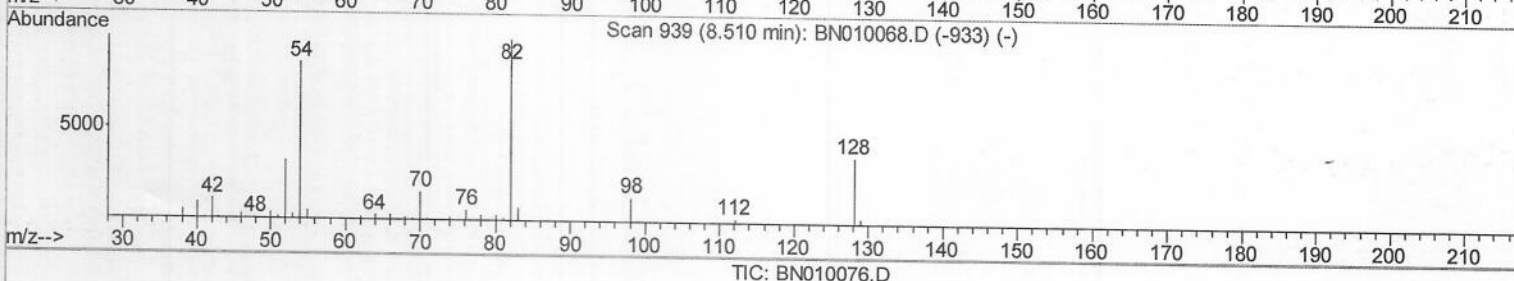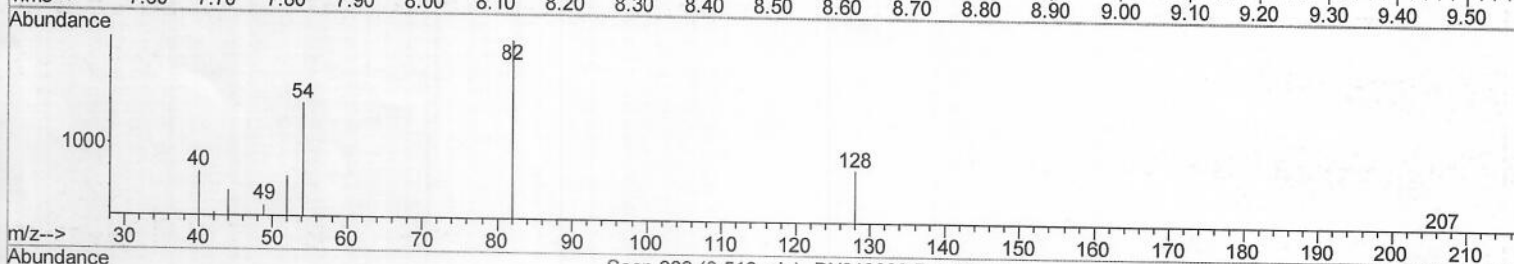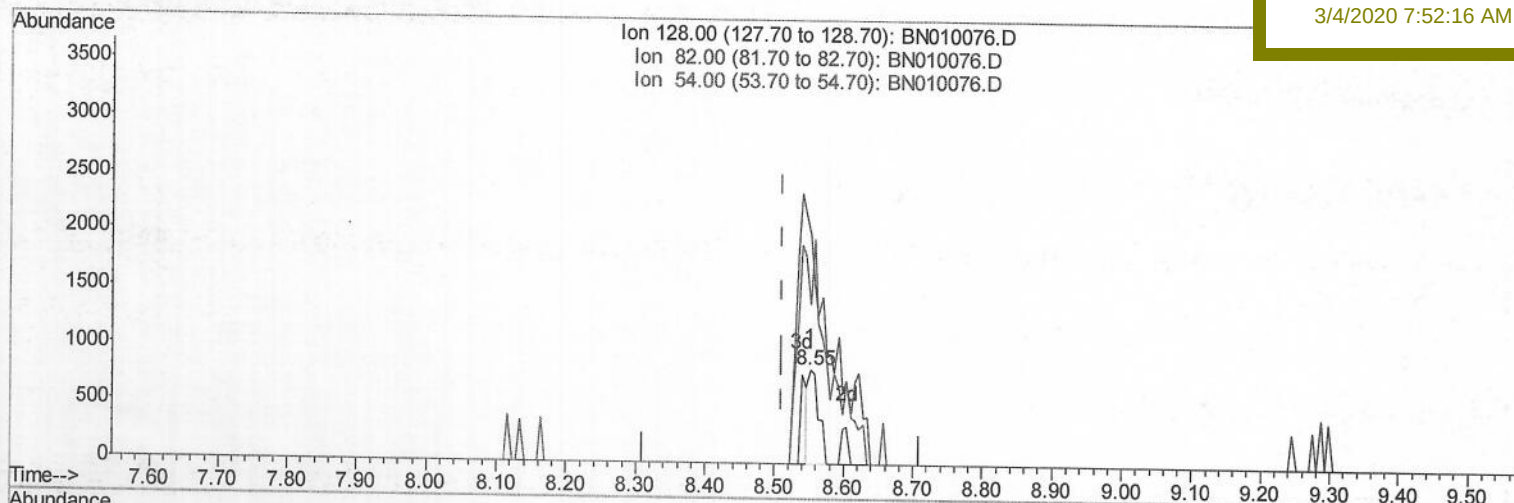

(19) Nitrobenzene-d5 (S)

8.552min (+0.041) 0.53ng/ul

response 834

Ion	Exp%	Act%
128.00	100	100
82.00	271.60	243.70
54.00	200.30	169.52
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030320\

Quantitation Report (Qedit)

Data File : BN010076.D

Acq On : 03 Mar 2020 23:58

Operator : CG/JU

Sample : L1619-06DL 50X

Misc :

ALS Vial : 20 Sample Multiplier: 1

Quant Time: Mar 04 01:33:14 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Wed Mar 04 01:30:16 2020

Response via : Initial Calibration

Instrument :

BNA_N

Client Sample ID :




DBDW0DL

Manual Integrations

APPROVED

mohammad

3/4/2020 7:52:16 AM

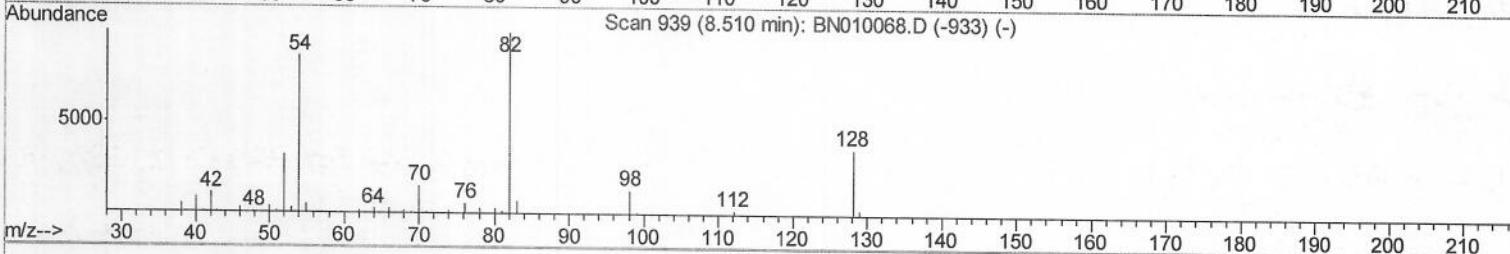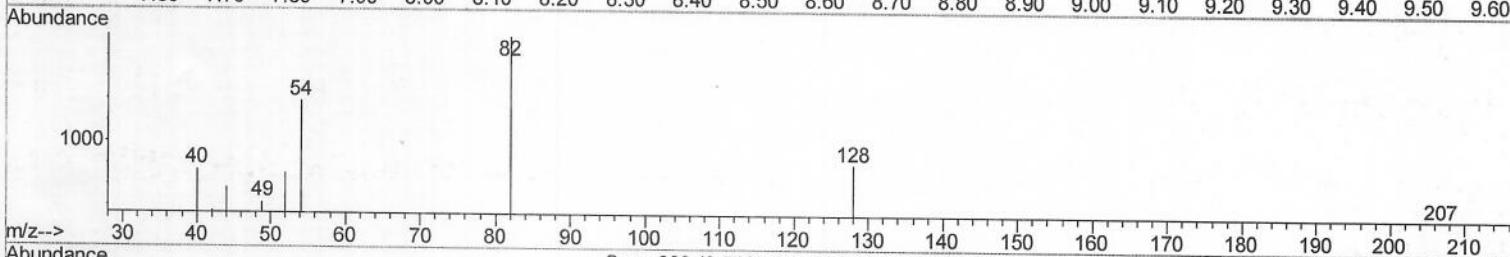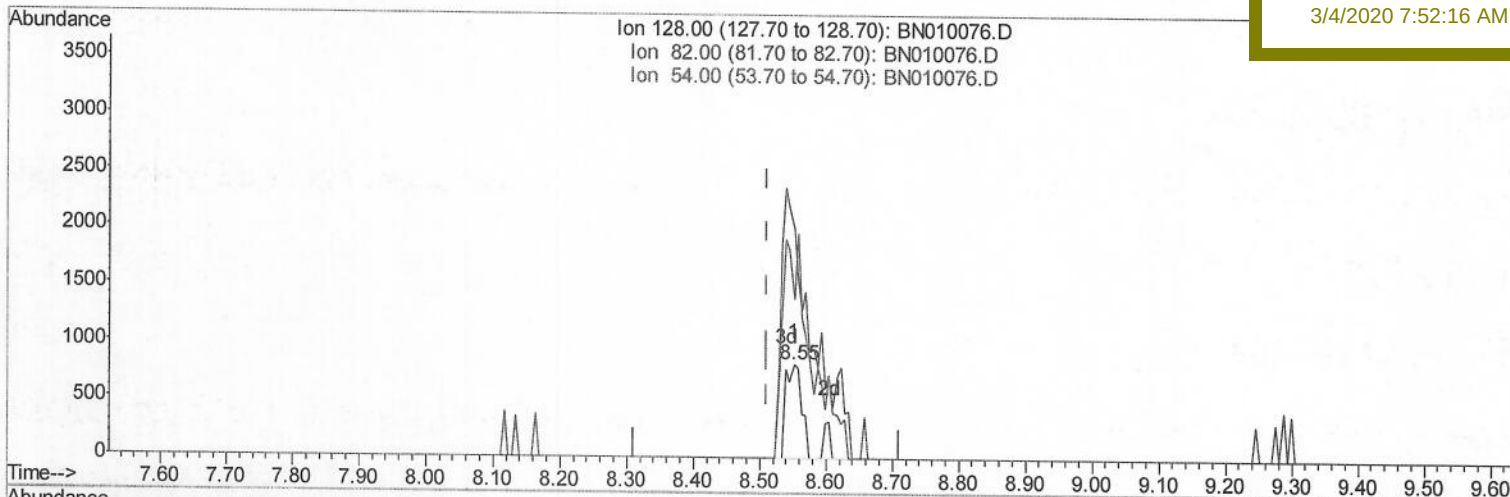

(19) Nitrobenzene-d5 (S)

8.552min (+0.041) 0.98ng/ul m

response 1559

Ion	Exp%	Act%
128.00	100	100
82.00	271.60	243.70
54.00	200.30	169.52
0.00	0.00	0.00

2 JU 03/04/20

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030320\
Quantitation Report (Qedit)




Data File : BN010076.D
Acq On : 03 Mar 2020 23:58
Operator : CG/JU
Sample : L1619-06DL 50X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Mar 04 01:33:14 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 04 01:30:16 2020
Response via : Initial Calibration

Instrument :
BNA_N
Client Sample Id :
DBDW0DL

Manual Integrations
APPROVED

mohammad
3/4/2020 7:52:16 AM

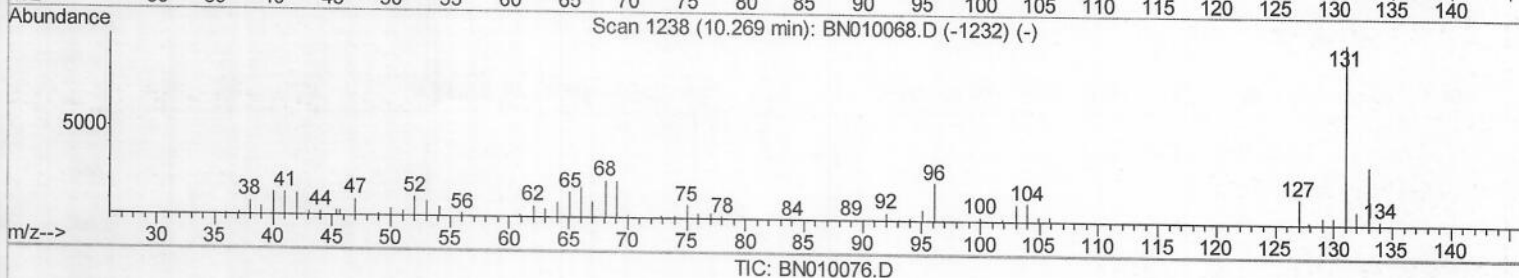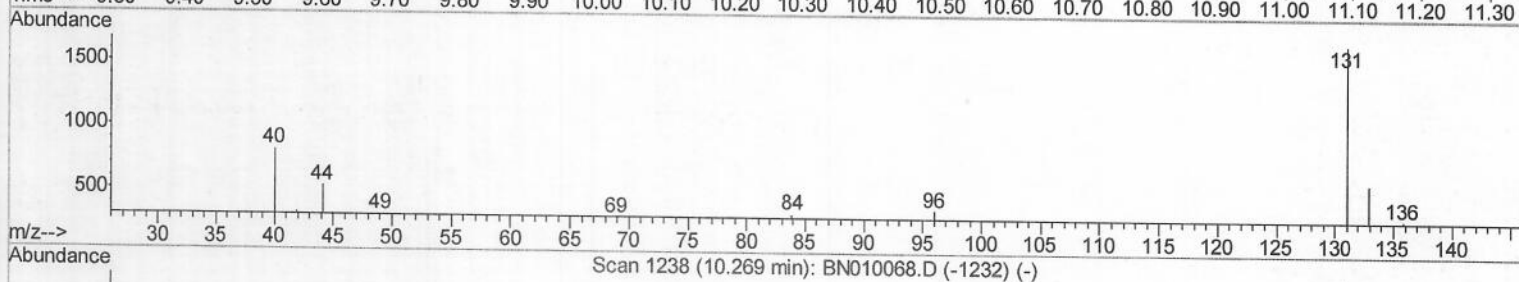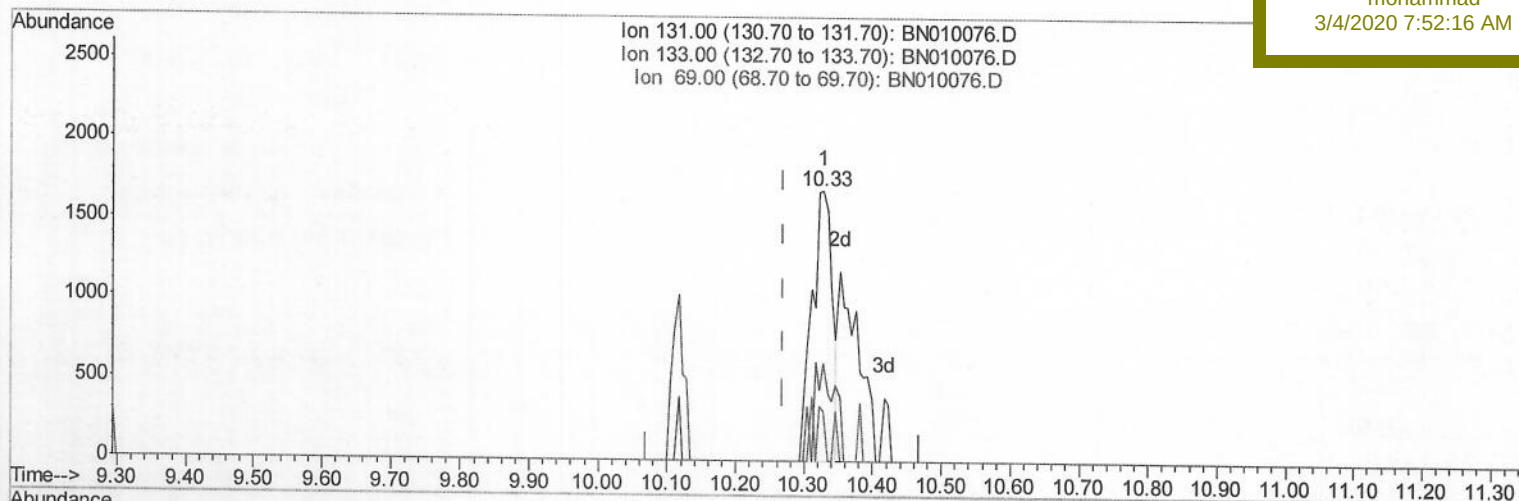

(29) 4-Chloroaniline-d4 (S)
10.328min (+0.059) 0.92ng/ul
response 3444

Ion	Exp%	Act%
131.00	100	100
133.00	33.00	35.73
69.00	22.10	18.19
0.00	0.00	0.00




Data File : BN010076.D
Acq On : 03 Mar 2020 23:58
Operator : CG/JU
Sample : L1619-06DL 50X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Mar 04 01:33:14 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 04 01:30:16 2020
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
DBDW0DL

Manual Integrations
APPROVED

mohammad
3/4/2020 7:52:16 AM

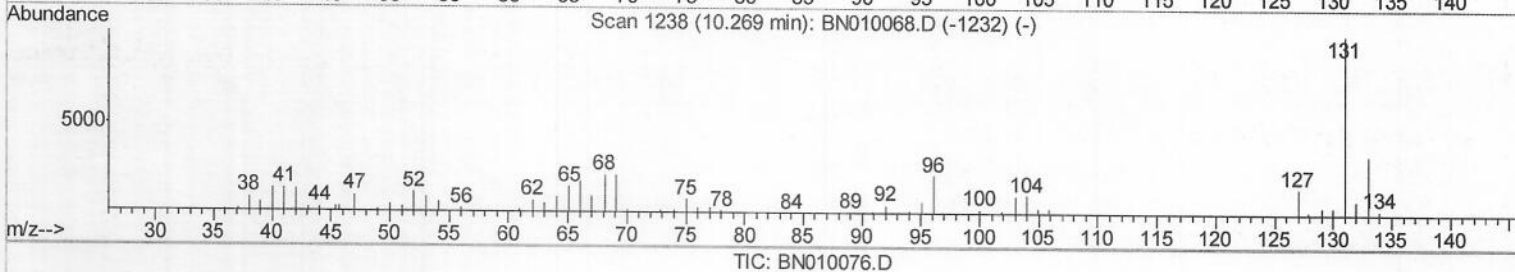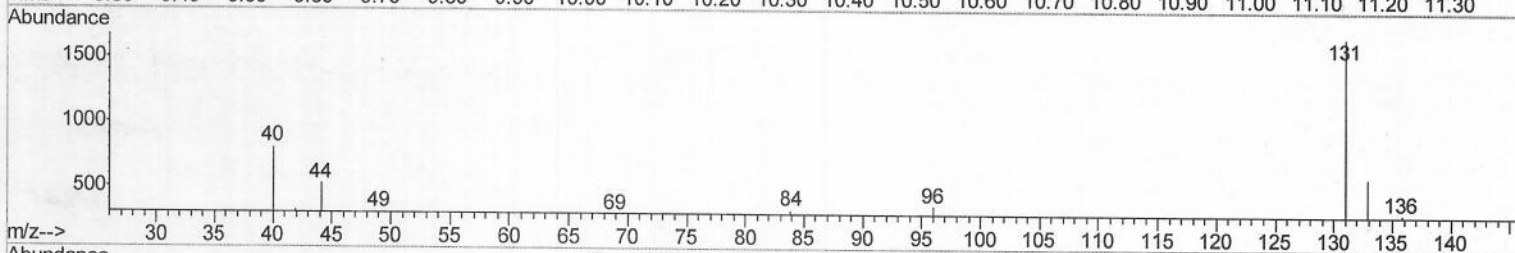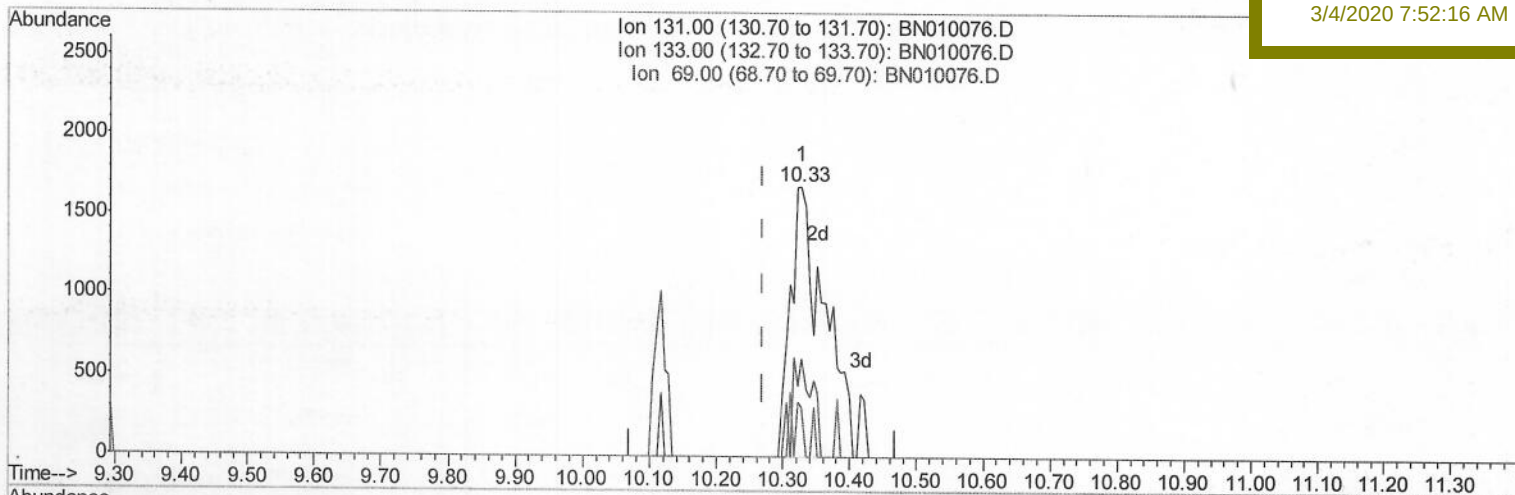

TIC: BN010076.D

(29) 4-Chloroaniline-d4 (S)

10.328min (+0.059) 1.56ng/ul m

response 5832

Ion	Exp%	Act%
131.00	100	100
133.00	33.00	35.73
69.00	22.10	18.19
0.00	0.00	0.00

> JU 03/04/20

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030320\

Quantitation Report (Qedit)

Data File : BN010076.D

Acq On : 03 Mar 2020 23:58

Operator : CG/JU

Sample : L1619-06DL 50X

Misc :

ALS Vial : 20 Sample Multiplier: 1

Quant Time: Mar 04 01:33:14 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Wed Mar 04 01:30:16 2020

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




DBDW0DL

Manual Integrations

APPROVED

mohammad

3/4/2020 7:52:16 AM

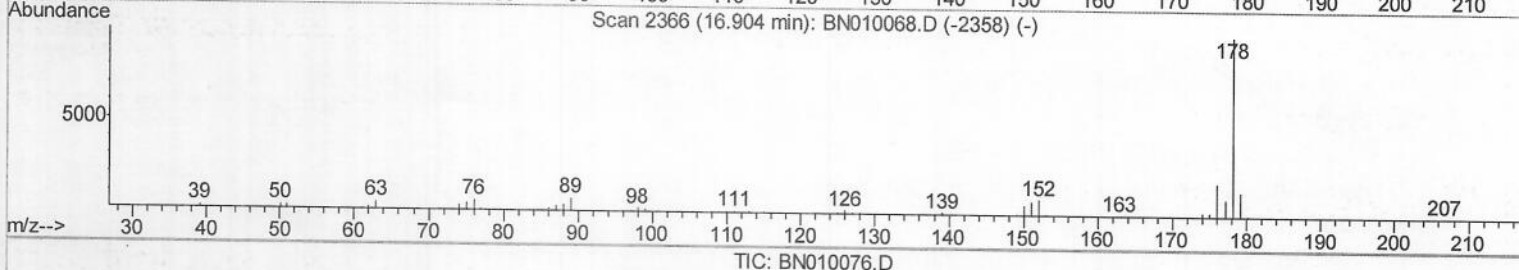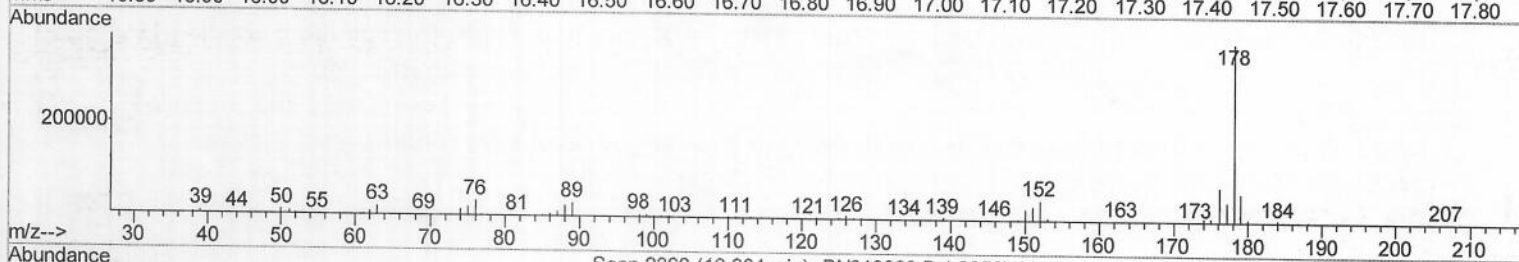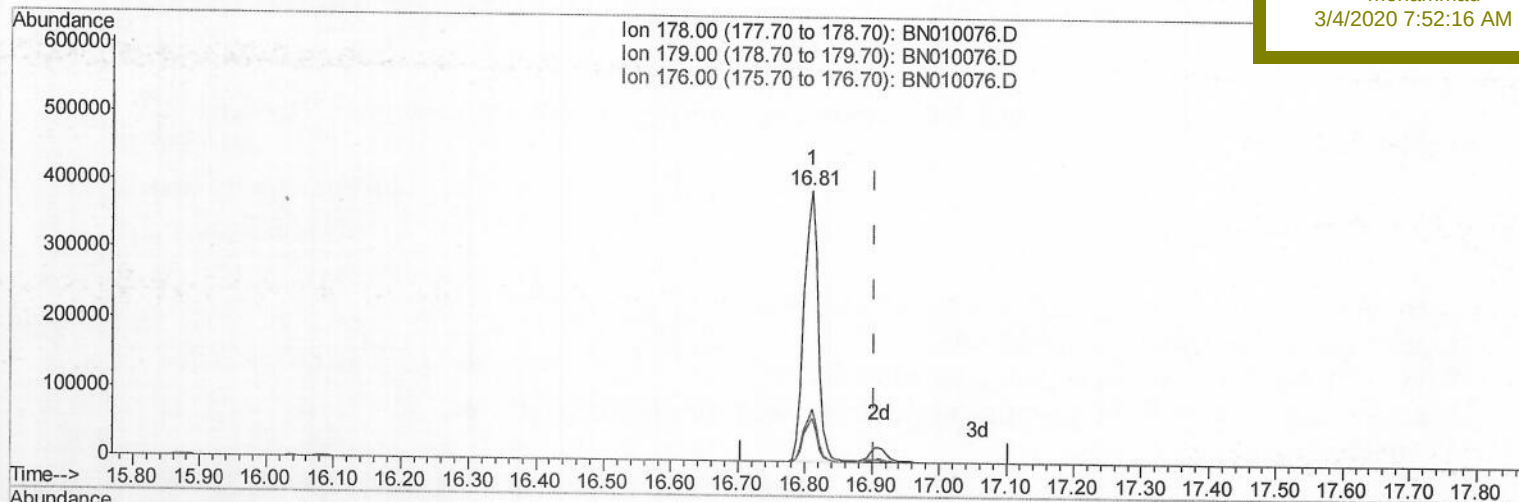

TIC: BN010076.D

(72) Anthracene

16.810min (-0.094) 24.38ng/ul

response 570124

Ion	Exp%	Act%
-----	------	------

178.00	100	100
--------	-----	-----

179.00	15.20	15.99
--------	-------	-------

176.00	18.20	19.17
--------	-------	-------

0.00	0.00	0.00
------	------	------

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030320\
Quantitation Report (Qedit)




Data File : BN010076.D
Acq On : 03 Mar 2020 23:58
Operator : CG/JU
Sample : L1619-06DL 50X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBDW0DL

Quant Time: Mar 04 01:33:14 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 04 01:30:16 2020
Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
3/4/2020 7:52:16 AM

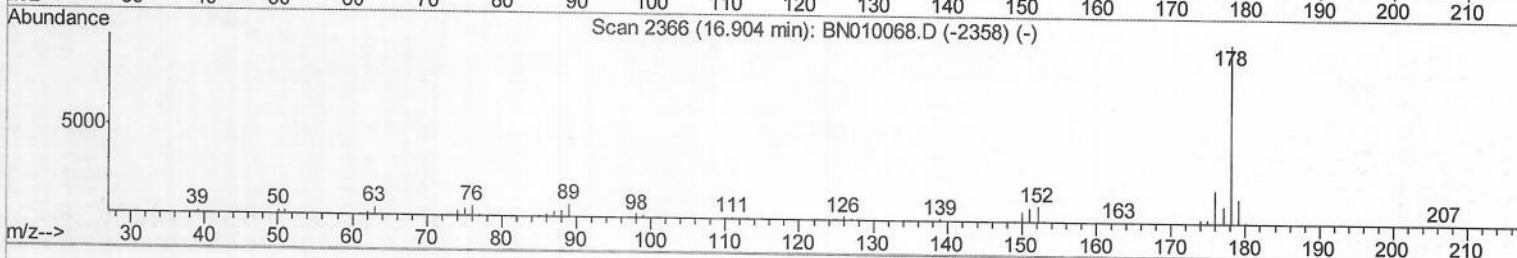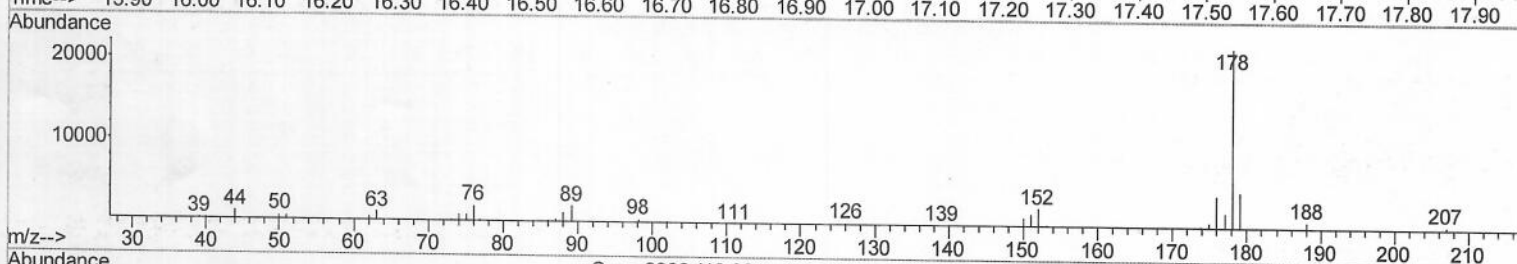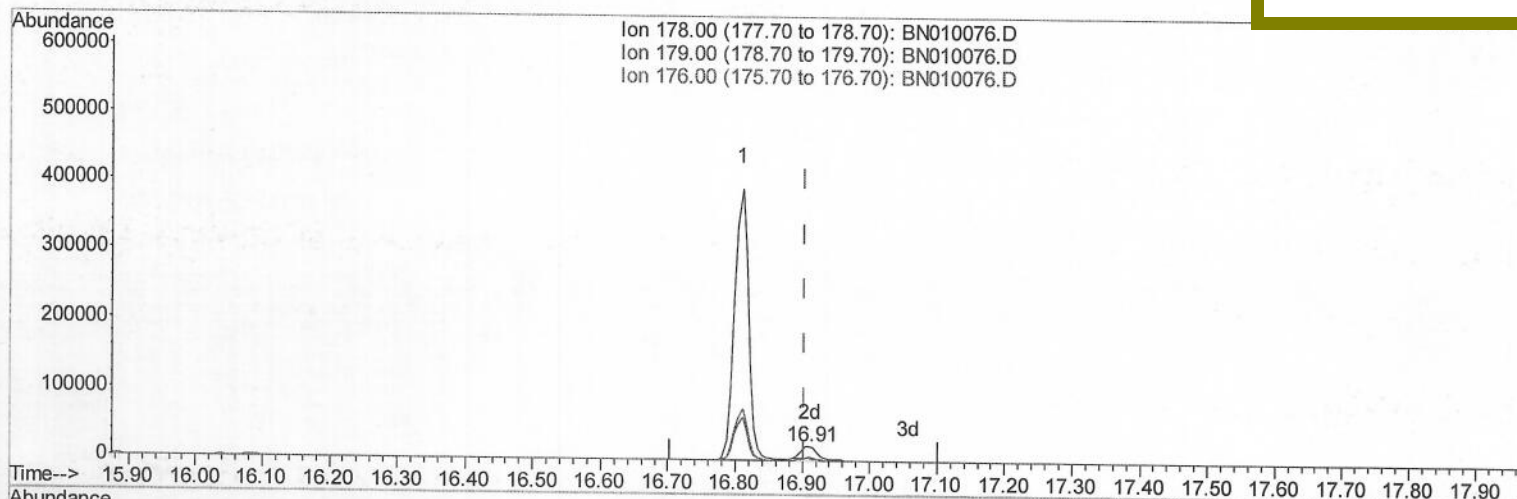

TIC: BN010076.D

(72) Anthracene

16.910min (+0.006) 1.77ng/ul m > JU 03/05/20

response 41366

Ion	Exp%	Act%
178.00	100	100
179.00	15.20	21.16#
176.00	18.20	19.27
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030320\
Quantitation Report (Qedit)




Data File : BN010076.D
Acq On : 03 Mar 2020 23:58
Operator : CG/JU
Sample : L1619-06DL 50X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Mar 04 01:33:14 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 04 01:30:16 2020
Response via : Initial Calibration

Instrument :
BNA_N
Client Sampled :
DBDW0DL

Manual Integrations
APPROVED

mohammad
3/4/2020 7:52:16 AM

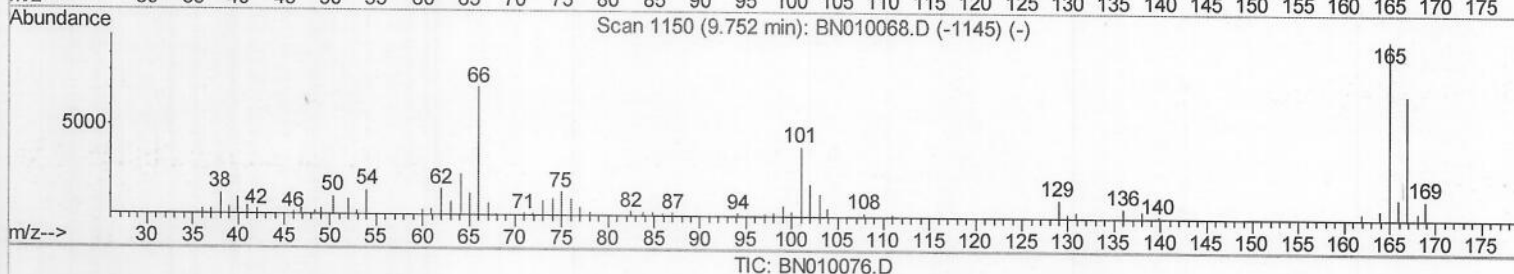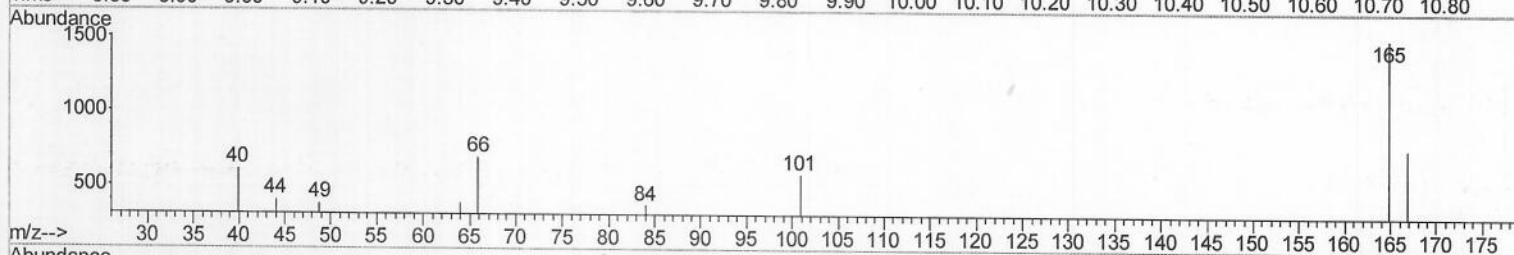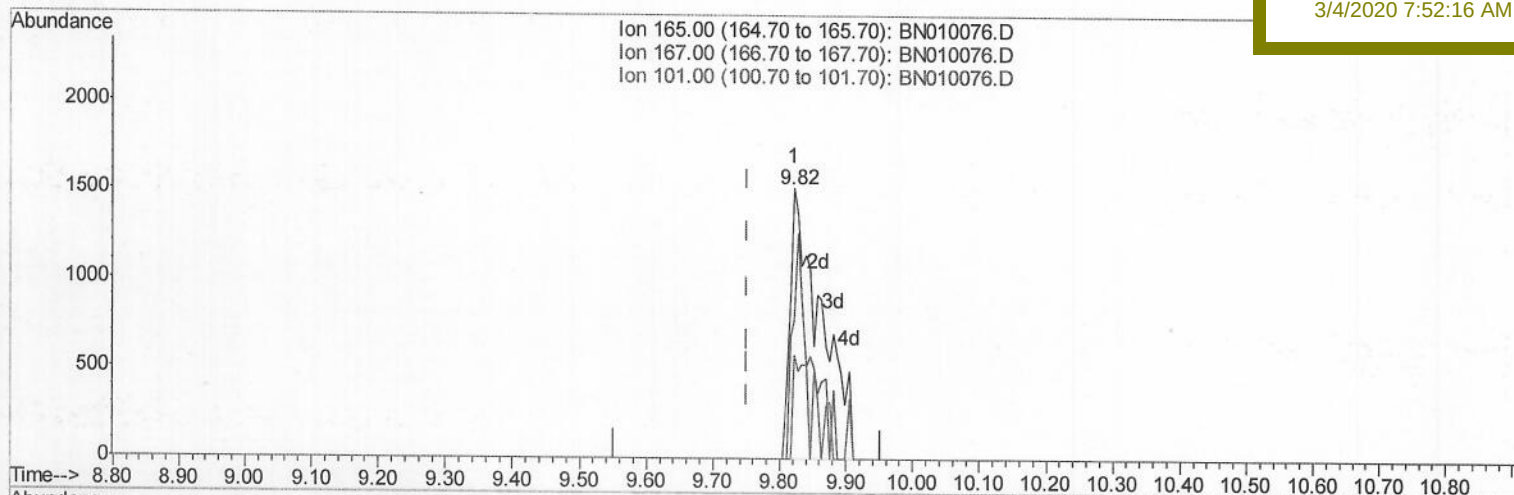

(26) 2,4-Dichlorophenol-d3 (S)

9.822min (+0.071) 1.44ng/ul m

7 JU03/05/20

response 4788

Ion	Exp%	Act%
165.00	100	100
167.00	64.20	50.93#
101.00	36.10	38.43
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030320\
Quantitation Report (Qedit)




Data File : BN010076.D
Acq On : 03 Mar 2020 23:58
Operator : CG/JU
Sample : L1619-06DL 50X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Mar 04 01:33:14 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 04 01:30:16 2020
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
DBDW0DL

Manual Integrations
APPROVED

mohammad
3/4/2020 7:52:16 AM

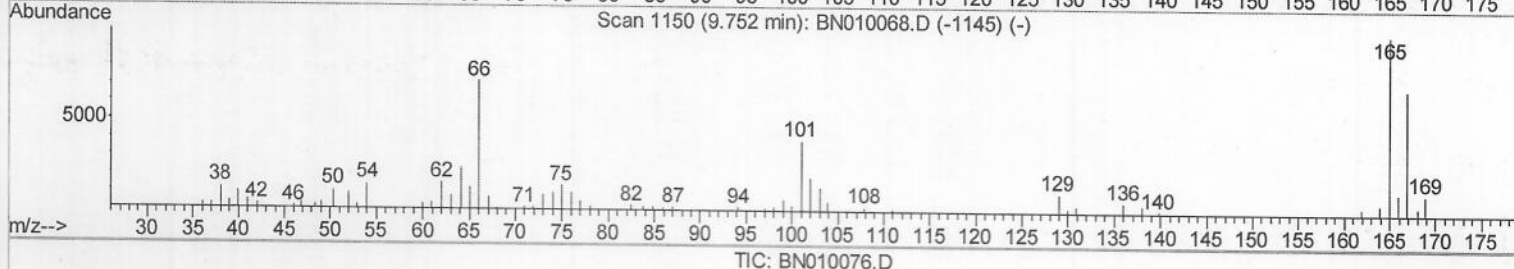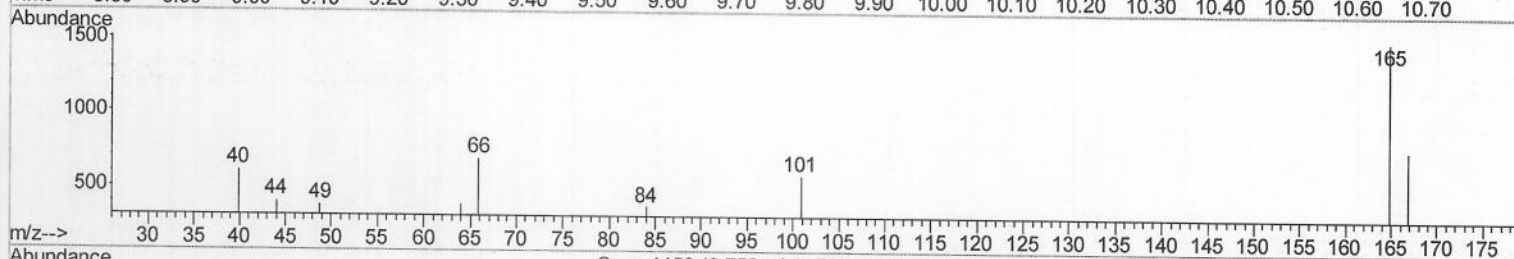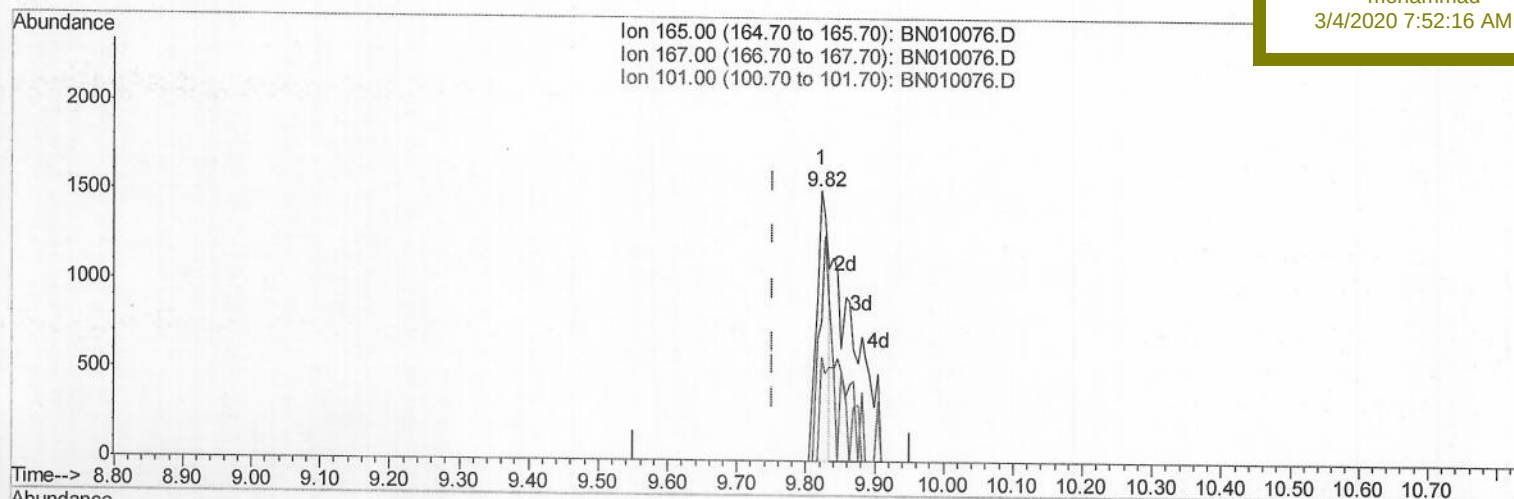

(26) 2,4-Dichlorophenol-d3 (S)

9.822min (+0.071) 0.56ng/ul

response 1857

Ion	Exp%	Act%
165.00	100	100
167.00	64.20	50.93#
101.00	36.10	38.43
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030320\
Quantitation Report (Qedit)




Data File : BN010076.D
Acq On : 03 Mar 2020 23:58
Operator : CG/JU
Sample : L1619-06DL 50X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Mar 04 01:33:14 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 04 01:30:16 2020
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
DBDW0DL

Manual Integrations
APPROVED

mohammad
3/4/2020 7:52:16 AM

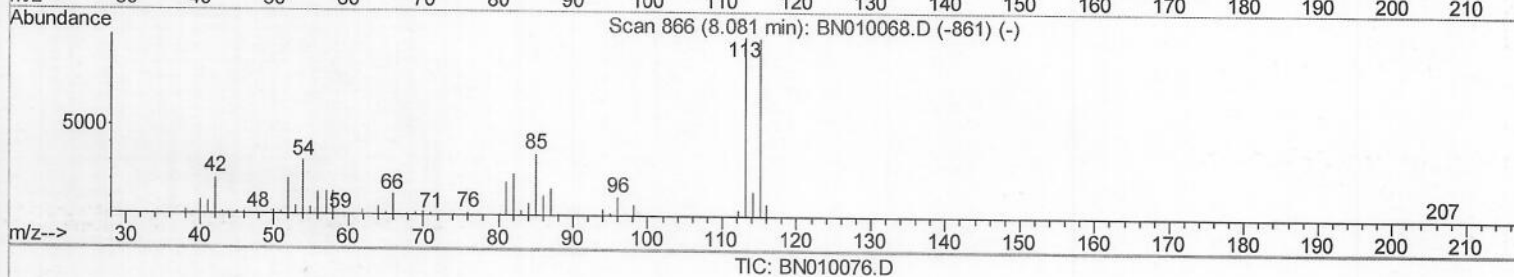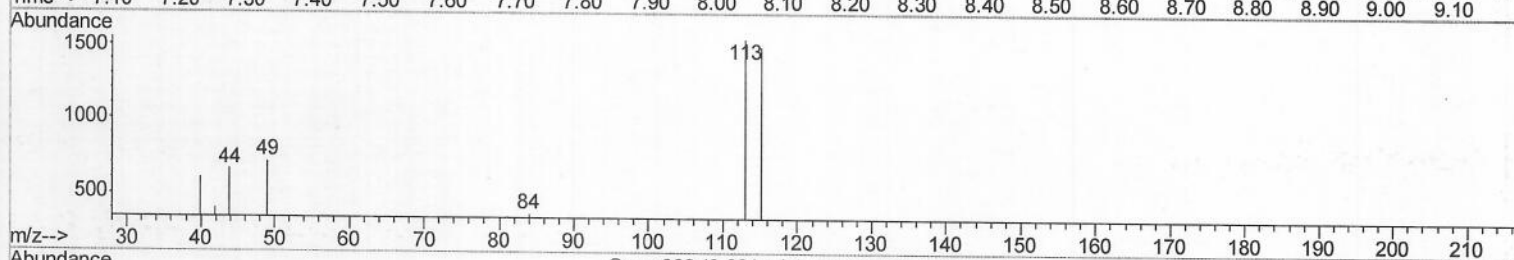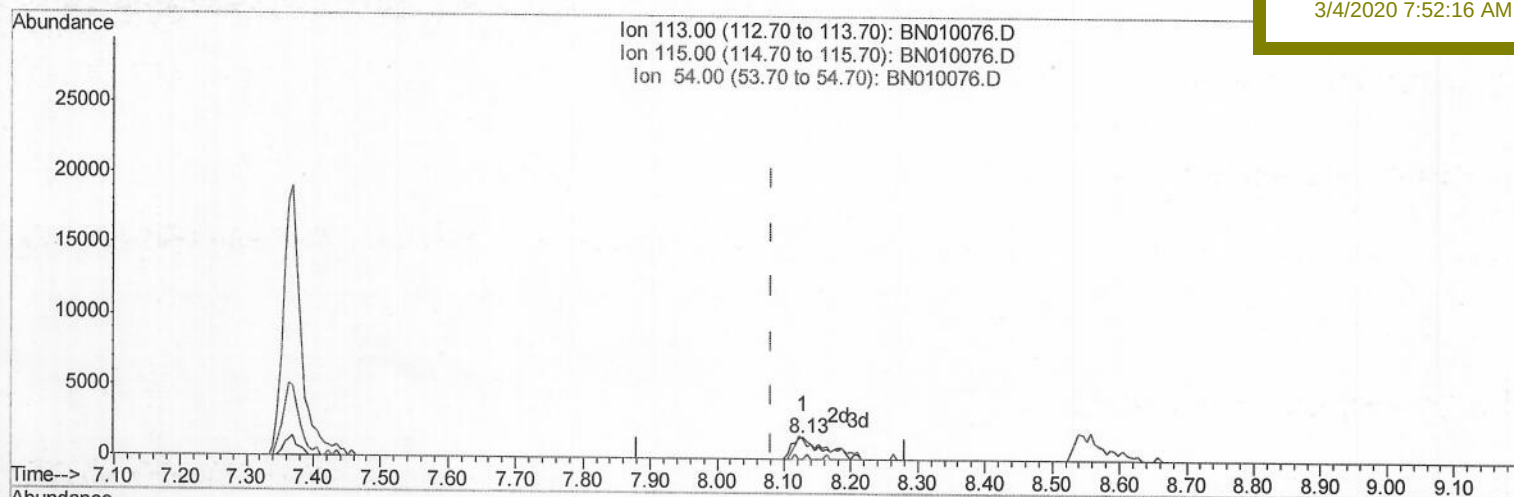

TIC: BN010076.D

(13) 4-Methylphenol-d8 (S)

8.128min (+0.047) 1.22ng/ul m

JU 03/05/20

response 4841

Ion	Exp%	Act%
113.00	100	100
115.00	90.70	96.77
54.00	21.20	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030320\
Quantitation Report (Qedit)




Data File : BN010076.D
Acq On : 03 Mar 2020 23:58
Operator : CG/JU
Sample : L1619-06DL 50X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Mar 04 01:33:14 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 04 01:30:16 2020
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
DBDW0DL

Manual Integrations
APPROVED

mohammad
3/4/2020 7:52:16 AM

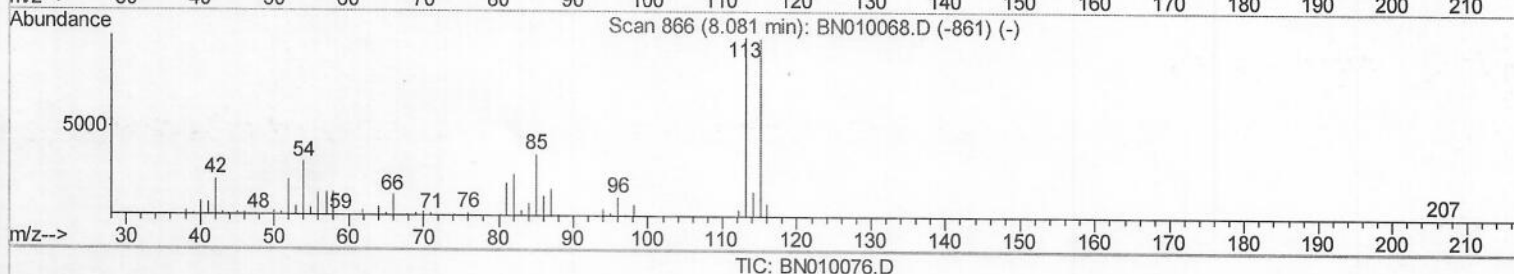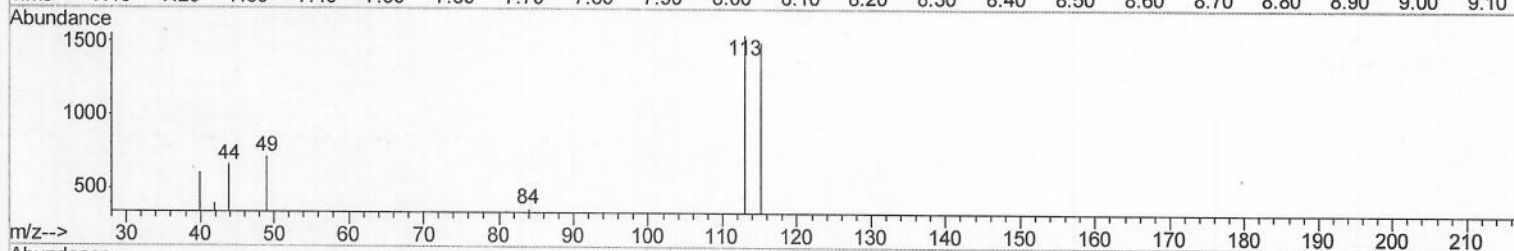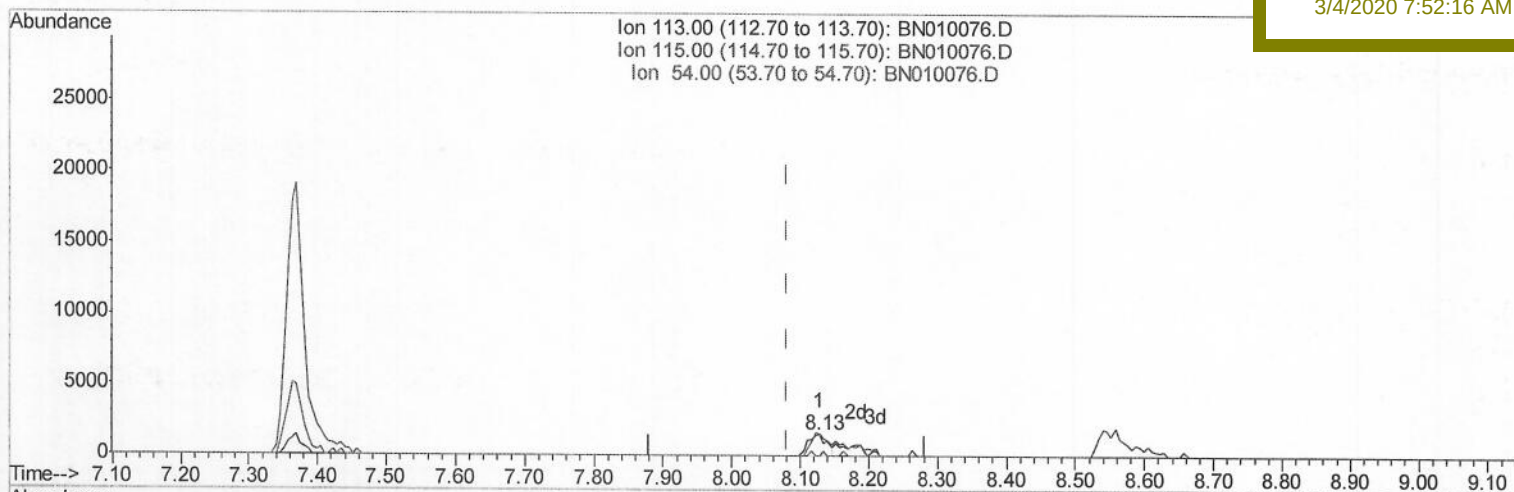

TIC: BN010076.D

(13) 4-Methylphenol-d8 (S)

8.128min (+0.047) 0.75ng/ul

response 2992

Ion	Exp%	Act%
113.00	100	100
115.00	90.70	96.77
54.00	21.20	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030320\
Quantitation Report (Qedit)




Data File : BN010076.D
Acq On : 03 Mar 2020 23:58
Operator : CG/JU
Sample : L1619-06DL 50X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Mar 04 01:33:14 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 04 01:30:16 2020
Response via : Initial Calibration

Instrument :
BNA_N
Client Sampled :
DBDW0DL

Manual Integrations
APPROVED

mohammad
3/4/2020 7:52:16 AM

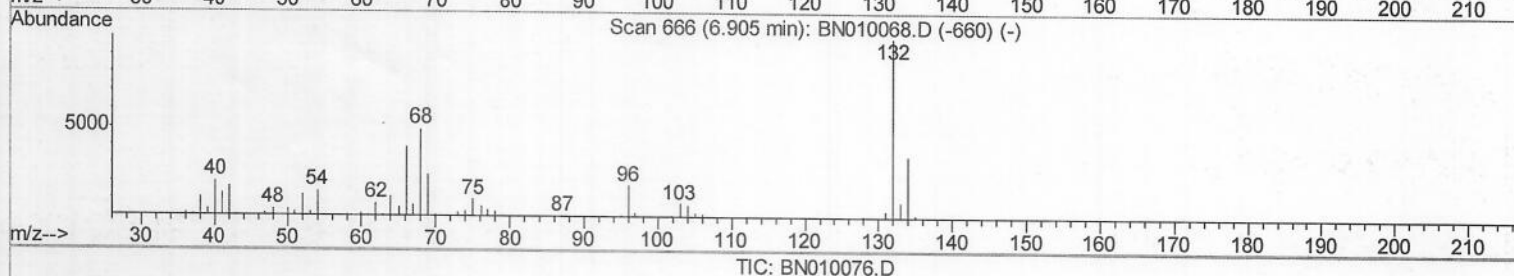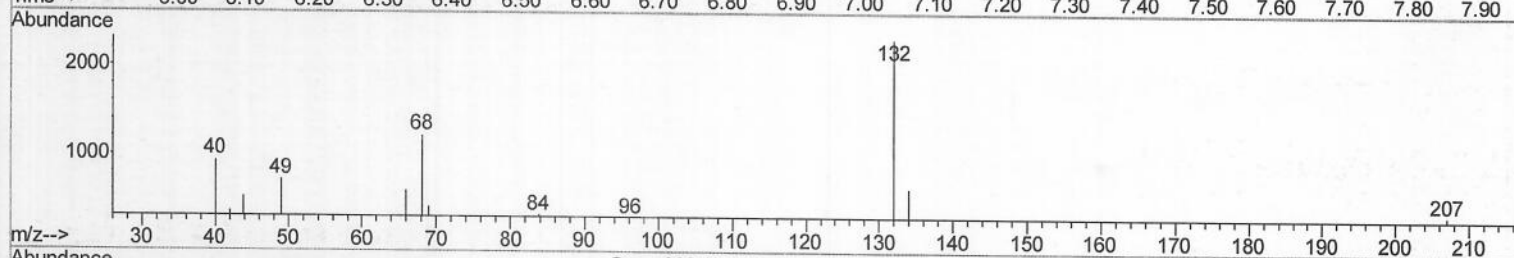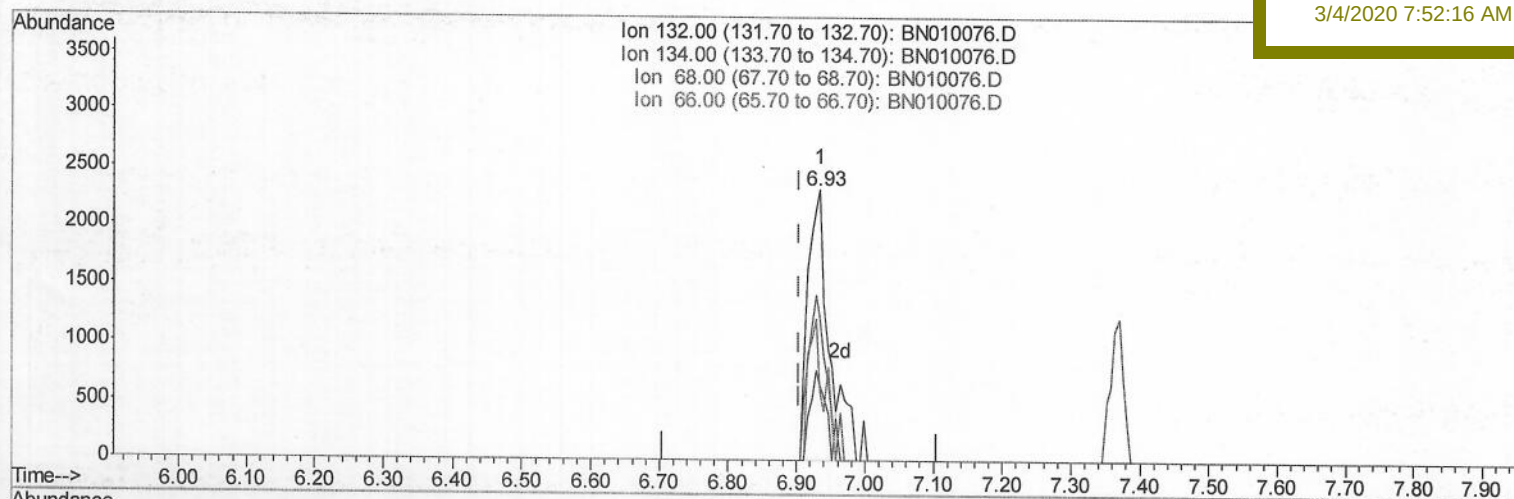

TIC: BN010076.D

(9) 2-Chlorophenol-d4 (S)

6.934min (+0.029) 1.16ng/ul

response 4367

Ion	Exp%	Act%
132.00	100	100
134.00	32.10	27.52
68.00	48.60	52.85
66.00	37.30	26.06#

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030320\
Quantitation Report (Qedit)




Data File : BN010076.D
Acq On : 03 Mar 2020 23:58
Operator : CG/JU
Sample : L1619-06DL 50X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Mar 04 01:33:14 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 04 01:30:16 2020
Response via : Initial Calibration

Instrument :
BNA_N
Client Sampled :
DBDW0DL

Manual Integrations
APPROVED

mohammad
3/4/2020 7:52:16 AM

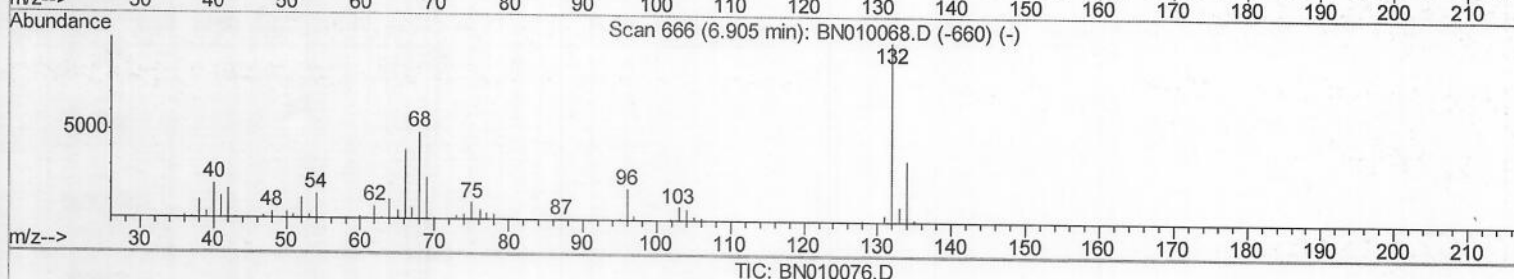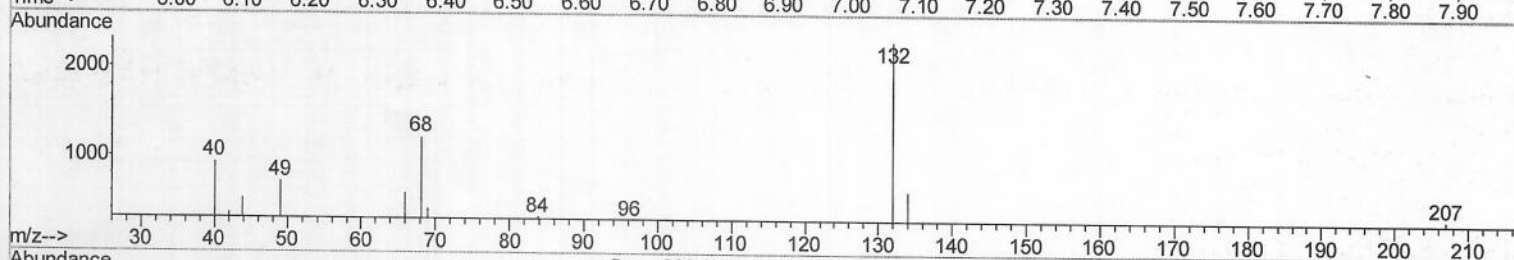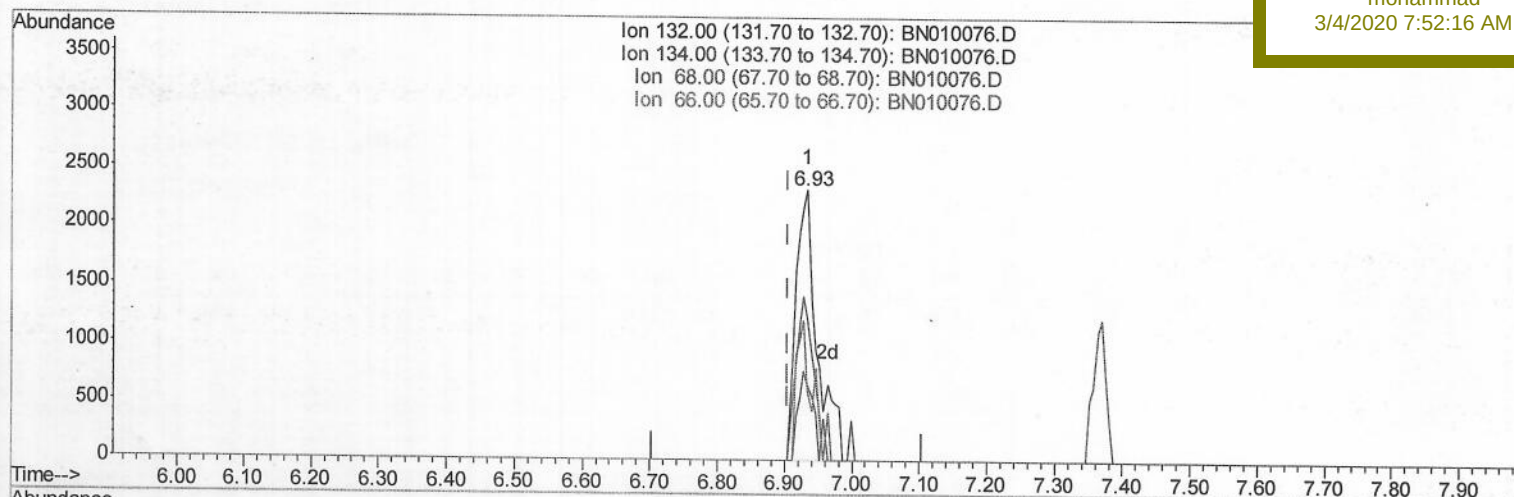

(9) 2-Chlorophenol-d4 (S)

6.934min (+0.029) 1.36ng/ul m

response 5119

Ion	Exp%	Act%
132.00	100	100
134.00	32.10	27.52
68.00	48.60	52.85
66.00	37.30	26.06#

25009/05/20

Data File : BN010076.D

Acq On : 03 Mar 2020 23:58

Operator : CG/JU

Sample : L1619-06DL 5X

Misc :

ALS Vial : 20 Sample Multiplier: 1

Quant Time: Mar 04 02:50:56 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Wed Mar 04 01:30:16 2020

Response via : Initial Calibration

Instrument :

BNA_N

Client Sampled :

DBDW0DL

Manual Integrations

APPROVED

mohammad

3/4/2020 7:52:16 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.37	152	58685	20.00	ng/ul	0.01
18) Naphthalene-d8	10.11	136	216630	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.00	164	190243	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.76	188	400869	20.00	ng/ul	0.00
78) Chrysene-d12	20.99	240	387518	20.00	ng/ul	0.00
86) Perylene-d12	23.08	264	423890	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.03	96	278	0.19	ng/uL	0.02
5) Phenol-d5	6.61	99	5998m	1.20	ng/ul	0.04
7) Bis-(2-Chloroethyl) ether-d	6.75	67	5037m	1.46	ng/ul	0.02
9) 2-Chlorophenol-d4	6.93	132	5119m	1.36	ng/ul	0.03
13) 4-Methylphenol-d8	8.13	113	4841m	1.22	ng/ul	0.05
19) Nitrobenzene-d5	8.55	128	1559m	0.98	ng/ul	0.04
22) 2-Nitrophenol-d4	9.26	143	1812m	1.05	ng/ul	0.04
26) 2,4-Dichlorophenol-d3	9.82	165	4788m	1.44	ng/ul	0.07
29) 4-Chloroaniline-d4	10.33	131	5832m	1.56	ng/ul	0.06
44) Dimethylphthalate-d6	13.45	166	25743	1.81	ng/ul	0.01
47) Acenaphthylene-d8	13.70	160	27492	1.64	ng/ul	0.00
52) 4-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
58) Fluorene-d10	15.02	176	24218	1.97	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	0.00	200	0	0.00	ng/ul	
71) Anthracene-d10	16.87	188	37704	2.05	ng/ul	0.00
79) Pyrene-d10	19.17	212	41572	2.05	ng/ul	0.00
90) Benzo(a)pyrene-d12	22.95	264	40556	1.92	ng/ul	0.00

Target Compounds

					Qvalue	
34) 2-Methylnaphthalene	11.80	142	37052	4.568	ng/ul	98
41) 1,1'-Biphenyl	12.83	154	24218	1.657	ng/ul#	91
50) Acenaphthene	14.07	153	144244	11.616	ng/ul	97
54) Dibenzofuran	14.42	168	144583	8.295	ng/ul	99
59) Fluorene	15.07	166	127978	8.749	ng/ul	98
70) Phenanthrene	16.81	178	570124	24.921	ng/ul	99
72) Anthracene	16.91	178	41366m	1.769	ng/ul	
77) Fluoranthene	18.84	202	334169	12.470	ng/ul	95
80) Pyrene	19.20	202	222222	7.954	ng/ul	95
83) Benzo(a)anthracene	20.97	228	42311	1.589	ng/ul	93
85) Chrysene	21.03	228	33556	1.280	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed