

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN030320\
 Data File : BN010045.D
 Acq On : 02 Mar 2020 18:14
 Operator : CG/JU
 Sample : PB127031BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK31

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.017	3	5	12	rVB2	28954	37124	1.71%	0.157%
2	3.187	32	34	36	rBV3	2036	2276	0.10%	0.010%
3	3.211	36	38	41	rVB4	3863	2816	0.13%	0.012%
4	3.387	66	68	71	rBV3	2268	2703	0.12%	0.011%
5	3.517	87	90	93	rBV3	2105	2776	0.13%	0.012%
6	3.693	119	120	126	rVB4	4489	5355	0.25%	0.023%
7	4.146	192	197	199	rVB4	2613	3687	0.17%	0.016%
8	5.440	414	417	421	rVB5	1663	2226	0.10%	0.009%
9	6.140	532	536	540	rVV2	2230	3446	0.16%	0.015%
10	6.575	602	610	624	rBV	399189	716968	33.07%	3.035%
11	6.669	624	626	631	rVV5	4032	5737	0.26%	0.024%
12	6.728	631	636	650	rVV	296815	481420	22.20%	2.038%
13	6.911	661	667	681	rVB	432996	692222	31.93%	2.930%
14	7.305	729	734	736	rBV2	1353	2521	0.12%	0.011%
15	7.369	738	745	757	rVV	299811	502217	23.16%	2.126%
16	8.087	861	867	884	rBV	460613	806024	37.18%	3.412%
17	8.516	932	940	955	rBV	401160	720329	33.22%	3.049%
18	8.610	955	956	962	rVV3	3899	5257	0.24%	0.022%
19	9.228	1054	1061	1078	rBV	331463	607858	28.04%	2.573%
20	9.763	1144	1152	1171	rBV	393611	790702	36.47%	3.347%
21	10.110	1205	1211	1220	rBV	419356	703504	32.45%	2.978%
22	10.275	1231	1239	1256	rBV	371169	854997	39.44%	3.620%
23	10.410	1260	1262	1267	rVB2	3345	3943	0.18%	0.017%
24	11.763	1486	1492	1498	rBV4	3904	8231	0.38%	0.035%
25	13.281	1744	1750	1753	rVB4	1306	2364	0.11%	0.010%
26	13.440	1771	1777	1790	rBV	820784	1276053	58.86%	5.402%
27	13.693	1814	1820	1834	rBV	908745	1413090	65.18%	5.982%
28	14.010	1867	1874	1883	rBV	631887	957178	44.15%	4.052%
29	14.275	1913	1919	1935	rBV	219968	559389	25.80%	2.368%
30	14.434	1944	1946	1949	rVB2	3422	3084	0.14%	0.013%
31	15.016	2039	2045	2056	rBV	1208518	1767622	81.53%	7.483%
32	15.181	2068	2073	2083	rBV	318457	563439	25.99%	2.385%
33	15.251	2083	2085	2092	rVV4	22296	42911	1.98%	0.182%
34	15.298	2092	2093	2097	rVB4	3271	2431	0.11%	0.010%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030320\
 Data File : BN010045.D
 Acq On : 02 Mar 2020 18:14
 Operator : CG/JU
 Sample : PB127031BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK31

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Title : SVOA CALIBRATION

35	15.404	2110	2111	2117	rVB2	2296	2880	0.13%	0.012%
36	15.804	2174	2179	2183	rBV3	3437	5136	0.24%	0.022%
37	16.769	2337	2343	2353	rBV	847555	1128117	52.03%	4.776%
38	16.869	2353	2360	2377	rVV	1286399	1899617	87.62%	8.042%
39	17.757	2506	2511	2517	rBV2	27814	47464	2.19%	0.201%
40	18.092	2566	2568	2574	rBV5	2058	3226	0.15%	0.014%
41	18.251	2591	2595	2596	rVB	2190	2483	0.11%	0.011%
42	18.775	2679	2684	2688	rVV5	6332	11399	0.53%	0.048%
43	18.816	2688	2691	2695	rVV2	12234	18629	0.86%	0.079%
44	18.863	2697	2699	2703	rVB3	2220	2903	0.13%	0.012%
45	18.910	2703	2707	2709	rBV4	3649	5149	0.24%	0.022%
46	19.063	2729	2733	2737	rVB	8555	11627	0.54%	0.049%
47	19.175	2744	2752	2767	rBV2	1467676	2168073	100.00%	9.178%
48	19.951	2881	2884	2885	rVB2	5722	4422	0.20%	0.019%
49	20.686	3004	3009	3012	rBV	30875	47796	2.20%	0.202%
50	20.739	3014	3018	3022	rVV	48493	67998	3.14%	0.288%
51	20.792	3023	3027	3034	rVV	103277	153487	7.08%	0.650%
52	20.992	3055	3061	3069	rBV	895427	1226605	56.58%	5.193%
53	22.951	3388	3394	3410	rVB	1151028	2065447	95.27%	8.744%
54	23.080	3410	3416	3427	rBV	673106	1197400	55.23%	5.069%


Sum of corrected areas: 23621758

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN030320\
Data File : BN010045.D
Acq On : 02 Mar 2020 18:14
Operator : CG/JU
Sample : PB127031BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK31

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

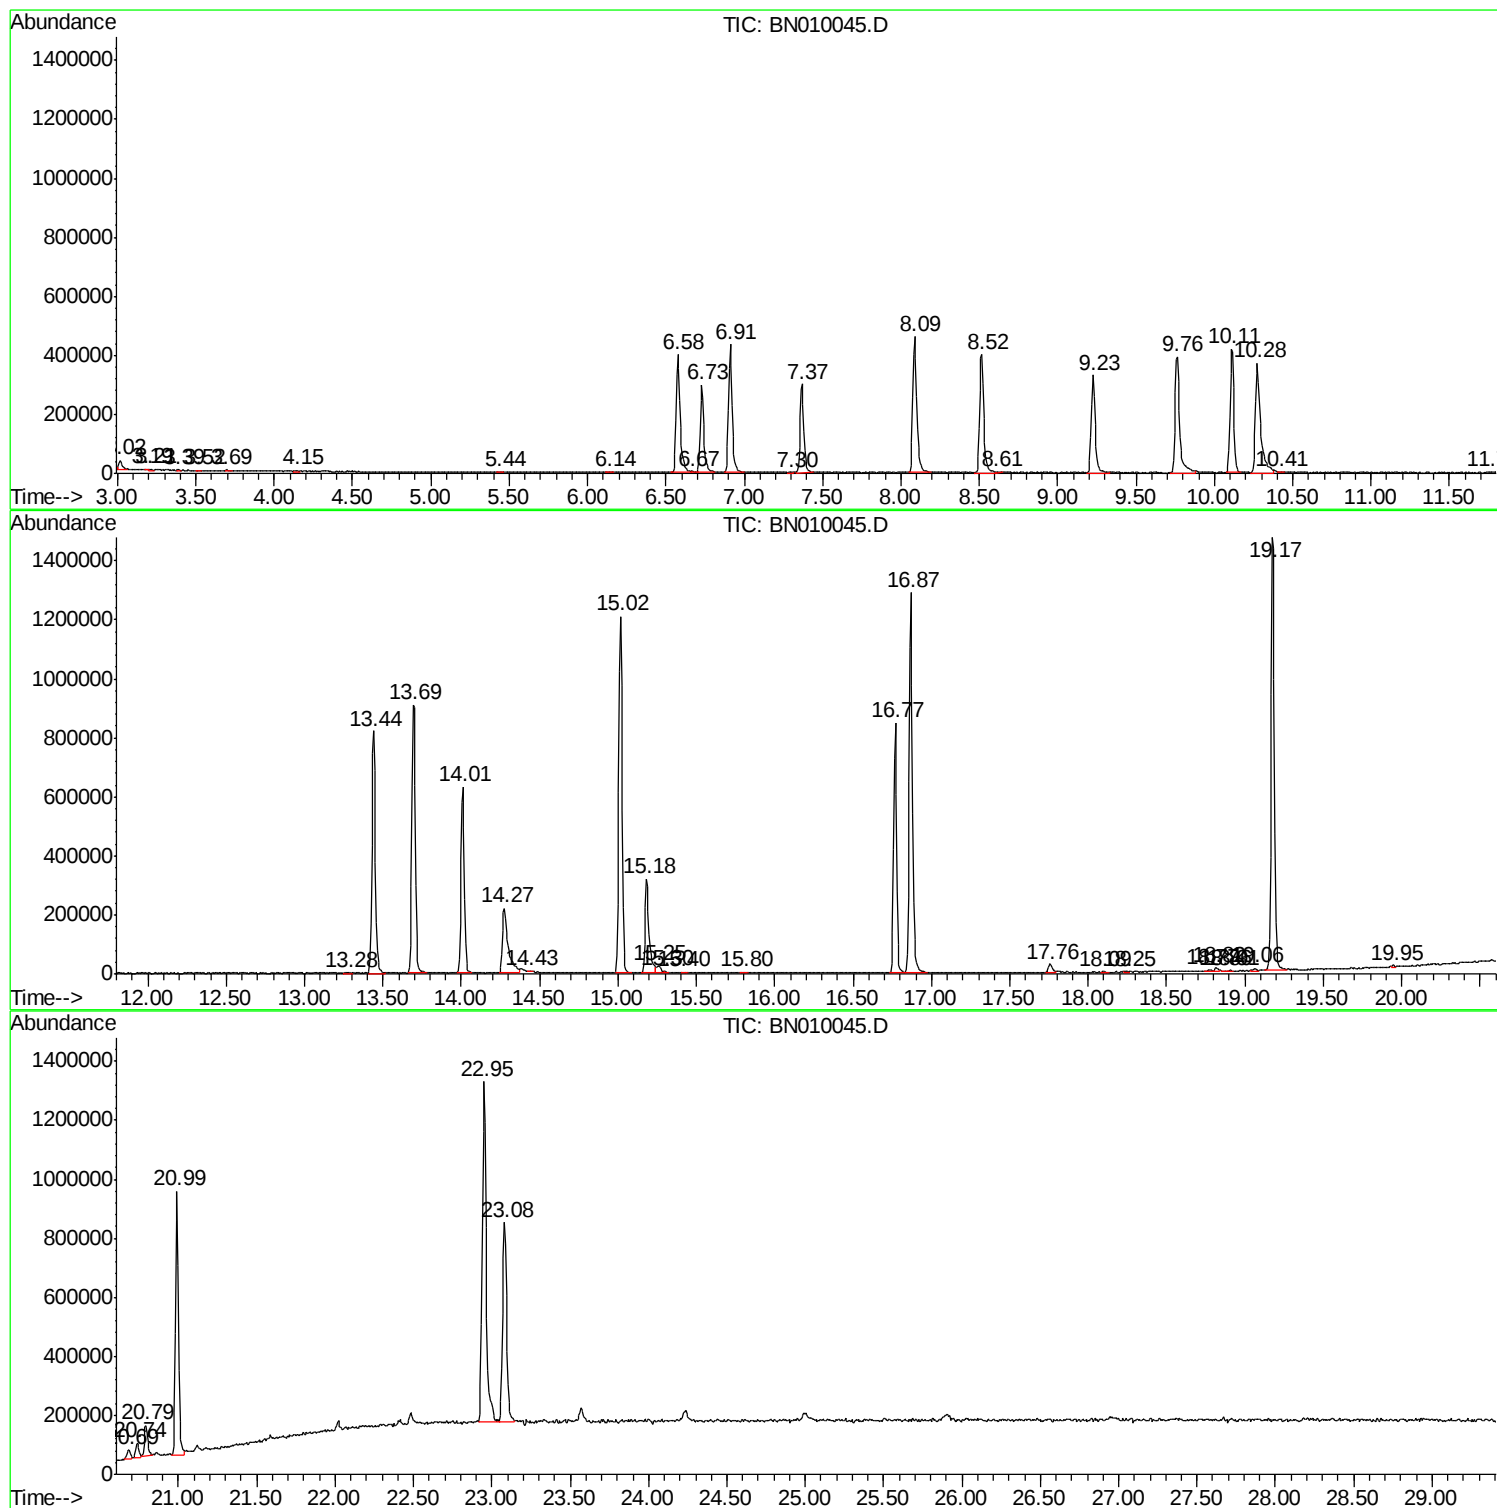

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN030320\
Data File : BN010045.D
Acq On : 02 Mar 2020 18:14
Operator : CG/JU
Sample : PB127031BL
Misc :
ALS Vial : 3 Sample Multiplier: 1










Instrument :
BNA_N
ClientSampleId :
SBLK31

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Diethylene glycol dibenzoate Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.		
20.79	2.50 ng/ul	153487	Chrysene-d12	20.99		
Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1		Diethylene glycol dibenzoate	314	C18H18O5	000120-55-8	78
2		2,2'-(Ethane-1,2-diylbis(oxv))bi...	358	C20H22O6	1000366-99-4	53
3		1-Propanone, 3-hydroxy-1-phenyl-	150	C9H10O2	005650-41-9	49
4		Vinyl benzoate	148	C9H8O2	000769-78-8	46
5		Pyrazine-2-carboxylic acid, 4,5-...	301	C15H15N3O4	1000259-49-5	43

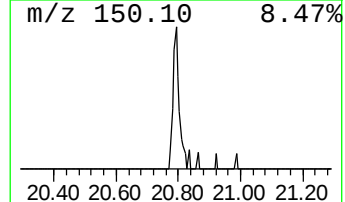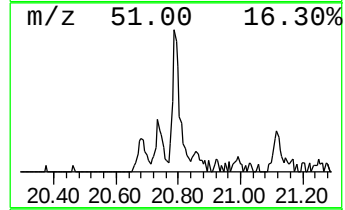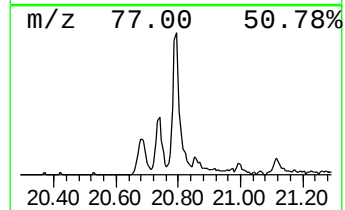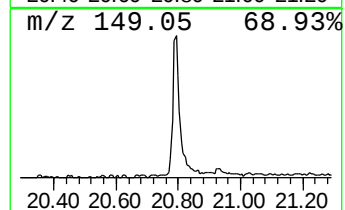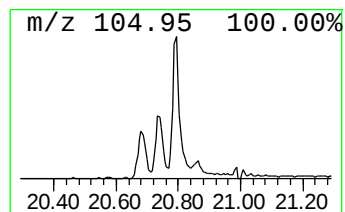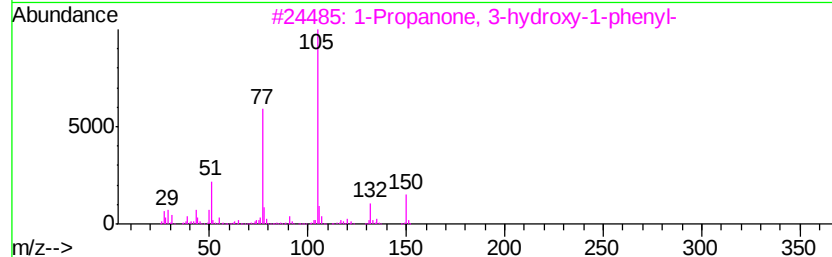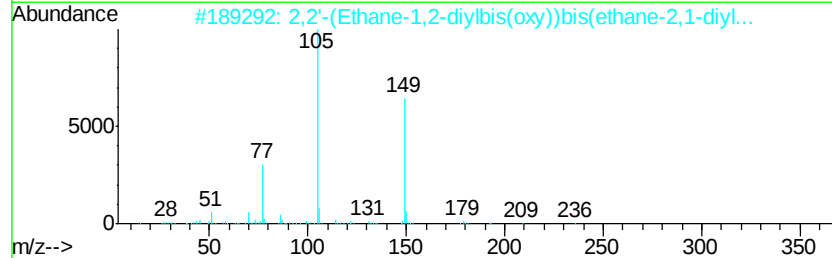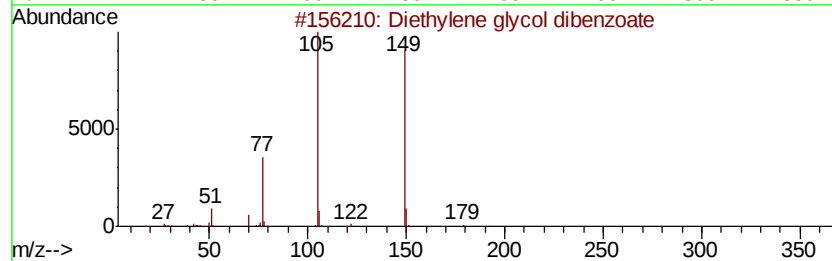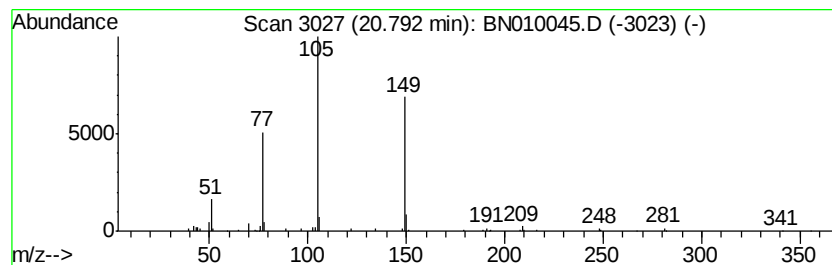

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030320\
Data File : BN010045.D
Acq On : 02 Mar 2020 18:14
Operator : CG/JU
Sample : PB127031BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK31

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Diethylene glycol...	20.79	2.5	ng/ul	153487	5	20.99	1226610	20.0