

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN030320\
 Data File : BN010067.D
 Acq On : 03 Mar 2020 18:22
 Operator : CG/JU
 Sample : PB127065BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK65

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.017	3	5	14	rVB	31119	43233	3.31%	0.292%
2	3.699	118	121	123	rVB3	2673	2537	0.19%	0.017%
3	3.805	138	139	141	rBV2	2040	1363	0.10%	0.009%
4	4.164	198	200	205	rVV4	2047	2412	0.18%	0.016%
5	4.481	252	254	258	rVB2	1107	1377	0.11%	0.009%
6	4.834	311	314	315	rBV3	1385	1548	0.12%	0.010%
7	4.946	331	333	336	rBV	1170	1413	0.11%	0.010%
8	4.981	338	339	342	rBV3	1458	1319	0.10%	0.009%
9	5.117	360	362	364	rVV2	2072	1331	0.10%	0.009%
10	5.140	364	366	368	rVB	1642	1431	0.11%	0.010%
11	5.223	377	380	382	rVB2	1521	1900	0.15%	0.013%
12	5.246	382	384	386	rBV2	1420	1488	0.11%	0.010%
13	5.293	390	392	394	rVB2	1633	1431	0.11%	0.010%
14	5.323	394	397	400	rBV2	1674	2279	0.17%	0.015%
15	5.452	416	419	422	rBV	1692	2535	0.19%	0.017%
16	5.793	473	477	478	rVB	1253	1369	0.10%	0.009%
17	5.858	486	488	491	rVB2	1480	1311	0.10%	0.009%
18	5.905	491	496	498	rVB2	1070	1410	0.11%	0.010%
19	5.946	502	503	507	rBV	1459	1309	0.10%	0.009%
20	6.046	517	520	525	rBV	986	1864	0.14%	0.013%
21	6.181	541	543	546	rBV2	1236	1351	0.10%	0.009%
22	6.358	571	573	577	rVB3	1832	1938	0.15%	0.013%
23	6.569	604	609	627	rBV	279626	469794	35.95%	3.170%
24	6.722	628	635	648	rVV	187084	303748	23.24%	2.050%
25	6.905	660	666	675	rBV	289965	460758	35.26%	3.109%
26	7.364	738	744	755	rVB	201105	328303	25.12%	2.216%
27	7.840	822	825	832	rVB3	893	1598	0.12%	0.011%
28	8.081	860	866	880	rVV	323869	542363	41.50%	3.660%
29	8.193	883	885	887	rVV2	1780	1549	0.12%	0.010%
30	8.211	887	888	890	rVV	1812	1417	0.11%	0.010%
31	8.440	922	927	928	rBV	1130	1495	0.11%	0.010%
32	8.511	933	939	953	rVV	271448	481883	36.87%	3.252%
33	8.605	953	955	957	rVV2	2161	2080	0.16%	0.014%
34	8.628	957	959	961	rVB2	2062	1691	0.13%	0.011%

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN030320\
 Data File : BN010067.D
 Acq On : 03 Mar 2020 18:22
 Operator : CG/JU
 Sample : PB127065BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK65

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Title : SVOA CALIBRATION

35	8.875	999	1001	1006	rBV3	1177	1909	0.15%	0.013%
36	8.916	1006	1008	1010	rVB	1558	1381	0.11%	0.009%
37	8.946	1010	1013	1017	rBV3	1707	2736	0.21%	0.018%
38	9.040	1027	1029	1032	rVB2	1241	1382	0.11%	0.009%
39	9.222	1053	1060	1074	rBV	230309	402481	30.80%	2.716%
40	9.758	1145	1151	1166	rBV	267384	534916	40.93%	3.610%
41	9.911	1176	1177	1183	rVB3	1845	1812	0.14%	0.012%
42	10.105	1204	1210	1222	rBV	279755	463680	35.48%	3.129%
43	10.269	1231	1238	1258	rBV	250329	564034	43.16%	3.806%
44	11.457	1439	1440	1446	rBV	1336	2002	0.15%	0.014%
45	11.757	1487	1491	1498	rVB3	1843	3599	0.28%	0.024%
46	12.910	1684	1687	1690	rVB	1101	1431	0.11%	0.010%
47	13.434	1770	1776	1789	rBV	517184	813729	62.27%	5.491%
48	13.693	1814	1820	1832	rVV	632663	900618	68.92%	6.078%
49	14.004	1866	1873	1885	rVB2	421795	606663	46.42%	4.094%
50	14.275	1913	1919	1933	rBV	133459	346715	26.53%	2.340%
51	14.481	1952	1954	1957	rBV2	2082	2166	0.17%	0.015%
52	15.010	2038	2044	2055	rBV	747871	1116838	85.46%	7.537%
53	15.181	2069	2073	2084	rBV	150648	283362	21.68%	1.912%
54	15.257	2084	2086	2090	rVV3	13296	16675	1.28%	0.113%
55	15.304	2092	2094	2095	rVB	2277	1509	0.12%	0.010%
56	15.569	2135	2139	2142	rVB	1715	1391	0.11%	0.009%
57	15.922	2196	2199	2203	rVB3	846	1395	0.11%	0.009%
58	16.563	2304	2308	2312	rVB3	1367	2128	0.16%	0.014%
59	16.769	2337	2343	2353	rBV	483551	700785	53.62%	4.729%
60	16.869	2354	2360	2371	rBV	772719	1159465	88.72%	7.825%
61	17.222	2419	2420	2426	rVB3	1295	1413	0.11%	0.010%
62	17.351	2438	2442	2445	rBV2	1131	1444	0.11%	0.010%
63	17.540	2470	2474	2475	rBV3	1494	1757	0.13%	0.012%
64	17.763	2511	2512	2515	rBV2	2327	2518	0.19%	0.017%
65	17.810	2518	2520	2522	rVV	1423	1434	0.11%	0.010%
66	18.092	2566	2568	2572	rVB3	1503	1639	0.13%	0.011%
67	18.475	2630	2633	2638	rVB3	1753	2780	0.21%	0.019%
68	18.745	2677	2679	2680	rVB2	2399	1511	0.12%	0.010%
69	18.757	2680	2681	2684	rBV2	2327	1987	0.15%	0.013%
70	18.792	2684	2687	2688	rVV	1848	1705	0.13%	0.012%
71	18.816	2688	2691	2695	rVV2	4935	6368	0.49%	0.043%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030320\
 Data File : BN010067.D
 Acq On : 03 Mar 2020 18:22
 Operator : CG/JU
 Sample : PB127065BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK65

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Title : SVOA CALIBRATION

72	18.904	2705	2706	2710	rBV2	2132	1880	0.14%	0.013%
73	19.063	2729	2733	2737	rBV3	4318	6189	0.47%	0.042%
74	19.181	2746	2753	2761	rBV	888354	1306828	100.00%	8.819%
75	19.339	2778	2780	2782	rBV2	2780	2385	0.18%	0.016%
76	19.363	2782	2784	2787	rVV3	1978	1642	0.13%	0.011%
77	19.457	2798	2800	2802	rBV2	1895	2015	0.15%	0.014%
78	19.522	2809	2811	2814	rVB5	2525	1821	0.14%	0.012%
79	19.551	2814	2816	2817	rBV2	1932	1903	0.15%	0.013%
80	19.710	2840	2843	2844	rBV3	1673	1556	0.12%	0.011%
81	19.745	2847	2849	2851	rVV3	2057	1739	0.13%	0.012%
82	20.075	2903	2905	2907	rBV3	1984	1775	0.14%	0.012%
83	20.157	2917	2919	2920	rBV2	3075	2206	0.17%	0.015%
84	20.204	2924	2927	2929	rVV3	3524	3568	0.27%	0.024%
85	20.310	2943	2945	2947	rVB3	3640	2714	0.21%	0.018%
86	20.445	2966	2968	2969	rBV	3085	2104	0.16%	0.014%
87	20.633	2998	3000	3001	rBV	5390	3504	0.27%	0.024%
88	20.686	3005	3009	3014	rVV3	14925	24522	1.88%	0.165%
89	20.739	3015	3018	3023	rVV	17249	26571	2.03%	0.179%
90	20.798	3024	3028	3034	rVV	47746	69862	5.35%	0.471%
91	20.992	3056	3061	3071	rBV2	512483	718117	54.95%	4.846%
92	21.122	3080	3083	3088	rVB4	15316	20784	1.59%	0.140%
93	22.957	3389	3395	3409	rBV	684363	1274129	97.50%	8.598%
94	23.086	3411	3417	3428	rVB	375669	706171	54.04%	4.766%


Sum of corrected areas: 14818171

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN030320\
Data File : BN010067.D
Acq On : 03 Mar 2020 18:22
Operator : CG/JU
Sample : PB127065BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK65

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

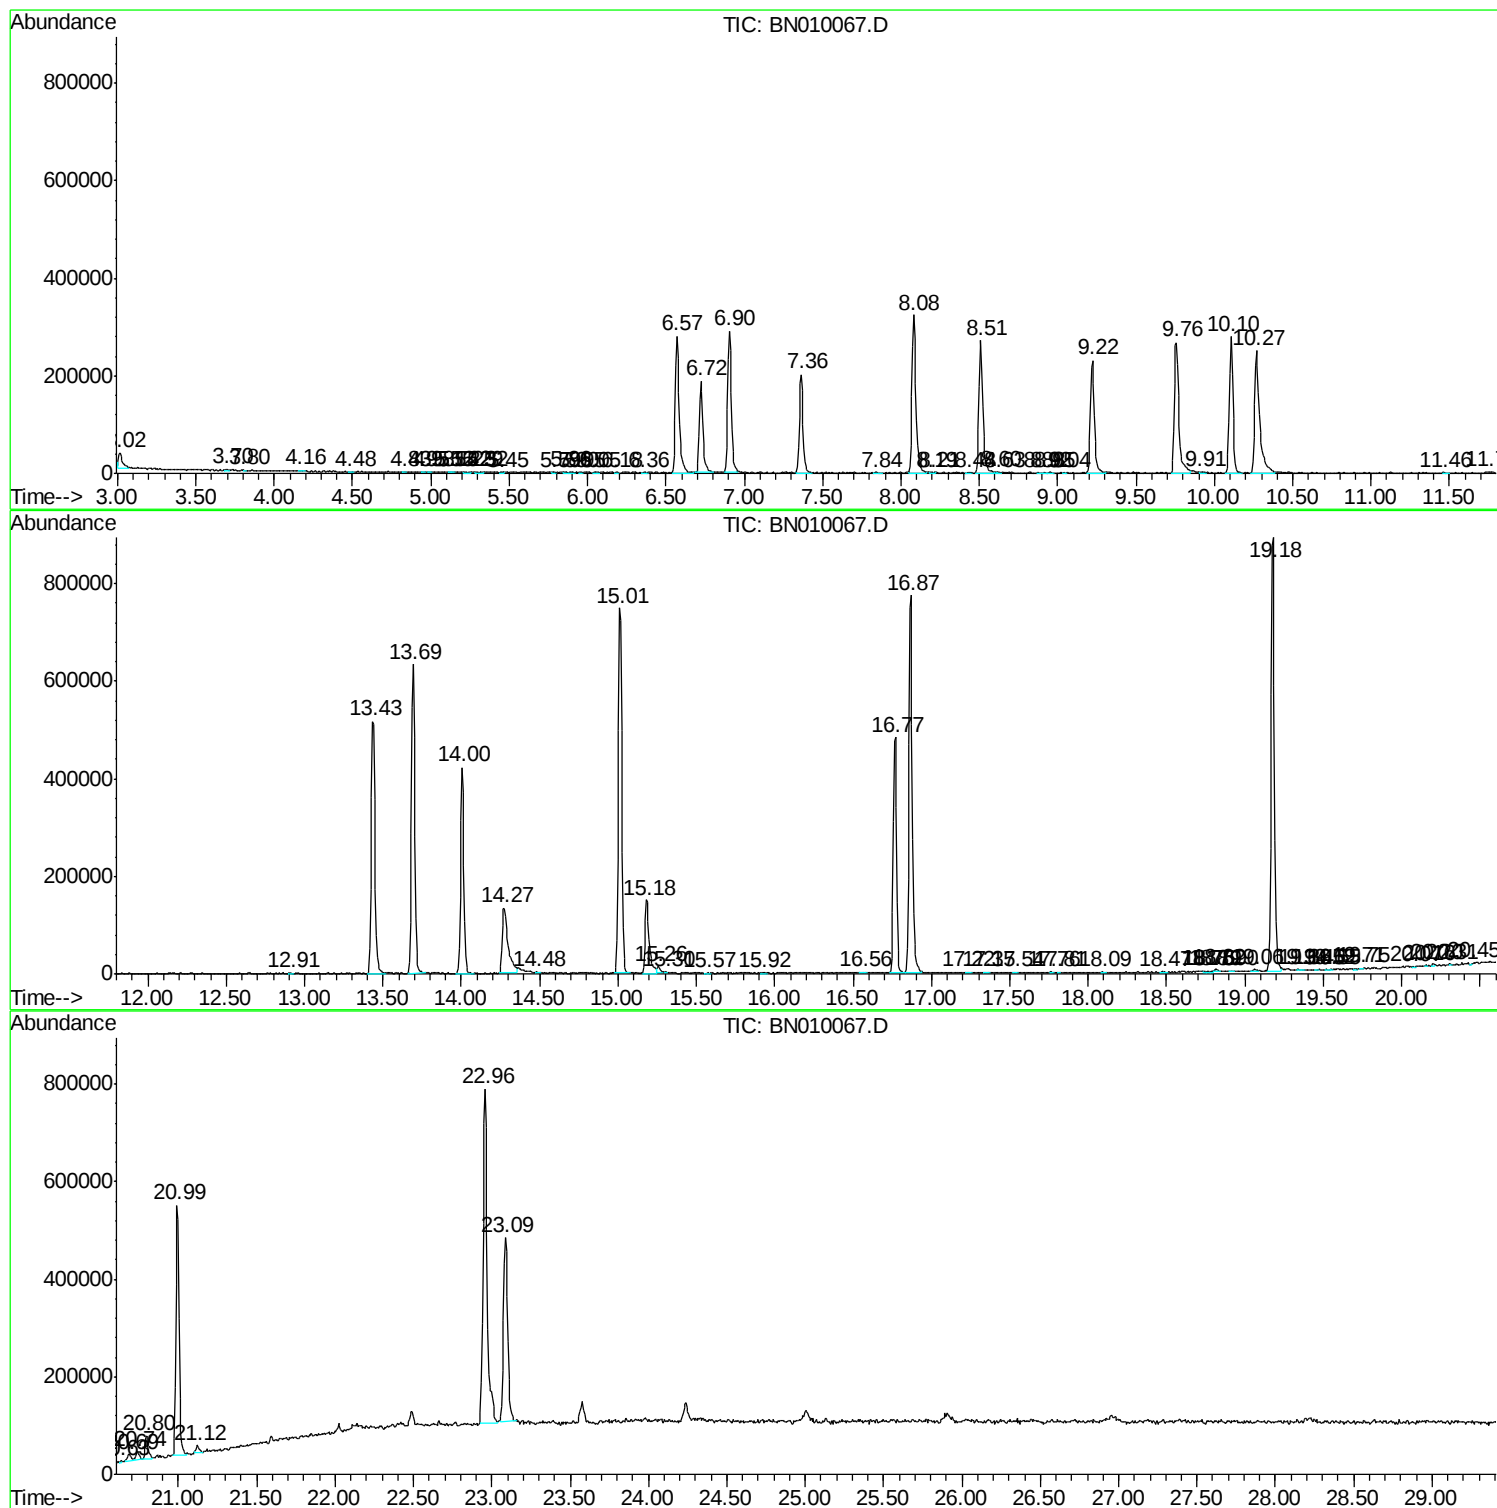

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030320\
Data_File : BN010067.D
Acq_On : 03-Mar-2020 18:222
Operator : CG/JUU
Sample : PB127065BLL
Misc :
ALS_Vial : 12 Sample_Multiplier: 11

Instrument :
BNA_N
ClientSampleId :
SBLK65

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.MM
Quant_Title : SVOA_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
