

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030419\
 Data File : BN004587.D
 Acq On : 04 Mar 2019 12:09
 Operator : JU/SJ
 Sample : K1622-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BF5H6

Quant Time: Mar 05 03:35:07 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 05 03:32:21 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.73	152	25944	20.00	ng/ul	-0.02
18) Naphthalene-d8	10.52	136	128358	20.00	ng/ul	-0.02
36) Acenaphthene-d10	14.37	164	84187	20.00	ng/ul	-0.02
62) Phenanthrene-d10	17.12	188	204642	20.00	ng/ul	-0.02
78) Chrysene-d12	21.32	240	260148	20.00	ng/ul	0.00
86) Perylene-d12	23.59	264	291365	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.23	96	2866	6.64	ng/uL	-0.01
5) Phenol-d5	6.89	99	29401	12.72	ng/ul	-0.01
7) Bis-(2-Chloroethyl)ether-d	7.07	67	17093	14.73	ng/ul	-0.02
9) 2-Chlorophenol-d4	7.26	132	26321	14.04	ng/ul	-0.02
13) 4-Methylphenol-d8	8.42	113	26065	13.12	ng/ul	-0.02
19) Nitrobenzene-d5	8.89	128	13571	15.97	ng/ul	-0.01
22) 2-Nitrophenol-d4	9.60	143	14942	16.85	ng/ul	-0.02
26) 2,4-Dichlorophenol-d3	10.13	165	28436	14.14	ng/ul	-0.01
29) 4-Chloroaniline-d4	10.66	131	42198	18.97	ng/ul	-0.02
44) Dimethylphthalate-d6	13.78	166	113360	15.88	ng/ul	-0.02
47) Acenaphthylene-d8	14.06	160	122702	14.51	ng/ul	-0.02
52) 4-Nitrophenol-d4	14.57	143	14312	10.47	ng/ul	-0.01
58) Fluorene-d10	15.36	176	94566	15.05	ng/ul	-0.02
63) 4,6-Dinitro-2-methylphenol	15.49	200	13398	11.23	ng/ul	-0.01
71) Anthracene-d10	17.22	188	153381	15.64	ng/ul	-0.02
79) Pyrene-d10	19.52	212	183962	15.78	ng/ul	-0.01
90) Benzo(a)pyrene-d12	23.45	264	213787	13.98	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.83	163	17667	2.503	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030419\
Data File : BN004587.D
Acq On : 04 Mar 2019 12:09
Operator : JU/SJ
Sample : K1622-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BF5H6

Quant Time: Mar 05 03:35:07 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 05 03:32:21 2019
Response via : Initial Calibration

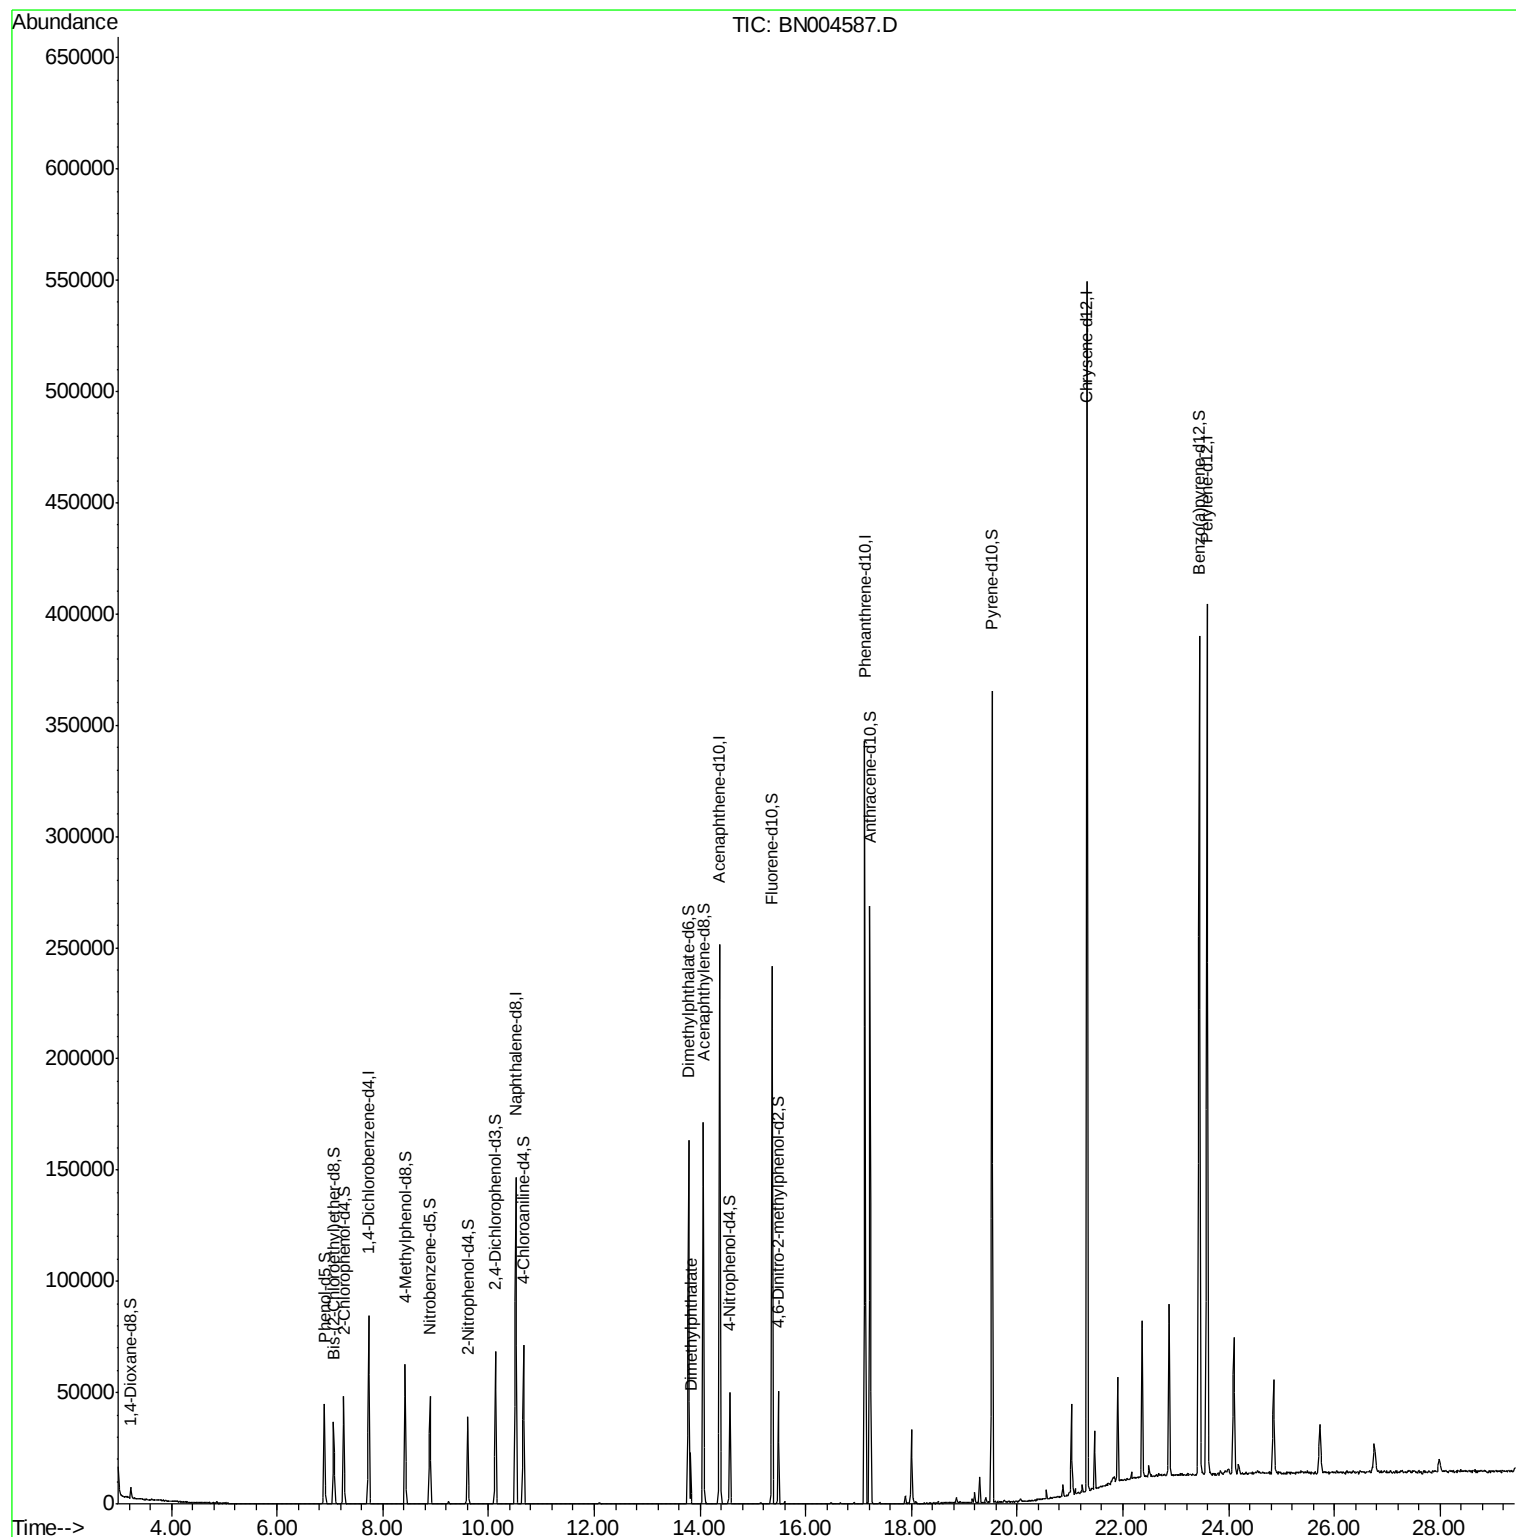

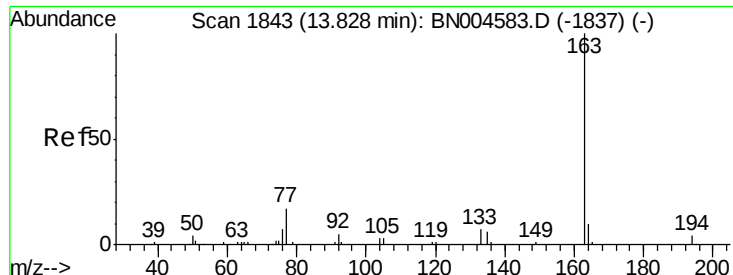

#45

Dimethylphthalate

Concen: 2.503 ng/ul

RT: 13.83 min Scan# 1843

Delta R.T. -0.02 min

Lab File: BN004587.D


Acq: 04 Mar 2019 12:09

Instrument :

BNA_N

ClientSampleId :

BF5H6

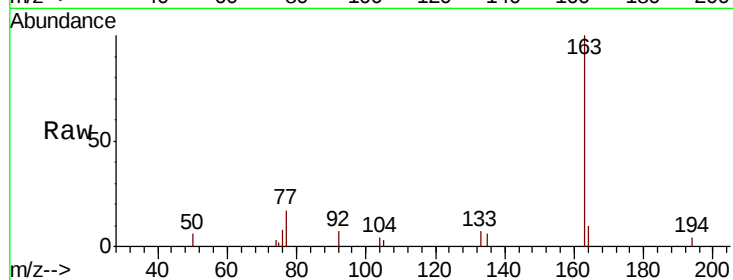


Tgt Ion:163 Resp: 17667

Ion Ratio Lower Upper

163 100

194 4.3 3.4 5.2

164 9.5 7.9 11.9

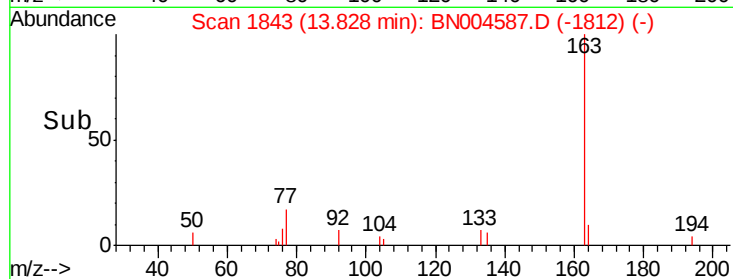

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

