

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030419\
 Data File : BN004588.D
 Acq On : 04 Mar 2019 12:44
 Operator : JU/SJ
 Sample : K1622-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BF5H7

Quant Time: Mar 05 03:35:12 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 05 03:32:21 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.73	152	33161	20.00	ng/ul	-0.01
18) Naphthalene-d8	10.52	136	161681	20.00	ng/ul	-0.02
36) Acenaphthene-d10	14.37	164	105654	20.00	ng/ul	-0.02
62) Phenanthrene-d10	17.12	188	257437	20.00	ng/ul	-0.02
78) Chrysene-d12	21.32	240	328322	20.00	ng/ul	0.00
86) Perylene-d12	23.59	264	368977	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.23	96	3927	7.12	ng/uL	-0.01
5) Phenol-d5	6.89	99	37927	12.83	ng/ul	-0.01
7) Bis-(2-Chloroethyl)ether-d	7.07	67	21771	14.68	ng/ul	-0.02
9) 2-Chlorophenol-d4	7.26	132	33996	14.18	ng/ul	-0.02
13) 4-Methylphenol-d8	8.42	113	35348	13.92	ng/ul	-0.02
19) Nitrobenzene-d5	8.89	128	17758	16.59	ng/ul	-0.01
22) 2-Nitrophenol-d4	9.60	143	19956	17.86	ng/ul	-0.02
26) 2,4-Dichlorophenol-d3	10.13	165	37345	14.74	ng/ul	-0.01
29) 4-Chloroaniline-d4	10.66	131	55878	19.95	ng/ul	-0.02
44) Dimethylphthalate-d6	13.78	166	149354	16.67	ng/ul	-0.02
47) Acenaphthylene-d8	14.06	160	162744	15.33	ng/ul	-0.02
52) 4-Nitrophenol-d4	14.56	143	21367	12.46	ng/ul	-0.02
58) Fluorene-d10	15.36	176	125072	15.86	ng/ul	-0.02
63) 4,6-Dinitro-2-methylphenol	15.49	200	19972	13.30	ng/ul	-0.01
71) Anthracene-d10	17.22	188	208119	16.87	ng/ul	-0.02
79) Pyrene-d10	19.52	212	249528	16.96	ng/ul	-0.01
90) Benzo(a)pyrene-d12	23.44	264	293422	15.15	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.83	163	26367	2.977	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030419\
Data File : BN004588.D
Acq On : 04 Mar 2019 12:44
Operator : JU/SJ
Sample : K1622-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BF5H7

Quant Time: Mar 05 03:35:12 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 05 03:32:21 2019
Response via : Initial Calibration

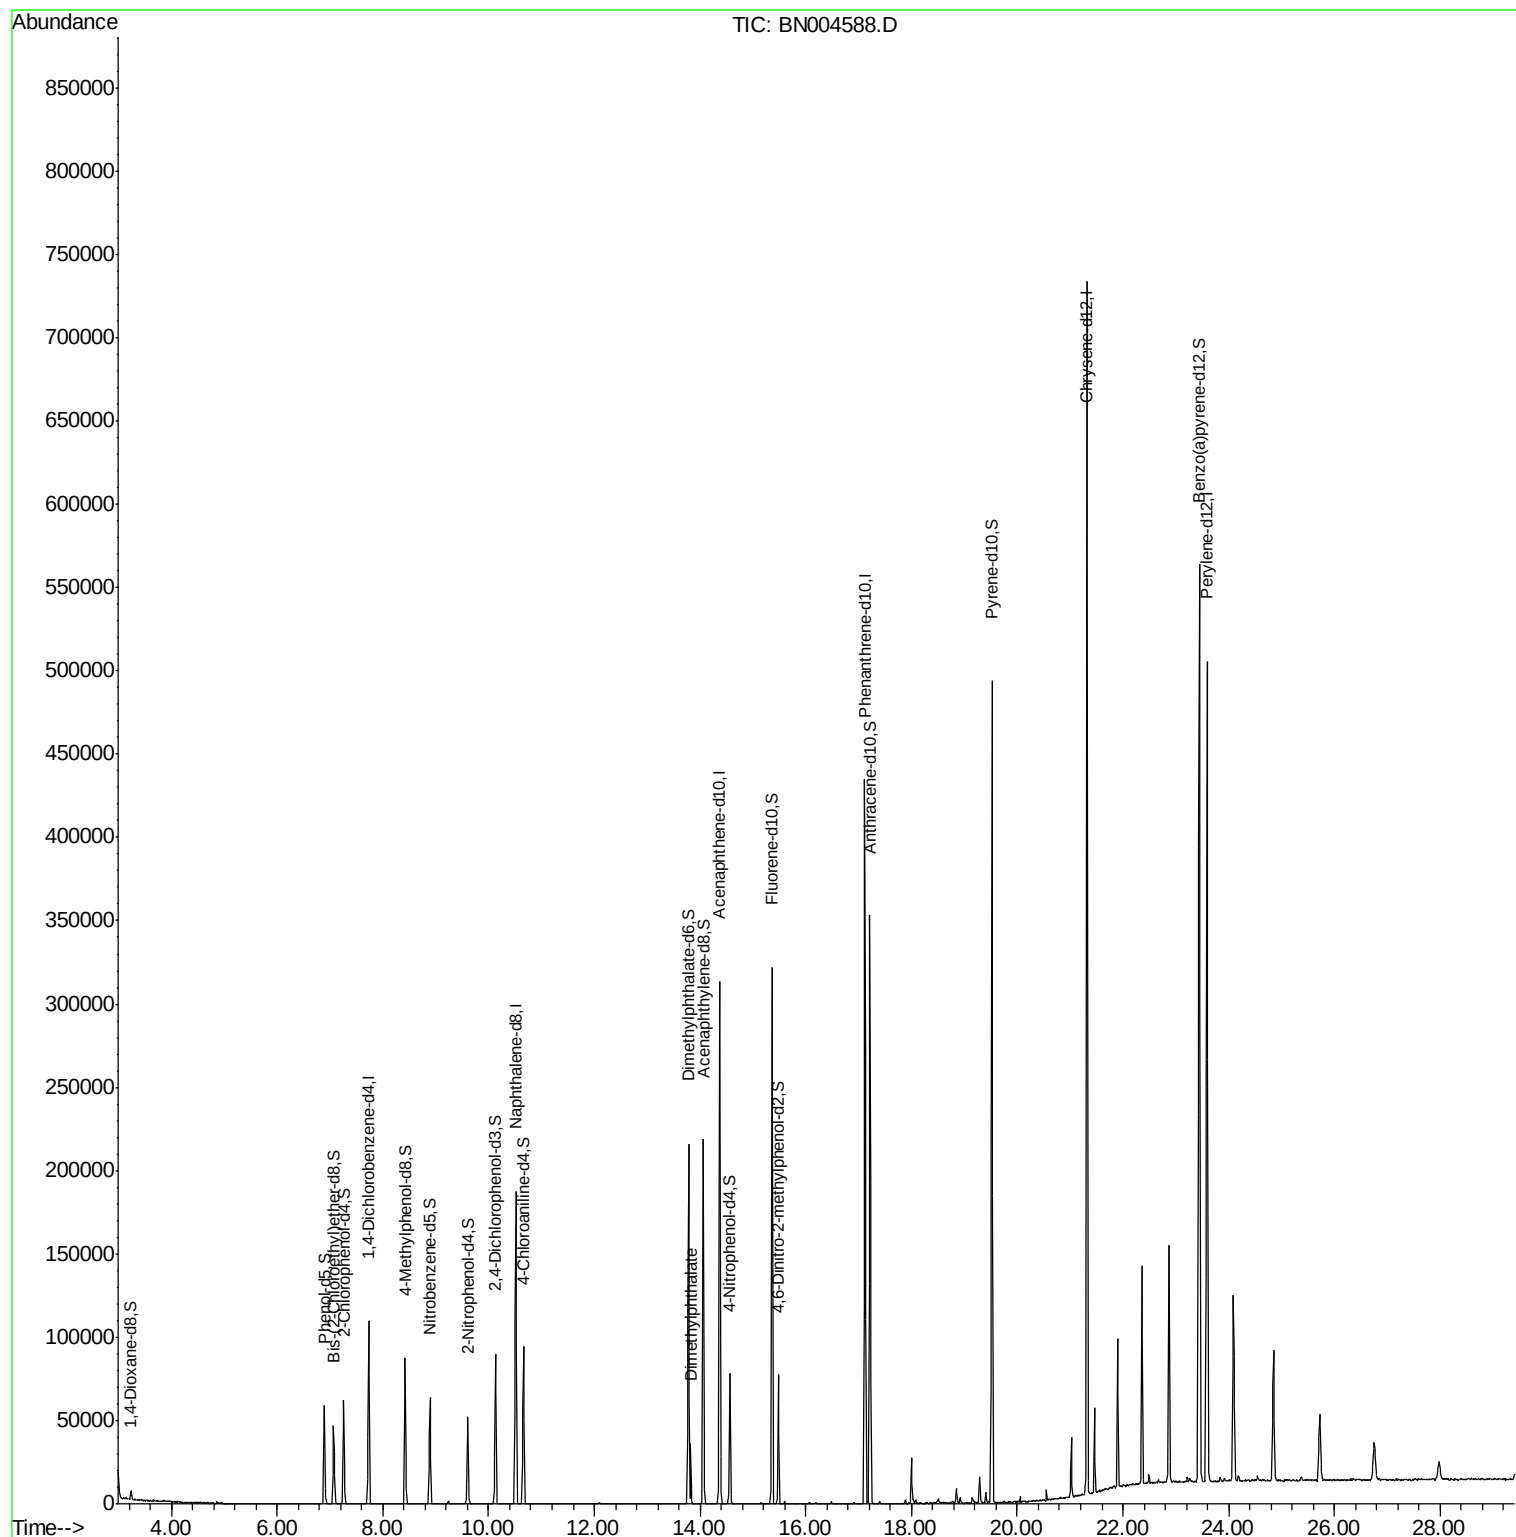

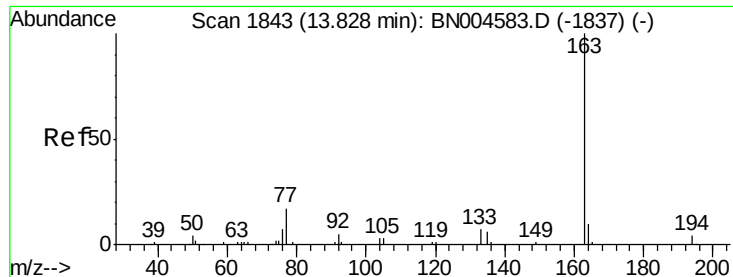

#45

Dimethylphthalate

Concen: 2.977 ng/ul

RT: 13.83 min Scan# 1843

Delta R.T. -0.02 min

Lab File: BN004588.D

Acq: 04 Mar 2019 12:44

Instrument :

BNA_N

ClientSampleId :

BF5H7


Tgt Ion:163 Resp: 26367

Ion Ratio Lower Upper

163 100

194 4.6 3.4 5.2

164 10.0 7.9 11.9

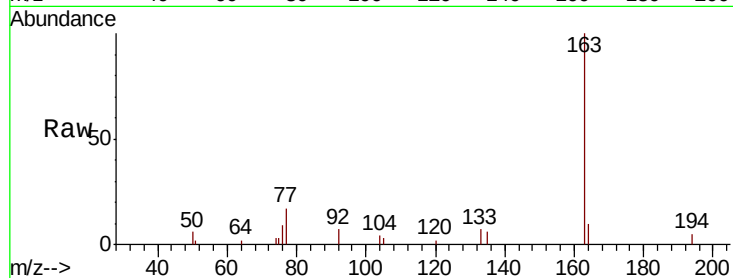

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

