

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030419\
 Data File : BN004585.D
 Acq On : 04 Mar 2019 10:59
 Operator : JU/SJ
 Sample : K1622-08
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BF5J2

Quant Time: Mar 05 04:34:58 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 05 03:32:21 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.73	152	28132	20.00	ng/ul	-0.02
18) Naphthalene-d8	10.52	136	139317	20.00	ng/ul	-0.02
36) Acenaphthene-d10	14.37	164	90928	20.00	ng/ul	-0.02
62) Phenanthrene-d10	17.12	188	220706	20.00	ng/ul	-0.01
78) Chrysene-d12	21.32	240	285875	20.00	ng/ul	0.00
86) Perylene-d12	23.59	264	320948	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.23	96	1293	2.76	ng/uL	-0.01
5) Phenol-d5	6.89	99	30692	12.24	ng/ul	-0.02
7) Bis-(2-Chloroethyl)ether-d	7.07	67	18047	14.35	ng/ul	-0.02
9) 2-Chlorophenol-d4	7.26	132	28001	13.77	ng/ul	-0.02
13) 4-Methylphenol-d8	8.42	113	27513	12.77	ng/ul	-0.02
19) Nitrobenzene-d5	8.89	128	14134	15.33	ng/ul	-0.01
22) 2-Nitrophenol-d4	9.60	143	15905	16.52	ng/ul	-0.02
26) 2,4-Dichlorophenol-d3	10.13	165	29880	13.69	ng/ul	-0.02
29) 4-Chloroaniline-d4	10.66	131	44298	18.35	ng/ul	-0.02
44) Dimethylphthalate-d6	13.78	166	117081	15.18	ng/ul	-0.02
47) Acenaphthylene-d8	14.06	160	127826	13.99	ng/ul	-0.02
52) 4-Nitrophenol-d4	14.56	143	13711	9.29	ng/ul	-0.02
58) Fluorene-d10	15.36	176	98764	14.55	ng/ul	-0.02
63) 4,6-Dinitro-2-methylphenol	15.48	200	13305	10.34	ng/ul	-0.02
71) Anthracene-d10	17.22	188	156508	14.80	ng/ul	-0.02
79) Pyrene-d10	19.52	212	185312	14.46	ng/ul	-0.01
90) Benzo(a)pyrene-d12	23.44	264	212559	12.62	ng/ul	-0.02


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.82	163	16823	2.207	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030419\
Data File : BN004585.D
Acq On : 04 Mar 2019 10:59
Operator : JU/SJ
Sample : K1622-08
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BF5J2

Quant Time: Mar 05 04:34:58 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 05 03:32:21 2019
Response via : Initial Calibration

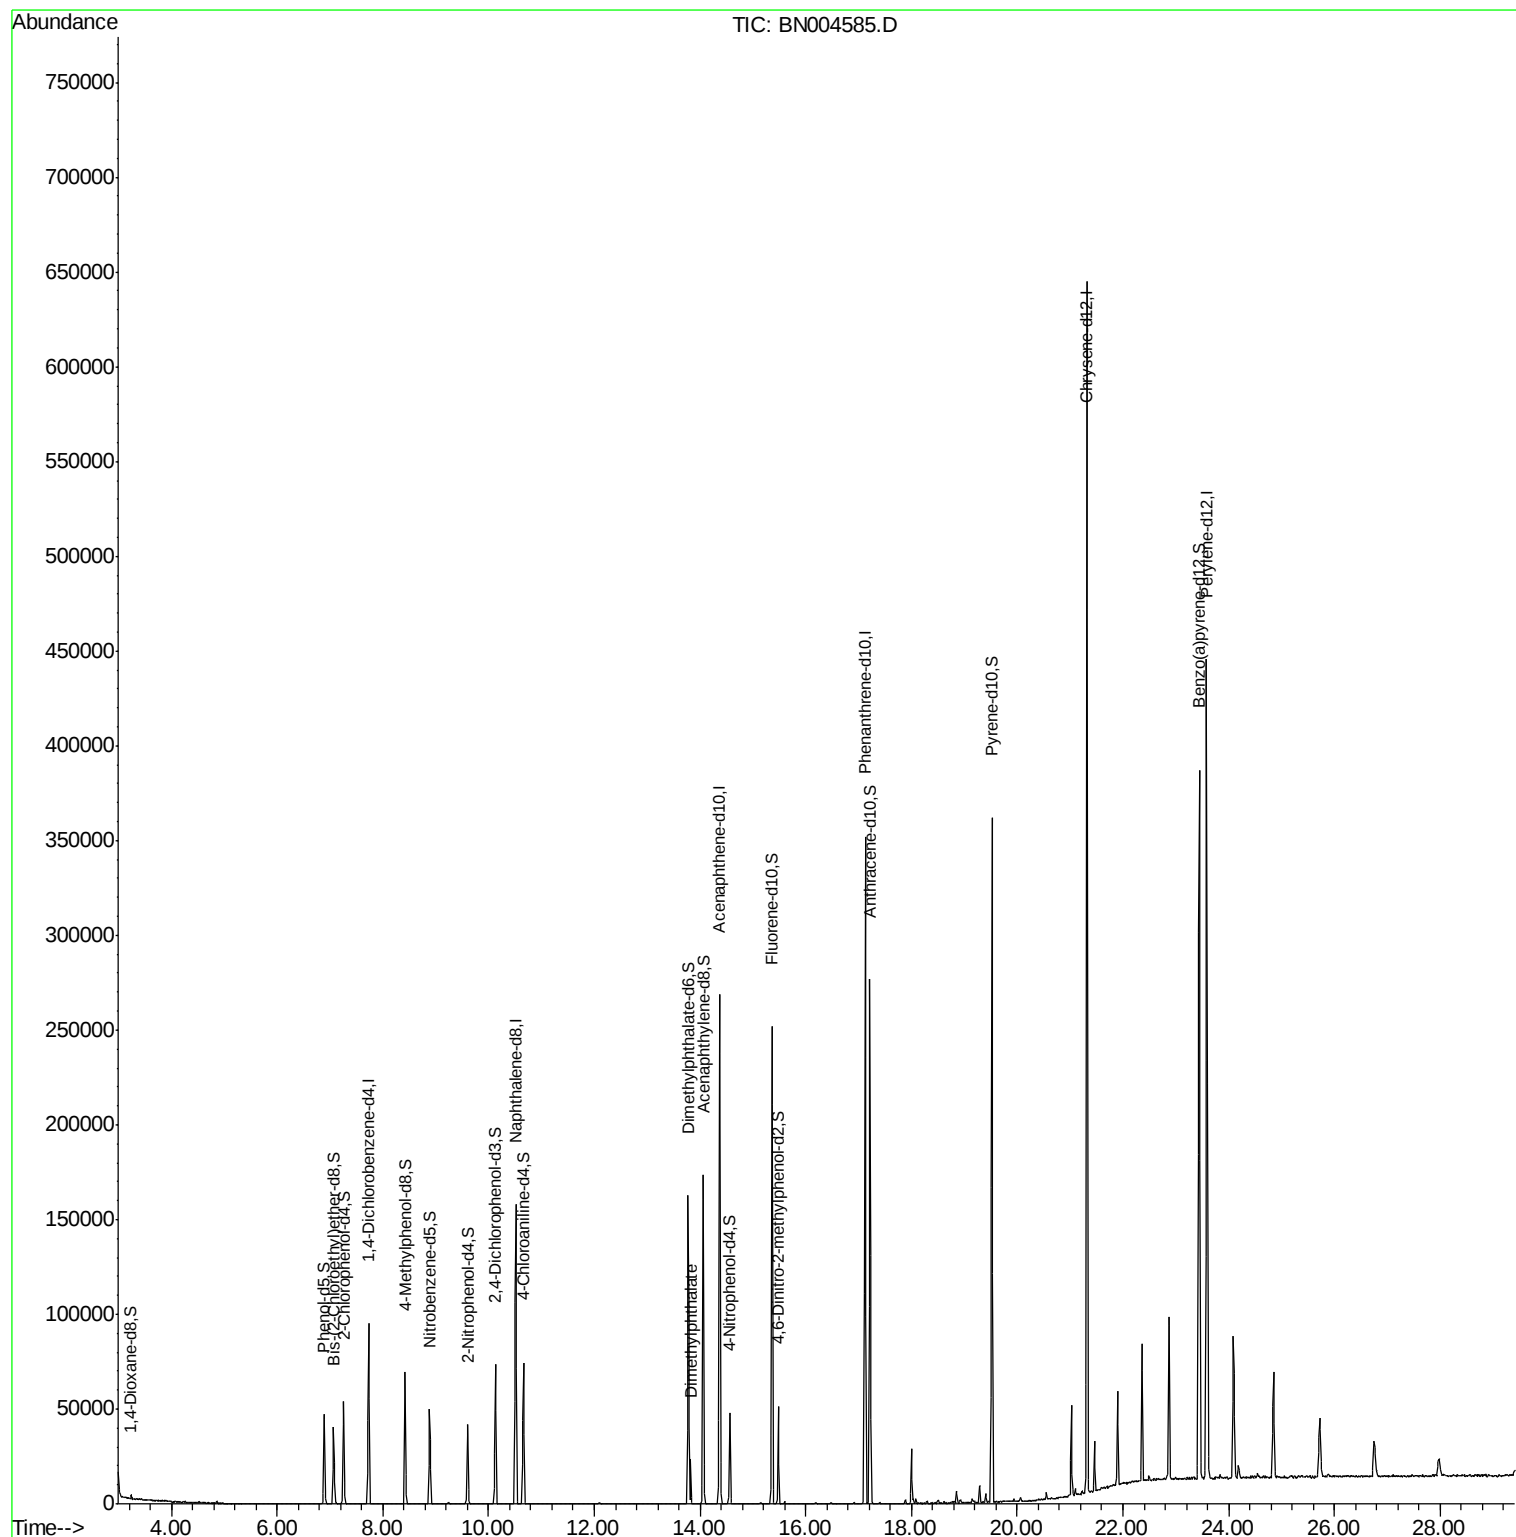

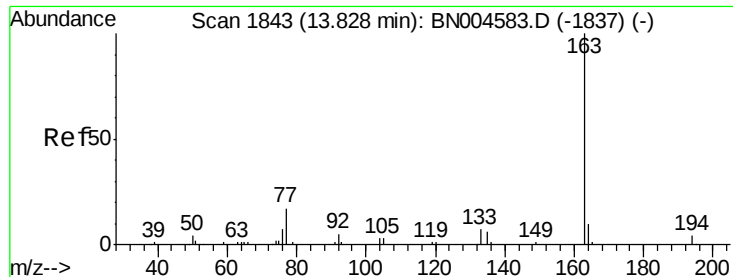

#45

Dimethylphthalate

Concen: 2.207 ng/ul

RT: 13.82 min Scan# 1842

Delta R.T. -0.02 min

Lab File: BN004585.D

Acq: 04 Mar 2019 10:59

Instrument :

BNA_N

ClientSampleId :

BF5J2


Tgt Ion:163 Resp: 16823

Ion Ratio Lower Upper

163 100

194 4.4 3.4 5.2

164 10.4 7.9 11.9

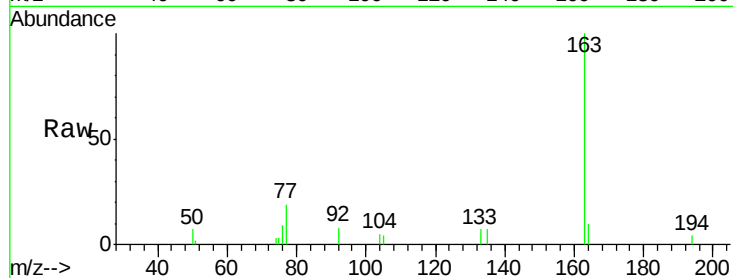

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

