


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030419\
Data File : BN004582.D
Acq On : 04 Mar 2019 09:12
Operator : JU/SJ
Sample : DFTPP13
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP13

Integration File: LSCINT.P

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020719MA.M
Title : SVOA CALIBRATION
Last Update : Tue Mar 05 05:46:57 2019

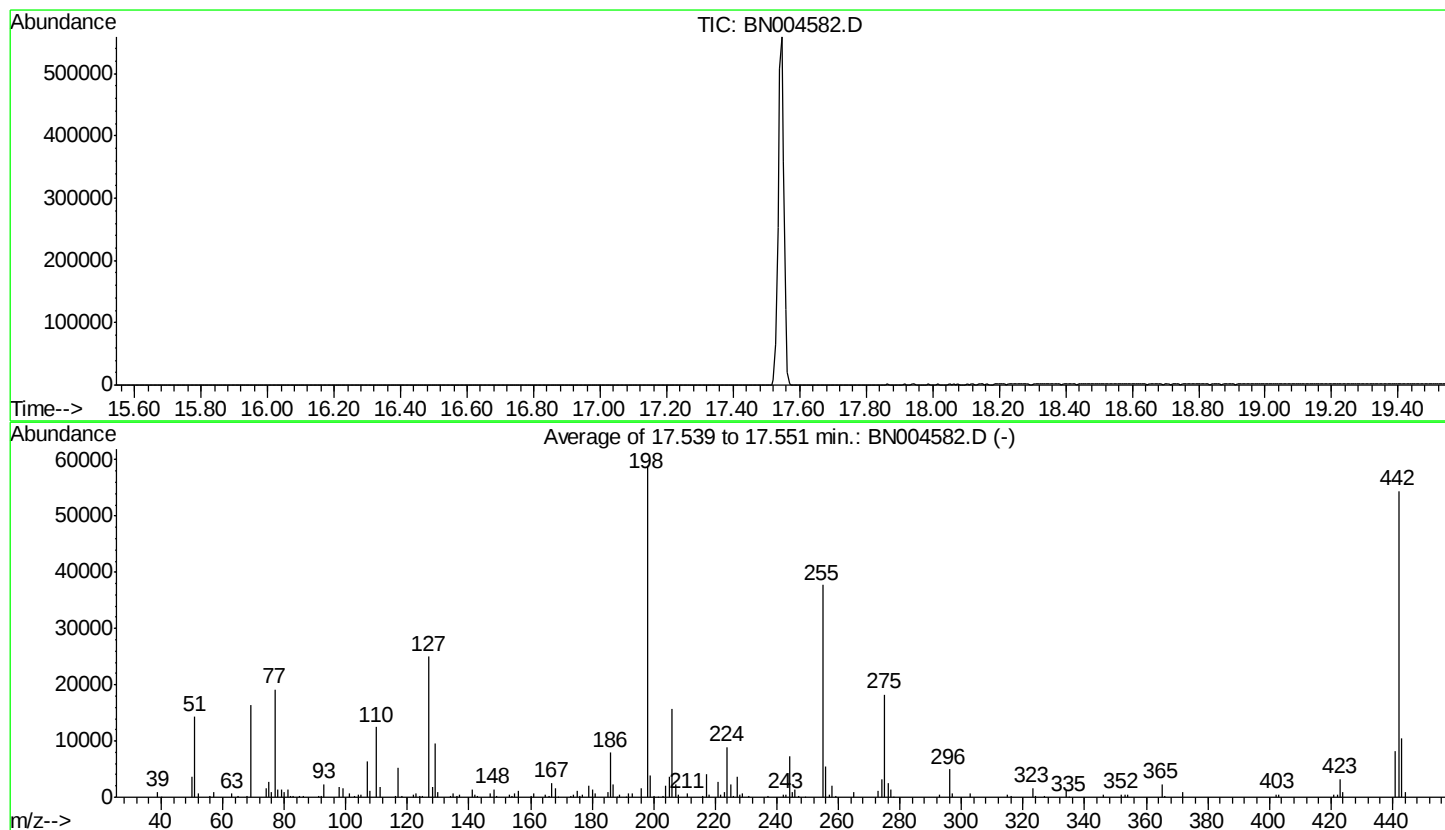

AutoFind: Scans 2474, 2475, 2476; Background Corrected with Scan 2469

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.2	14246	PASS
68	69	0.00	2	1.5	240	PASS
69	198	0.00	100	27.9	16477	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.5	25042	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	58976	PASS
199	198	5	9	6.8	3982	PASS
275	198	10	60	30.9	18244	PASS
365	198	1	100	3.9	2322	PASS
441	198	0.01	100	14.0	8284	PASS
442	198	50	100	92.4	54493	PASS
443	442	15	24	19.1	10417	PASS

Scan 2469 (17.510 min): BN004582.D
DFTPP13

m/z	Abundance
39.90	314.0
44.00	485.0

Instrument :
BNA_N
ClientSampleId :
DFTPP13

m/z	Abundance
39.00	1176.0
39.90	356.0
44.00	482.0
50.00	4595.0
51.00	17320.0
52.00	937.0
56.00	535.0
57.00	1197.0
63.00	706.0
65.00	360.0
68.00	392.0
69.00	19624.0
74.00	1967.0
75.00	3268.0
76.00	1110.0
77.00	22920.0
78.00	1626.0
79.00	1544.0
80.00	1284.0
81.00	1744.0
81.90	431.0
82.90	366.0
84.90	314.0
86.00	513.0
91.00	409.0
92.00	406.0
93.00	2765.0
98.00	2027.0
99.00	1867.0
101.00	939.0
102.90	388.0
104.00	622.0
105.00	596.0
107.00	7571.0
108.00	1184.0
110.00	14387.0
111.00	2359.0
116.00	430.0
117.00	6081.0
118.00	526.0
121.90	514.0
123.00	772.0
123.90	381.0
125.00	358.0
127.00	28984.0
128.00	2310.0
129.00	10851.0
130.00	922.0
134.00	322.0
135.00	923.0
136.00	362.0
137.00	514.0
141.00	1438.0
141.90	449.0
142.90	330.0
147.00	748.0
148.00	1705.0
149.00	368.0
153.00	436.0
154.00	350.0
155.00	793.0
156.00	1199.0
160.00	412.0
161.00	726.0
164.90	571.0
166.00	473.0
167.00	2888.0
168.00	1872.0
168.90	340.0
173.00	333.0
174.00	625.0
175.00	1233.0
176.00	328.0
177.00	539.0
179.00	2201.0
180.00	1524.0
181.00	735.0
185.00	1032.0
186.00	8632.0
187.00	2573.0
188.00	307.0
188.90	542.0
192.00	750.0
193.00	862.0
196.00	1821.0
198.00	63208.0
199.00	4465.0
203.00	458.0
204.00	2411.0
205.00	3848.0
206.00	16728.0

Instrument :
BNA_N
ClientSampleId :
DFTPP13

207.00	2445.0
208.00	619.0
211.00	617.0
216.00	358.0
217.00	4344.0
218.00	631.0
221.00	2932.0
221.80	702.0
223.00	990.0
224.00	9580.0
225.00	2442.0
226.00	327.0
227.00	3749.0
228.00	565.0
228.90	840.0
231.00	376.0
237.00	484.0
242.10	505.0
243.00	520.0
244.00	7576.0
245.00	1021.0
246.00	1523.0
247.00	325.0
249.00	312.0
255.00	38656.0
256.00	5879.0
257.00	502.0
258.00	2162.0
258.90	356.0
264.90	937.0
273.00	1184.0
274.00	3175.0
275.00	18632.0
276.00	2552.0
277.00	1517.0
293.00	362.0
296.00	4867.0
297.00	698.0
303.00	608.0
315.00	535.0
316.00	302.0
323.00	1596.0
324.00	321.0
334.00	1067.0
345.90	326.0
352.00	501.0
353.00	331.0
354.00	585.0
365.00	2178.0
366.00	344.0
372.00	913.0
402.00	355.0
403.00	471.0
420.90	372.0
422.00	413.0
423.00	2910.0
424.00	905.0
441.00	7070.0
442.00	46128.0
443.00	9318.0
444.00	886.0

Instrument :
BNA_N
ClientSampleId :
DFTPP13

m/z	Abundance
39.00	1136.0
39.90	347.0
44.00	428.0
50.00	4177.0
51.00	16111.0
52.00	822.0
56.00	504.0
57.00	1225.0
63.00	701.0
65.00	386.0
68.10	328.0
69.00	18968.0
74.00	2019.0
75.00	3176.0
76.00	1126.0
77.00	21960.0
78.00	1520.0
79.00	1665.0
80.00	1128.0
81.00	1580.0
82.00	436.0
83.00	335.0
84.90	311.0
86.00	500.0
91.00	337.0
91.90	460.0
93.00	2596.0
98.00	2133.0
99.00	1801.0
101.00	909.0
102.90	388.0
104.00	641.0
104.90	589.0
107.00	7351.0
108.00	1195.0
110.00	14515.0
111.00	2120.0
116.00	432.0
117.00	6097.0
118.00	467.0
122.00	545.0
122.90	785.0
123.90	379.0
125.00	313.0
127.00	28856.0
128.00	2118.0
129.00	11081.0
130.00	943.0
134.00	371.0
135.00	890.0
136.00	369.0
137.00	511.0
141.00	1456.0
142.00	532.0
142.90	308.0
147.00	760.0
148.00	1729.0
149.00	420.0
152.90	470.0
153.90	390.0
155.00	804.0
156.00	1276.0
160.00	541.0
161.00	700.0
165.00	563.0
166.00	431.0
167.00	2955.0
168.00	1683.0
172.90	370.0
174.00	627.0
175.00	1172.0
175.90	363.0
176.90	606.0
179.00	2310.0
180.00	1723.0
181.00	815.0
185.00	1187.0
186.00	9294.0
187.00	2676.0
189.00	543.0
191.00	310.0
192.00	781.0
193.00	778.0
196.00	2031.0
198.00	69344.0
199.00	4608.0
200.00	374.0
201.40	338.0
203.00	441.0
204.00	2402.0
205.00	4297.0

Instrument :
BNA_N
ClientSampleId :
DFTPP13

206.00	18584.0
207.00	2685.0
208.00	626.0
211.00	716.0
216.00	393.0
217.00	4701.0
218.00	643.0
221.00	3171.0
223.00	1109.0
224.00	10567.0
225.00	2711.0
226.00	346.0
227.00	4085.0
228.00	613.0
229.00	888.0
231.00	396.0
237.00	425.0
241.90	551.0
243.00	636.0
244.00	8335.0
245.00	1145.0
246.00	1668.0
246.90	367.0
255.00	44584.0
256.00	6487.0
257.00	539.0
258.00	2525.0
259.00	430.0
265.00	1003.0
273.00	1317.0
274.00	3622.0
275.00	21720.0
276.00	2846.0
277.00	1720.0
278.00	312.0
293.00	416.0
296.00	5844.0
297.00	762.0
303.00	649.0
314.90	673.0
316.00	385.0
323.00	2003.0
324.00	354.0
326.90	387.0
334.00	1200.0
335.00	341.0
346.00	452.0
352.00	646.0
353.00	404.0
354.00	626.0
365.00	2752.0
365.90	366.0
372.00	1105.0
402.00	471.0
403.00	698.0
421.00	535.0
422.00	579.0
423.00	3848.0
424.00	990.0
441.00	9686.0
442.00	64720.0
443.00	12076.0
444.00	1060.0

Instrument :
BNA_N
ClientSampleId :
DFTPP13

m/z	Abundance
39.00	639.0
39.90	371.0
43.90	463.0
50.00	2385.0
51.00	9307.0
52.00	481.0
57.00	655.0
63.00	429.0
69.00	10839.0
74.00	1121.0
75.00	1848.0
76.00	580.0
77.00	12608.0
78.00	895.0
79.00	929.0
80.00	654.0
81.00	982.0
93.00	1483.0
98.00	1199.0
99.00	1065.0
101.00	548.0
104.00	371.0
104.90	369.0
107.00	4358.0
108.00	718.0
110.00	8585.0
111.00	1232.0
117.00	3682.0
121.90	307.0
123.00	515.0
127.00	17288.0
128.00	1330.0
129.00	6667.0
130.00	576.0
135.00	552.0
137.00	311.0
140.90	896.0
142.00	308.0
147.00	477.0
148.00	977.0
152.90	306.0
155.00	504.0
156.00	778.0
161.00	451.0
165.00	390.0
167.00	1858.0
168.00	1056.0
174.00	444.0
175.00	786.0
176.90	377.0
178.90	1417.0
180.00	1047.0
181.00	430.0
185.00	681.0
186.00	5864.0
187.00	1676.0
188.90	347.0
192.00	517.0
193.00	599.0
196.00	1252.0
198.00	44376.0
199.00	2874.0
204.00	1583.0
205.00	2811.0
206.00	11663.0
207.00	1803.0
208.00	426.0
211.10	491.0
217.00	2977.0
218.00	391.0
221.00	2010.0
221.80	487.0
223.00	770.0
224.00	6615.0
225.00	1750.0
227.00	2807.0
228.00	402.0
229.00	642.0
242.00	371.0
243.00	393.0
244.00	5671.0
245.10	758.0
246.00	1034.0
255.00	30024.0
256.00	4171.0
257.00	346.0
258.00	1594.0
265.00	675.0
273.00	972.0
274.00	2571.0
275.00	14380.0

Instrument :
BNA_N
ClientSampleId :
DFTPP13

276.00	1956.0
277.00	1222.0
293.00	305.0
296.00	4062.0
297.00	496.0
303.00	540.0
315.00	497.0
323.00	1357.0
334.00	957.0
346.00	325.0
352.00	438.0
353.00	331.0
354.00	479.0
365.00	2038.0
372.00	846.0
402.00	366.0
403.00	476.0
421.00	450.0
422.10	435.0
423.00	3134.0
424.00	814.0
441.00	8097.0
442.00	52632.0
443.00	9857.0
444.00	813.0

Instrument :
BNA_N
ClientSampleId :
DFTPP13