

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030420\
Quantitation Report (Qedit)




Data File : BN010096.D
Acq On : 05 Mar 2020 01:51
Operator : CG/JU
Sample : L1641-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Quant Time: Mar 05 07:52:34 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 04 01:30:16 2020
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
CB6Y5

Manual Integrations
APPROVED

mohammad
3/5/2020 3:56:37 PM

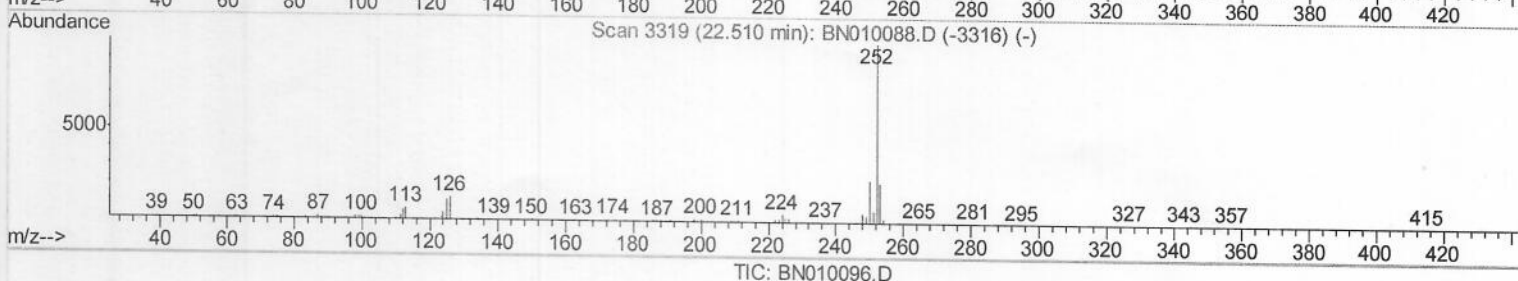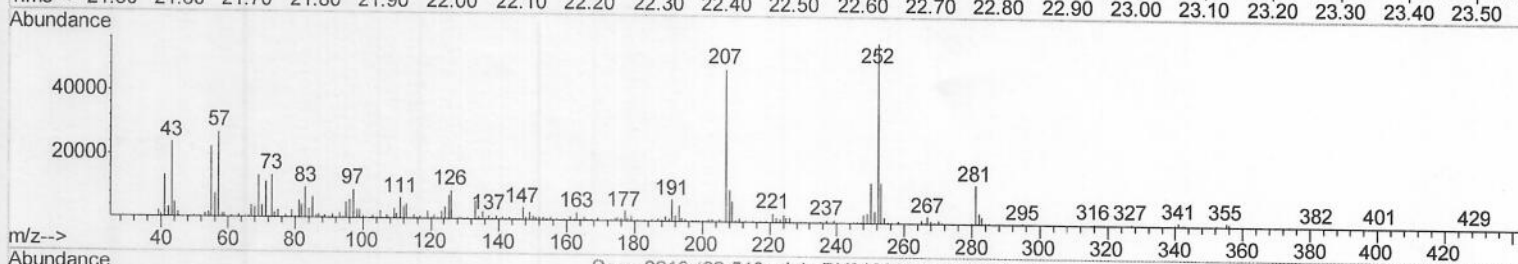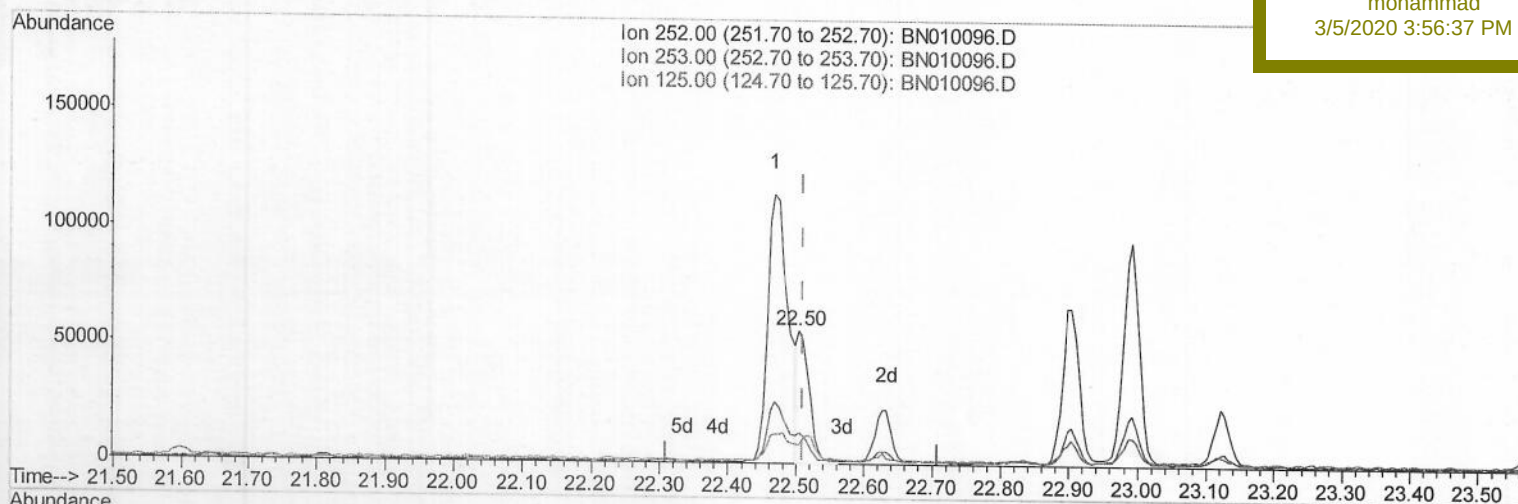

(89) Benzo(k)fluoranthene

22.504min (-0.006) 2.30ng/ul m) JU 03/05/20

response 71015

Ion	Exp%	Act%
252.00	100	100
253.00	22.50	22.80
125.00	10.20	13.83#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030420\
Quantitation Report (Qedit)


Data File : BN010096.D
Acq On : 05 Mar 2020 01:51
Operator : CG/JU
Sample : L1641-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB6Y5

Manual Integrations
APPROVED

mohammad
3/5/2020 3:56:37 PM

Quant Time: Mar 05 07:52:34 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 04 01:30:16 2020
Response via : Initial Calibration

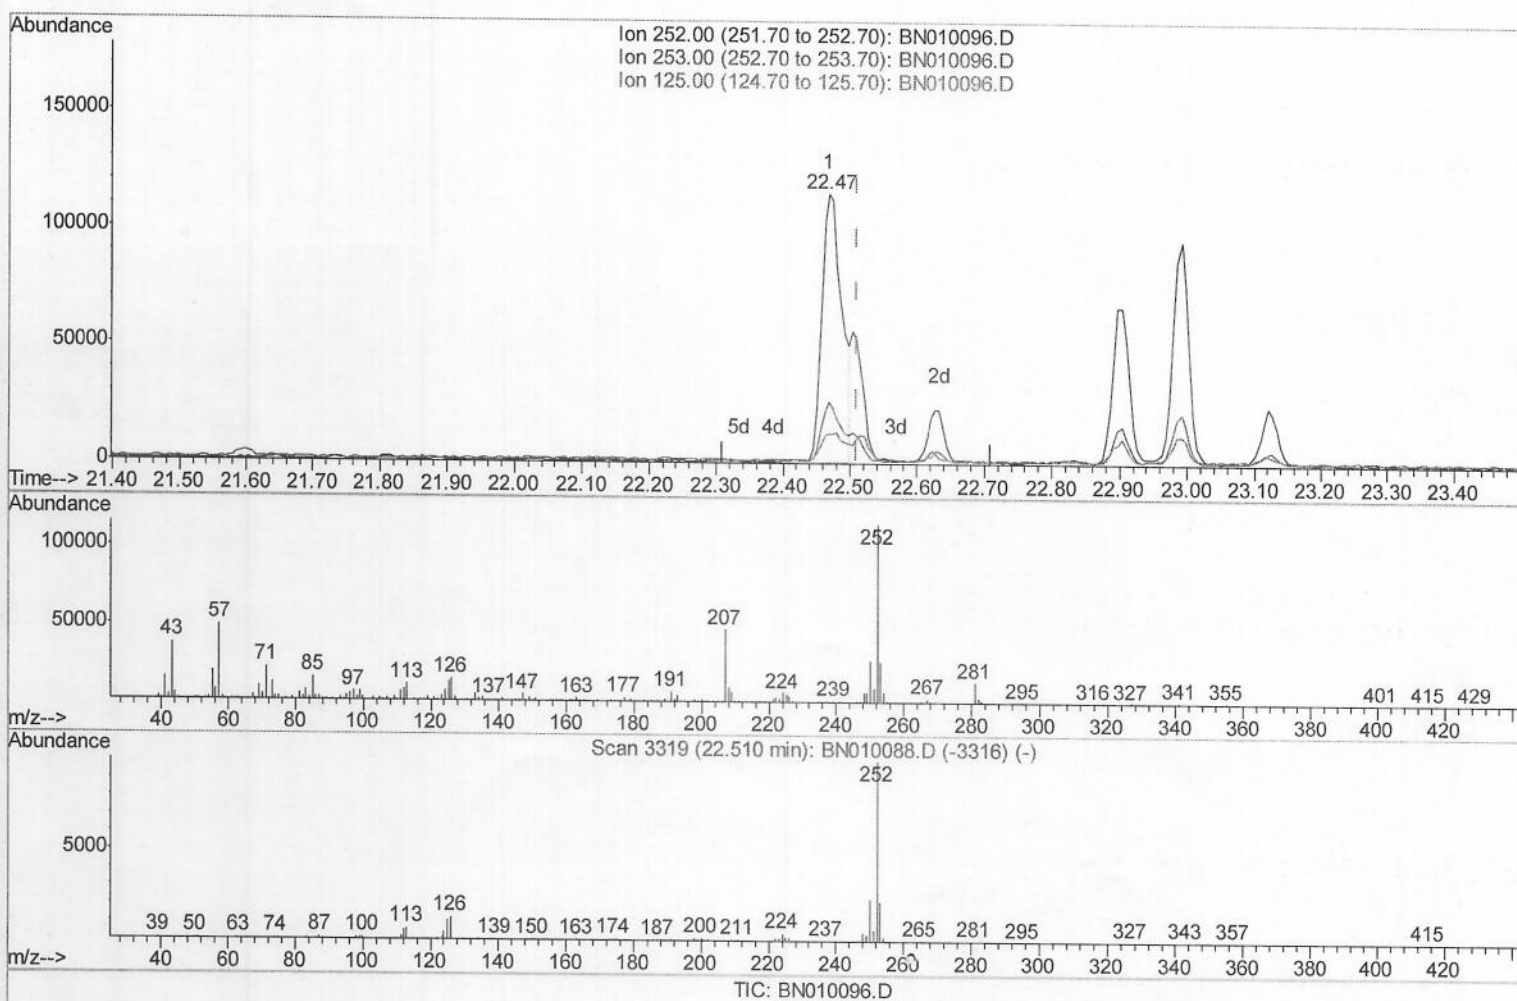

(89) Benzo(k)fluoranthene

22.468min (-0.041) 7.72ng/ul

response 238262

Ion	Exp%	Act%
252.00	100	100
253.00	22.50	22.67
125.00	10.20	10.91
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030420\
Quantitation Report (Qedit)


Data File : BN010096.D
Acq On : 05 Mar 2020 01:51
Operator : CG/JU
Sample : L1641-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB6Y5

Manual Integrations
APPROVED

mohammad
3/5/2020 3:56:37 PM

Quant Time: Mar 05 07:52:34 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 04 01:30:16 2020
Response via : Initial Calibration

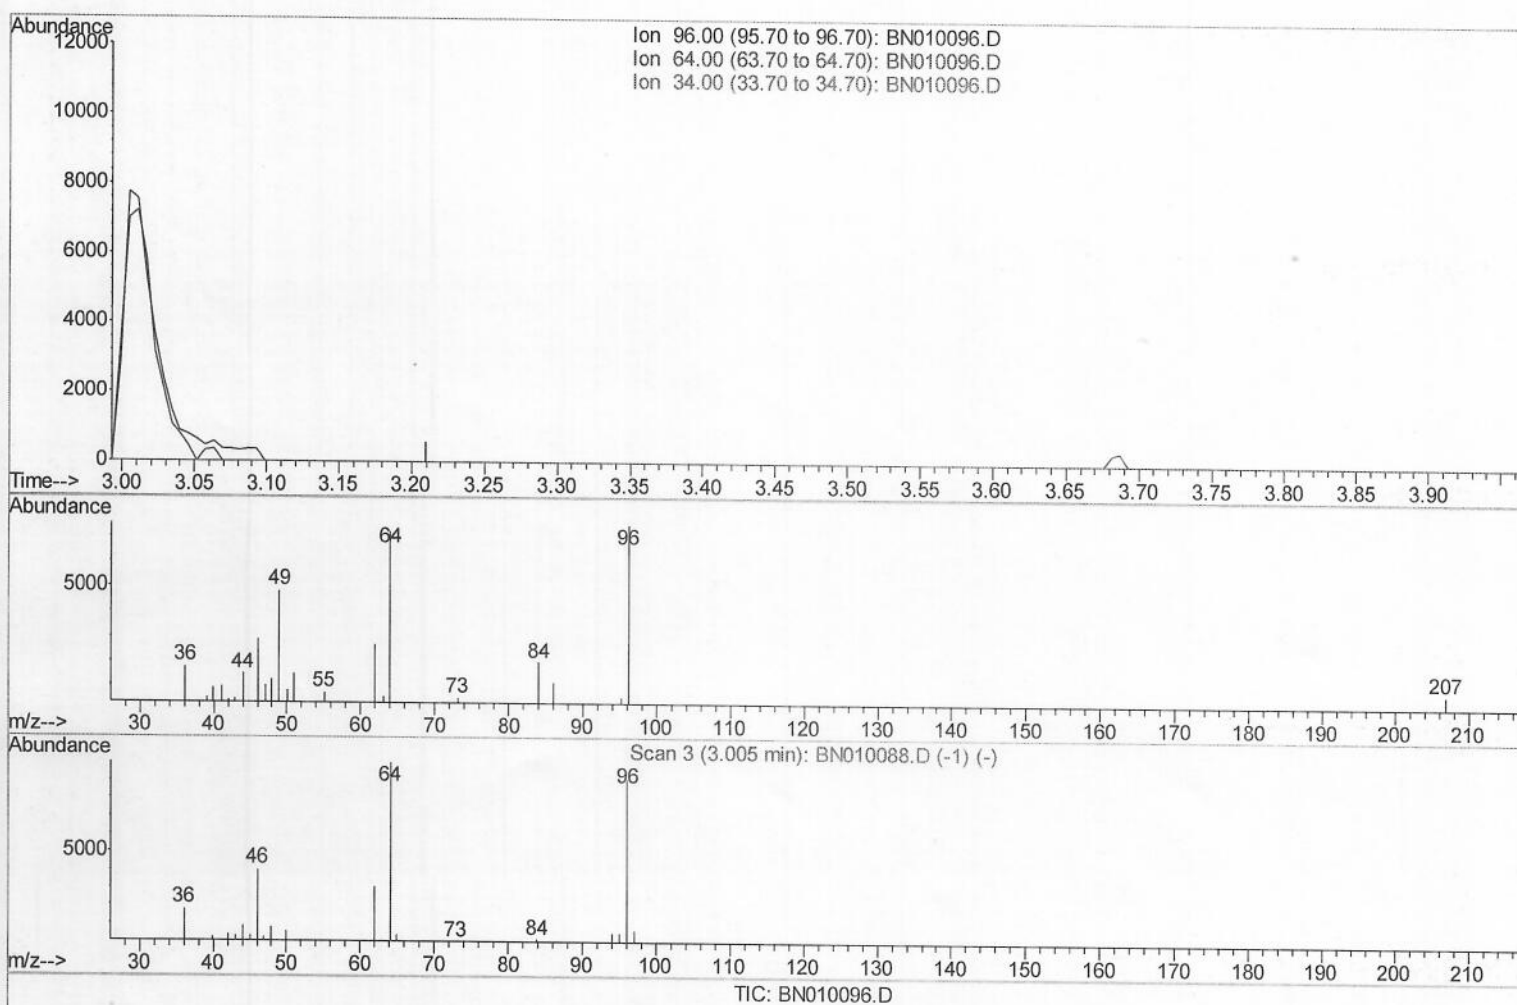

(3) 1,4-Dioxane-d8 (S)

3.011min (-3.011) 0.00ng/uL

response 0

Ion	Exp%	Act%
96.00	100	0.00
64.00	93.60	0.00#
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030420\
Quantitation Report (Qedit)




Data File : BN010096.D
Acq On : 05 Mar 2020 01:51
Operator : CG/JU
Sample : L1641-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Quant Time: Mar 05 07:52:34 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 04 01:30:16 2020
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
CB6Y5

Manual Integrations
APPROVED

mohammad
3/5/2020 3:56:37 PM

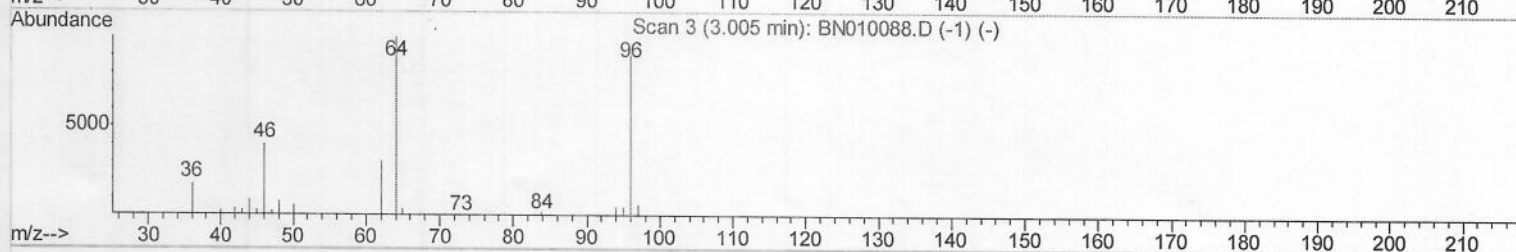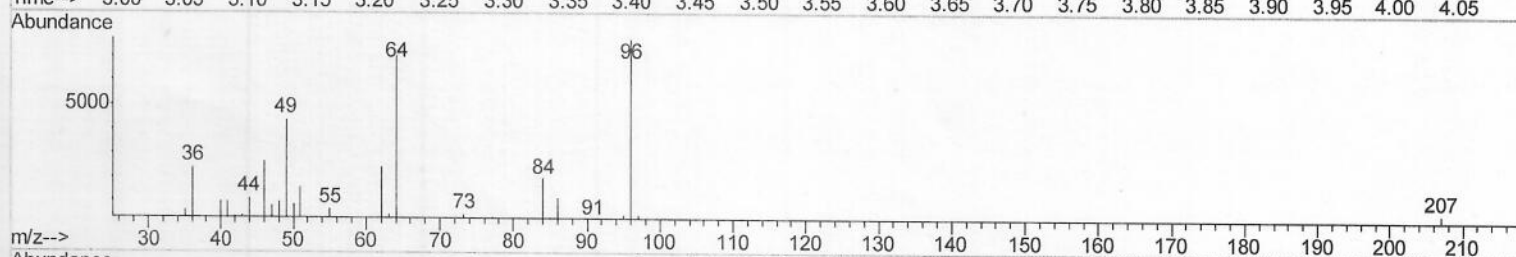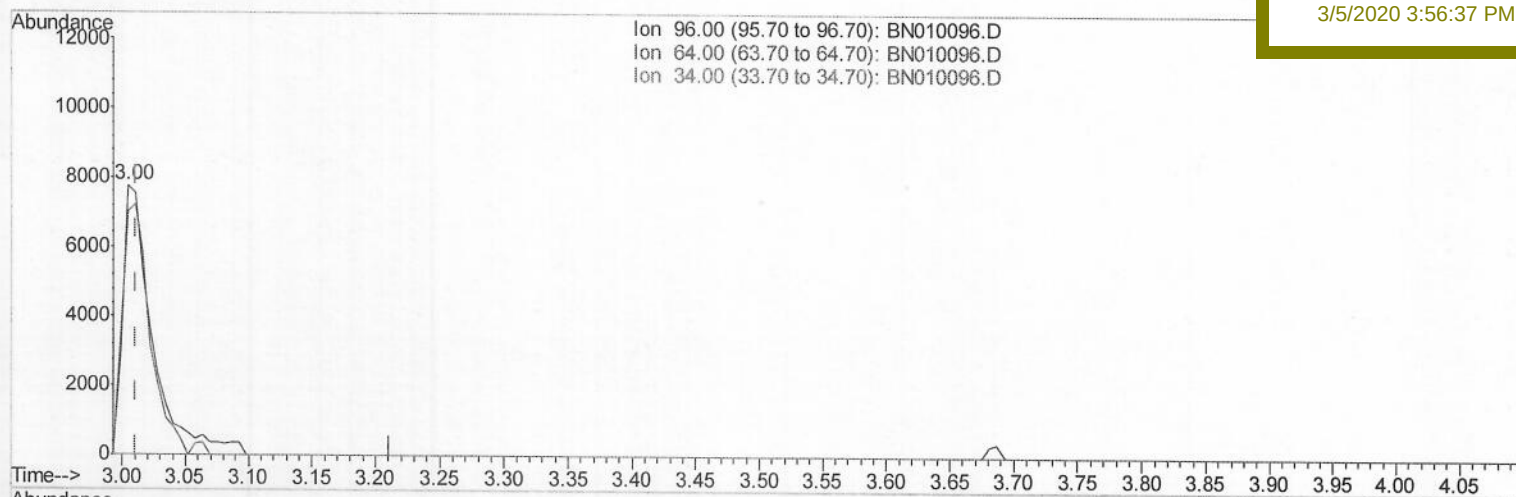

TIC: BN010096.D

(3) 1,4-Dioxane-d8 (S)

3.005min (-0.006) 5.22ng/uL m) JU 03/05/20

response 12688

Ion	Exp%	Act%
96.00	100	100
64.00	93.60	90.62
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030420\

Quantitation Report (QT Reviewed)

Data File : BN010096.D

Acq On : 05 Mar 2020 01:51

Operator : CG/JU

Sample : L1641-02

Misc :

ALS Vial : 23 Sample Multiplier: 1

Instrument :

BNA_N

Client Sampled :

CB6Y5

Manual Integrations

APPROVED

mohammad

3/5/2020 3:56:37 PM

Quant Time: Mar 05 08:14:25 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Wed Mar 04 01:30:16 2020

Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.36	152	99924	20.00	ng/ul	0.00
18) Naphthalene-d8	10.10	136	420829	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.00	164	266478	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.76	188	530138	20.00	ng/ul	0.00
78) Chrysene-d12	20.99	240	467501	20.00	ng/ul	0.00
86) Perylene-d12	23.08	264	502512	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.00	96	12688m)	5.22	ng/uL	0.00
5) Phenol-d5	6.56	99	250853	29.51	ng/ul	0.00
7) Bis-(2-Chloroethyl) ether-d	6.72	67	181607	30.96	ng/ul	0.00
9) 2-Chlorophenol-d4	6.90	132	199661	31.20	ng/ul	0.00
13) 4-Methylphenol-d8	8.08	113	141385	20.91	ng/ul	0.00
19) Nitrobenzene-d5	8.50	128	104914	34.08	ng/ul	-0.01
22) 2-Nitrophenol-d4	9.21	143	117487	34.88	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.75	165	188513	29.11	ng/ul	0.00
29) 4-Chloroaniline-d4	10.26	131	160881	22.11	ng/ul	0.00
44) Dimethylphthalate-d6	13.43	166	654587	32.89	ng/ul	0.00
47) Acenaphthylene-d8	13.69	160	792174	33.79	ng/ul	0.00
52) 4-Nitrophenol-d4	14.26	143	89727	24.68	ng/ul	0.00
58) Fluorene-d10	15.01	176	565064	32.88	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.17	200	92375	28.05	ng/ul	0.00
71) Anthracene-d10	16.86	188	765929	31.52	ng/ul	0.00
79) Pyrene-d10	19.17	212	923658	37.80	ng/ul	0.00
90) Benzo(a)pyrene-d12	22.95	264	888892	35.42	ng/ul	0.00

JU 03/05/20

Target Compounds

					Qvalue	
45) Dimethylphthalate	13.48	163	24104	1.161	ng/ul	98
70) Phenanthrene	16.80	178	176984	5.850	ng/ul	100
72) Anthracene	16.90	178	35663	1.153	ng/ul	97
77) Fluoranthene	18.84	202	328392	9.266	ng/ul	96
80) Pyrene	19.20	202	300524	8.916	ng/ul	98
83) Benzo(a)anthracene	20.97	228	163688	5.095	ng/ul	97
85) Chrysene	21.02	228	167332	5.291	ng/ul	97
88) Benzo(b)fluoranthene	22.47	252	238262	7.313	ng/ul	97
89) Benzo(k)fluoranthene	22.50	252	71015m)	2.302	ng/ul	
91) Benzo(a)pyrene	22.99	252	154678	5.278	ng/ul	98
92) Indeno(1,2,3-cd)pyrene	25.11	276	114959	3.304	ng/ul	94
93) Dibenzo(a,h)anthracene	25.11	278	33295	1.119	ng/ul#	76
94) Benzo(g,h,i)perylene	25.73	276	80203	2.749	ng/ul	98

JU 03/05/20

(#)=qualifier out of range (m)=manual integration (+)=signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030420\
Quantitation Report (QT Reviewed)

Data File : BN010096.D
Acq On : 05 Mar 2020 01:51
Operator : CG/JU
Sample : L1641-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Quant Time: Mar 05 08:14:25 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 04 01:30:16 2020
Response via : Initial Calibration

Instrument :
BNA_N
Client Sample Id :
CB6Y5

Manual Integrations
APPROVED

mohammad
3/5/2020 3:56:37 PM

