


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030420\
Data File : BN010106.D
Acq On : 05 Mar 2020 09:11
Operator : CG/JU
Sample : SSTDCCC020EC
Misc :
ALS Vial : 33 Sample Multiplier: 1

Quant Time: Mar 05 16:41:10 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 05 14:04:18 2020
Response via : Initial Calibration

Instrument :
BNA_N
LabSampleId :
SSTD02082

Manual Integrations

mohammad
3/6/2020 10:25:12 AM

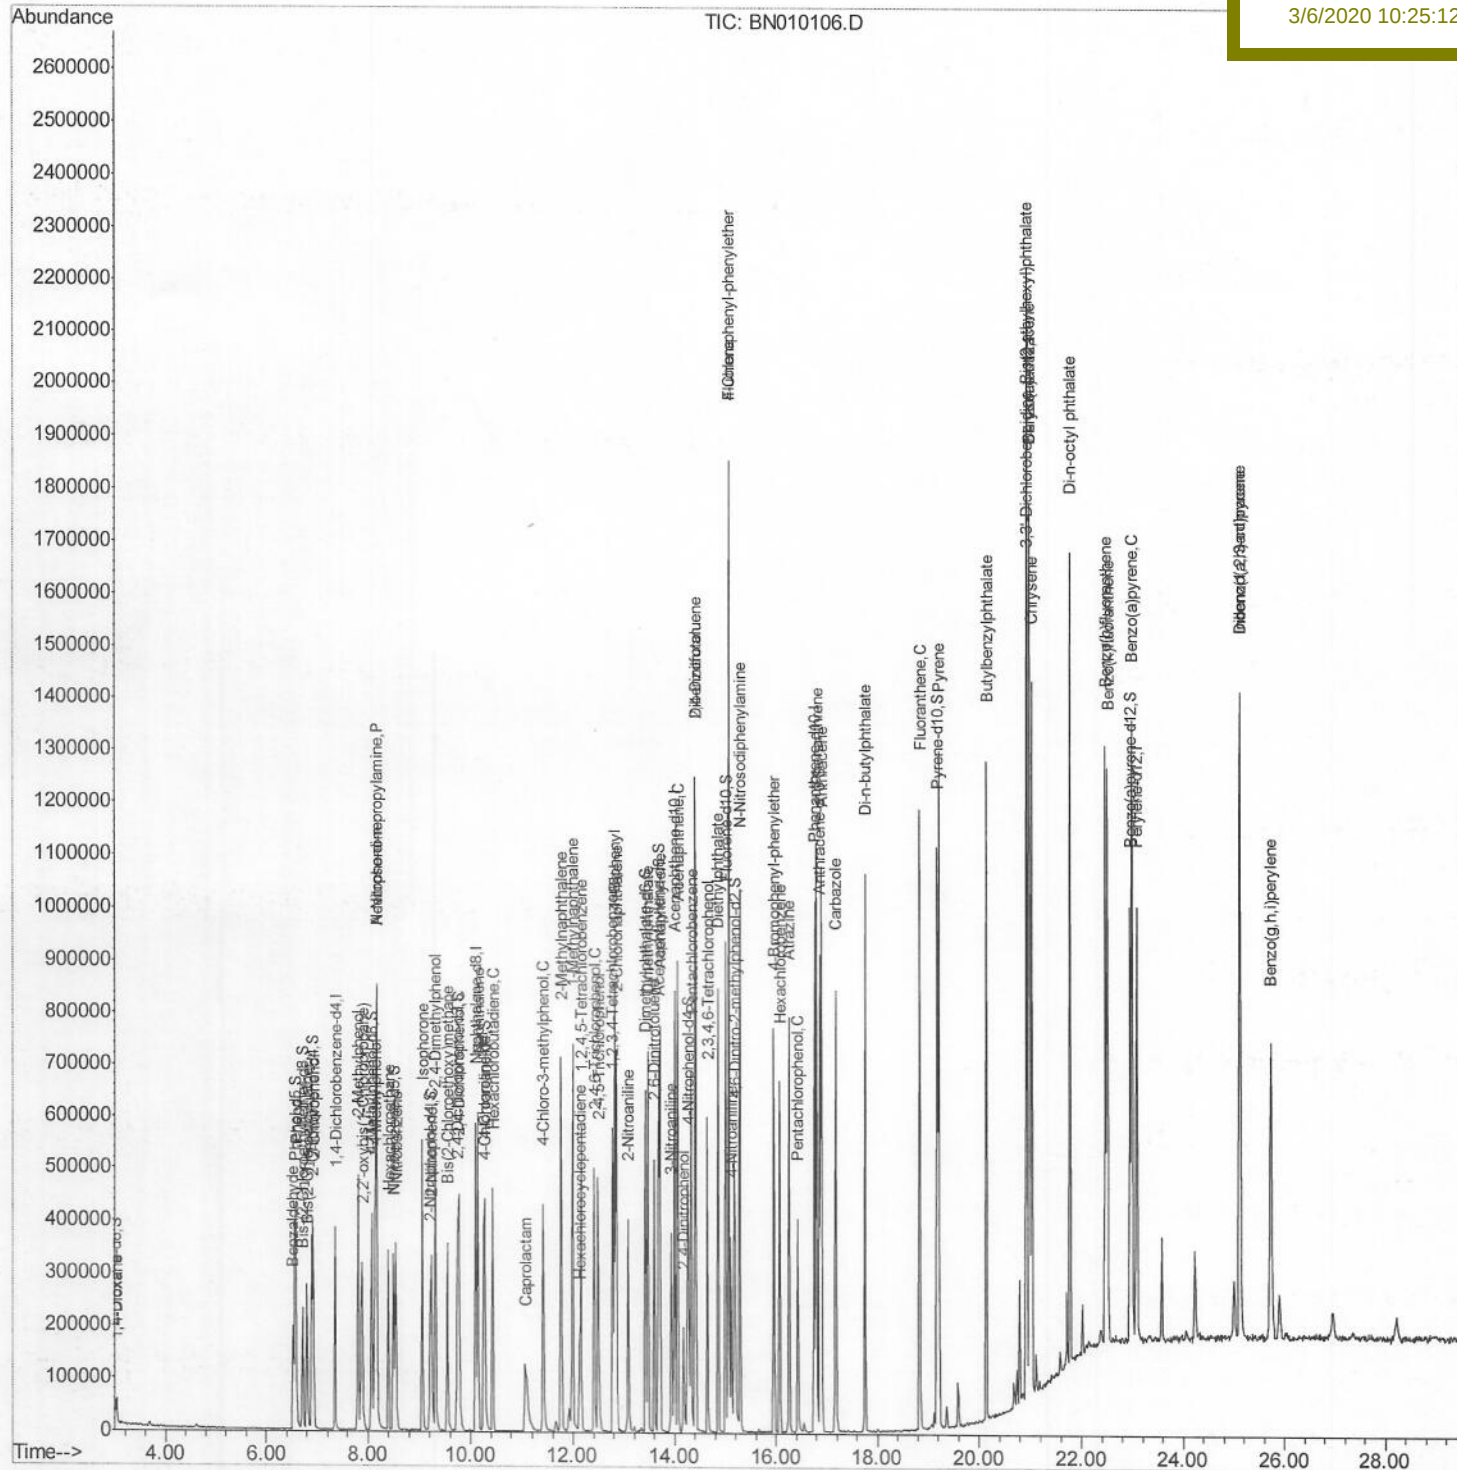

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030420\

Data File : BN010106.D

Acq On : 05 Mar 2020 09:11

Operator : CG/JU

Sample : SSTDCCC020EC

Misc :

ALS Vial : 33 Sample Multiplier: 1

Quant Time: Mar 05 16:39:54 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Thu Mar 05 14:04:18 2020

Response via : Initial Calibration

Instrument :

BNA_N

LabSampleId :




SSTD02082

Manual Integrations

APPROVED

mohammad

3/6/2020 10:25:12 AM

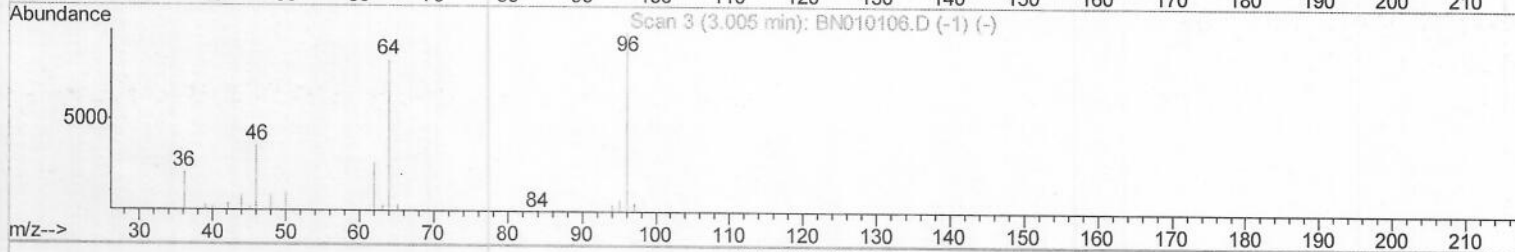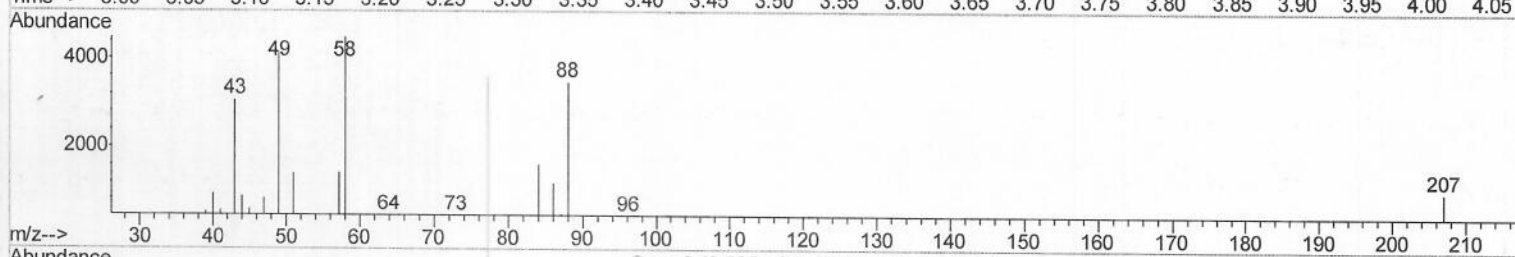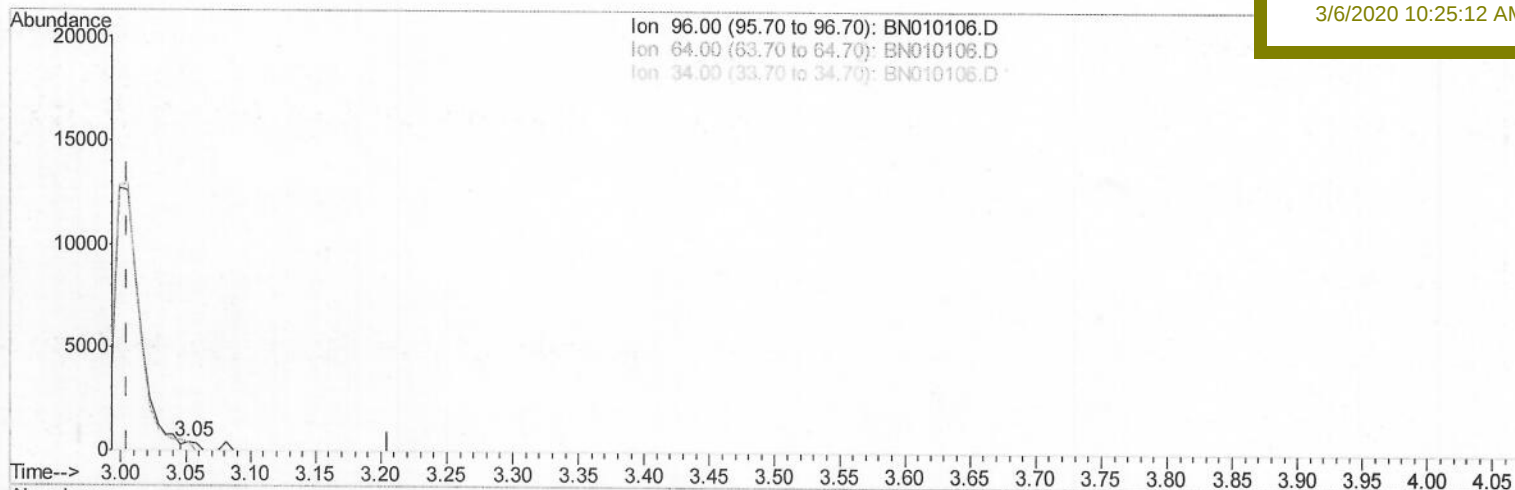

TIC: BN010106.D

(3) 1,4-Dioxane-d8 (S)

3.052min (+0.047) 0.12ng/uL

response 272

Ion	Exp%	Act%
96.00	100	100
64.00	93.60	101.39
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030420\
Data File : BN010106.D
Acq On : 05 Mar 2020 09:11
Operator : CG/JU
Sample : SSTDCCC020EC
Misc :
ALS Vial : 33 Sample Multiplier: 1

Quant Time: Mar 05 16:39:54 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 05 14:04:18 2020
Response via : Initial Calibration

Instrument :
BNA_N
LabSampleId :
SSTD02082

Manual Integrations
APPROVED

mohammad
3/6/2020 10:25:12 AM

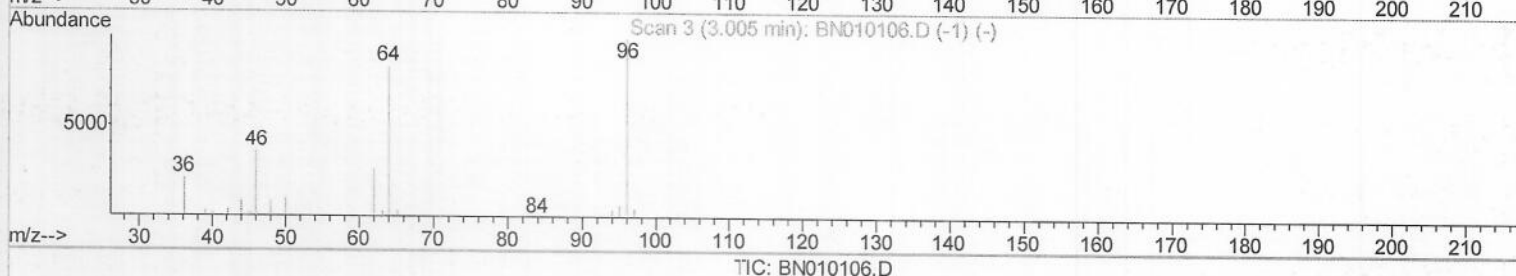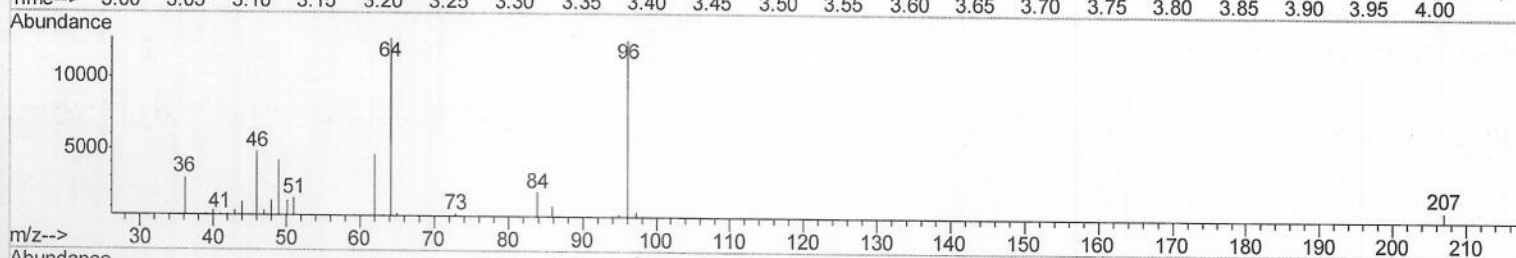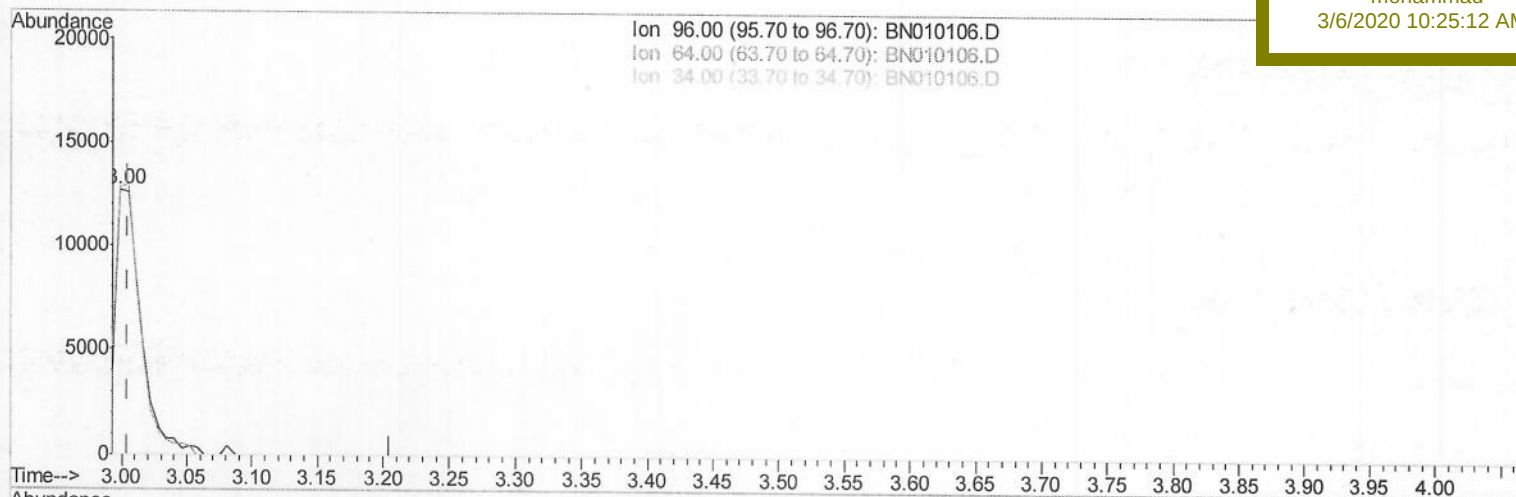

(3) 1,4-Dioxane-d8 (S)

2.999min (-0.006) 6.99ng/uL m

response 15977

Ion	Exp%	Act%
96.00	100	100
64.00	93.60	100.68
34.00	0.00	0.00
0.00	0.00	0.00

JU 03/06/20

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030420\
 Data File : BN010106.D
 Acq On : 05 Mar 2020 09:11
 Operator : CG/JU
 Sample : SSTDCCC020EC
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Quant Time: Mar 05 16:39:54 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 05 14:04:18 2020
 Response via : Initial Calibration

Instrument :
 BNA_N
 LabSampleId :
 SSTD02082

Manual Integrations
 APPROVED

mohammad
 3/6/2020 10:25:12 AM

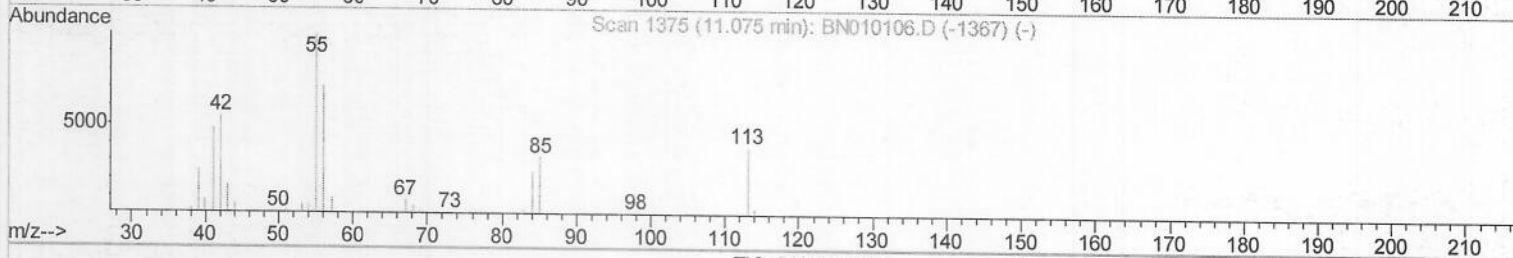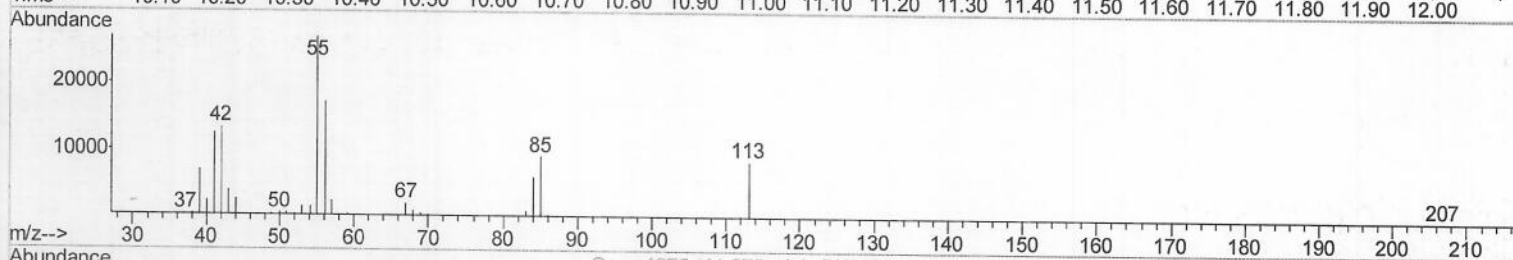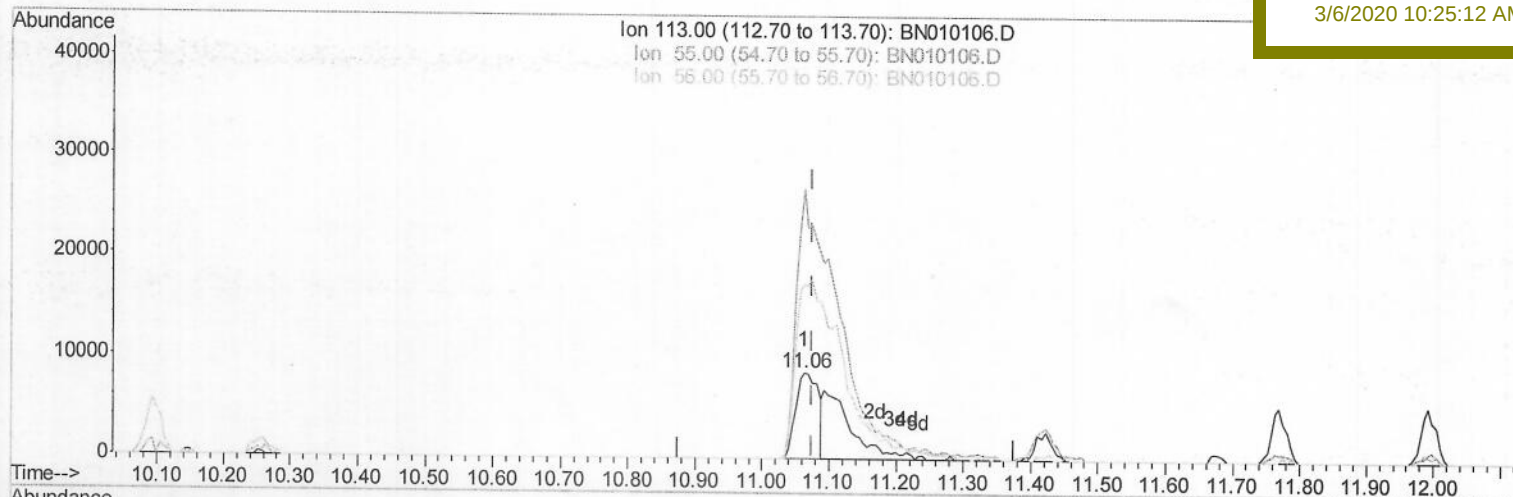

TIC: BN010106.D

(32) Caprolactam

11.063min (-0.012) 9.03ng/ul

response 19406

Ion	Exp%	Act%
113.00	100	100
55.00	261.40	313.92#
56.00	202.00	201.36
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030420\
 Data File : BN010106.D
 Acq On : 05 Mar 2020 09:11
 Operator : CG/JU
 Sample : SSTDCCC020EC
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Quant Time: Mar 05 16:39:54 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 05 14:04:18 2020
 Response via : Initial Calibration

Instrument :
 BNA_N
LabSampleId :
 SSTD02082

Manual Integrations
APPROVED

mohammad
 3/6/2020 10:25:12 AM

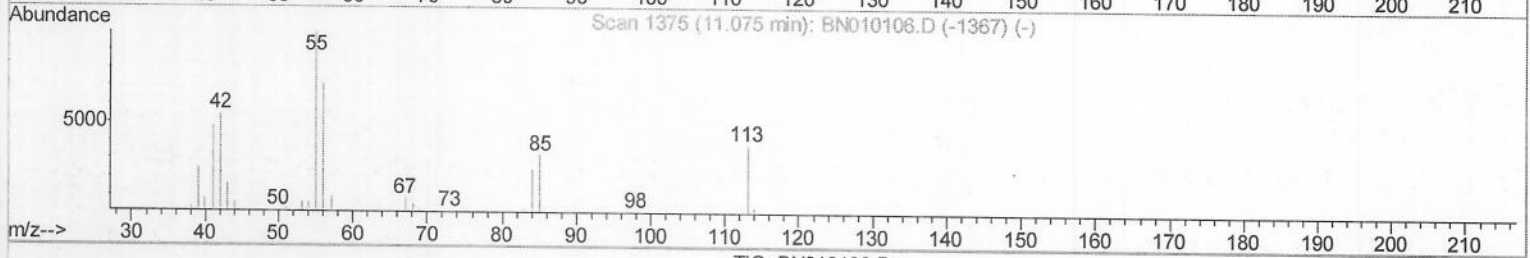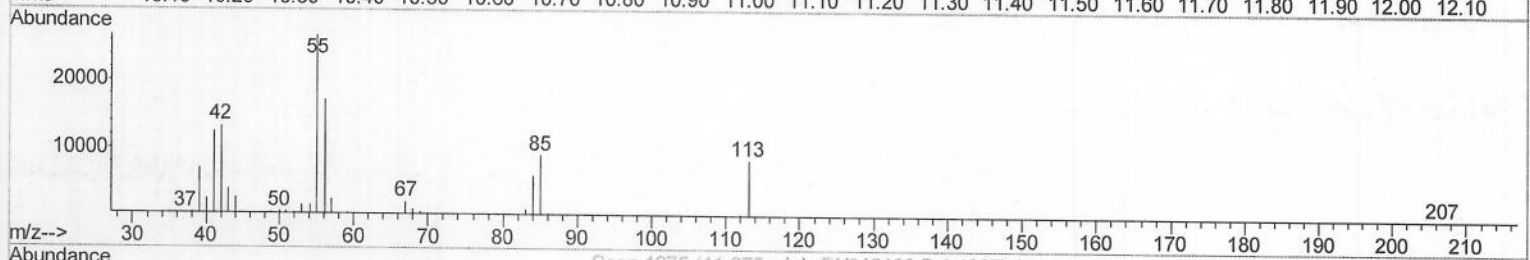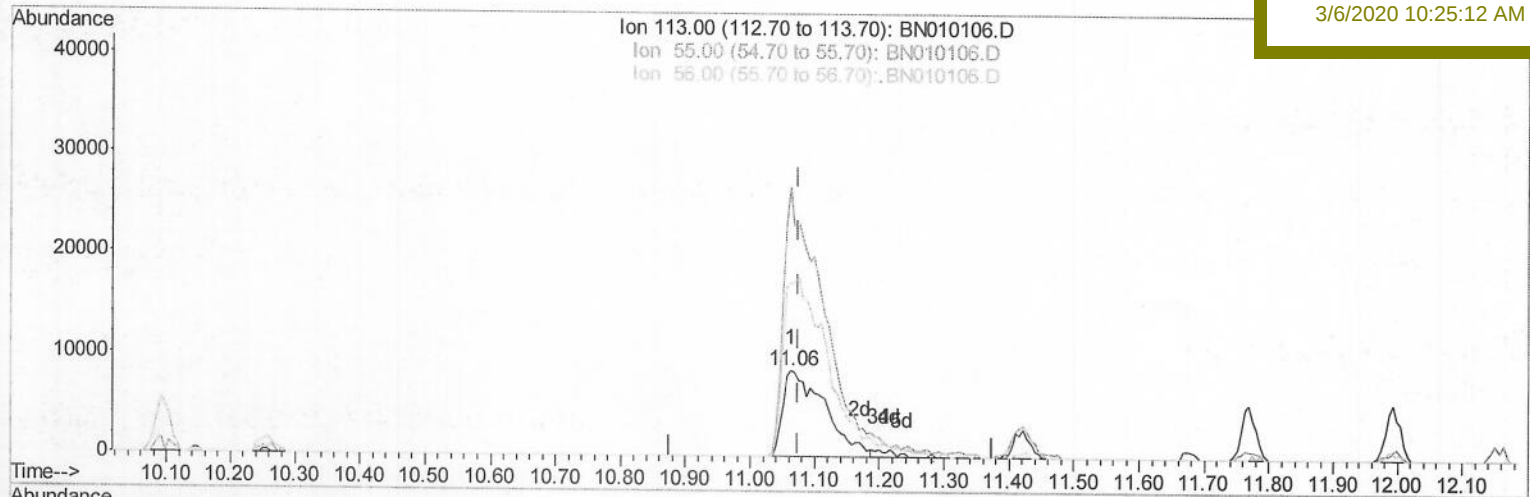

TIC: BN010106.D

(32) Caprolactam

11.063min (-0.012) 18.03ng/ul m

response 38745

Ion	Exp%	Act%
113.00	100	100
55.00	261.40	313.92#
56.00	202.00	201.36
0.00	0.00	0.00

> 5003/06/20

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030420\
 Data File : BN010106.D
 Acq On : 05 Mar 2020 09:11
 Operator : CG/JU
 Sample : SSTDCCC020EC
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_N
 LabSampleId :
 SSTD02082

Manual Integrations
 APPROVED

mohammad
 3/6/2020 10:25:12 AM

Quant Time: Mar 05 16:41:10 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 05 14:04:18 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.35	152	94050	20.00	ng/ul	0.00
18) Naphthalene-d8	10.09	136	412824	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.00	164	264437	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.76	188	560123	20.00	ng/ul	0.00
78) Chrysene-d12	20.99	240	496226	20.00	ng/ul	0.00
86) Perylene-d12	23.09	264	539406	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.00	96	15977m	6.99	ng/uL	0.00
5) Phenol-d5	6.56	99	165624	20.70	ng/ul	0.00
7) Bis-(2-Chloroethyl) ether-d	6.71	67	108327	19.62	ng/ul	0.00
9) 2-Chlorophenol-d4	6.89	132	126202	20.95	ng/ul	0.00
13) 4-Methylphenol-d8	8.07	113	128848	20.25	ng/ul	0.00
19) Nitrobenzene-d5	8.49	128	61061	20.22	ng/ul	0.00
22) 2-Nitrophenol-d4	9.21	143	69511	21.04	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.74	165	128612	20.25	ng/ul	0.00
29) 4-Chloroaniline-d4	10.26	131	158703	22.24	ng/ul	0.00
44) Dimethylphthalate-d6	13.43	166	385929	19.54	ng/ul	0.00
47) Acenaphthylene-d8	13.68	160	447717	19.25	ng/ul	0.00
52) 4-Nitrophenol-d4	14.26	143	60453	16.76	ng/ul	0.00
58) Fluorene-d10	15.00	176	334157	19.59	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.17	200	63020	18.11	ng/ul	0.00
71) Anthracene-d10	16.86	188	495271	19.29	ng/ul	0.00
79) Pyrene-d10	19.17	212	530922	20.47	ng/ul	0.00
90) Benzo(a)pyrene-d12	22.95	264	526271	19.54	ng/ul	0.00

JU
 03/06/20

Target Compounds

					Qvalue
2) 1,4-Dioxane	3.03	88	18489	7.04	ng/uL 94
4) Benzaldehyde	6.52	77	70732	13.30	ng/ul 89
6) Phenol	6.59	94	173509	20.24	ng/ul 93
8) Bis(2-Chloroethyl) ether	6.80	93	135790	20.15	ng/ul 96
10) 2-Chlorophenol	6.92	128	134728	21.24	ng/ul 97
11) 2-Methylphenol	7.80	108	128396	20.47	ng/ul 99
12) 2,2'-oxybis(1-Chloropropan	7.89	45	341355	20.67	ng/ul 98
14) Acetophenone	8.17	105	216691	20.90	ng/ul 99
15) N-Nitroso-di-n-propylamine	8.16	70	120874	22.31	ng/ul 98
16) 4-Methylphenol	8.13	108	142280	20.67	ng/ul 93
17) Hexachloroethane	8.39	117	58145	20.15	ng/ul 93
20) Nitrobenzene	8.54	77	176805	19.87	ng/ul 97
21) Isophorone	9.06	82	319293	20.39	ng/ul 99
23) 2-Nitrophenol	9.24	139	77571	20.98	ng/ul 100
24) 2,4-Dimethylphenol	9.31	107	165877	20.66	ng/ul 99
25) Bis(2-Chloroethoxy)methane	9.55	93	187081	19.54	ng/ul 99
27) 2,4-Dichlorophenol	9.77	162	133123	20.77	ng/ul 99
28) Naphthalene	10.15	128	432785	19.44	ng/ul 99
30) 4-Chloroaniline	10.28	127	169147	23.15	ng/ul 100
31) Hexachlorobutadiene	10.43	225	83813	19.56	ng/ul# 86
32) Caprolactam	11.06	113	38745m	18.03	ng/ul
33) 4-Chloro-3-methylphenol	11.42	107	153133	20.90	ng/ul 99
34) 2-Methylnaphthalene	11.77	142	318124	20.58	ng/ul 97

JU
 03/06/20

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030420\
 Data File : BN010106.D
 Acq On : 05 Mar 2020 09:11
 Operator : CG/JU
 Sample : SSTDCCC020EC
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Quant Time: Mar 05 16:41:10 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 05 14:04:18 2020
 Response via : Initial Calibration

Instrument :
 BNA_N
 LabSampleId :
 SSTD02082

Manual Integrations
 APPROVED

mohammad
 3/6/2020 10:25:12 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
35) 1-Methylnaphthalene	11.99	142	299590	19.34	ng/uL	99
37) 1,2,4,5-Tetrachlorobenzene	12.16	216	162788	20.77	ng/uL	96
38) Hexachlorocyclopentadiene	12.13	237	39313	11.59	ng/uL	99
39) 2,4,6-Trichlorophenol	12.42	196	105012	21.11	ng/uL	96
40) 2,4,5-Trichlorophenol	12.49	196	111453	20.88	ng/uL	98
41) 1,1'-Biphenyl	12.82	154	418175	20.59	ng/uL	98
42) 2-Chloronaphthalene	12.85	162	321776	19.95	ng/uL	99
43) 2-Nitroaniline	13.09	65	125314	21.24	ng/uL	98
45) Dimethylphthalate	13.47	163	396805	19.25	ng/uL	99
46) 2,6-Dinitrotoluene	13.60	165	81334	20.16	ng/uL	97
48) Acenaphthylene	13.71	152	491554	19.52	ng/uL	99
49) 3-Nitroaniline	13.93	138	76024	20.41	ng/uL	90
50) Acenaphthene	14.06	153	335739	19.45	ng/uL	96
51) 2,4-Dinitrophenol	14.17	184	39599	17.10	ng/uL	96
53) 4-Nitrophenol	14.27	109	60172	18.49	ng/uL	92
54) Dibenzofuran	14.40	168	486597	20.09	ng/uL	97
55) 2,4-Dinitrotoluene	14.41	165	120666	20.18	ng/uL	96
56) 2,3,4,6-Tetrachlorophenol	14.65	232	95533	20.82	ng/uL	98
57) Diethylphthalate	14.86	149	406884	19.23	ng/uL	98
59) Fluorene	15.06	166	395201	19.44	ng/uL	98
60) 4-Chlorophenyl-phenylether	15.06	204	194748	19.42	ng/uL	96
61) 4-Nitroaniline	15.11	138	76014	16.73	ng/uL	91
64) 4,6-Dinitro-2-methylphenol	15.19	198	66744	17.81	ng/uL	98
65) N-Nitrosodiphenylamine	15.29	169	346161	20.83	ng/uL	99
66) 4-Bromophenyl-phenylether	15.96	248	112289	20.03	ng/uL	95
67) Hexachlorobenzene	16.07	284	121275	19.55	ng/uL	94
68) Atrazine	16.26	200	118482	18.79	ng/uL	94
69) Pentachlorophenol	16.43	266	63725	17.78	ng/uL	95
70) Phenanthrene	16.80	178	607857	19.02	ng/uL	99
72) Anthracene	16.89	178	626116	19.16	ng/uL	100
73) 1,2,3,4-Tetrachlorobenzene	12.77	216	158030	19.31	ng/uL	95
74) Pentachlorobenzene	14.33	250	152215	19.29	ng/uL	93
75) Carbazole	17.18	167	552268	19.19	ng/uL	98
76) Di-n-butylphthalate	17.76	149	686104	19.32	ng/uL	99
77) Fluoranthene	18.84	202	690194	18.43	ng/uL	96
80) Pyrene	19.20	202	717714	20.06	ng/uL	96
81) Butylbenzylphthalate	20.14	149	309998	21.08	ng/uL	95
82) 3,3'-Dichlorobenzidine	20.92	252	208870	19.31	ng/uL	99
83) Benzo(a)anthracene	20.97	228	701892	20.58	ng/uL	96
84) Bis(2-ethylhexyl)phthalate	20.93	149	462665	20.61	ng/uL	97
85) Chrysene	21.03	228	649598	19.35	ng/uL	96
87) Di-n-octyl phthalate	21.78	149	777285	19.04	ng/uL	100
88) Benzo(b)fluoranthene	22.47	252	677412	19.37	ng/uL	98
89) Benzo(k)fluoranthene	22.52	252	654885	19.78	ng/uL	95
91) Benzo(a)pyrene	23.00	252	639866	20.34	ng/uL	99
92) Indeno(1,2,3-cd)pyrene	25.12	276	717463	19.21	ng/uL	95
93) Dibenzo(a,h)anthracene	25.12	278	610138	19.10	ng/uL	97
94) Benzo(g,h,i)perylene	25.73	276	592420	18.92	ng/uL	98

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030420\
Data File : BN010106.D
Acq On : 05 Mar 2020 09:11
Operator : CG/JU
Sample : SSTDCCC020EC
Misc :
ALS Vial : 33 Sample Multiplier: 1

Quant Time: Mar 05 16:41:10 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 05 14:04:18 2020
Response via : Initial Calibration

Instrument :
BNA_N
LabSampleId :
SSTD02082

Manual Integrations
APPROVED

mohammad
3/6/2020 10:25:12 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)

(#) = qualifier out of range (m) = manual integration (+) = signals summed						