

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030519\NOT REVIEWED DATA\
 Data File : BN004624.D
 Acq On : 05 Mar 2019 14:38
 Operator : JU/SJ
 Sample : K1626-12
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BF672

Quant Time: Mar 06 00:32:17 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 06 00:29:18 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.73	152	24352	20.00	ng/ul	-0.02
18) Naphthalene-d8	10.52	136	118286	20.00	ng/ul	-0.02
36) Acenaphthene-d10	14.37	164	75700	20.00	ng/ul	-0.02
62) Phenanthrene-d10	17.12	188	188065	20.00	ng/ul	-0.02
78) Chrysene-d12	21.32	240	255111	20.00	ng/ul	0.00
86) Perylene-d12	23.59	264	273780	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.23	96	3232	7.98	ng/uL	-0.01
5) Phenol-d5	6.89	99	38704	17.83	ng/ul	-0.01
7) Bis-(2-Chloroethyl)ether-d	7.07	67	21062	19.34	ng/ul	-0.02
9) 2-Chlorophenol-d4	7.26	132	35314	20.06	ng/ul	-0.02
13) 4-Methylphenol-d8	8.42	113	35410	18.98	ng/ul	-0.02
19) Nitrobenzene-d5	8.89	128	17877	22.83	ng/ul	-0.01
22) 2-Nitrophenol-d4	9.60	143	20194	24.71	ng/ul	-0.02
26) 2,4-Dichlorophenol-d3	10.13	165	37815	20.41	ng/ul	-0.01
29) 4-Chloroaniline-d4	10.66	131	53715	26.21	ng/ul	-0.02
44) Dimethylphthalate-d6	13.78	166	131995	20.56	ng/ul	-0.02
47) Acenaphthylene-d8	14.06	160	157131	20.66	ng/ul	-0.02
52) 4-Nitrophenol-d4	14.57	143	18049	14.69	ng/ul	-0.01
58) Fluorene-d10	15.36	176	116030	20.53	ng/ul	-0.02
63) 4,6-Dinitro-2-methylphenol	15.49	200	13570	12.37	ng/ul	-0.01
71) Anthracene-d10	17.22	188	191187	21.21	ng/ul	-0.02
79) Pyrene-d10	19.52	212	234076	20.47	ng/ul	-0.01
90) Benzo(a)pyrene-d12	23.44	264	277347	19.30	ng/ul	-0.02


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
6) Phenol	6.92	94	2466	1.138	ng/ul	97
45) Dimethylphthalate	13.83	163	20658	3.255	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030519\NOT REVIEWED DATA\
Data File : BN004624.D
Acq On : 05 Mar 2019 14:38
Operator : JU/SJ
Sample : K1626-12
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BF672

Quant Time: Mar 06 00:32:17 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 06 00:29:18 2019
Response via : Initial Calibration

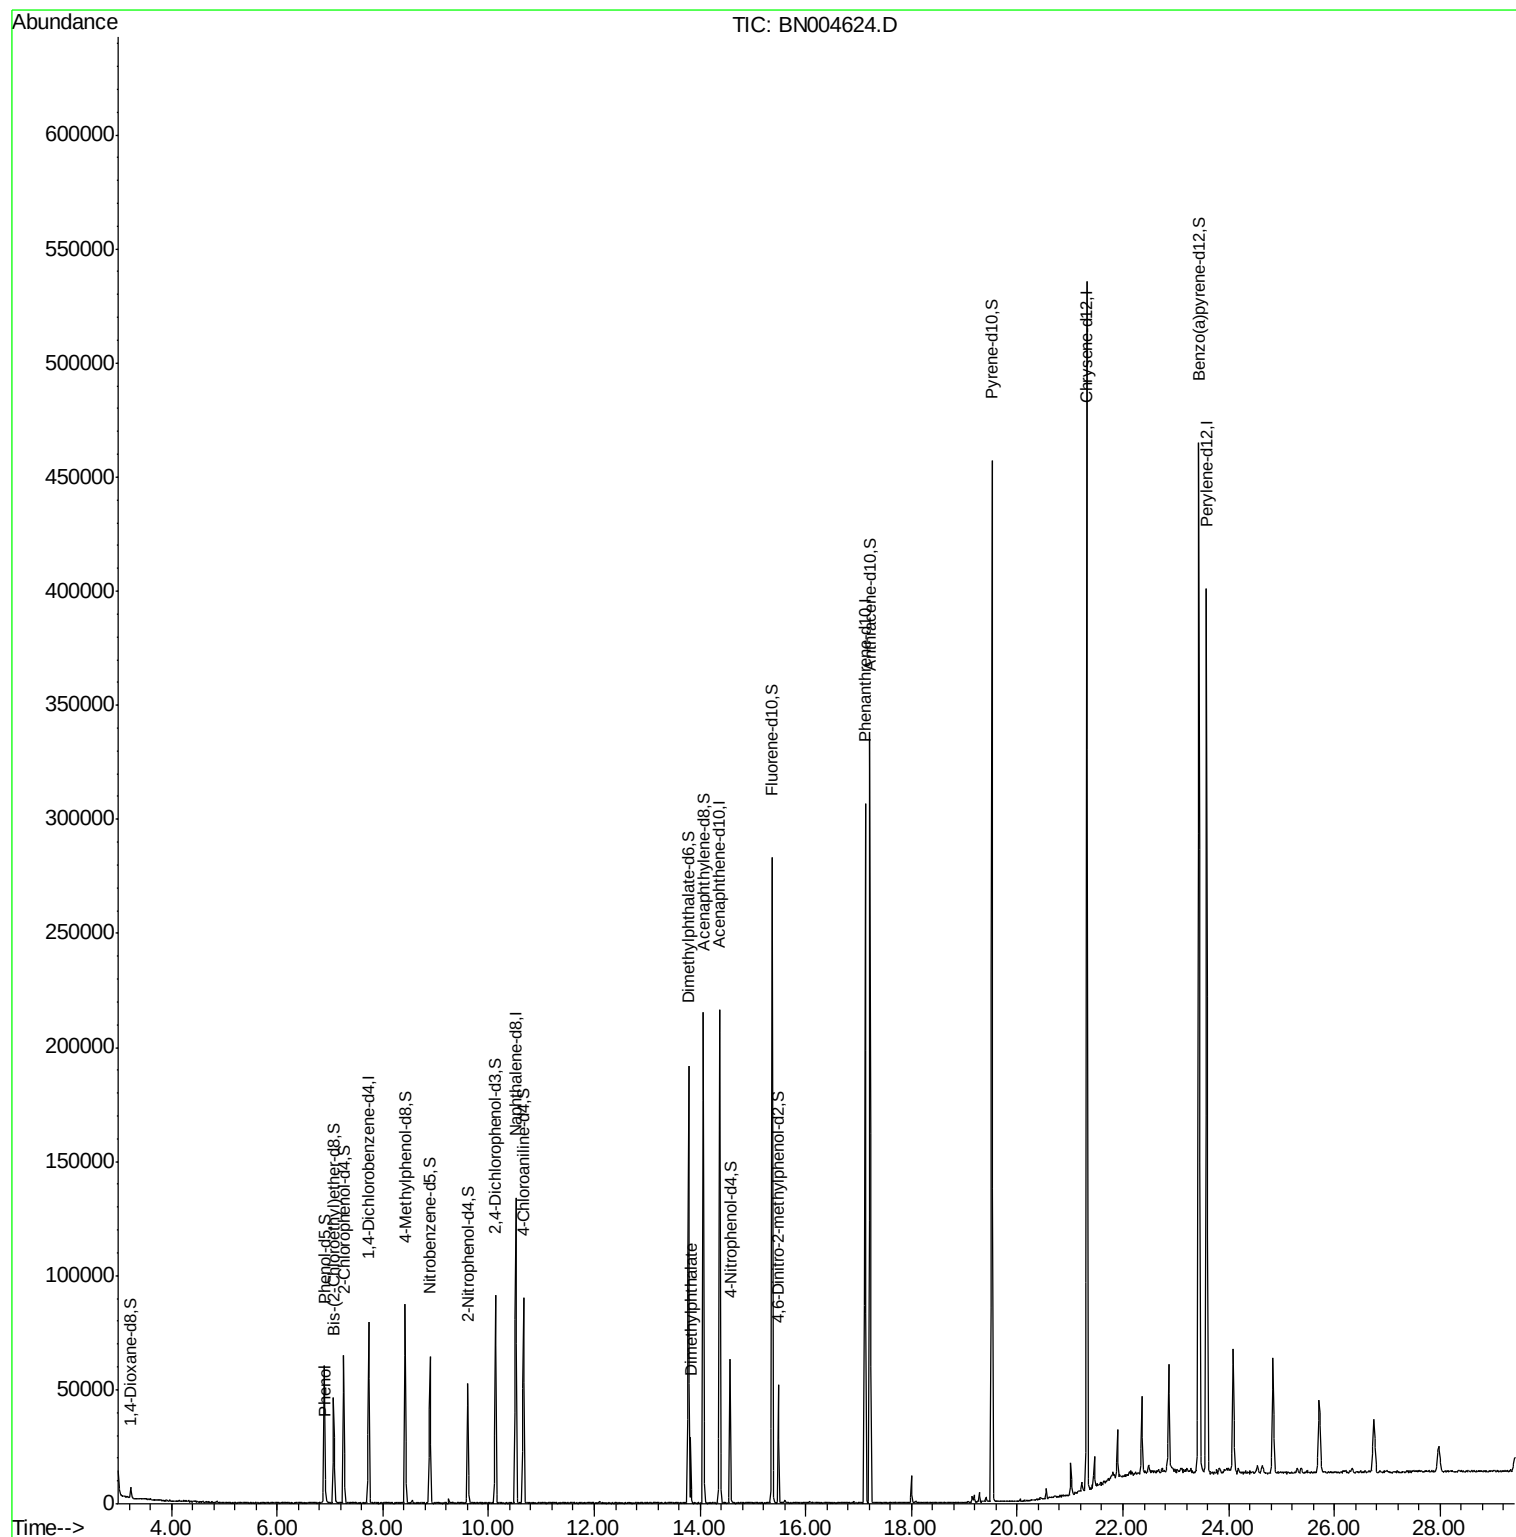

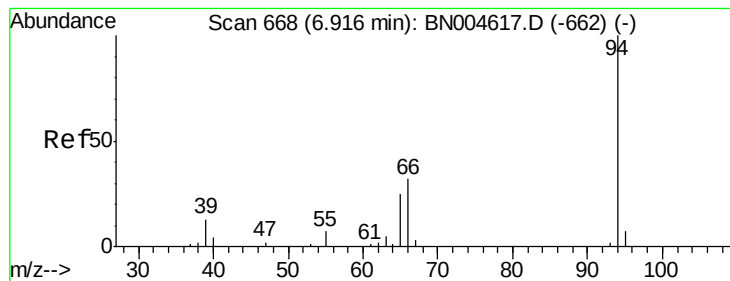

#6

Phenol

Concen: 1.138 ng/ul

RT: 6.92 min Scan# 668

Delta R.T. -0.02 min

Lab File: BN004624.D

Acq: 05 Mar 2019 14:38

Instrument :

BNA_N

ClientSampleId :

BF672


Tgt Ion: 94 Resp: 2466

Ion Ratio Lower Upper

94 100

65 23.2 20.2 30.4

66 36.6 28.2 42.2



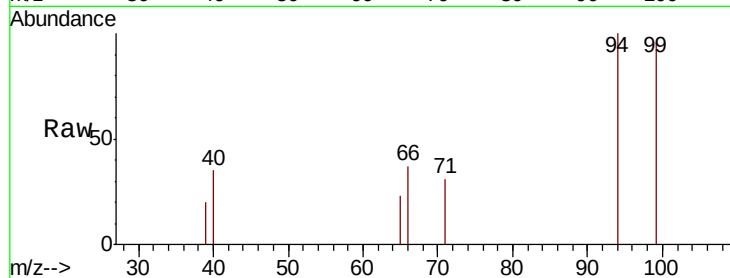


Abundance

Ion 94.00 (93.70 to 94.70): BN0

Ion 65.00 (64.70 to 65.70): BN0

Ion 66.00 (65.70 to 66.70): BN0

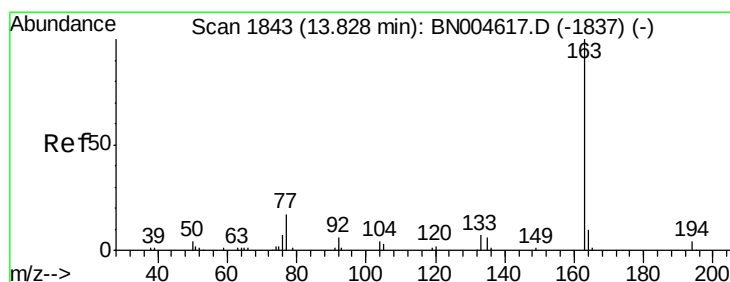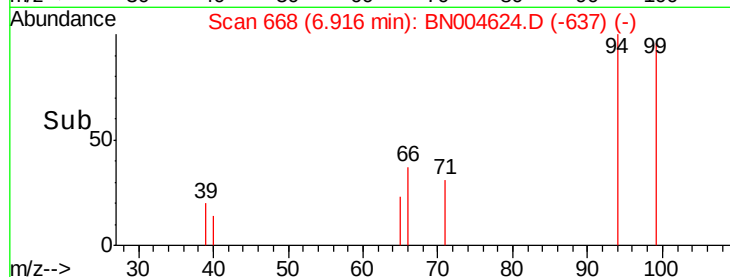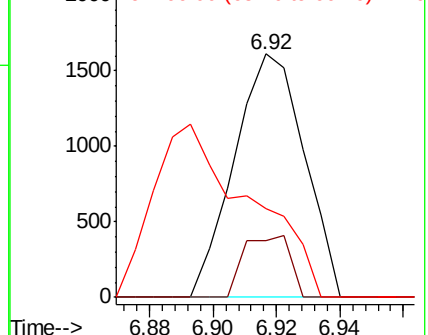

#45

Dimethylphthalate

Concen: 3.255 ng/ul

RT: 13.83 min Scan# 1843

Delta R.T. -0.02 min

Lab File: BN004624.D

Acq: 05 Mar 2019 14:38


Tgt Ion: 163 Resp: 20658

Ion Ratio Lower Upper

163 100

194 4.6 3.4 5.2

164 10.1 7.9 11.9

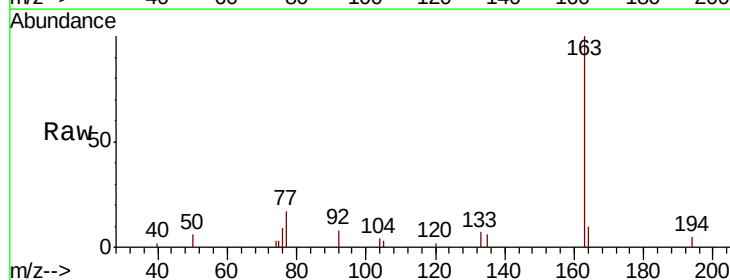

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

