

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030519\NOT REVIEWED DATA\
 Data File : BN004626.D
 Acq On : 05 Mar 2019 15:49
 Operator : JU/SJ
 Sample : K1626-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BF663

Quant Time: Mar 06 00:32:27 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 06 00:29:18 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.73	152	24321	20.00	ng/ul	-0.02
18) Naphthalene-d8	10.52	136	116892	20.00	ng/ul	-0.02
36) Acenaphthene-d10	14.37	164	72391	20.00	ng/ul	-0.02
62) Phenanthrene-d10	17.12	188	178499	20.00	ng/ul	-0.01
78) Chrysene-d12	21.32	240	238445	20.00	ng/ul	0.00
86) Perylene-d12	23.59	264	238081	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.23	96	2125	5.25	ng/uL	-0.01
5) Phenol-d5	6.89	99	27744	12.80	ng/ul	-0.01
7) Bis-(2-Chloroethyl)ether-d	7.07	67	15181	13.96	ng/ul	-0.02
9) 2-Chlorophenol-d4	7.26	132	25259	14.37	ng/ul	-0.01
13) 4-Methylphenol-d8	8.42	113	24232	13.01	ng/ul	-0.02
19) Nitrobenzene-d5	8.89	128	12287	15.88	ng/ul	-0.01
22) 2-Nitrophenol-d4	9.60	143	13548	16.77	ng/ul	-0.02
26) 2,4-Dichlorophenol-d3	10.13	165	26856	14.66	ng/ul	-0.01
29) 4-Chloroaniline-d4	10.66	131	29145	14.39	ng/ul	-0.02
44) Dimethylphthalate-d6	13.78	166	89650	14.60	ng/ul	-0.02
47) Acenaphthylene-d8	14.06	160	106526	14.65	ng/ul	-0.02
52) 4-Nitrophenol-d4	14.57	143	10193	8.67	ng/ul	-0.01
58) Fluorene-d10	15.36	176	82507	15.27	ng/ul	-0.02
63) 4,6-Dinitro-2-methylphenol	15.49	200	7058	6.78	ng/ul	-0.01
71) Anthracene-d10	17.22	188	129639	15.15	ng/ul	-0.02
79) Pyrene-d10	19.52	212	156351	14.63	ng/ul	-0.01
90) Benzo(a)pyrene-d12	23.44	264	182300	14.59	ng/ul	-0.02


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.83	163	12429	2.048	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030519\NOT REVIEWED DATA\
Data File : BN004626.D
Acq On : 05 Mar 2019 15:49
Operator : JU/SJ
Sample : K1626-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BF663

Quant Time: Mar 06 00:32:27 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 06 00:29:18 2019
Response via : Initial Calibration

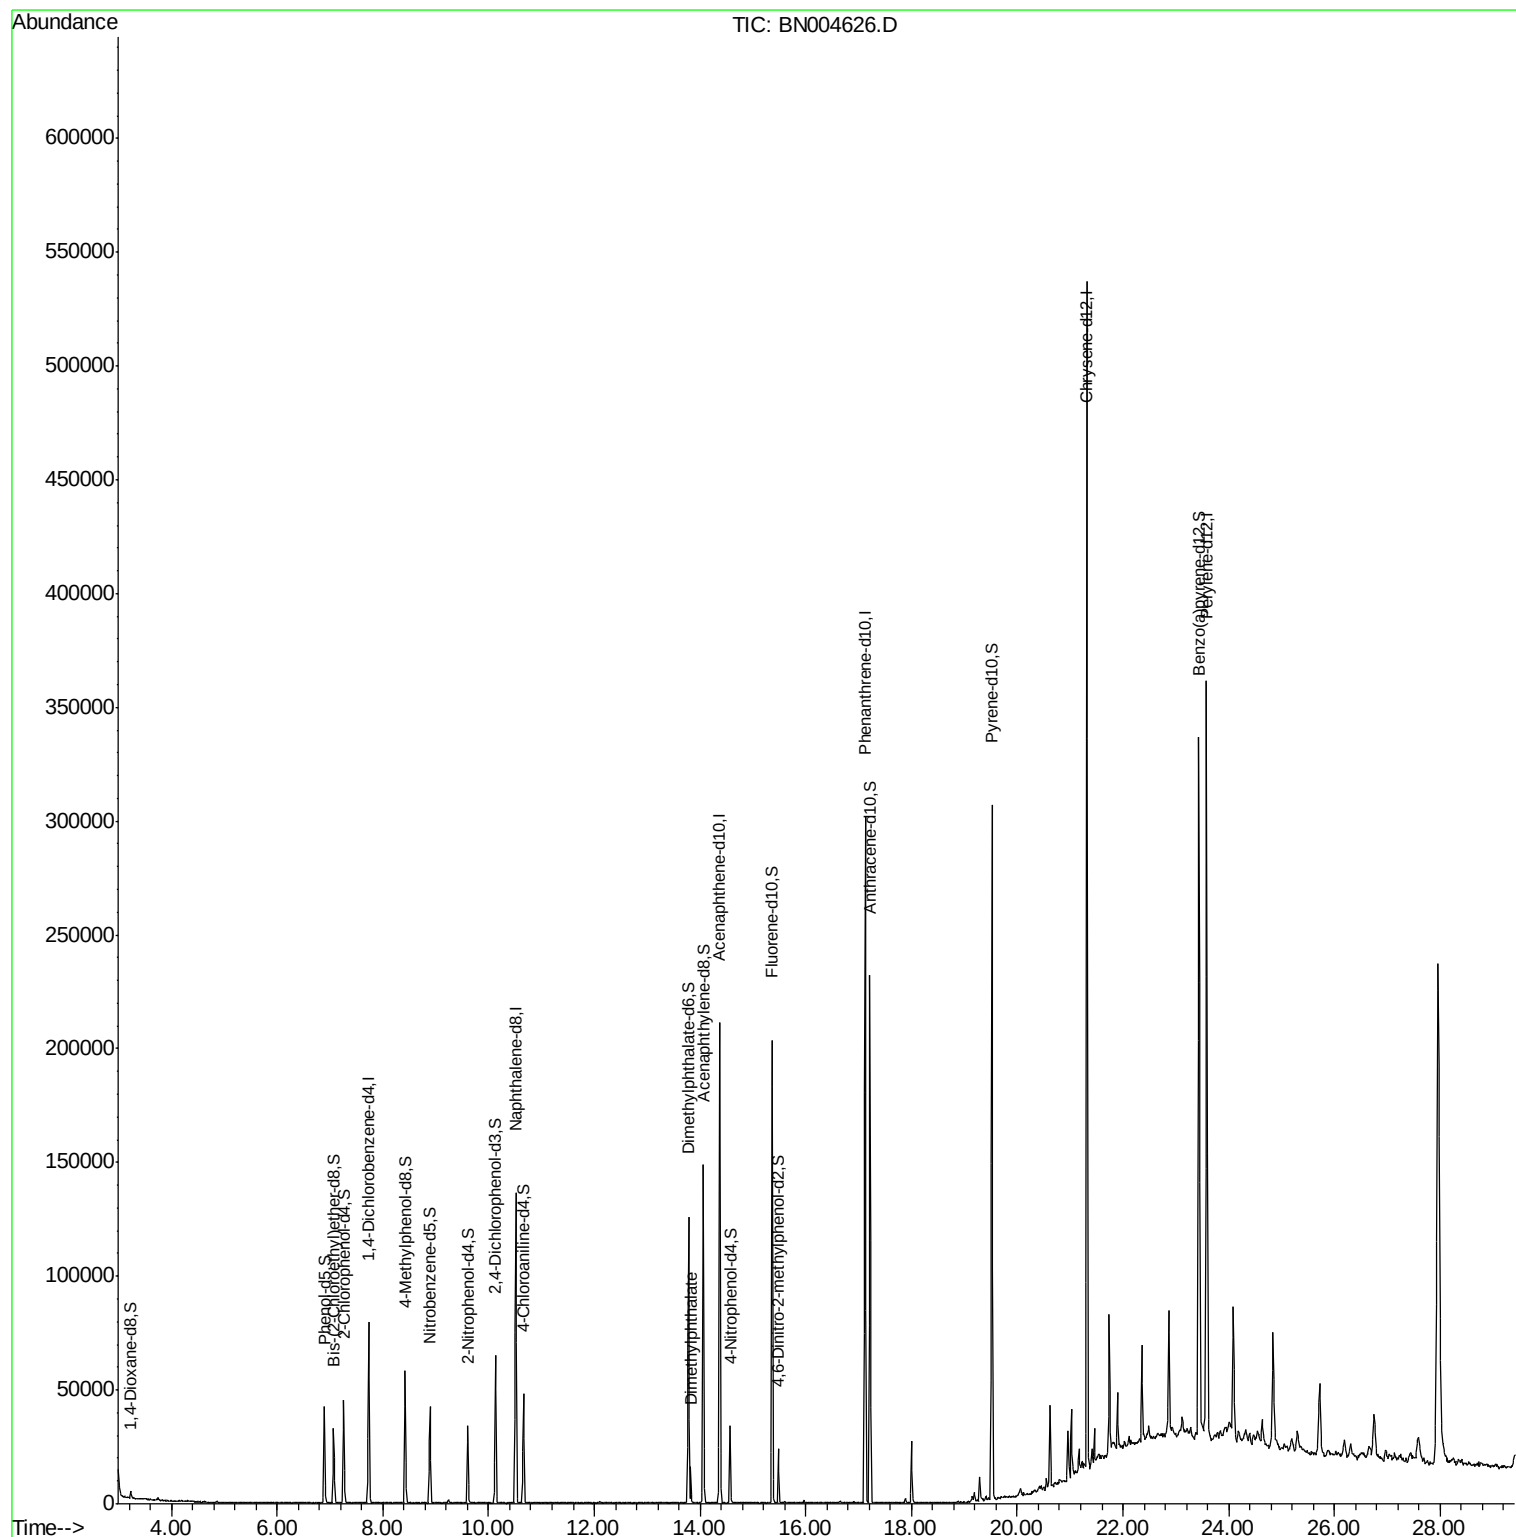

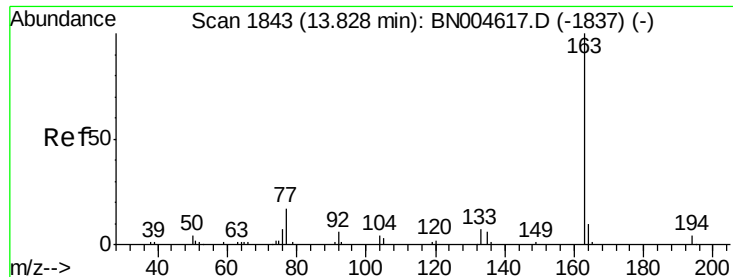

#45

Dimethylphthalate

Concen: 2.048 ng/ul

RT: 13.83 min Scan# 1843

Delta R.T. -0.02 min

Lab File: BN004626.D

Acq: 05 Mar 2019 15:49

Instrument :

BNA_N

ClientSampleId :

BF663


Tgt Ion:163 Resp: 12429

Ion Ratio Lower Upper

163 100

194 4.3 3.4 5.2

164 9.8 7.9 11.9

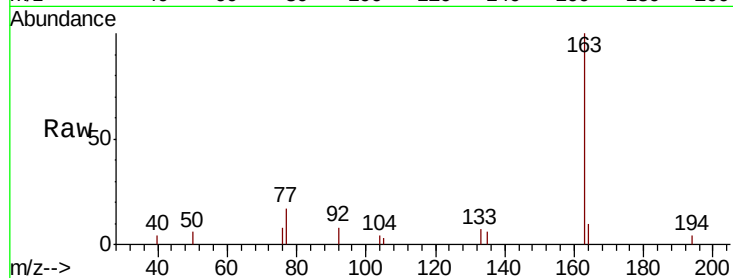

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

