

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN030520\
 Data File : BN010112.D
 Acq On : 05 Mar 2020 19:36
 Operator : CG/JU
 Sample : L1641-17
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB700

Manual Integrations
 APPROVED

mohammad
 3/6/2020 10:18:34 PM

Quant Time: Mar 06 04:18:08 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 05 14:04:18 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.36	152	68493	20.00	ng/ul	0.00
18) Naphthalene-d8	10.10	136	291681	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.00	164	191202	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.76	188	403662	20.00	ng/ul	0.00
78) Chrysene-d12	20.99	240	352791	20.00	ng/ul	0.00
86) Perylene-d12	23.08	264	381827	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.00	96	8642	5.19	ng/uL	0.00
5) Phenol-d5	6.56	99	168429	28.91	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.72	67	117337	29.19	ng/ul	0.00
9) 2-Chlorophenol-d4	6.90	132	131326	29.94	ng/ul	0.00
13) 4-Methylphenol-d8	8.08	113	133960	28.91	ng/ul	0.00
19) Nitrobenzene-d5	8.50	128	65121	30.52	ng/ul	0.00
22) 2-Nitrophenol-d4	9.22	143	73572	31.51	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.75	165	131506	29.30	ng/ul	0.00
29) 4-Chloroaniline-d4	10.26	131	184126	36.52	ng/ul	0.00
44) Dimethylphthalate-d6	13.43	166	450400	31.54	ng/ul	0.00
47) Acenaphthylene-d8	13.69	160	543249	32.30	ng/ul	0.00
52) 4-Nitrophenol-d4	14.27	143	58171m	22.30	ng/ul	0.01
58) Fluorene-d10	15.00	176	390753	31.69	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.17	200	51850	20.68	ng/ul	0.00
71) Anthracene-d10	16.86	188	600789	32.47	ng/ul	0.00
79) Pyrene-d10	19.17	212	628006	34.06	ng/ul	0.00
90) Benzo(a)pyrene-d12	22.95	264	620954	32.57	ng/ul	0.00

Target Compounds

					Ovalue	
2) 1,4-Dioxane	3.04	88	2636	1.378	ng/uL	86
70) Phenanthrene	16.80	178	32631	1.416	ng/ul	96
77) Fluoranthene	18.84	202	48389	1.793	ng/ul	98
80) Pyrene	19.20	202	45928	1.806	ng/ul	98
83) Benzo(a)anthracene	20.97	228	26733	1.103	ng/ul	95
85) Chrysene	21.03	228	24961	1.046	ng/ul	93
88) Benzo(b)fluoranthene	22.47	252	28209	1.139	ng/ul#	88

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030520\
Data File : BN010112.D
Acq On : 05 Mar 2020 19:36
Operator : CG/JU
Sample : L1641-17
Misc :
ALS Vial : 6 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
CB700

Manual Integrations
APPROVED

mohammad
3/6/2020 10:18:34 PM

Quant Time: Mar 06 04:18:08 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 05 14:04:18 2020
Response via : Initial Calibration

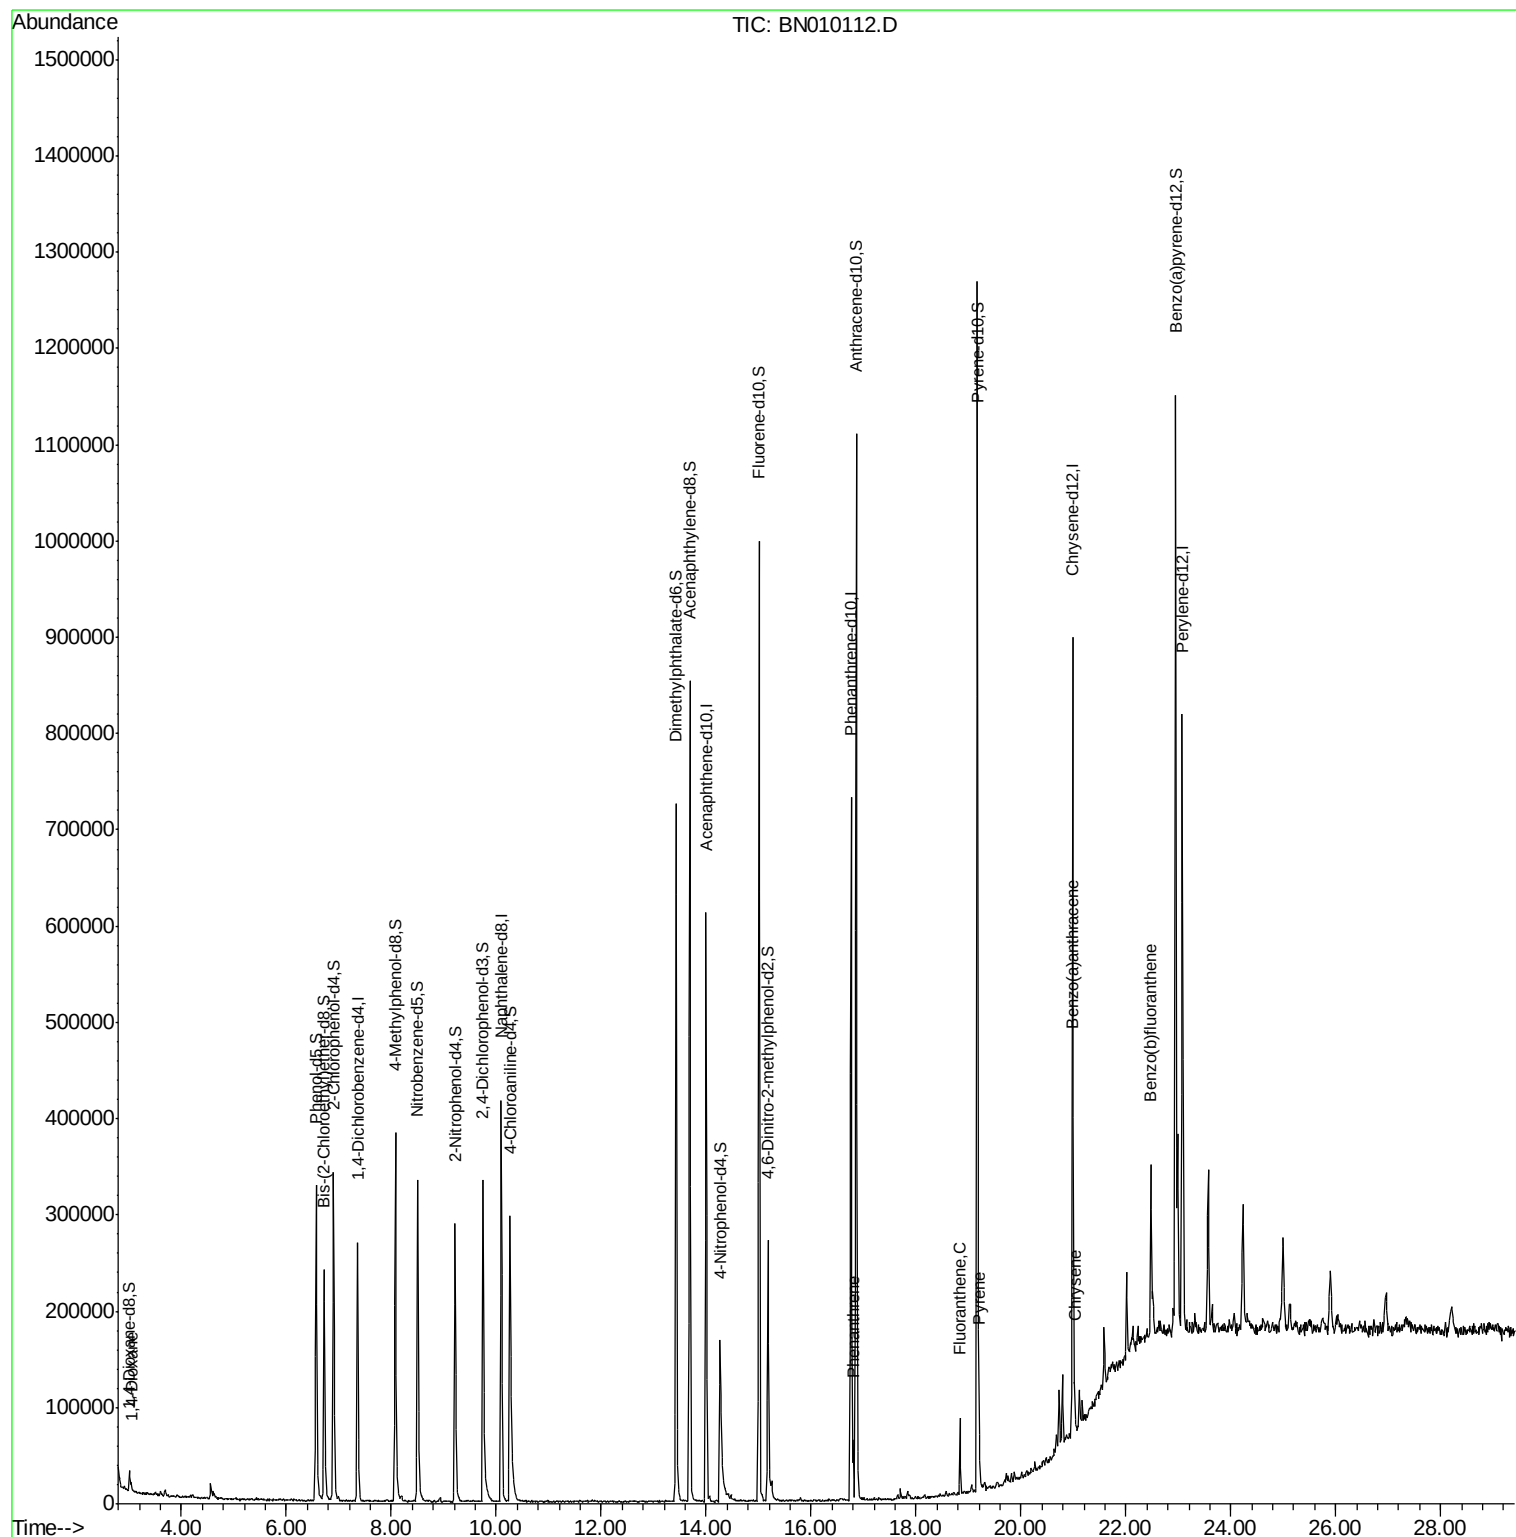

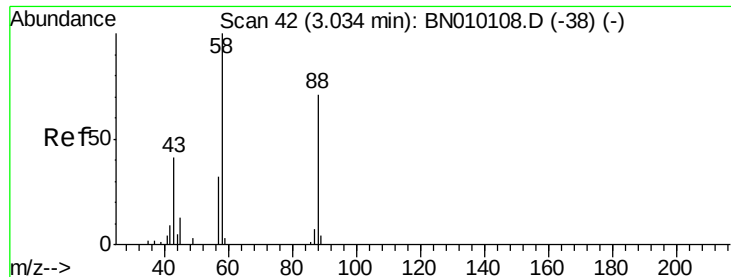

#2

1,4-Dioxane

Concen: 1.378 ng/uL

RT: 3.04 min Scan# 43

Delta R.T. -0.00 min

Lab File: BN010112.D

Acq: 05 Mar 2020 19:36

Instrument :

BNA_N





ClientSampleId :

CB700

Tot Ion:	88	Resp:	2636
Ion	Ratio	Lower	Upper
88	100		
43	46.1	44.7	67.1
58	135.6	96.2	144.2

Manual Integrations
APPROVED

mohammad
3/6/2020 10:18:34 PM

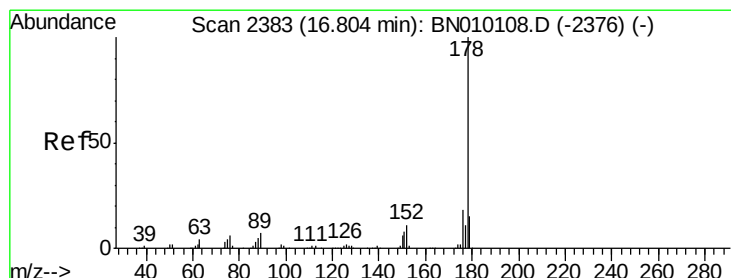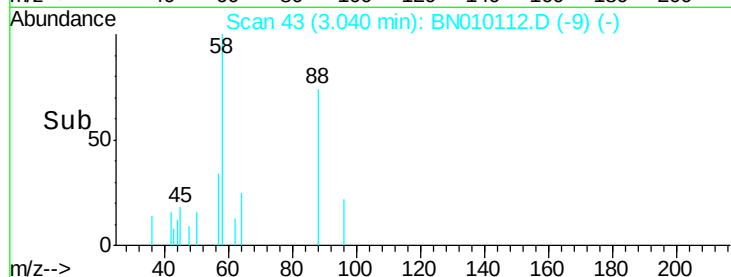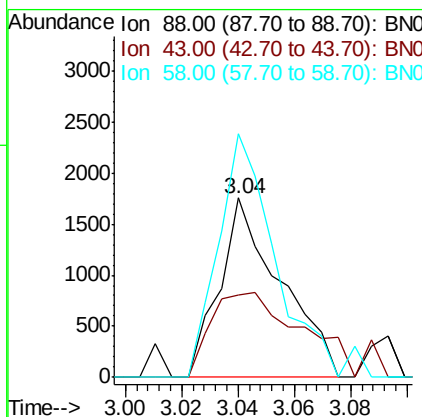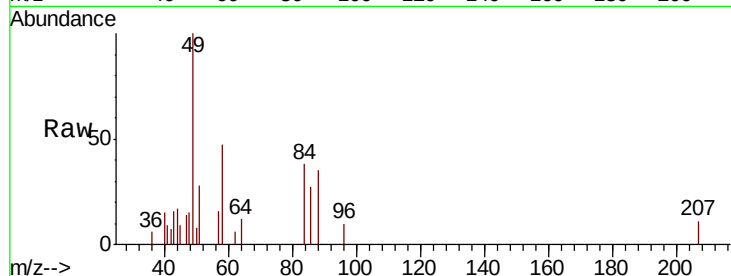

#70

Phenanthrene

Concen: 1.416 ng/uL




RT: 16.80 min Scan# 2383


Delta R.T. -0.00 min

Lab File: BN010112.D

Acq: 05 Mar 2020 19:36

Tgt Ion:	178	Resp:	32631
Ion	Ratio	Lower	Upper
178	100		
179	17.9	12.5	18.7
176	17.3	14.6	22.0

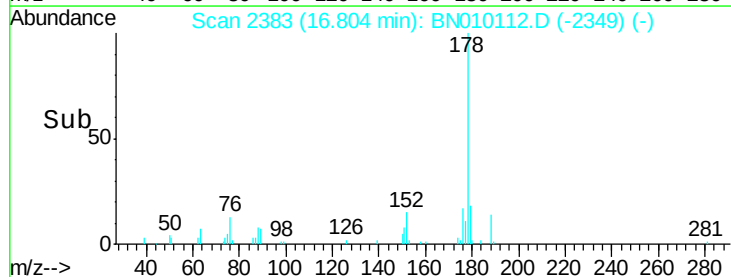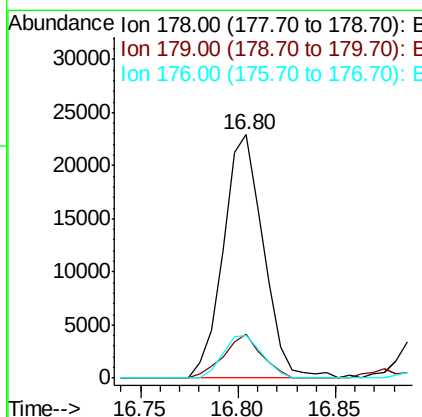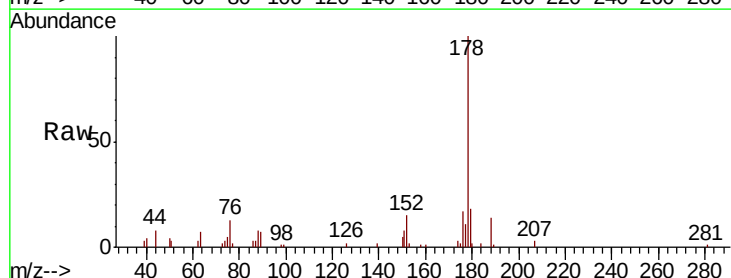

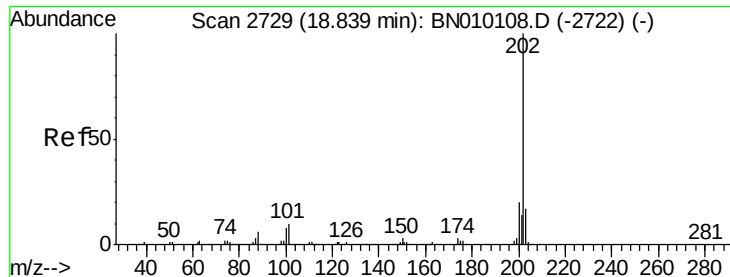





#77
Fluoranthene
Concen: 1.793 ng/ul
RT: 18.84 min Scan# 2729
Delta R.T. -0.00 min
Lab File: BN010112.D
Acq: 05 Mar 2020 19:36

Instrument :
BNA_N
ClientSampleId :
CB700

Tot Ion	Ratio	Resp	Lower	Upper
202	100	48389		
101	12.2		9.4	14.2
100	7.4		7.2	10.8




Manual Integrations
APPROVED


mohammad
3/6/2020 10:18:34 PM

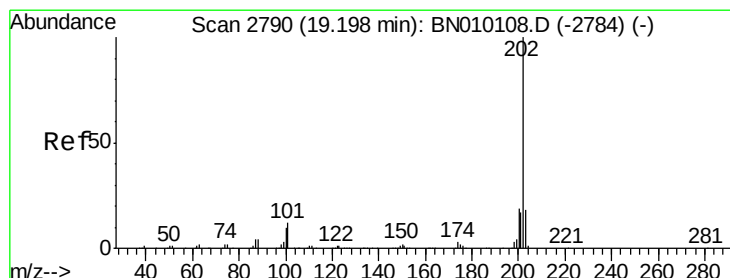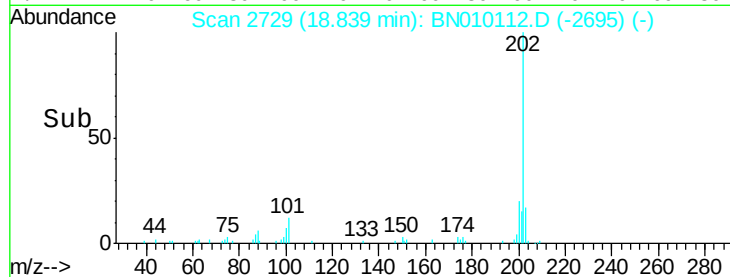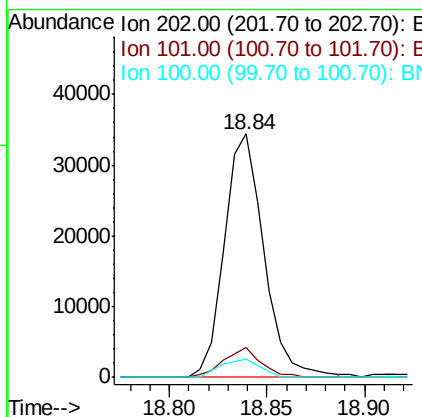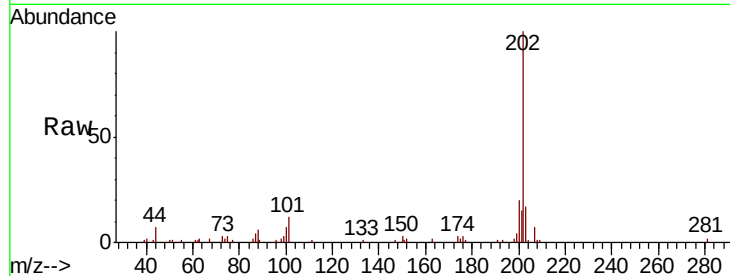

#80
Pyrene
Concen: 1.806 ng/ul
RT: 19.20 min Scan# 2791
Delta R.T. -0.00 min
Lab File: BN010112.D
Acq: 05 Mar 2020 19:36

Tgt Ion	Ratio	Resp	Lower	Upper
202	100	45928		
101	12.7		11.3	16.9
100	11.7		9.0	13.6

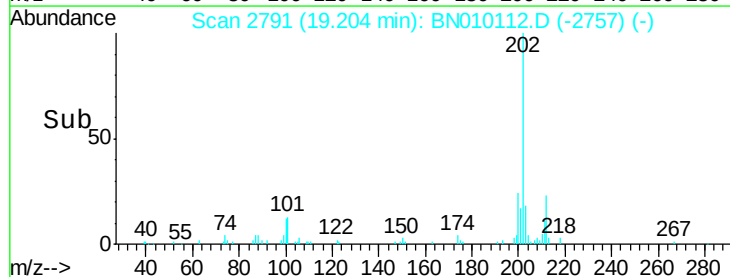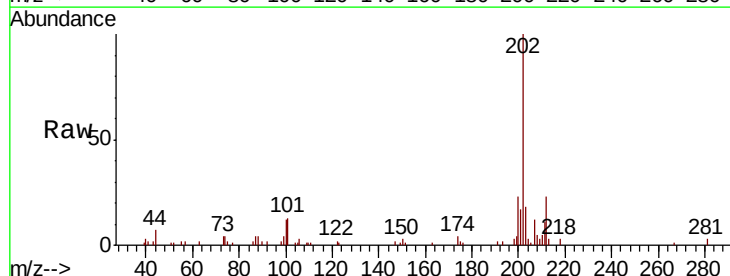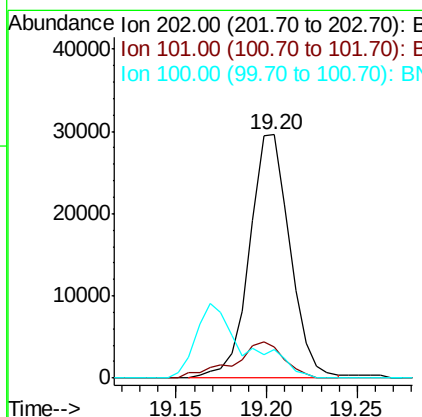

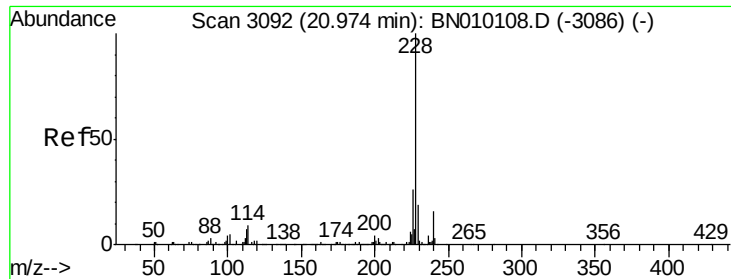





#83
Benzo(a)anthracene
Concen: 1.103 ng/ul
RT: 20.97 min Scan# 3091
Delta R.T. -0.00 min
Lab File: BN010112.D
Acq: 05 Mar 2020 19:36

Instrument :
BNA_N
ClientSampled :
CB700

Tot Ion	Ratio	Lower	Upper
228	100		
229	20.6	15.0	22.4
226	29.5	21.4	32.2




Manual Integrations
APPROVED


mohammad
3/6/2020 10:18:34 PM

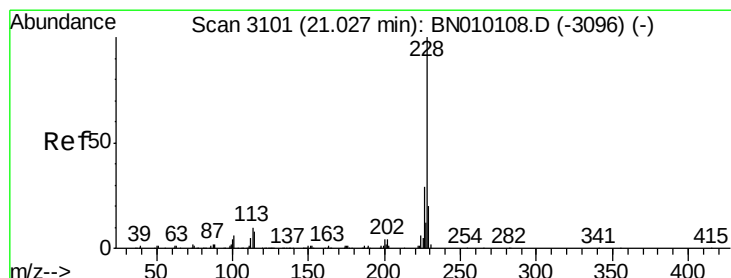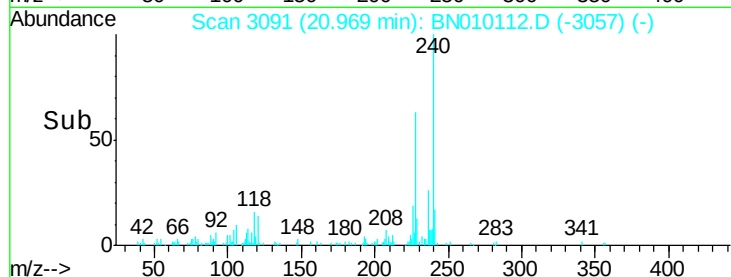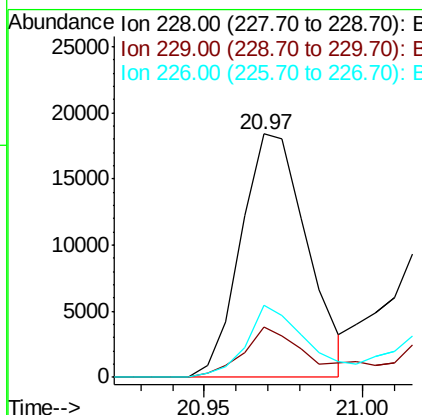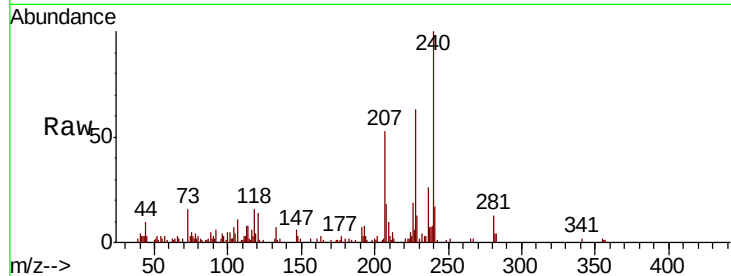

#85
Chrysene
Concen: 1.046 ng/ul
RT: 21.03 min Scan# 3101
Delta R.T. 0.01 min
Lab File: BN010112.D
Acq: 05 Mar 2020 19:36

Tgt Ion	Ratio	Lower	Upper
228	100		
226	25.5	23.4	35.2
229	22.4	15.0	22.4

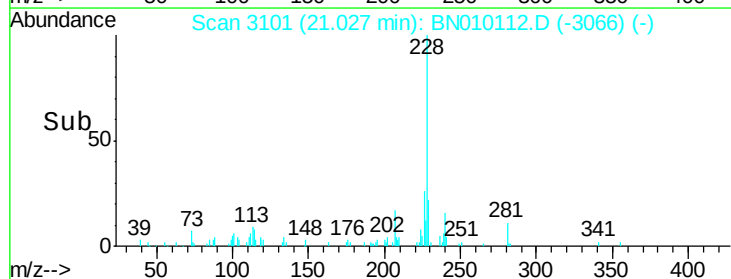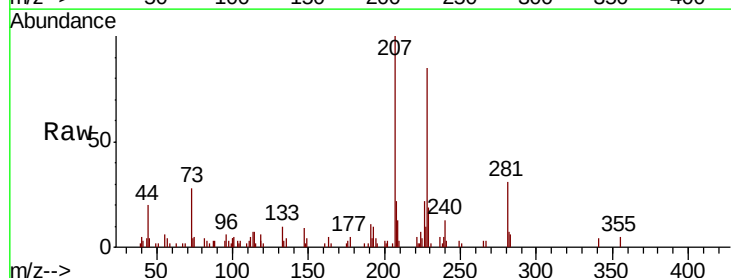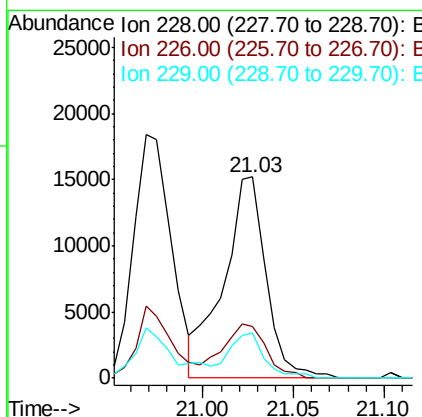

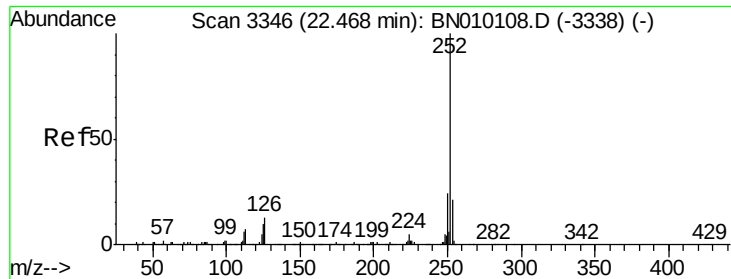

#88

Benzo(b)fluoranthene

Concen: 1.139 ng/ul

RT: 22.47 min Scan# 3347

Delta R.T. 0.01 min

Lab File: BN010112.D

Acq: 05 Mar 2020 19:36

Instrument :

BNA_N

ClientSampleId :

CB700

Tot Ion	Ratio	Resp Lower	Upper
252	100		
253	23.4	17.0	25.4
125	20.1	8.0	12.0

Manual Integrations
APPROVED

mohammad
3/6/2020 10:18:34 PM

