

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN030620\
 Data File : BN010129.D
 Acq On : 06 Mar 2020 21:09
 Operator : CG/JU
 Sample : L1788-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Mar 07 01:59:49 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 05 14:04:18 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.35	152	73317	20.00	ng/ul	0.00
18) Naphthalene-d8	10.10	136	300873	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.00	164	198167	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.76	188	422701	20.00	ng/ul	0.00
78) Chrysene-d12	20.99	240	384840	20.00	ng/ul	0.00
86) Perylene-d12	23.08	264	434260	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.00	96	9182	5.15	ng/uL	0.00
5) Phenol-d5	6.57	99	39507	6.33	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.72	67	120362	27.97	ng/ul	0.00
9) 2-Chlorophenol-d4	6.90	132	111311	23.71	ng/ul	0.00
13) 4-Methylphenol-d8	8.08	113	70061	14.12	ng/ul	0.00
19) Nitrobenzene-d5	8.50	128	64411	29.26	ng/ul	0.00
22) 2-Nitrophenol-d4	9.21	143	76673	31.84	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.75	165	124877	26.98	ng/ul	0.00
29) 4-Chloroaniline-d4	0.00	131	0	0.00	ng/ul	
44) Dimethylphthalate-d6	13.43	166	522867	35.32	ng/ul	0.00
47) Acenaphthylene-d8	13.69	160	560307	32.14	ng/ul	0.00
52) 4-Nitrophenol-d4	14.29	143	10850	4.01	ng/ul	0.03
58) Fluorene-d10	15.00	176	461085	36.08	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.17	200	72699	27.69	ng/ul	0.00
71) Anthracene-d10	16.86	188	754088	38.92	ng/ul	0.00
79) Pyrene-d10	19.17	212	837528	41.64	ng/ul	0.00
90) Benzo(a)pyrene-d12	22.95	264	854475	39.40	ng/ul	0.00


Target Compounds				Ovalue
45) Dimethylphthalate	13.47	163	20486	1.326 ng/ul 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030620\
Data File : BN010129.D
Acq On : 06 Mar 2020 21:09
Operator : CG/JU
Sample : L1788-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Mar 07 01:59:49 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 05 14:04:18 2020
Response via : Initial Calibration

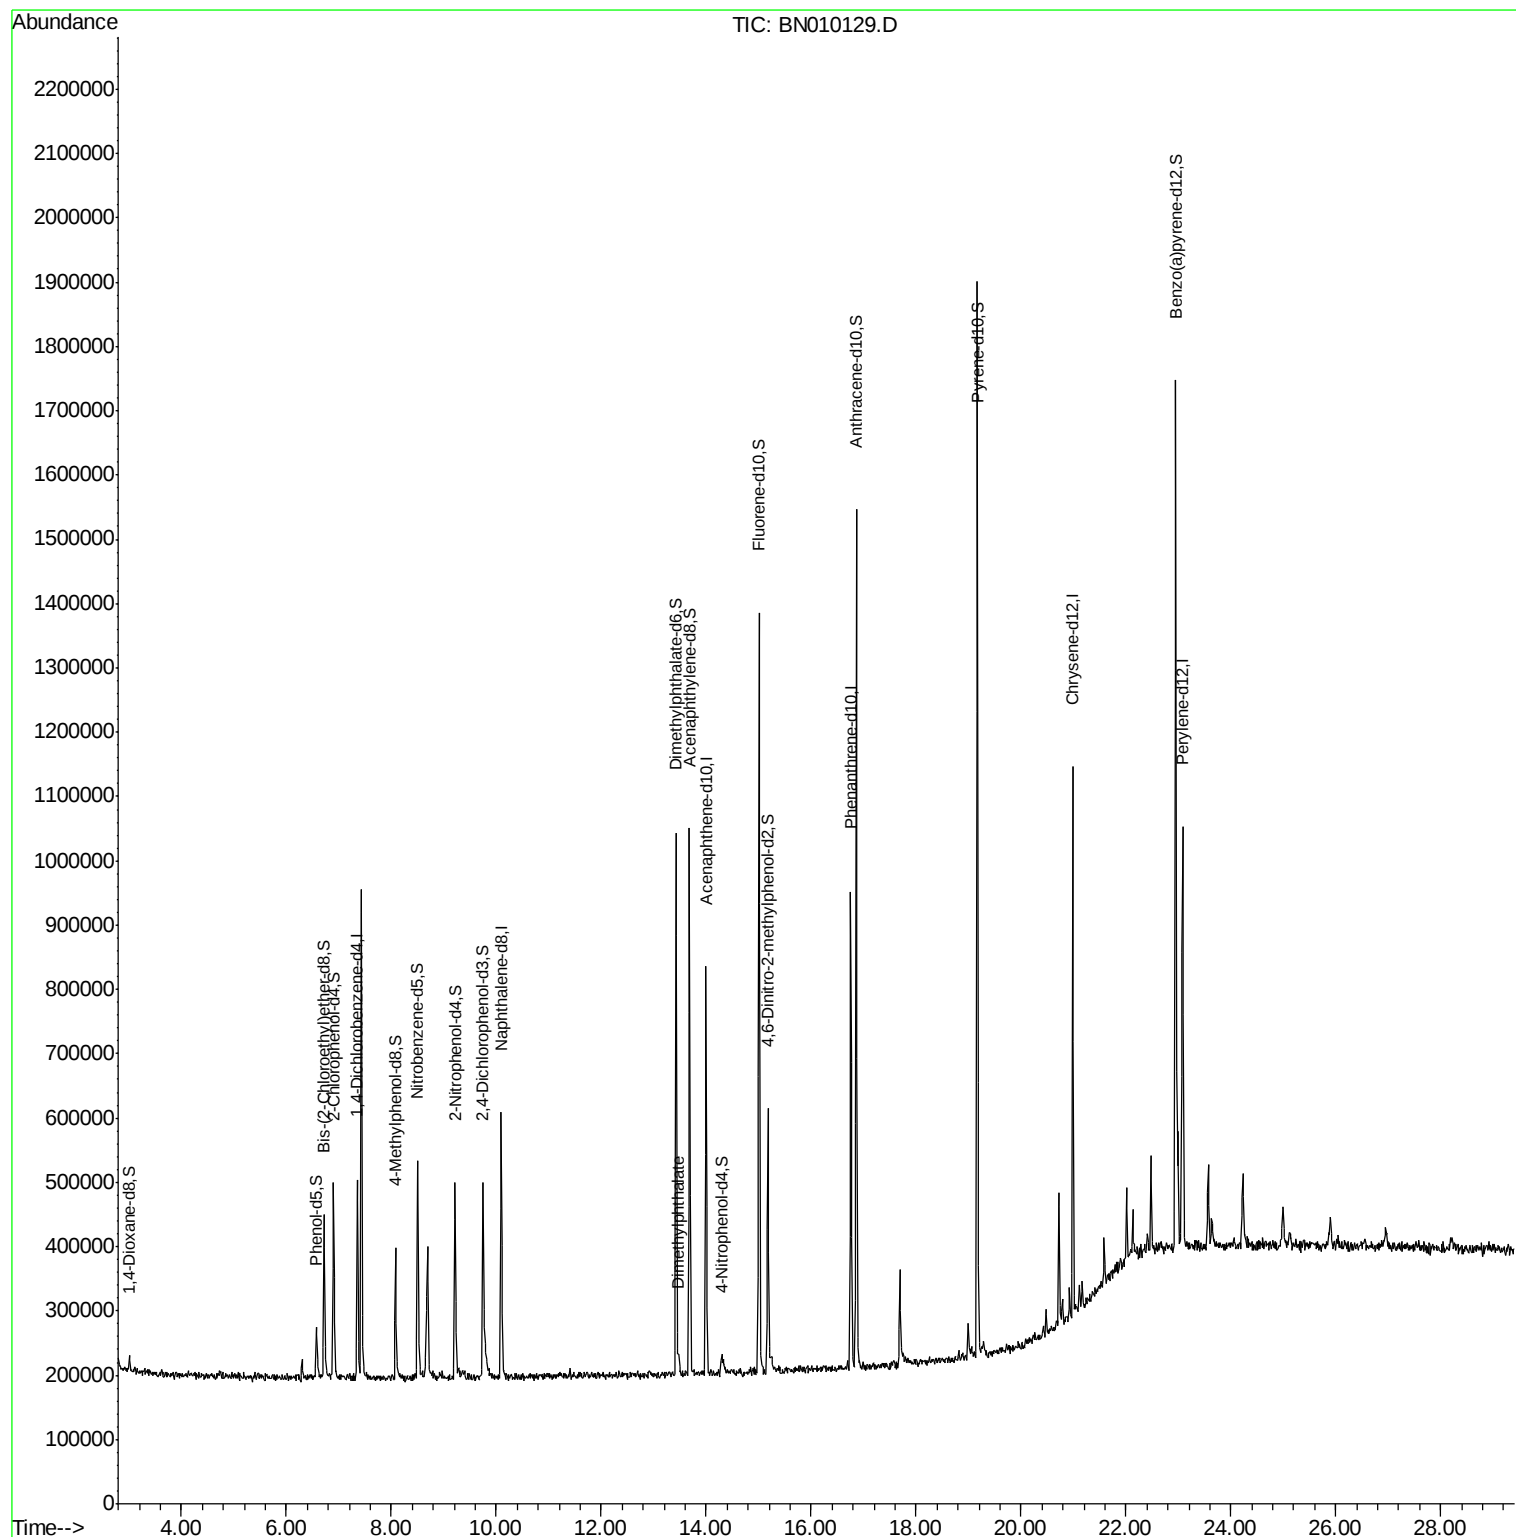

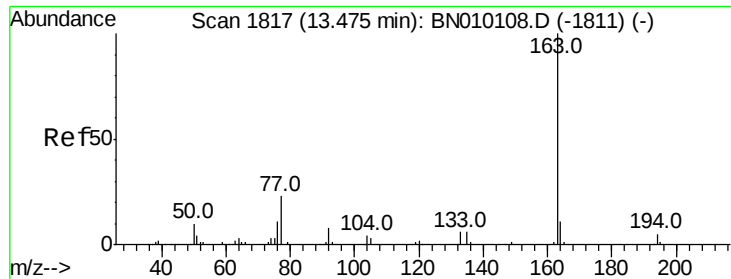

#45

Dimethylphthalate

Concen: 1.326 ng/ul

RT: 13.47 min Scan# 1817

Delta R.T. -0.00 min

Lab File: BN010129.D

Acq: 06 Mar 2020 21:09

Instrument :

BNA_N

ClientSampleId :


Tot Ion:163 Resp: 20486

Ion Ratio Lower Upper

163 100

194 4.5 3.4 5.0

164 11.3 8.0 12.0

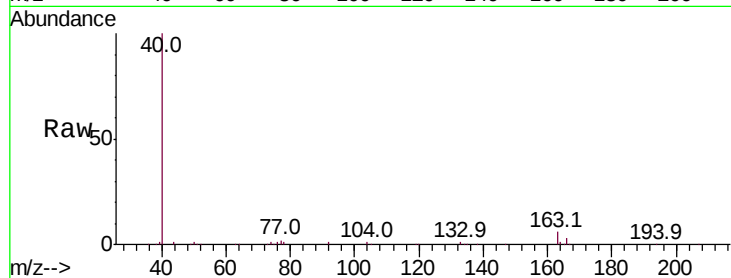

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

