

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN030620\
 Data File : BN010118.D
 Acq On : 06 Mar 2020 14:29
 Operator : CG/JU
 Sample : L1641-07
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB6Z0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.005	35	37	39	rBV	25499	20857	1.52%	0.131%
2	3.311	87	89	92	rVB	9150	6913	0.50%	0.043%
3	3.422	106	108	111	rBV	8722	8137	0.59%	0.051%
4	3.575	132	134	136	rBV2	6380	7196	0.52%	0.045%
5	3.746	161	163	166	rVB	10520	7032	0.51%	0.044%
6	3.769	166	167	169	rBV	9242	7757	0.57%	0.049%
7	3.846	177	180	184	rBV	10053	14795	1.08%	0.093%
8	3.887	184	187	193	rVV	8753	16847	1.23%	0.106%
9	3.940	193	196	198	rVV	6678	7762	0.57%	0.049%
10	3.958	198	199	201	rVB	13852	7151	0.52%	0.045%
11	3.981	201	203	204	rBV	10562	9718	0.71%	0.061%
12	4.111	224	225	228	rBV	6504	7442	0.54%	0.047%
13	4.158	231	233	236	rVV	10899	9153	0.67%	0.058%
14	4.181	236	237	239	rVV	9178	6386	0.47%	0.040%
15	4.205	239	241	244	rVB	10353	7005	0.51%	0.044%
16	4.311	257	259	261	rBV	12808	9431	0.69%	0.059%
17	4.487	287	289	291	rBV	8261	8958	0.65%	0.056%
18	4.587	303	306	311	rVB2	18501	28077	2.05%	0.177%
19	4.675	320	321	324	rBV	9699	6763	0.49%	0.043%
20	4.752	331	334	337	rBV	6183	8878	0.65%	0.056%
21	4.911	358	361	363	rBV	10770	11498	0.84%	0.072%
22	4.934	363	365	367	rVV	7569	7789	0.57%	0.049%
23	5.069	386	388	391	rVV	10420	11258	0.82%	0.071%
24	5.169	402	405	406	rBV	12464	10153	0.74%	0.064%
25	5.240	413	417	418	rBV	6626	7361	0.54%	0.046%
26	5.287	420	425	426	rBV	5614	8203	0.60%	0.052%
27	5.687	490	493	495	rBV	9419	12261	0.89%	0.077%
28	5.799	510	512	515	rBV	7722	7500	0.55%	0.047%
29	5.869	523	524	526	rBV	10172	6869	0.50%	0.043%
30	5.905	528	530	531	rBV	9539	6069	0.44%	0.038%
31	6.034	549	552	553	rBV	10653	7323	0.53%	0.046%
32	6.175	573	576	579	rBV	8251	10081	0.73%	0.063%
33	6.505	628	632	633	rBV	7611	7671	0.56%	0.048%
34	6.563	637	642	652	rVB2	241559	452945	32.99%	2.848%

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN030620\
 Data File : BN010118.D
 Acq On : 06 Mar 2020 14:29
 Operator : CG/JU
 Sample : L1641-07
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB6Z0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Title : SVOA CALIBRATION

35	6.716	662	668	674	rBV2	173858	302129	22.01%	1.900%
36	6.893	692	698	706	rBV	276519	450897	32.85%	2.835%
37	7.110	729	735	736	rVV	6703	8709	0.63%	0.055%
38	7.234	753	756	758	rBV	8334	9582	0.70%	0.060%
39	7.352	769	776	786	rVV	296568	501309	36.52%	3.152%
40	7.440	789	791	796	rBV	13471	13866	1.01%	0.087%
41	7.505	800	802	805	rBV	9458	13504	0.98%	0.085%
42	7.599	815	818	820	rBV	8476	12581	0.92%	0.079%
43	7.669	828	830	832	rBV	5773	7025	0.51%	0.044%
44	7.710	834	837	840	rBV	8955	9324	0.68%	0.059%
45	7.793	849	851	854	rBV	5494	5992	0.44%	0.038%
46	7.822	854	856	858	rVB	12055	6098	0.44%	0.038%
47	7.893	866	868	870	rVB	9839	6655	0.48%	0.042%
48	8.069	893	898	908	rBV	278555	523150	38.11%	3.289%
49	8.152	911	912	914	rBV	12194	10118	0.74%	0.064%
50	8.193	918	919	921	rVB	14222	8714	0.63%	0.055%
51	8.216	921	923	926	rVB	12750	10469	0.76%	0.066%
52	8.240	926	927	929	rBV	9630	7011	0.51%	0.044%
53	8.305	937	938	942	rVB	10668	10292	0.75%	0.065%
54	8.346	942	945	946	rBV	7103	7448	0.54%	0.047%
55	8.399	953	954	957	rVB	8929	6338	0.46%	0.040%
56	8.499	963	971	979	rBV2	258225	485881	35.39%	3.055%
57	8.746	1011	1013	1014	rBV	8372	6495	0.47%	0.041%
58	8.910	1040	1041	1044	rBV	7726	6941	0.51%	0.044%
59	9.063	1065	1067	1069	rBV	7476	7916	0.58%	0.050%
60	9.146	1079	1081	1083	rBV	12649	11663	0.85%	0.073%
61	9.210	1086	1092	1103	rVV2	208334	399293	29.09%	2.511%
62	9.446	1128	1132	1133	rBV	8753	12297	0.90%	0.077%
63	9.463	1133	1135	1137	rBV	8422	6896	0.50%	0.043%
64	9.693	1171	1174	1175	rBV	6084	6462	0.47%	0.041%
65	9.752	1178	1184	1197	rBV	254645	523235	38.12%	3.290%
66	10.099	1237	1243	1251	rVB	392022	673907	49.09%	4.237%
67	10.263	1264	1271	1285	rBV2	227599	601343	43.80%	3.781%
68	10.504	1310	1312	1314	rBV	11151	7929	0.58%	0.050%
69	10.663	1338	1339	1343	rBV	7025	10179	0.74%	0.064%
70	10.728	1346	1350	1353	rBV	8816	10653	0.78%	0.067%
71	10.816	1363	1365	1369	rVB	9870	13958	1.02%	0.088%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030620\
 Data File : BN010118.D
 Acq On : 06 Mar 2020 14:29
 Operator : CG/JU
 Sample : L1641-07
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB6Z0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Title : SVOA CALIBRATION

72	10.999	1393	1396	1398	rBV	7729	10571	0.77%	0.066%
73	11.016	1398	1399	1402	rVV	9057	7672	0.56%	0.048%
74	11.051	1403	1405	1406	rVB	14381	7310	0.53%	0.046%
75	11.246	1436	1438	1441	rBV	9826	9838	0.72%	0.062%
76	11.281	1443	1444	1446	rBV	12689	7590	0.55%	0.048%
77	11.328	1451	1452	1455	rBV	12395	9918	0.72%	0.062%
78	11.399	1460	1464	1465	rBV	7774	6235	0.45%	0.039%
79	11.628	1498	1503	1505	rBV	13877	18263	1.33%	0.115%
80	11.846	1538	1540	1541	rBV	10628	7705	0.56%	0.048%
81	12.210	1601	1602	1606	rVB	9338	9663	0.70%	0.061%
82	12.422	1636	1638	1639	rBV	14053	8640	0.63%	0.054%
83	12.769	1695	1697	1698	rBV	9943	6680	0.49%	0.042%
84	12.857	1709	1712	1715	rBV	13046	18001	1.31%	0.113%
85	12.975	1730	1732	1736	rBV	12067	13600	0.99%	0.086%
86	13.216	1771	1773	1777	rBV	15018	21392	1.56%	0.135%
87	13.322	1789	1791	1793	rBV	9715	6873	0.50%	0.043%
88	13.428	1802	1809	1820	rBV	544844	874815	63.73%	5.501%
89	13.551	1828	1830	1832	rBV	12916	12862	0.94%	0.081%
90	13.687	1847	1853	1862	rBV	627812	951473	69.31%	5.983%
91	13.998	1900	1906	1913	rVB	606037	893525	65.09%	5.618%
92	14.269	1948	1952	1960	rBV	111367	244554	17.81%	1.538%
93	14.616	2009	2011	2013	rBV	12277	9058	0.66%	0.057%
94	15.004	2072	2077	2084	rVB	756795	1148617	83.67%	7.222%
95	15.181	2102	2107	2115	rBV	177641	326434	23.78%	2.053%
96	16.763	2371	2376	2386	rVB	744428	1047620	76.31%	6.587%
97	16.863	2388	2393	2403	rVB	827682	1226329	89.33%	7.711%
98	19.175	2781	2786	2795	rBV	996252	1372773	100.00%	8.632%
99	20.992	3091	3095	3104	rBV2	793124	1069455	77.90%	6.724%
100	22.957	3425	3429	3434	rBV	686903	1067126	77.74%	6.710%


Sum of corrected areas: 15904090

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN030620\
Data File : BN010118.D
Acq On : 06 Mar 2020 14:29
Operator : CG/JU
Sample : L1641-07
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB6Z0

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

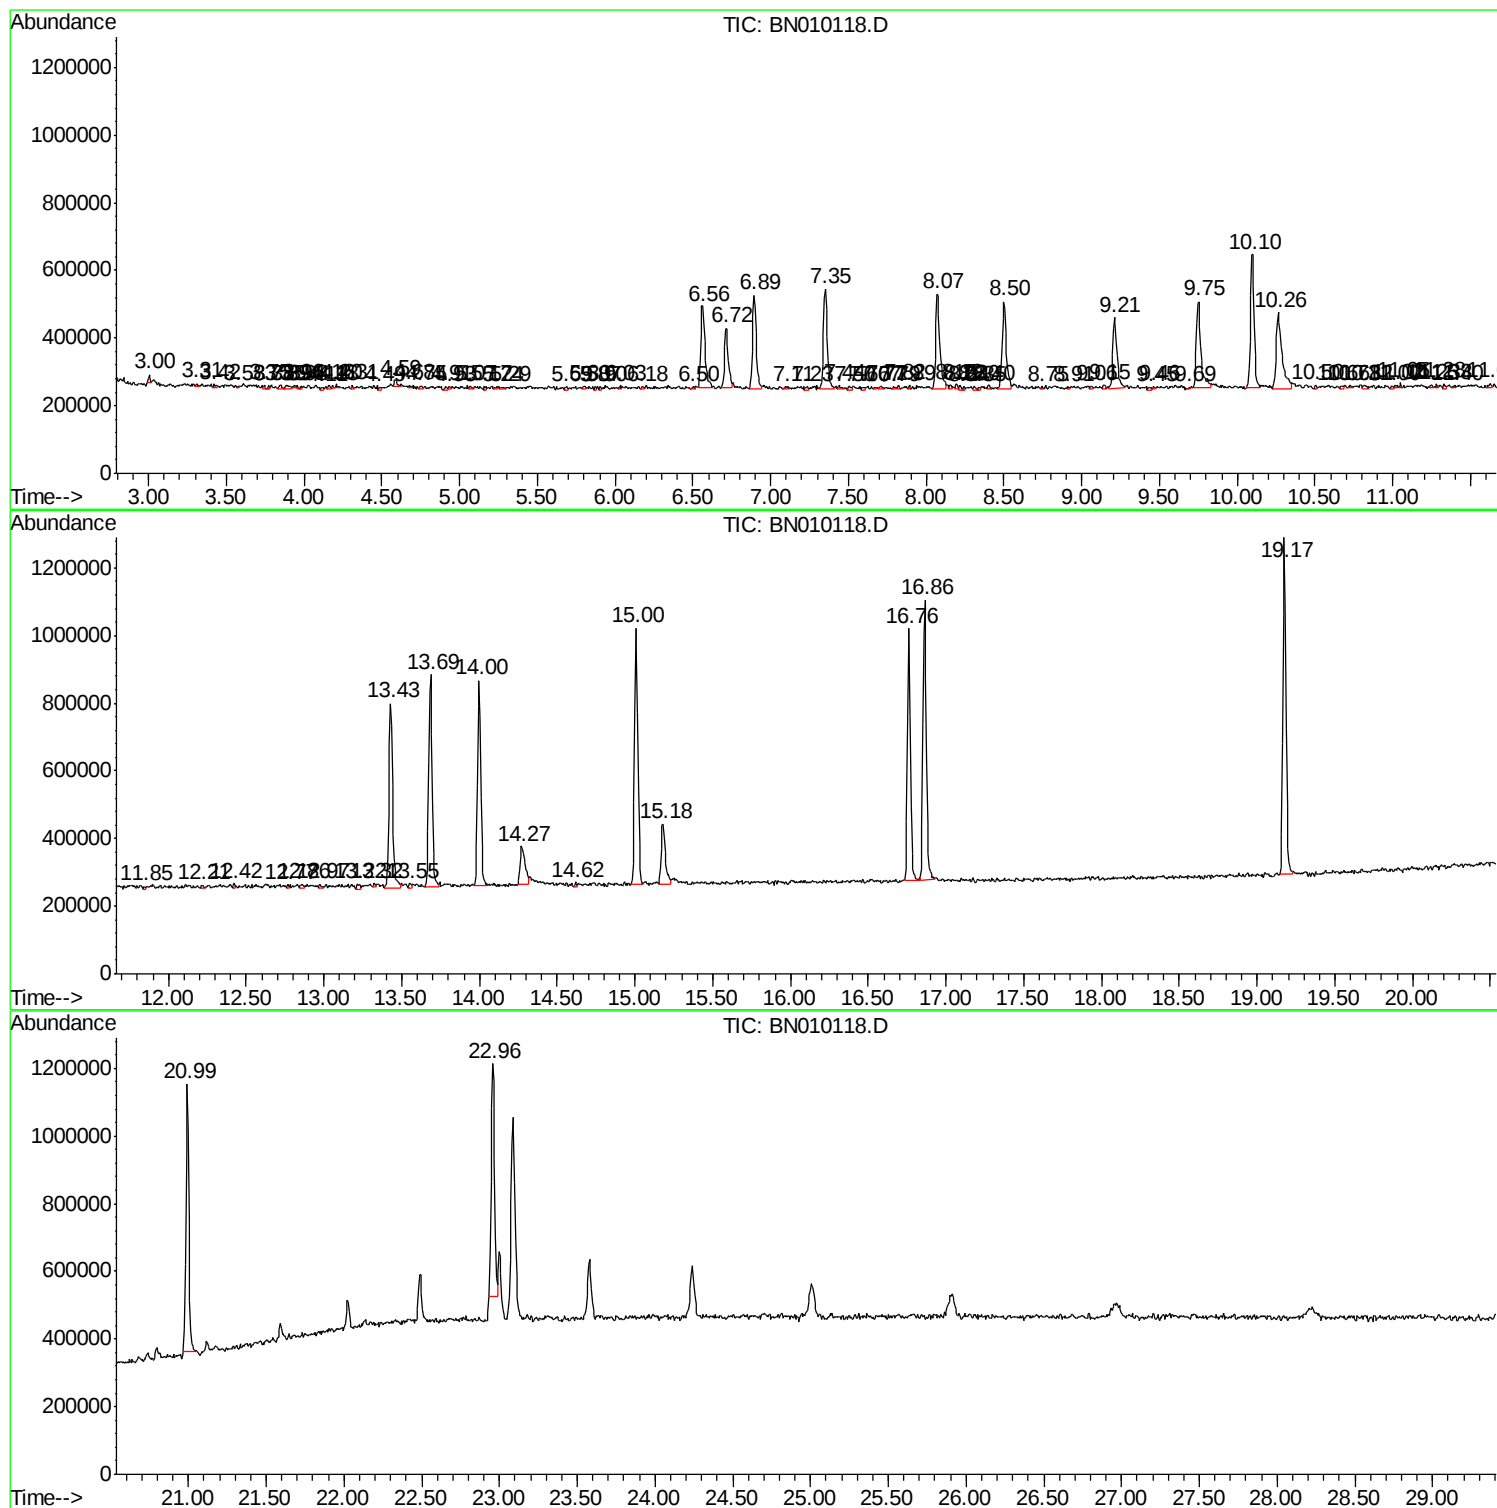

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030620\
Data File : BN010118.D
Acq On : 06 Mar 2020 14:29
Operator : CG/JU
Sample : L1641-07
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB6Z0

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030620\
Data File : BN010118.D
Acq On : 06 Mar 2020 14:29
Operator : CG/JU
Sample : L1641-07
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB6Z0

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc