

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN030620\
 Data File : BN010119.D
 Acq On : 06 Mar 2020 15:05
 Operator : CG/JU
 Sample : L1641-11
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB6Z4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.070	46	48	52	rBV	11241	12602	1.10%	0.105%
2	3.346	93	95	96	rBV	10515	5849	0.51%	0.049%
3	3.922	191	193	196	rBV	9917	11089	0.97%	0.092%
4	4.011	206	208	211	rBV	6558	5569	0.49%	0.046%
5	4.305	256	258	263	rVB	14040	20762	1.82%	0.172%
6	4.693	321	324	326	rBV	10006	12641	1.11%	0.105%
7	4.811	343	344	347	rBV	9129	8043	0.70%	0.067%
8	4.840	347	349	351	rBV	8807	6361	0.56%	0.053%
9	4.911	359	361	363	rBV	7559	5890	0.51%	0.049%
10	4.952	366	368	371	rVB	9502	10607	0.93%	0.088%
11	4.981	371	373	374	rBV	11343	10850	0.95%	0.090%
12	5.117	394	396	399	rVB	6642	6771	0.59%	0.056%
13	5.211	410	412	414	rVB	7158	5625	0.49%	0.047%
14	5.399	443	444	450	rBV	10926	15441	1.35%	0.128%
15	5.446	450	452	455	rVV	7112	7040	0.62%	0.058%
16	5.481	455	458	459	rVV	7205	6352	0.56%	0.053%
17	5.522	463	465	468	rVB	11200	11652	1.02%	0.097%
18	5.564	468	472	473	rBV	10565	10046	0.88%	0.083%
19	5.622	480	482	484	rBV	8694	10197	0.89%	0.085%
20	5.681	491	492	494	rVB	11475	6747	0.59%	0.056%
21	5.699	494	495	499	rBV	14098	9905	0.87%	0.082%
22	5.758	503	505	507	rBV	7182	8697	0.76%	0.072%
23	5.811	513	514	516	rBV	9382	6330	0.55%	0.053%
24	5.940	530	536	538	rVB	10290	17200	1.50%	0.143%
25	5.964	538	540	543	rBV	10541	11483	1.00%	0.095%
26	6.134	568	569	572	rVV	10172	6509	0.57%	0.054%
27	6.258	588	590	591	rBV	9914	6218	0.54%	0.052%
28	6.311	596	599	601	rBV	8752	8416	0.74%	0.070%
29	6.328	601	602	604	rVB	9500	5403	0.47%	0.045%
30	6.446	620	622	625	rVV	7492	6983	0.61%	0.058%
31	6.511	631	633	635	rBV	8035	8768	0.77%	0.073%
32	6.564	638	642	652	rVV	166479	313190	27.38%	2.600%
33	6.716	664	668	677	rVB	121540	195932	17.13%	1.626%
34	6.864	690	693	694	rBV	7944	8387	0.73%	0.070%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030620\
 Data File : BN010119.D
 Acq On : 06 Mar 2020 15:05
 Operator : CG/JU
 Sample : L1641-11
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB6Z4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Title : SVOA CALIBRATION

35	6.899	694	699	709	rVB2	183782	327944	28.67%	2.722%
36	7.022	718	720	723	rVB	7814	8399	0.73%	0.070%
37	7.116	734	736	737	rVB	9927	6624	0.58%	0.055%
38	7.205	749	751	752	rVB	10741	5784	0.51%	0.048%
39	7.352	771	776	785	rBV	306581	519445	45.42%	4.312%
40	7.458	793	794	797	rVB	9423	6442	0.56%	0.053%
41	7.481	797	798	800	rBV	7041	5677	0.50%	0.047%
42	7.581	811	815	816	rBV	10876	14321	1.25%	0.119%
43	7.599	816	818	823	rVB	10470	13971	1.22%	0.116%
44	7.640	823	825	827	rVB	10449	9038	0.79%	0.075%
45	7.658	827	828	832	rBV	9354	11824	1.03%	0.098%
46	7.781	848	849	852	rBV	13357	9230	0.81%	0.077%
47	7.811	852	854	856	rBV	9323	9302	0.81%	0.077%
48	7.834	856	858	861	rVB	10669	8540	0.75%	0.071%
49	7.946	876	877	879	rBV	9857	7283	0.64%	0.060%
50	8.075	894	899	909	rBV2	188030	372233	32.55%	3.090%
51	8.246	926	928	930	rVB	11168	8620	0.75%	0.072%
52	8.275	930	933	934	rBV	7953	7146	0.62%	0.059%
53	8.322	940	941	943	rBV	9709	6384	0.56%	0.053%
54	8.452	960	963	964	rBV	11438	9584	0.84%	0.080%
55	8.505	966	972	979	rVV2	170363	326009	28.50%	2.706%
56	8.881	1034	1036	1038	rVB	13496	7870	0.69%	0.065%
57	8.905	1038	1040	1043	rBV	10428	12397	1.08%	0.103%
58	8.952	1046	1048	1050	rVV	6580	5786	0.51%	0.048%
59	9.005	1055	1057	1060	rVB	7082	6930	0.61%	0.058%
60	9.040	1060	1063	1065	rBV	7656	7337	0.64%	0.061%
61	9.216	1088	1093	1102	rVB	136547	241777	21.14%	2.007%
62	9.328	1111	1112	1114	rBV	11154	6472	0.57%	0.054%
63	9.352	1114	1116	1117	rVB	11134	7242	0.63%	0.060%
64	9.363	1117	1118	1119	rBV	8560	5916	0.52%	0.049%
65	9.422	1124	1128	1129	rBV	6085	6563	0.57%	0.054%
66	9.569	1152	1153	1157	rBV	8764	7914	0.69%	0.066%
67	9.757	1179	1185	1196	rBV2	157259	330354	28.88%	2.742%
68	9.887	1205	1207	1210	rVB	13665	12395	1.08%	0.103%
69	9.916	1210	1212	1213	rBV	9025	9047	0.79%	0.075%
70	9.952	1215	1218	1219	rBV	9454	7389	0.65%	0.061%
71	10.099	1237	1243	1251	rVV	443538	729816	63.81%	6.058%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030620\
 Data File : BN010119.D
 Acq On : 06 Mar 2020 15:05
 Operator : CG/JU
 Sample : L1641-11
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB6Z4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Title : SVOA CALIBRATION

72	10.269	1267	1272	1284	rBV2	142916	344721	30.14%	2.861%
73	10.481	1306	1308	1309	rVB	10069	5523	0.48%	0.046%
74	10.563	1319	1322	1324	rBV	7006	10107	0.88%	0.084%
75	10.752	1351	1354	1355	rBV	8062	10109	0.88%	0.084%
76	10.787	1359	1360	1363	rVB	9143	7822	0.68%	0.065%
77	10.887	1375	1377	1378	rVB	13568	7947	0.69%	0.066%
78	10.899	1378	1379	1381	rBV	14323	12068	1.06%	0.100%
79	10.993	1391	1395	1400	rVB	8159	12309	1.08%	0.102%
80	11.040	1402	1403	1407	rBV	8746	10623	0.93%	0.088%
81	11.228	1433	1435	1438	rBV	8402	8999	0.79%	0.075%
82	11.340	1453	1454	1456	rBV	10379	7641	0.67%	0.063%
83	11.410	1465	1466	1468	rBV	13920	6088	0.53%	0.051%
84	11.622	1500	1502	1504	rVB	9807	6634	0.58%	0.055%
85	11.640	1504	1505	1506	rBV	12651	6288	0.55%	0.052%
86	11.951	1556	1558	1560	rBV	9268	8877	0.78%	0.074%
87	12.963	1727	1730	1732	rBV	12736	20267	1.77%	0.168%
88	13.210	1768	1772	1775	rBV	14219	23821	2.08%	0.198%
89	13.434	1804	1810	1819	rBV	363862	599908	52.45%	4.980%
90	13.610	1839	1840	1842	rBV	13018	6259	0.55%	0.052%
91	13.687	1847	1853	1864	rBV	463928	694039	60.68%	5.761%
92	13.998	1900	1906	1914	rBV	656787	982687	85.92%	8.157%
93	14.281	1951	1954	1962	rVB2	50989	103815	9.08%	0.862%
94	14.610	2008	2010	2012	rBV	11272	6327	0.55%	0.053%
95	15.010	2072	2078	2087	rBV	555624	846932	74.05%	7.030%
96	15.181	2103	2107	2117	rBV	110435	224624	19.64%	1.864%
97	16.763	2371	2376	2385	rVB	833168	1143737	100.00%	9.494%
98	16.863	2388	2393	2402	rVB	577359	886636	77.52%	7.360%
99	19.175	2781	2786	2795	rBV2	688502	997953	87.25%	8.284%
100	20.992	3091	3095	3101	rBV	885669	1142104	99.86%	9.480%


Sum of corrected areas: 12047425

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN030620\
Data File : BN010119.D
Acq On : 06 Mar 2020 15:05
Operator : CG/JU
Sample : L1641-11
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
CB6Z4

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

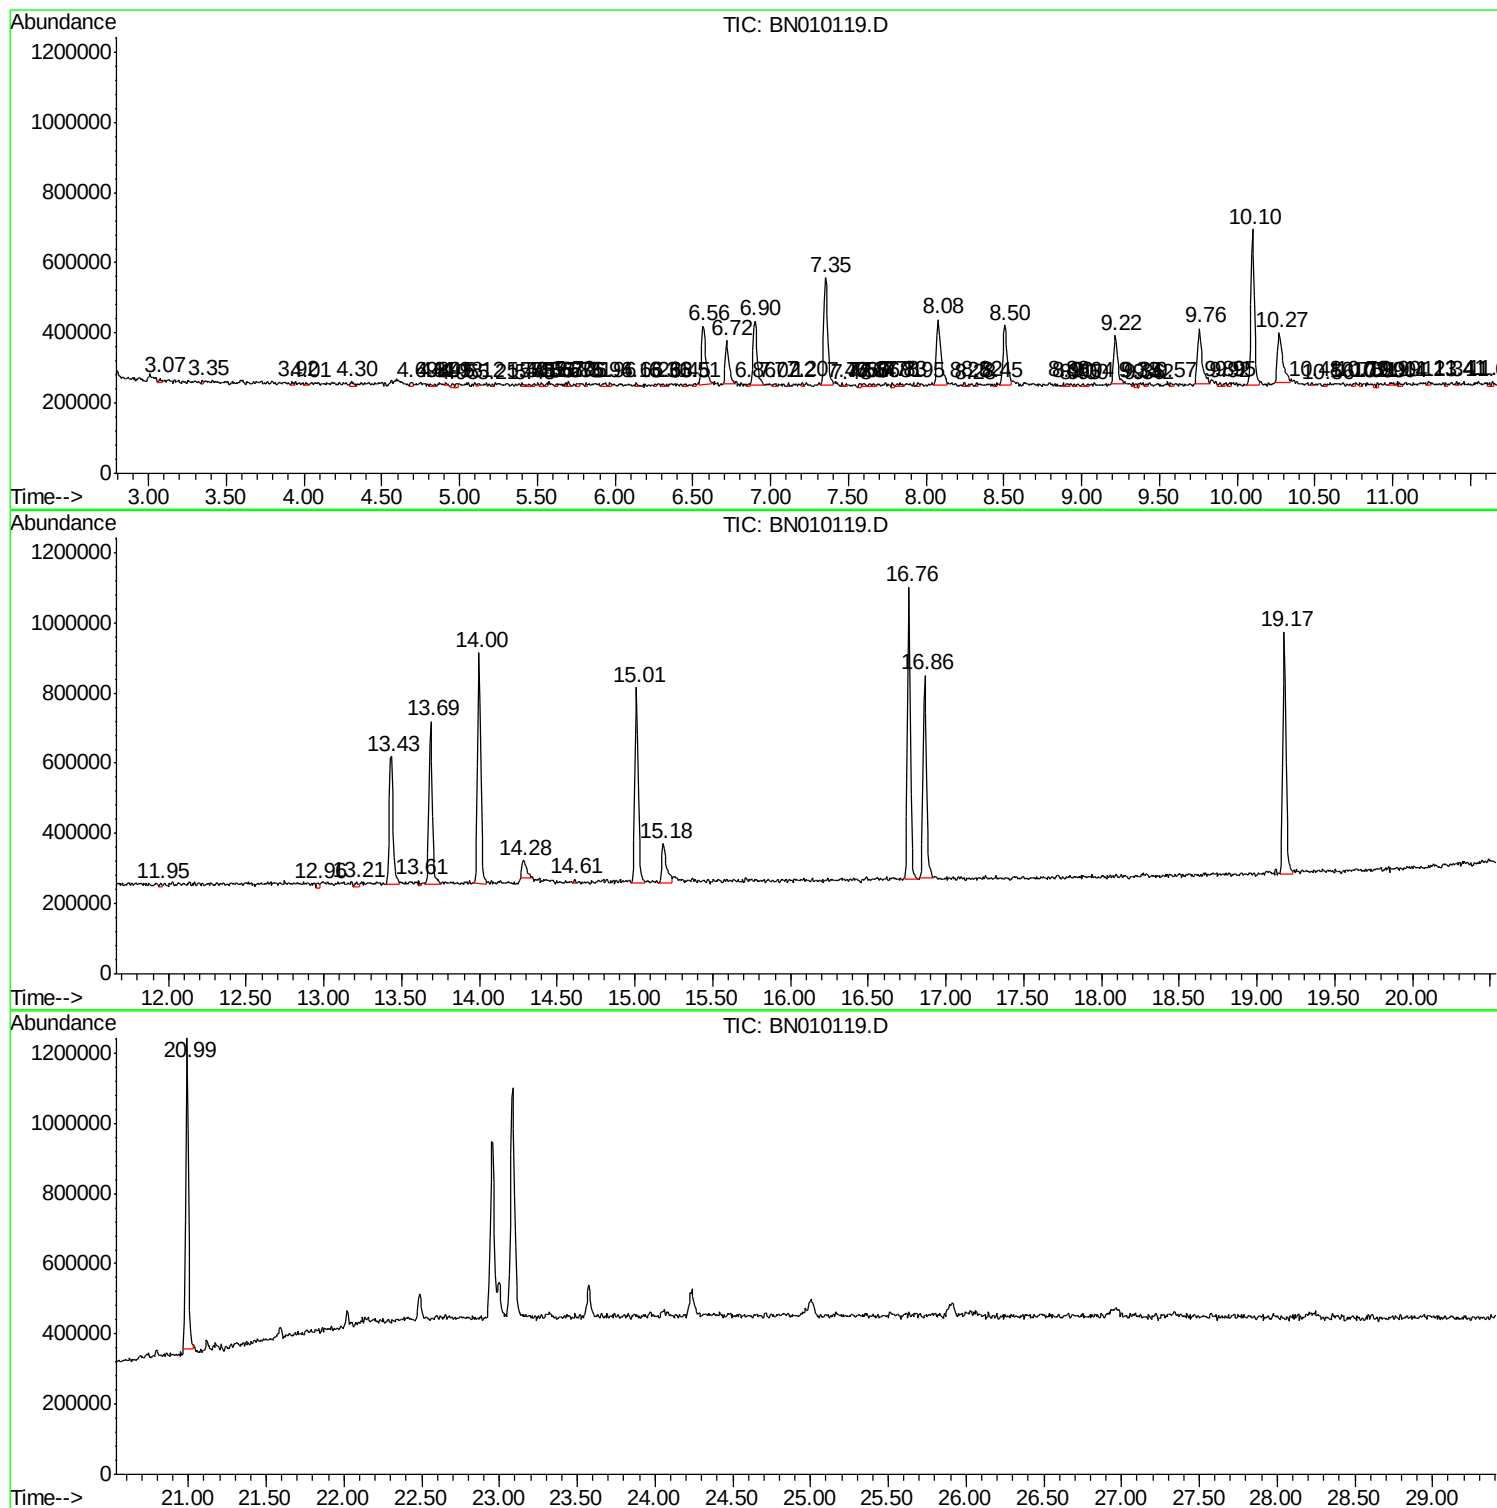

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030620\
Data File : BN010119.D
Acq On : 06 Mar 2020 15:05
Operator : CG/JU
Sample : L1641-11
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB6Z4

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030620\
Data File : BN010119.D
Acq On : 06 Mar 2020 15:05
Operator : CG/JU
Sample : L1641-11
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB6Z4

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc