

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030620\
 Data File : BN010120.D
 Acq On : 06 Mar 2020 15:41
 Operator : CG/JU
 Sample : L1641-08
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB6Z1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.581	133	135	136	rBV	10431	8947	0.66%	0.055%
2	4.011	206	208	209	rBV	10203	5705	0.42%	0.035%
3	4.281	253	254	258	rBV	10884	13833	1.02%	0.085%
4	4.317	258	260	261	rVB	12615	5567	0.41%	0.034%
5	4.340	262	264	267	rVB	8099	7623	0.56%	0.047%
6	4.405	272	275	278	rBV	15085	20051	1.47%	0.123%
7	4.481	286	288	290	rBV	6665	6709	0.49%	0.041%
8	4.558	299	301	303	rBV	14661	17293	1.27%	0.106%
9	4.870	351	354	355	rVB	12717	10746	0.79%	0.066%
10	4.893	355	358	359	rBV	10997	9933	0.73%	0.061%
11	4.952	366	368	372	rVB	9854	8895	0.65%	0.055%
12	5.064	384	387	389	rBV	8925	8517	0.63%	0.052%
13	5.164	402	404	410	rVB	8440	10718	0.79%	0.066%
14	5.446	449	452	456	rBV	12180	19989	1.47%	0.123%
15	5.558	469	471	474	rVB	11968	14645	1.08%	0.090%
16	5.581	474	475	476	rBV	10706	6463	0.48%	0.040%
17	5.822	514	516	520	rVB	7765	6738	0.50%	0.041%
18	5.881	523	526	528	rBV	7479	10118	0.74%	0.062%
19	6.252	587	589	591	rBV	7086	5657	0.42%	0.035%
20	6.346	604	605	608	rBV	9722	7251	0.53%	0.045%
21	6.446	621	622	624	rBV	9527	8125	0.60%	0.050%
22	6.505	631	632	634	rBV	5799	5697	0.42%	0.035%
23	6.528	634	636	637	rVB	9248	5880	0.43%	0.036%
24	6.564	637	642	650	rBV	249489	451527	33.19%	2.776%
25	6.717	662	668	678	rBV	188687	336799	24.76%	2.070%
26	6.858	690	692	693	rBV	7966	7853	0.58%	0.048%
27	6.899	693	699	706	rVV	263486	442409	32.52%	2.720%
28	7.081	728	730	732	rBV	8208	7024	0.52%	0.043%
29	7.128	735	738	740	rVB	7036	7471	0.55%	0.046%
30	7.158	740	743	745	rBV	5266	6209	0.46%	0.038%
31	7.205	749	751	753	rVV	11494	8648	0.64%	0.053%
32	7.240	755	757	760	rVB	9649	7669	0.56%	0.047%
33	7.352	771	776	785	rBV	300269	523057	38.45%	3.215%
34	7.622	821	822	824	rBV	7823	6811	0.50%	0.042%

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN030620\
 Data File : BN010120.D
 Acq On : 06 Mar 2020 15:41
 Operator : CG/JU
 Sample : L1641-08
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB6Z1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Title : SVOA CALIBRATION

35	7.758	843	845	848 rBV	8290	8470	0.62%	0.052%
36	7.869	861	864	865 rVB	8062	6151	0.45%	0.038%
37	7.905	868	870	871 rBV	12554	8256	0.61%	0.051%
38	8.016	887	889	891 rBV	7026	7096	0.52%	0.044%
39	8.075	894	899	909 rVV2	281934	520041	38.23%	3.197%
40	8.246	927	928	931 rBV	8671	8934	0.66%	0.055%
41	8.416	955	957	961 rVV	6202	7139	0.52%	0.044%
42	8.505	966	972	980 rVV	258511	459020	33.74%	2.822%
43	8.640	992	995	997 rBV	6583	8077	0.59%	0.050%
44	8.687	1001	1003	1004 rVB	10292	6180	0.45%	0.038%
45	8.699	1004	1005	1007 rBV	6821	5744	0.42%	0.035%
46	8.716	1007	1008	1013 rVB	7806	6877	0.51%	0.042%
47	9.034	1060	1062	1065 rBV	6612	6756	0.50%	0.042%
48	9.216	1087	1093	1101 rBV	211730	390438	28.70%	2.400%
49	9.381	1119	1121	1124 rBV	8283	9754	0.72%	0.060%
50	9.411	1124	1126	1127 rVV	10877	6185	0.45%	0.038%
51	9.452	1131	1133	1134 rBV	11151	11100	0.82%	0.068%
52	9.481	1137	1138	1140 rVB	10425	5501	0.40%	0.034%
53	9.516	1140	1144	1145 rBV	4367	5774	0.42%	0.035%
54	9.646	1162	1166	1167 rBV	10132	12684	0.93%	0.078%
55	9.675	1167	1171	1172 rBV	9156	10825	0.80%	0.067%
56	9.752	1178	1184	1197 rBV2	253097	520262	38.25%	3.198%
57	9.869	1202	1204	1207 rBV	10302	9044	0.66%	0.056%
58	10.099	1237	1243	1252 rVV	439810	731939	53.81%	4.499%
59	10.163	1252	1254	1255 rVB	11048	7424	0.55%	0.046%
60	10.228	1261	1265	1266 rBV	6912	8025	0.59%	0.049%
61	10.269	1266	1272	1282 rBV2	225715	545315	40.09%	3.352%
62	10.505	1310	1312	1313 rBV	9798	8081	0.59%	0.050%
63	10.863	1371	1373	1376 rVB	10498	10248	0.75%	0.063%
64	10.893	1376	1378	1380 rBV	7481	7532	0.55%	0.046%
65	11.063	1405	1407	1410 rBV	10123	12270	0.90%	0.075%
66	11.328	1448	1452	1454 rBV	8642	11397	0.84%	0.070%
67	11.352	1454	1456	1457 rVB	9103	5895	0.43%	0.036%
68	11.752	1523	1524	1527 rVB	9670	5677	0.42%	0.035%
69	11.781	1527	1529	1531 rBV	8983	6770	0.50%	0.042%
70	11.875	1544	1545	1547 rBV	8751	5483	0.40%	0.034%
71	11.928	1553	1554	1555 rBV	13769	6090	0.45%	0.037%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030620\
 Data File : BN010120.D
 Acq On : 06 Mar 2020 15:41
 Operator : CG/JU
 Sample : L1641-08
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB6Z1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Title : SVOA CALIBRATION

72	11.957	1558	1559	1561	rVB	10441	6341	0.47%	0.039%
73	11.981	1561	1563	1565	rBV	12966	13027	0.96%	0.080%
74	12.028	1568	1571	1573	rBV	8669	8743	0.64%	0.054%
75	12.152	1588	1592	1593	rBV	8392	8544	0.63%	0.053%
76	12.246	1606	1608	1612	rBV	8028	9270	0.68%	0.057%
77	12.363	1625	1628	1633	rVB	8744	12577	0.92%	0.077%
78	12.399	1633	1634	1636	rBV	11221	7676	0.56%	0.047%
79	12.622	1671	1672	1674	rBV	8022	7263	0.53%	0.045%
80	12.769	1695	1697	1699	rBV	10534	6174	0.45%	0.038%
81	12.863	1710	1713	1714	rBV	8171	7945	0.58%	0.049%
82	13.046	1741	1744	1745	rBV	8504	5988	0.44%	0.037%
83	13.104	1752	1754	1755	rBV	7284	5809	0.43%	0.036%
84	13.163	1762	1764	1766	rBV	9611	7936	0.58%	0.049%
85	13.428	1804	1809	1818	rBV	551198	835460	61.42%	5.136%
86	13.551	1828	1830	1833	rBV	10519	12069	0.89%	0.074%
87	13.687	1847	1853	1861	rVB	607712	935600	68.78%	5.751%
88	13.998	1901	1906	1914	rVB2	659151	963788	70.85%	5.925%
89	14.269	1948	1952	1970	rVV	118934	335401	24.66%	2.062%
90	14.646	2014	2016	2017	rBV	13321	8142	0.60%	0.050%
91	14.816	2042	2045	2046	rBV	11000	7928	0.58%	0.049%
92	14.945	2064	2067	2068	rBV	12120	12431	0.91%	0.076%
93	15.010	2072	2078	2085	rVV	773404	1186503	87.22%	7.294%
94	15.181	2102	2107	2113	rBV2	176286	327218	24.05%	2.012%
95	15.481	2156	2158	2160	rBV	10726	7171	0.53%	0.044%
96	16.757	2371	2375	2383	rBV	778136	1108054	81.46%	6.812%
97	16.863	2387	2393	2401	rBV	822998	1225983	90.13%	7.536%
98	19.175	2781	2786	2795	rVB	965362	1360298	100.00%	8.362%
99	20.992	3090	3095	3109	rBV	876761	1202486	88.40%	7.392%
100	22.957	3424	3429	3434	rBV	707901	1188493	87.37%	7.306%


Sum of corrected areas: 16267349

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN030620\
Data File : BN010120.D
Acq On : 06 Mar 2020 15:41
Operator : CG/JU
Sample : L1641-08
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB6Z1

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

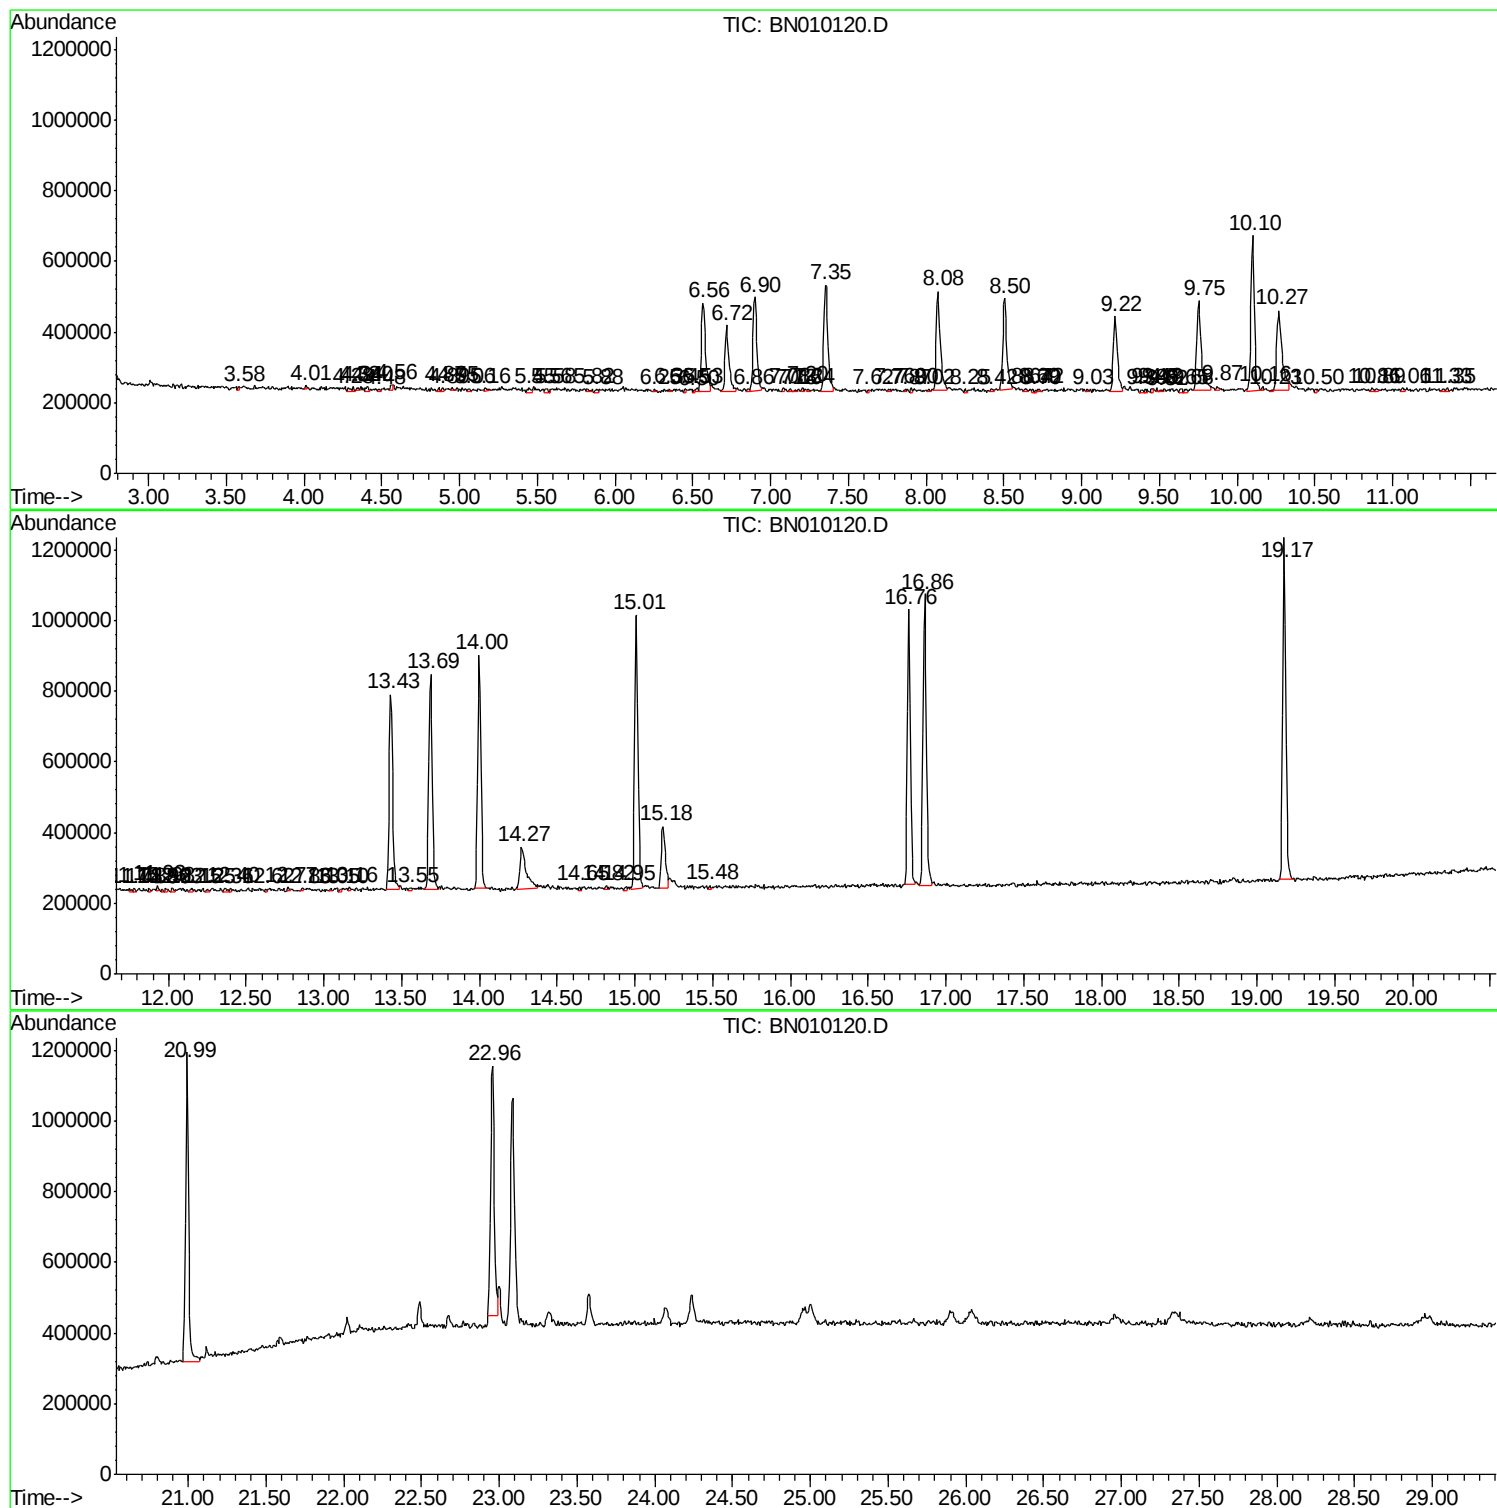

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030620\
Data File : BN010120.D
Acq On : 06 Mar 2020 15:41
Operator : CG/JU
Sample : L1641-08
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB6Z1

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030620\
Data File : BN010120.D
Acq On : 06 Mar 2020 15:41
Operator : CG/JU
Sample : L1641-08
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB6Z1

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc