

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN030620\
 Data File : BN010121.D
 Acq On : 06 Mar 2020 16:17
 Operator : CG/JU
 Sample : L1641-10
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB6Z3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.793	339	341	343	rVB	11894	7642	0.65%	0.068%
2	4.834	345	348	349	rBV	6508	5815	0.49%	0.052%
3	4.911	359	361	364	rBV	7559	6974	0.59%	0.062%
4	5.175	404	406	408	rBV	11463	8219	0.69%	0.073%
5	5.252	417	419	421	rBV	7536	6911	0.58%	0.062%
6	5.281	423	424	426	rBV	9213	8352	0.70%	0.074%
7	5.381	439	441	442	rBV	11199	9473	0.80%	0.084%
8	5.516	463	464	466	rBV	6269	6146	0.52%	0.055%
9	5.575	473	474	476	rBV	9308	5626	0.47%	0.050%
10	5.622	480	482	484	rVB	7345	6678	0.56%	0.060%
11	5.652	484	487	488	rBV	9876	9091	0.77%	0.081%
12	5.669	488	490	492	rVV	10382	11014	0.93%	0.098%
13	5.705	494	496	499	rVV	11661	10102	0.85%	0.090%
14	5.728	499	500	501	rVB	12536	4425	0.37%	0.039%
15	5.746	501	503	506	rBV	7600	7243	0.61%	0.065%
16	5.775	506	508	510	rVB	11243	8458	0.71%	0.075%
17	6.016	547	549	550	rBV	5945	4306	0.36%	0.038%
18	6.128	566	568	569	rVB	9816	5011	0.42%	0.045%
19	6.269	590	592	596	rVB	7776	9170	0.77%	0.082%
20	6.446	620	622	623	rBV	6903	4485	0.38%	0.040%
21	6.516	633	634	636	rBV	6473	4155	0.35%	0.037%
22	6.569	638	643	655	rVV2	147437	304794	25.73%	2.718%
23	6.675	659	661	663	rBV	10592	8308	0.70%	0.074%
24	6.716	664	668	677	rVV2	108229	189609	16.00%	1.691%
25	6.899	693	699	710	rBV2	163866	311862	26.32%	2.781%
26	6.999	714	716	718	rVB	14143	9960	0.84%	0.089%
27	7.034	718	722	724	rBV	9384	11657	0.98%	0.104%
28	7.110	734	735	738	rBV	6652	6615	0.56%	0.059%
29	7.269	758	762	764	rBV	9674	12481	1.05%	0.111%
30	7.352	770	776	787	rVB	293053	517564	43.69%	4.615%
31	7.457	793	794	797	rVB	8188	5794	0.49%	0.052%
32	7.481	797	798	800	rBV	9991	8301	0.70%	0.074%
33	7.587	814	816	818	rBV	9119	5637	0.48%	0.050%
34	7.746	841	843	845	rVB	8966	6941	0.59%	0.062%

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN030620\
 Data File : BN010121.D
 Acq On : 06 Mar 2020 16:17
 Operator : CG/JU
 Sample : L1641-10
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB6Z3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Title : SVOA CALIBRATION

35	7.763	845	846	847	rBV	9824	6073	0.51%	0.054%
36	7.816	853	855	856	rBV	9306	6886	0.58%	0.061%
37	7.834	856	858	861	rVV	9217	7220	0.61%	0.064%
38	7.928	871	874	876	rBV	8976	10670	0.90%	0.095%
39	8.081	895	900	910	rBV3	169519	334669	28.25%	2.984%
40	8.346	944	945	946	rBV	8903	5140	0.43%	0.046%
41	8.363	946	948	952	rVV	7057	11944	1.01%	0.107%
42	8.504	967	972	981	rBV2	151327	288560	24.36%	2.573%
43	8.651	996	997	999	rVB	8239	4131	0.35%	0.037%
44	8.793	1020	1021	1022	rBV	11455	5663	0.48%	0.050%
45	9.057	1065	1066	1071	rBV	4846	8539	0.72%	0.076%
46	9.216	1087	1093	1103	rBV	131712	276005	23.30%	2.461%
47	9.463	1134	1135	1137	rVV	7098	5064	0.43%	0.045%
48	9.551	1146	1150	1153	rBV	10887	17550	1.48%	0.156%
49	9.575	1153	1154	1158	rBV	7924	10484	0.88%	0.093%
50	9.687	1171	1173	1176	rBV	6578	5584	0.47%	0.050%
51	9.710	1176	1177	1180	rBV	7980	8533	0.72%	0.076%
52	9.757	1180	1185	1196	rVV3	137643	292120	24.66%	2.605%
53	10.098	1237	1243	1253	rBV	419467	724747	61.18%	6.463%
54	10.169	1253	1255	1256	rVB	8587	4342	0.37%	0.039%
55	10.275	1268	1273	1285	rBV3	123440	310578	26.22%	2.769%
56	10.516	1312	1314	1316	rBV	9234	10433	0.88%	0.093%
57	10.551	1318	1320	1321	rVB	11531	7185	0.61%	0.064%
58	10.569	1321	1323	1325	rBV	12538	13277	1.12%	0.118%
59	10.757	1353	1355	1357	rVB	8644	6914	0.58%	0.062%
60	10.775	1357	1358	1360	rBV	10467	9194	0.78%	0.082%
61	10.957	1385	1389	1390	rBV	7310	8798	0.74%	0.078%
62	10.993	1393	1395	1397	rBV	6581	5924	0.50%	0.053%
63	11.069	1405	1408	1410	rBV	8297	7139	0.60%	0.064%
64	11.275	1440	1443	1444	rBV	7771	7578	0.64%	0.068%
65	11.310	1447	1449	1452	rBV	11480	11447	0.97%	0.102%
66	11.498	1479	1481	1483	rVB	6296	4547	0.38%	0.041%
67	11.540	1483	1488	1489	rBV	9087	9699	0.82%	0.086%
68	11.651	1505	1507	1509	rBV	8889	9719	0.82%	0.087%
69	11.698	1513	1515	1516	rBV	12554	11140	0.94%	0.099%
70	11.840	1537	1539	1544	rBV	11089	17694	1.49%	0.158%
71	11.898	1548	1549	1551	rVB	10452	5410	0.46%	0.048%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030620\
 Data File : BN010121.D
 Acq On : 06 Mar 2020 16:17
 Operator : CG/JU
 Sample : L1641-10
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB6Z3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Title : SVOA CALIBRATION

72	11.922	1551	1553	1554	rBV	8473	6005	0.51%	0.054%
73	12.016	1567	1569	1570	rBV	7603	5368	0.45%	0.048%
74	12.151	1589	1592	1593	rBV	6786	6199	0.52%	0.055%
75	12.392	1632	1633	1634	rBV	9797	4695	0.40%	0.042%
76	12.616	1669	1671	1672	rBV	10736	4514	0.38%	0.040%
77	12.822	1705	1706	1711	rBV	8214	11204	0.95%	0.100%
78	12.857	1711	1712	1714	rBV	9622	5719	0.48%	0.051%
79	13.045	1742	1744	1745	rBV	10439	6384	0.54%	0.057%
80	13.063	1745	1747	1748	rBV	8008	5201	0.44%	0.046%
81	13.104	1753	1754	1757	rVB	8652	5799	0.49%	0.052%
82	13.228	1773	1775	1778	rVB	7446	7919	0.67%	0.071%
83	13.434	1805	1810	1818	rVB	319473	503241	42.48%	4.487%
84	13.610	1838	1840	1841	rBV	8324	5363	0.45%	0.048%
85	13.687	1847	1853	1862	rBV	415775	611478	51.61%	5.453%
86	13.816	1871	1875	1876	rVB	8097	9870	0.83%	0.088%
87	13.834	1876	1878	1879	rBV	8114	6630	0.56%	0.059%
88	13.998	1900	1906	1915	rBV	651346	977318	82.50%	8.715%
89	14.157	1932	1933	1935	rBV	7880	6227	0.53%	0.056%
90	14.192	1937	1939	1941	rBV	8651	5388	0.45%	0.048%
91	14.228	1943	1945	1947	rVB	9688	6368	0.54%	0.057%
92	14.281	1951	1954	1962	rVV3	39725	89162	7.53%	0.795%
93	14.722	2027	2029	2030	rBV	7311	4625	0.39%	0.041%
94	15.010	2072	2078	2085	rBV2	480159	764288	64.51%	6.815%
95	15.186	2104	2108	2118	rBV2	82498	156934	13.25%	1.399%
96	15.792	2210	2211	2213	rBV	9283	6607	0.56%	0.059%
97	16.763	2370	2376	2383	rBV	780956	1129096	95.31%	10.068%
98	16.863	2388	2393	2403	rVB	506172	784163	66.19%	6.992%
99	19.174	2781	2786	2793	rBV2	601612	854544	72.13%	7.620%
100	20.992	3090	3095	3104	rBV	845752	1184692	100.00%	10.564%


Sum of corrected areas: 11214420

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN030620\
Data File : BN010121.D
Acq On : 06 Mar 2020 16:17
Operator : CG/JU
Sample : L1641-10
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB6Z3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

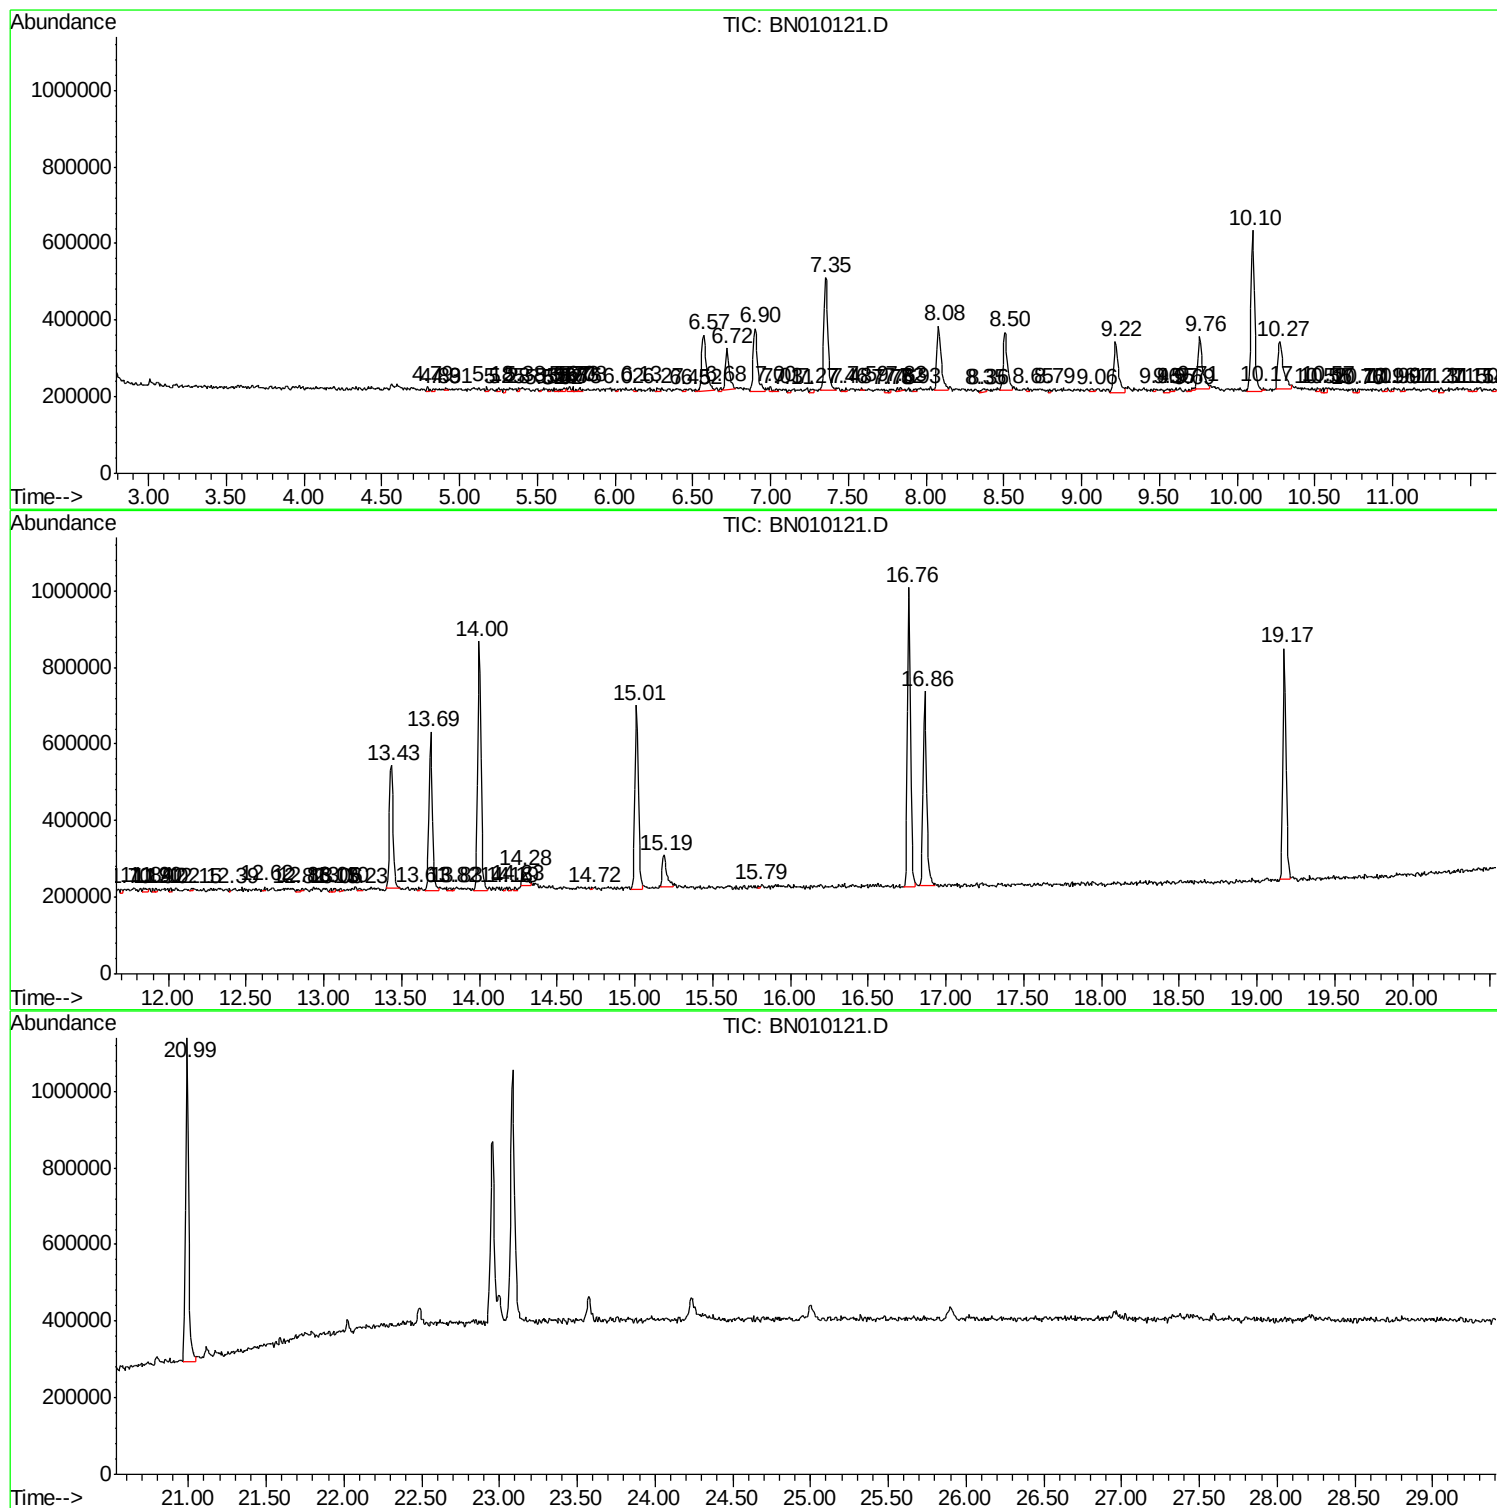

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030620\
Data File : BN010121.D
Acq On : 06 Mar 2020 16:17
Operator : CG/JU
Sample : L1641-10
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB6Z3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030620\
Data File : BN010121.D
Acq On : 06 Mar 2020 16:17
Operator : CG/JU
Sample : L1641-10
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB6Z3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc