

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN030620\
 Data File : BN010122.D
 Acq On : 06 Mar 2020 16:53
 Operator : CG/JU
 Sample : L1641-12
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB6Z5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.428	107	109	111	rBV	10940	12800	1.10%	0.091%
2	4.069	215	218	220	rBV	10725	15214	1.31%	0.109%
3	4.328	260	262	264	rVB	9702	7892	0.68%	0.056%
4	4.387	271	272	273	rBV	9613	5729	0.49%	0.041%
5	4.564	300	302	304	rBV2	14778	14777	1.27%	0.105%
6	5.140	398	400	402	rBV	7187	7391	0.64%	0.053%
7	5.346	433	435	436	rBV	7417	6249	0.54%	0.045%
8	5.428	448	449	452	rBV	5769	5669	0.49%	0.040%
9	5.516	462	464	467	rBV	9194	11363	0.98%	0.081%
10	5.575	472	474	476	rBV	11268	11440	0.99%	0.082%
11	5.599	476	478	482	rVB	9645	8139	0.70%	0.058%
12	5.646	482	486	487	rVB	9091	10250	0.88%	0.073%
13	5.664	487	489	490	rBV	9887	6336	0.55%	0.045%
14	5.722	498	499	502	rVB	6250	5435	0.47%	0.039%
15	5.811	513	514	516	rBV	8044	7352	0.63%	0.052%
16	5.922	529	533	534	rBV	5083	5386	0.46%	0.038%
17	6.034	550	552	554	rBV	7664	5479	0.47%	0.039%
18	6.058	554	556	558	rVB	13054	9649	0.83%	0.069%
19	6.081	558	560	561	rBV	9816	8499	0.73%	0.061%
20	6.128	565	568	569	rVB	9687	8925	0.77%	0.064%
21	6.146	569	571	572	rBV	7975	5611	0.48%	0.040%
22	6.305	596	598	599	rBV	8781	5345	0.46%	0.038%
23	6.322	599	601	603	rVV	5179	6504	0.56%	0.046%
24	6.458	622	624	626	rBV	10472	9739	0.84%	0.070%
25	6.563	637	642	651	rVV2	196272	374018	32.25%	2.670%
26	6.716	663	668	681	rBV2	144233	274990	23.71%	1.963%
27	6.846	689	690	691	rBV	11005	6132	0.53%	0.044%
28	6.899	694	699	709	rVV	221377	385309	33.22%	2.750%
29	7.158	741	743	745	rVB	7622	5388	0.46%	0.038%
30	7.234	754	756	759	rBV	9073	5726	0.49%	0.041%
31	7.352	771	776	786	rVV	288631	495295	42.71%	3.535%
32	7.552	807	810	812	rBV	7751	9110	0.79%	0.065%
33	7.652	825	827	830	rVB	7435	7197	0.62%	0.051%
34	7.763	843	846	850	rVB	5628	7869	0.68%	0.056%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030620\
 Data File : BN010122.D
 Acq On : 06 Mar 2020 16:53
 Operator : CG/JU
 Sample : L1641-12
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB6Z5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Title : SVOA CALIBRATION

35	7.852	860	861	863	rBV	8510	5986	0.52%	0.043%
36	7.969	880	881	884	rBV	8232	6755	0.58%	0.048%
37	8.034	887	892	893	rBV	7609	6340	0.55%	0.045%
38	8.075	894	899	910	rVV2	240429	450325	38.83%	3.214%
39	8.228	923	925	927	rBV	10850	9453	0.82%	0.067%
40	8.281	931	934	936	rVB	8707	6824	0.59%	0.049%
41	8.405	953	955	957	rBV	5153	6198	0.53%	0.044%
42	8.505	967	972	980	rBV2	214170	374909	32.33%	2.676%
43	8.628	991	993	996	rVB	7468	6195	0.53%	0.044%
44	8.710	1005	1007	1009	rBV	6765	6773	0.58%	0.048%
45	8.946	1045	1047	1049	rBV	9508	6501	0.56%	0.046%
46	8.999	1054	1056	1059	rBV	4732	5648	0.49%	0.040%
47	9.169	1084	1085	1088	rBV	5358	6083	0.52%	0.043%
48	9.216	1088	1093	1105	rVV	174069	335176	28.90%	2.392%
49	9.322	1109	1111	1113	rBV	6455	5802	0.50%	0.041%
50	9.452	1130	1133	1134	rVB	7743	6974	0.60%	0.050%
51	9.505	1140	1142	1145	rVB	8983	9037	0.78%	0.065%
52	9.581	1153	1155	1157	rVB	9883	5652	0.49%	0.040%
53	9.693	1170	1174	1175	rBV	8572	11599	1.00%	0.083%
54	9.752	1179	1184	1193	rVV	202292	390979	33.71%	2.791%
55	9.946	1214	1217	1218	rBV	9451	8087	0.70%	0.058%
56	10.022	1228	1230	1231	rVB	9283	5436	0.47%	0.039%
57	10.099	1235	1243	1251	rBV	405595	701714	60.51%	5.009%
58	10.263	1266	1271	1281	rBV	184532	429786	37.06%	3.068%
59	10.440	1299	1301	1302	rBV	9279	6860	0.59%	0.049%
60	10.475	1305	1307	1309	rBV	12719	14119	1.22%	0.101%
61	10.604	1327	1329	1332	rBV	8194	10556	0.91%	0.075%
62	10.704	1341	1346	1347	rBV	7831	10943	0.94%	0.078%
63	10.722	1347	1349	1354	rVV	7137	9598	0.83%	0.069%
64	10.816	1362	1365	1366	rBV	10475	12069	1.04%	0.086%
65	10.928	1382	1384	1385	rBV	11822	6443	0.56%	0.046%
66	11.022	1396	1400	1401	rBV	8268	9956	0.86%	0.071%
67	11.104	1413	1414	1416	rBV	13262	6021	0.52%	0.043%
68	11.175	1424	1426	1429	rBV	6128	7220	0.62%	0.052%
69	11.234	1434	1436	1441	rBV	11565	15369	1.33%	0.110%
70	11.451	1472	1473	1477	rBV	9578	9576	0.83%	0.068%
71	11.522	1484	1485	1487	rBV	6696	5375	0.46%	0.038%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030620\
 Data File : BN010122.D
 Acq On : 06 Mar 2020 16:53
 Operator : CG/JU
 Sample : L1641-12
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB6Z5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Title : SVOA CALIBRATION

72	11.704	1514	1516	1520	rVB	10491	9893	0.85%	0.071%
73	11.740	1520	1522	1524	rBV	8929	8010	0.69%	0.057%
74	11.904	1547	1550	1551	rBV	10502	7716	0.67%	0.055%
75	12.016	1566	1569	1571	rVB	7549	8522	0.73%	0.061%
76	12.304	1614	1618	1620	rBV	7397	8566	0.74%	0.061%
77	12.475	1646	1647	1649	rVB	11929	5941	0.51%	0.042%
78	12.657	1676	1678	1681	rBV	8335	11401	0.98%	0.081%
79	12.687	1681	1683	1685	rBV	8978	9399	0.81%	0.067%
80	12.828	1705	1707	1709	rBV	8716	6178	0.53%	0.044%
81	12.887	1715	1717	1721	rVB	7432	7333	0.63%	0.052%
82	13.081	1748	1750	1753	rVB	8071	5301	0.46%	0.038%
83	13.293	1784	1786	1788	rBV	9083	7839	0.68%	0.056%
84	13.328	1790	1792	1794	rVB	8229	7785	0.67%	0.056%
85	13.428	1804	1809	1823	rVB	445559	740420	63.84%	5.285%
86	13.687	1847	1853	1860	rVV	539170	794415	68.50%	5.671%
87	13.863	1881	1883	1885	rBV	8861	7110	0.61%	0.051%
88	13.998	1900	1906	1916	rVB	623985	923112	79.60%	6.589%
89	14.092	1920	1922	1924	rBV	9130	6795	0.59%	0.049%
90	14.145	1929	1931	1936	rBV	6941	9263	0.80%	0.066%
91	14.275	1948	1953	1961	rBV3	87779	215455	18.58%	1.538%
92	14.704	2024	2026	2027	rBV	10524	7520	0.65%	0.054%
93	14.781	2038	2039	2045	rBV	10502	11374	0.98%	0.081%
94	15.010	2072	2078	2086	rVB	658453	1000056	86.23%	7.138%
95	15.181	2102	2107	2116	rBV3	139030	272873	23.53%	1.948%
96	16.763	2370	2376	2382	rBV	738558	1064747	91.81%	7.600%
97	16.863	2387	2393	2405	rVB	688508	1077028	92.87%	7.688%
98	19.175	2781	2786	2795	rBV	842706	1159717	100.00%	8.278%
99	20.986	3090	3094	3104	rBV2	752804	1085560	93.61%	7.749%
100	22.945	3424	3427	3433	rVB2	566632	825663	71.20%	5.894%


Sum of corrected areas: 14009536

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN030620\
Data File : BN010122.D
Acq On : 06 Mar 2020 16:53
Operator : CG/JU
Sample : L1641-12
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB6Z5

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

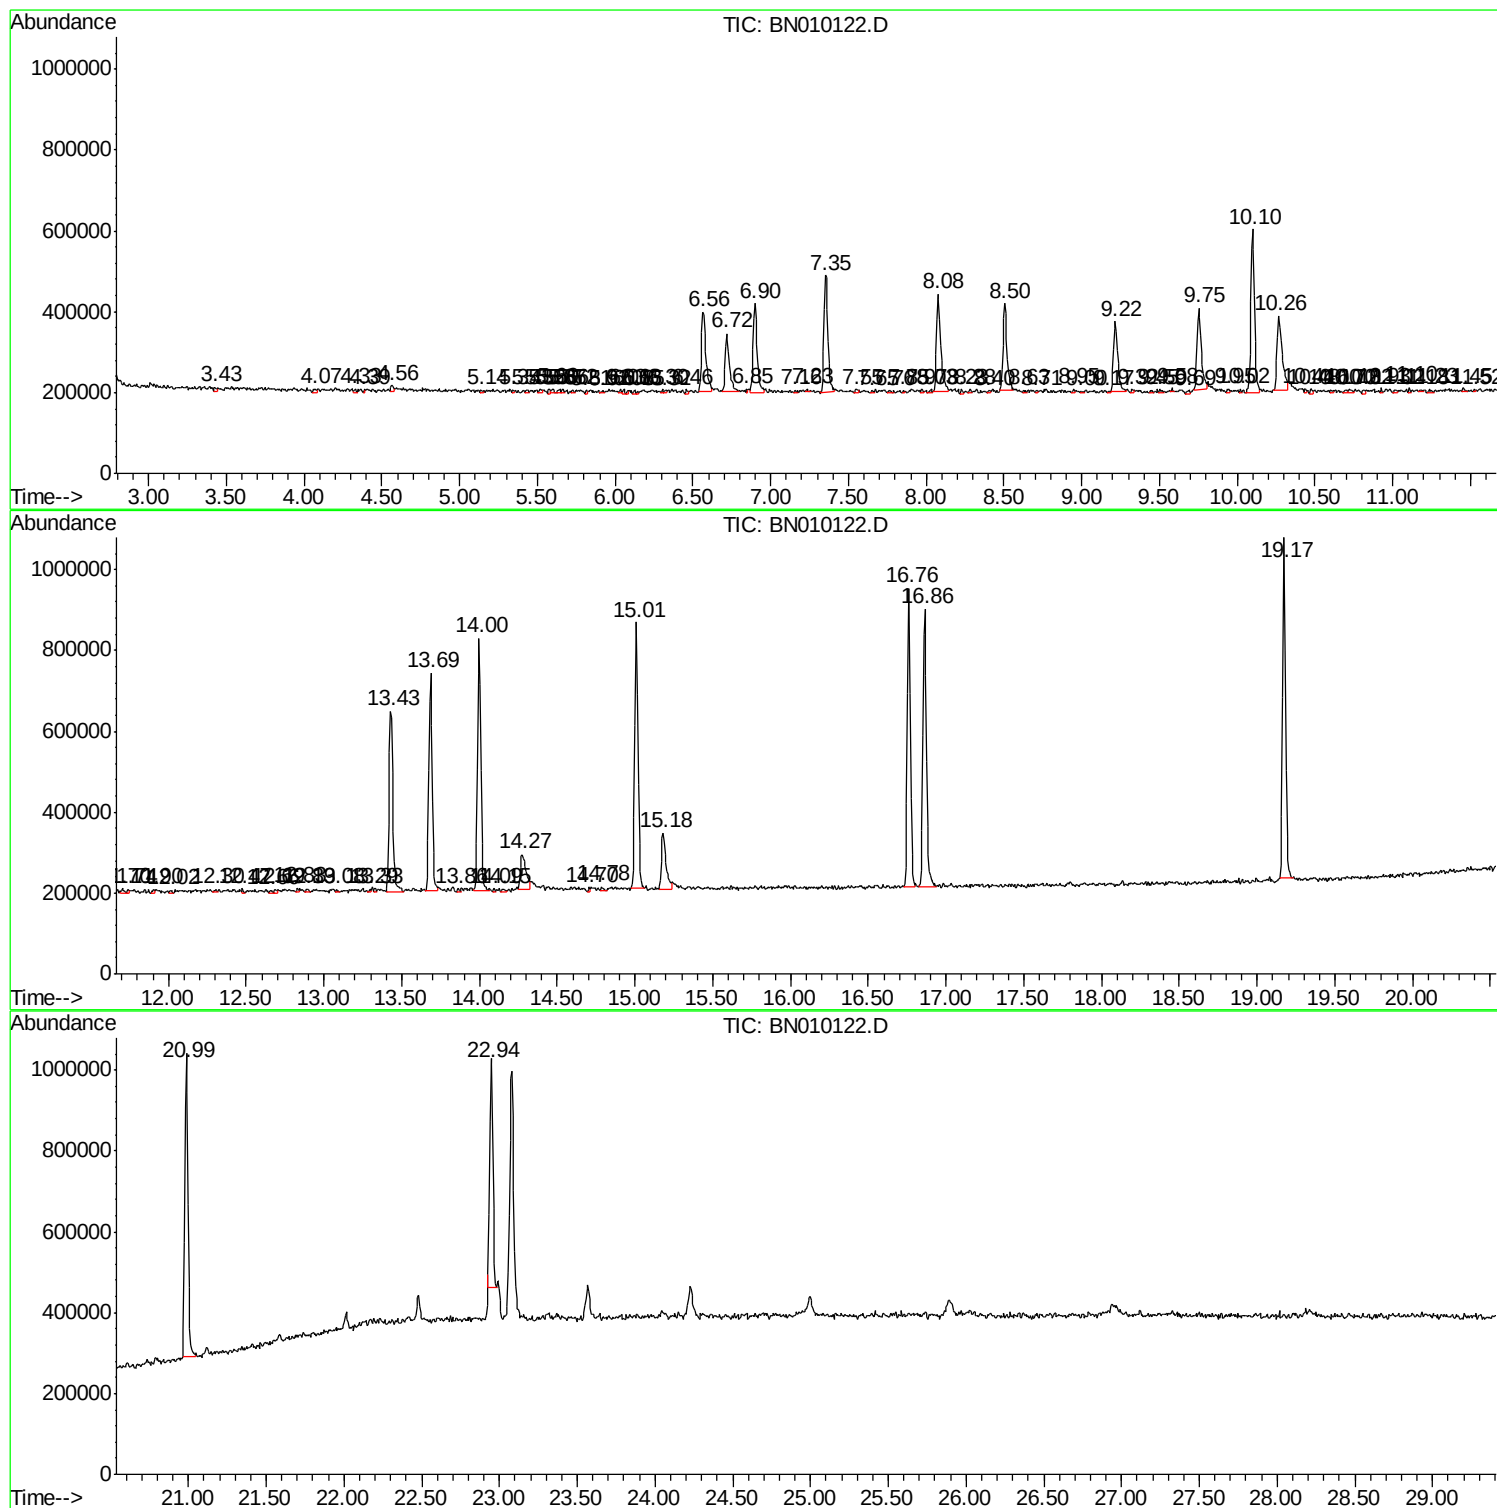

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030620\
Data File : BN010122.D
Acq On : 06 Mar 2020 16:53
Operator : CG/JU
Sample : L1641-12
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB6Z5

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030620\
Data File : BN010122.D
Acq On : 06 Mar 2020 16:53
Operator : CG/JU
Sample : L1641-12
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB6Z5

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc