

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN030620\
 Data File : BN010125.D
 Acq On : 06 Mar 2020 18:42
 Operator : CG/JU
 Sample : TESTBL02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 TESTBL02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.687	151	153	157	rBV	9058	12798	1.28%	0.106%
2	3.964	198	200	202	rVB	9549	7402	0.74%	0.061%
3	4.199	238	240	241	rBV	8390	7806	0.78%	0.065%
4	4.464	283	285	287	rBV	9025	8579	0.86%	0.071%
5	4.599	306	308	309	rBV	8090	4872	0.49%	0.040%
6	4.670	318	320	321	rBV	5100	4860	0.49%	0.040%
7	4.899	357	359	362	rBV	8613	9588	0.96%	0.079%
8	4.922	362	363	364	rBV	7902	4258	0.43%	0.035%
9	5.099	390	393	394	rBV	9937	8266	0.83%	0.068%
10	5.152	400	402	404	rVB	7652	5241	0.52%	0.043%
11	5.270	421	422	425	rBV	5276	4827	0.48%	0.040%
12	5.381	440	441	442	rBV	8164	5126	0.51%	0.042%
13	5.399	442	444	445	rVV	11880	6779	0.68%	0.056%
14	5.417	445	447	449	rVV	4423	4545	0.46%	0.038%
15	5.505	460	462	464	rBV	4190	5168	0.52%	0.043%
16	5.922	530	533	534	rBV	6270	6689	0.67%	0.055%
17	5.999	544	546	548	rVB	8930	6329	0.63%	0.052%
18	6.028	548	551	553	rBV	9407	12904	1.29%	0.107%
19	6.287	591	595	596	rBV	5664	5757	0.58%	0.048%
20	6.375	607	610	611	rBV	9481	8600	0.86%	0.071%
21	6.393	611	613	614	rBV	8256	6471	0.65%	0.054%
22	6.475	625	627	630	rVB	11079	7923	0.79%	0.066%
23	6.505	630	632	633	rBV	6396	4394	0.44%	0.036%
24	6.534	635	637	638	rBV	8038	7220	0.72%	0.060%
25	6.564	638	642	652	rVV	158428	308690	30.91%	2.555%
26	6.717	664	668	677	rBV2	138042	225162	22.54%	1.864%
27	6.899	694	699	709	rBV	195044	334539	33.50%	2.769%
28	7.187	747	748	750	rBV	7210	4689	0.47%	0.039%
29	7.293	763	766	769	rBV	5625	6894	0.69%	0.057%
30	7.352	769	776	787	rBV2	251887	464324	46.49%	3.844%
31	7.652	825	827	829	rBV	6455	5393	0.54%	0.045%
32	7.828	855	857	858	rVB	10104	6248	0.63%	0.052%
33	7.846	858	860	863	rBV	5798	6781	0.68%	0.056%
34	7.869	863	864	866	rVV	8628	5690	0.57%	0.047%

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN030620\
 Data File : BN010125.D
 Acq On : 06 Mar 2020 18:42
 Operator : CG/JU
 Sample : TESTBL02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 TESTBL02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Title : SVOA CALIBRATION

35	7.893	866	868	870	rVB	7812	7058	0.71%	0.058%
36	8.016	887	889	891	rVB	8059	6411	0.64%	0.053%
37	8.040	891	893	895	rBV	4817	5188	0.52%	0.043%
38	8.075	895	899	912	rVV2	192901	377846	37.83%	3.128%
39	8.164	912	914	918	rVV	8320	6939	0.69%	0.057%
40	8.199	918	920	924	rVB	7608	6431	0.64%	0.053%
41	8.246	924	928	931	rVB	11372	12140	1.22%	0.100%
42	8.275	931	933	935	rBV	7909	5963	0.60%	0.049%
43	8.358	944	947	950	rBV	10688	15295	1.53%	0.127%
44	8.505	966	972	981	rBV2	182359	341406	34.18%	2.826%
45	8.605	988	989	991	rVB	9061	4555	0.46%	0.038%
46	8.628	991	993	995	rBV	6906	7125	0.71%	0.059%
47	8.675	998	1001	1002	rBV	4498	4320	0.43%	0.036%
48	8.769	1015	1017	1020	rBV	7709	8350	0.84%	0.069%
49	8.846	1029	1030	1035	rVB	5837	5662	0.57%	0.047%
50	8.934	1043	1045	1049	rVB	8383	9660	0.97%	0.080%
51	8.969	1049	1051	1054	rBV	8736	10044	1.01%	0.083%
52	9.046	1061	1064	1066	rBV	5849	6224	0.62%	0.052%
53	9.081	1066	1070	1071	rVV	5264	4580	0.46%	0.038%
54	9.140	1076	1080	1084	rVB	7195	12411	1.24%	0.103%
55	9.216	1088	1093	1102	rBV3	136653	264453	26.48%	2.189%
56	9.369	1117	1119	1120	rBV	6398	4649	0.47%	0.038%
57	9.605	1158	1159	1161	rBV	7240	5721	0.57%	0.047%
58	9.752	1180	1184	1197	rVV	146833	320465	32.09%	2.653%
59	10.099	1237	1243	1253	rBV	351893	586572	58.73%	4.856%
60	10.193	1258	1259	1262	rVB	8354	7352	0.74%	0.061%
61	10.269	1266	1272	1296	rBV2	134520	397601	39.81%	3.291%
62	10.416	1296	1297	1300	rVB	9463	8715	0.87%	0.072%
63	10.446	1300	1302	1303	rBV	6847	5702	0.57%	0.047%
64	10.516	1312	1314	1317	rBV	10267	13622	1.36%	0.113%
65	10.622	1330	1332	1333	rBV	6459	4318	0.43%	0.036%
66	10.710	1345	1347	1348	rBV	7469	5982	0.60%	0.050%
67	10.916	1378	1382	1383	rBV	6445	6729	0.67%	0.056%
68	10.946	1385	1387	1389	rVB	7487	5971	0.60%	0.049%
69	10.975	1389	1392	1395	rBV	6005	8275	0.83%	0.069%
70	11.069	1404	1408	1409	rBV	6563	6677	0.67%	0.055%
71	11.128	1415	1418	1419	rBV	6885	5824	0.58%	0.048%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030620\
 Data File : BN010125.D
 Acq On : 06 Mar 2020 18:42
 Operator : CG/JU
 Sample : TESTBL02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 TESTBL02

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Title : SVOA CALIBRATION

72	11.269	1440	1442	1443	rBV	8015	4439	0.44%	0.037%
73	11.387	1458	1462	1463	rBV	7431	7002	0.70%	0.058%
74	11.499	1479	1481	1483	rBV	7103	5508	0.55%	0.046%
75	11.522	1483	1485	1486	rVB	7449	4708	0.47%	0.039%
76	11.628	1501	1503	1504	rBV	5833	4655	0.47%	0.039%
77	11.669	1508	1510	1513	rVB	5936	6456	0.65%	0.053%
78	11.699	1513	1515	1517	rBV	6167	7184	0.72%	0.059%
79	11.946	1555	1557	1558	rBV	6773	4282	0.43%	0.035%
80	12.175	1592	1596	1597	rBV	10001	10272	1.03%	0.085%
81	12.410	1634	1636	1637	rBV	7260	5685	0.57%	0.047%
82	12.499	1648	1651	1655	rBV	9955	13532	1.35%	0.112%
83	12.557	1660	1661	1665	rBV	11212	12233	1.22%	0.101%
84	12.593	1665	1667	1669	rBV	6218	4446	0.45%	0.037%
85	12.793	1700	1701	1702	rBV	10489	5526	0.55%	0.046%
86	13.128	1756	1758	1761	rBV	7861	7685	0.77%	0.064%
87	13.257	1776	1780	1782	rBV	9656	10921	1.09%	0.090%
88	13.428	1804	1809	1819	rBV	382374	633615	63.44%	5.245%
89	13.563	1830	1832	1833	rBV	10491	7124	0.71%	0.059%
90	13.687	1844	1853	1862	rBV	441191	660849	66.17%	5.471%
91	13.998	1900	1906	1913	rBV2	542047	793900	79.49%	6.572%
92	14.281	1949	1954	1963	rBV3	58416	153244	15.34%	1.269%
93	15.010	2072	2078	2087	rBV	536468	863320	86.44%	7.147%
94	15.181	2103	2107	2115	rBV2	106256	219909	22.02%	1.820%
95	15.963	2239	2240	2241	rBV	9628	4814	0.48%	0.040%
96	16.757	2370	2375	2383	rBV	627304	901943	90.31%	7.466%
97	16.863	2387	2393	2405	rVB	611138	933638	93.48%	7.729%
98	19.175	2781	2786	2793	rBV	699539	984682	98.59%	8.151%
99	20.992	3090	3095	3108	rBV	666102	998769	100.00%	8.268%
100	22.951	3424	3428	3433	rBV	501197	758558	75.95%	6.279%


Sum of corrected areas: 12079947

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN030620\
Data File : BN010125.D
Acq On : 06 Mar 2020 18:42
Operator : CG/JU
Sample : TESTBL02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
TESTBL02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

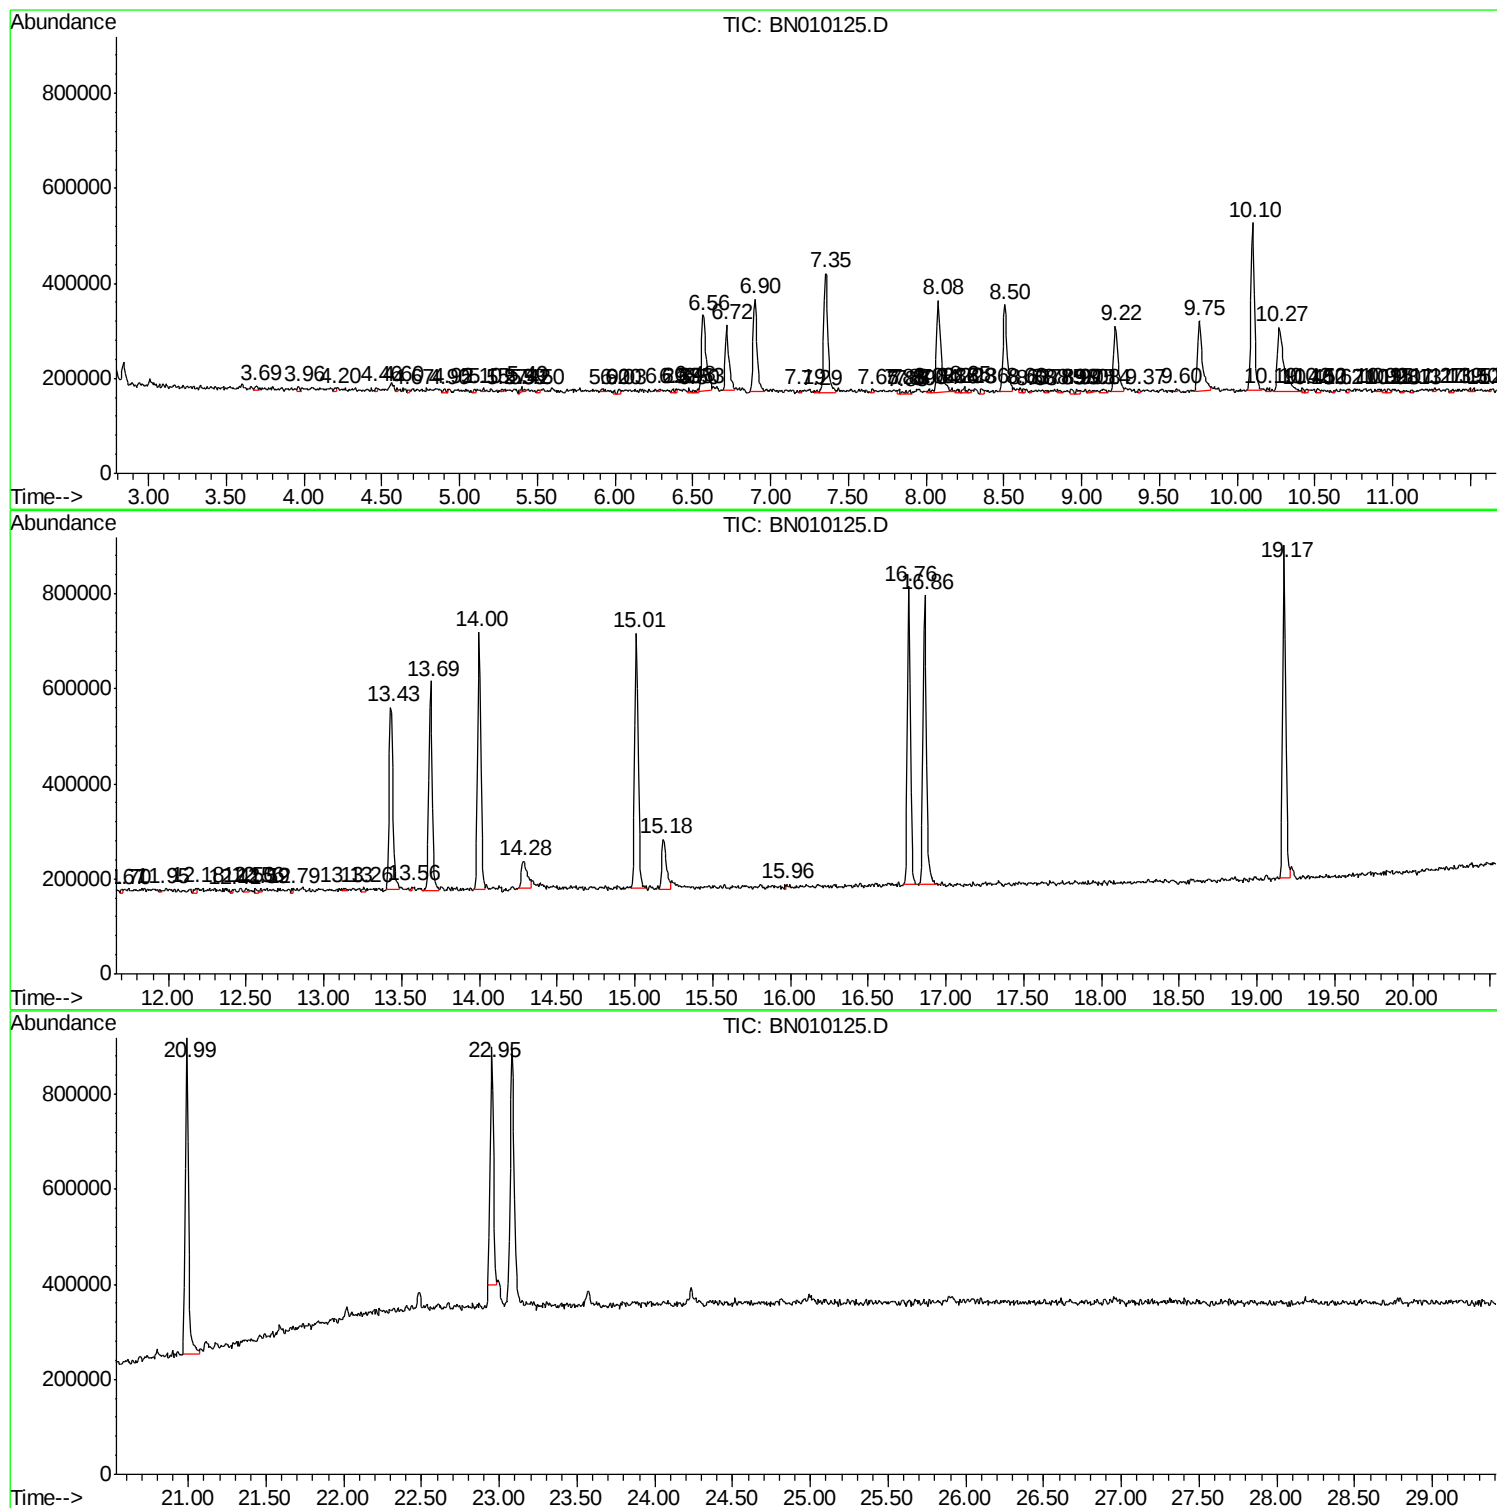

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030620\
Data File : BN010125.D
Acq On : 06 Mar 2020 18:42
Operator : CG/JU
Sample : TESTBL02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
TESTBL02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN030620\
Data File : BN010125.D
Acq On : 06 Mar 2020 18:42
Operator : CG/JU
Sample : TESTBL02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
TESTBL02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc